


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG053024\
Data File : BG061360.D
Acq On : 30 May 2024 15:08
Operator : MA/JU
Sample : DFTPP574
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP574

Integration File: LSCINT.P

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG052124.MA.M
Title : SVOA CALIBRATION
Last Update : Thu May 30 22:54:48 2024

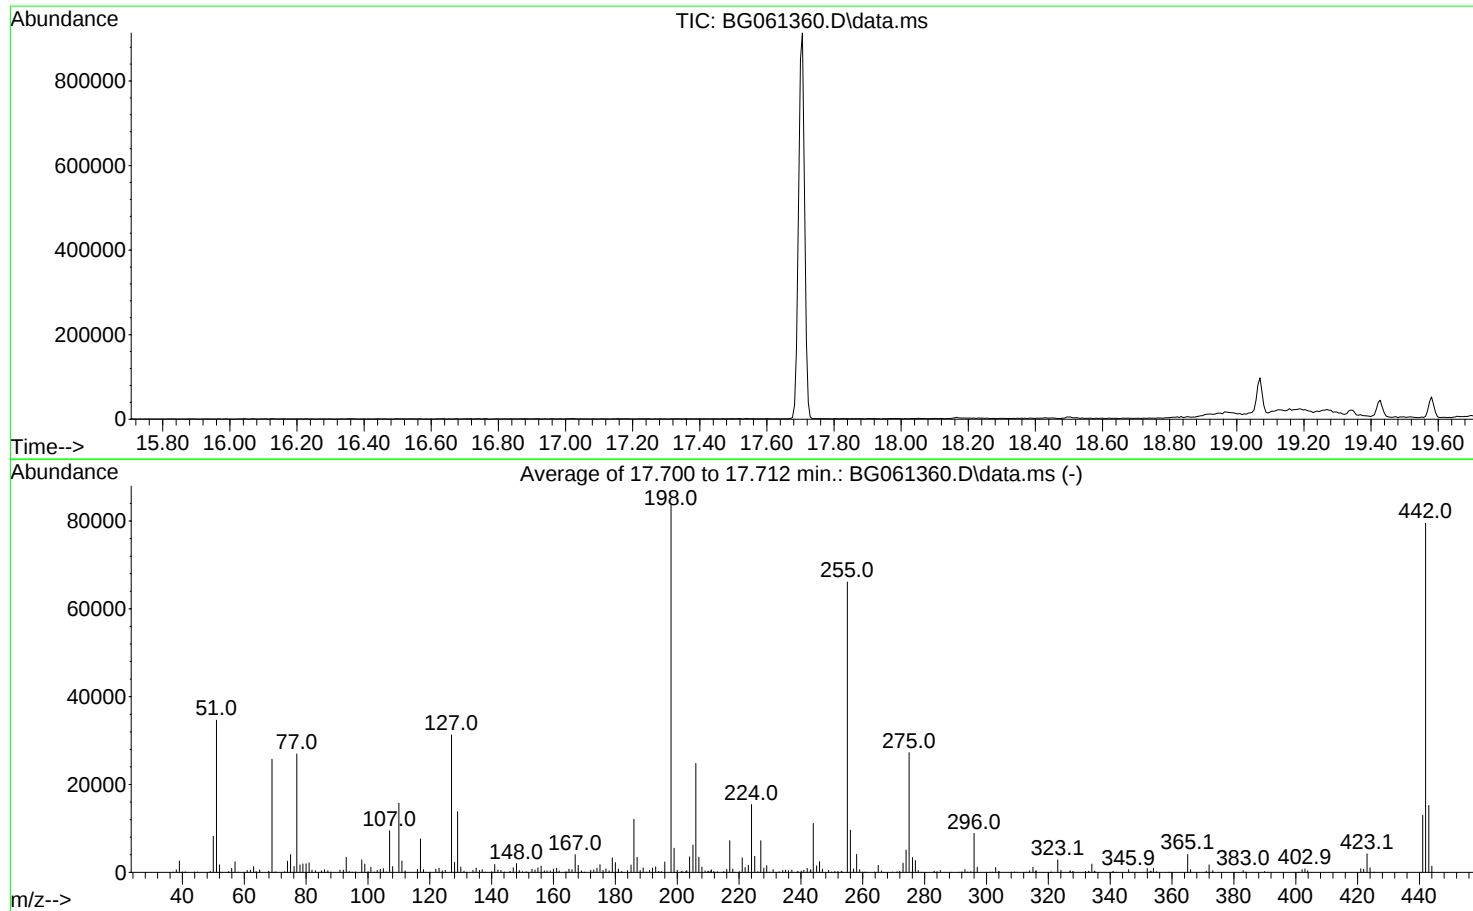

AutoFind: Scans 2504, 2505, 2506; Background Corrected with Scan 2498

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.4	34653	PASS
68	69	0.00	2	1.0	249	PASS
69	198	0.00	100	30.7	25747	PASS
70	69	0.00	2	0.5	128	PASS
127	198	10	80	37.4	31283	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	83755	PASS
199	198	5	9	6.6	5487	PASS
275	198	10	60	32.5	27251	PASS
365	198	1	100	4.9	4090	PASS
441	198	0.01	100	15.5	13022	PASS
442	198	50	100	94.9	79485	PASS
443	442	15	24	19.2	15227	PASS

Scan 2498 (17.665 min): BG061360.D\data.ms
DFTPP574

m/z	Abundance
43.10	212.0
43.90	654.0
107.10	153.0
207.10	262.0

Instrument :
BNA_G
ClientSampleId :
DFTPP574

m/z	Abundance
37.00	187.0
38.10	516.0
39.00	3063.0
40.90	187.0
44.00	710.0
50.00	10316.0
51.00	43632.0
52.00	2556.0
55.00	299.0
55.90	1017.0
57.00	3209.0
58.00	178.0
60.90	601.0
62.10	474.0
63.00	1783.0
65.10	770.0
69.00	32016.0
69.80	163.0
72.90	275.0
74.00	3209.0
75.00	4919.0
76.10	1599.0
77.00	32704.0
78.00	1843.0
79.00	2574.0
80.00	2539.0
81.00	2870.0
81.90	493.0
83.00	495.0
85.00	421.0
86.00	815.0
87.00	521.0
90.90	604.0
92.00	517.0
93.00	3937.0
94.00	267.0
95.90	168.0
98.00	3681.0
99.00	2474.0
100.00	191.0
100.90	1140.0
102.10	184.0
103.00	597.0
104.00	859.0
105.00	947.0
107.00	11983.0
108.00	1661.0
110.00	19200.0
111.00	2905.0
112.00	515.0
116.00	866.0
117.00	9436.0
118.00	743.0
120.10	163.0
122.00	942.0
123.00	1208.0
124.00	444.0
125.00	538.0
127.00	37664.0
128.00	2640.0
129.00	17496.0
130.00	1309.0
131.10	323.0
134.00	533.0
135.00	1439.0
136.10	550.0
136.90	778.0
138.00	204.0
139.90	217.0
141.00	2312.0
142.00	532.0
143.00	570.0
145.80	315.0
147.00	1318.0
148.00	2535.0
149.00	409.0
150.00	244.0
151.20	263.0
153.00	957.0
154.00	797.0
154.90	1300.0
156.00	1754.0
157.00	441.0
157.90	519.0
158.90	297.0
160.00	851.0
161.00	1175.0
161.90	368.0
163.80	183.0
164.40	270.0
165.00	701.0
165.90	682.0

Instrument :
BNA_G
ClientSampleId :
DFTPP574

167.00	5023.0
168.00	1777.0
169.10	300.0
170.00	188.0
172.10	596.0
173.10	480.0
174.00	1074.0
175.10	2246.0
176.00	488.0
176.90	970.0
178.00	494.0
179.00	3376.0
180.00	2422.0
181.00	1244.0
181.90	204.0
184.00	505.0
185.10	2255.0
186.00	13753.0
187.10	4418.0
188.00	518.0
189.00	1219.0
191.00	484.0
192.00	1092.0
193.10	1327.0
193.90	475.0
194.90	256.0
196.00	2526.0
198.00	95000.0
199.00	6079.0
200.00	530.0
201.90	279.0
202.80	641.0
204.00	3669.0
205.10	7601.0
206.00	27456.0
207.00	4278.0
208.00	1347.0
209.00	462.0
210.20	575.0
210.90	1020.0
212.10	234.0
214.90	415.0
216.00	668.0
217.00	8041.0
217.90	971.0
218.80	165.0
220.10	491.0
221.00	3708.0
222.00	1095.0
223.00	1956.0
224.00	17496.0
225.00	4225.0
226.10	584.0
227.00	7576.0
228.00	1222.0
229.00	1534.0
229.90	270.0
231.00	739.0
232.90	306.0
234.10	410.0
235.10	580.0
235.90	375.0
237.10	627.0
239.10	340.0
240.20	283.0
241.00	567.0
242.00	944.0
243.00	842.0
244.00	11628.0
245.10	1526.0
246.00	2549.0
247.00	843.0
248.90	487.0
249.90	211.0
250.90	240.0
252.00	193.0
253.30	374.0
255.00	71144.0
256.00	10228.0
257.10	832.0
258.00	4099.0
259.10	783.0
259.90	233.0
261.10	154.0
265.00	1910.0
266.00	428.0
271.10	221.0
272.00	160.0
273.00	2263.0
274.00	5383.0
275.00	27848.0
276.00	3691.0
277.00	2429.0
277.90	475.0
279.00	156.0
282.90	185.0

Instrument :
BNA_G
ClientSampleId :
DFTPP574

284.20	152.0
285.00	553.0
292.10	158.0
293.00	920.0
293.80	217.0
296.00	8902.0
297.00	1259.0
302.90	1000.0
304.00	308.0
308.00	175.0
314.00	383.0
315.00	1382.0
315.90	696.0
320.80	233.0
323.10	3142.0
324.10	645.0
326.90	486.0
327.90	295.0
328.10	289.0
332.00	257.0
333.00	405.0
334.10	2164.0
334.90	564.0
340.90	411.0
345.90	780.0
351.90	749.0
352.90	335.0
353.20	360.0
354.10	968.0
355.00	258.0
365.10	4407.0
366.00	656.0
371.10	317.0
372.00	1319.0
373.10	336.0
383.00	393.0
390.00	181.0
400.90	157.0
402.20	634.0
402.90	741.0
403.90	283.0
421.00	684.0
421.90	710.0
423.00	3759.0
424.10	731.0
441.10	11147.0
442.00	69864.0
443.00	14630.0
444.00	1100.0

Instrument :
BNA_G
ClientSampleId :
DFTPP574

m/z	Abundance
38.00	773.0
39.00	3172.0
40.00	238.0
41.10	256.0
44.00	687.0
44.90	179.0
49.00	506.0
50.00	10050.0
51.00	40056.0
52.00	1777.0
52.90	155.0
54.90	305.0
56.00	1137.0
57.00	2608.0
61.00	518.0
61.90	555.0
63.00	1402.0
63.90	326.0
64.90	794.0
67.90	748.0
69.00	30656.0
70.20	384.0
73.10	296.0
74.00	2791.0
75.00	5131.0
76.00	1671.0
77.00	31696.0
78.10	2027.0
78.90	2337.0
80.00	2411.0
81.00	2250.0
81.90	589.0
83.10	590.0
84.90	369.0
85.90	629.0
87.10	407.0
88.00	177.0
91.00	578.0
92.10	619.0
93.00	3950.0
93.80	284.0
94.90	177.0
98.00	3210.0
99.00	2126.0
100.00	270.0
101.00	1596.0
103.00	427.0
104.00	854.0
105.00	1117.0
107.00	11160.0
108.00	1580.0
110.00	18656.0
111.00	3228.0
112.00	592.0
116.00	781.0
117.00	8721.0
117.90	819.0
118.90	158.0
121.90	953.0
123.00	1057.0
124.00	468.0
125.00	503.0
127.00	37440.0
128.00	2684.0
129.00	14998.0
130.00	1437.0
131.00	180.0
131.80	156.0
133.90	414.0
135.00	1043.0
136.00	473.0
137.00	708.0
140.10	243.0
141.00	1946.0
142.00	736.0
143.00	482.0
144.20	172.0
146.00	530.0
147.00	1115.0
148.00	2445.0
148.90	525.0
150.00	160.0
151.10	315.0
151.70	158.0
153.10	798.0
154.00	489.0
155.00	1238.0
156.00	1748.0
157.10	420.0
157.90	350.0
159.00	428.0
160.00	971.0

Instrument :
BNA_G
ClientSampleId :
DFTPP574

161.00	1264.0
161.80	446.0
164.90	974.0
166.00	723.0
167.00	4590.0
168.00	1941.0
169.00	480.0
172.10	461.0
173.00	656.0
174.10	1083.0
175.00	1766.0
176.00	481.0
177.00	823.0
177.90	355.0
179.00	4103.0
180.00	2874.0
181.00	698.0
182.10	284.0
184.00	416.0
185.00	1528.0
186.00	13892.0
187.00	3575.0
188.00	538.0
189.00	1263.0
190.10	199.0
191.10	474.0
192.00	1119.0
193.10	1438.0
194.10	351.0
195.00	328.0
196.00	2849.0
198.00	99856.0
199.00	6533.0
200.10	565.0
201.30	278.0
201.60	338.0
203.00	768.0
204.00	4507.0
205.10	6878.0
206.00	29408.0
207.00	4576.0
208.00	1335.0
209.00	414.0
209.90	644.0
211.10	1271.0
211.70	428.0
213.00	246.0
215.10	316.0
216.10	945.0
217.00	8592.0
218.00	859.0
221.00	3897.0
221.80	1336.0
223.00	1705.0
224.00	17696.0
225.10	4000.0
227.00	8974.0
228.00	1034.0
228.90	1813.0
230.90	720.0
234.10	512.0
235.10	662.0
236.00	505.0
237.00	684.0
238.70	239.0
239.10	164.0
240.10	227.0
241.00	668.0
242.10	1166.0
243.20	1072.0
244.00	13640.0
245.10	1515.0
246.00	2964.0
247.00	686.0
249.00	524.0
251.00	235.0
251.90	340.0
253.00	569.0
255.00	79024.0
256.00	11601.0
257.10	934.0
258.00	5382.0
259.00	627.0
263.80	177.0
265.00	1617.0
266.10	307.0
269.60	201.0
271.10	190.0
271.90	371.0
273.00	2627.0
274.00	6223.0
275.00	32616.0
276.00	3822.0
277.00	3338.0
278.00	628.0
283.10	509.0

Instrument :
BNA_G
ClientSampleId :
DFTPP574

284.00	188.0
285.10	377.0
290.90	150.0
292.00	176.0
293.10	541.0
295.00	337.0
296.00	11107.0
297.00	1368.0
301.20	205.0
302.00	173.0
303.00	1434.0
303.90	454.0
309.10	164.0
309.90	155.0
312.90	197.0
313.90	392.0
315.00	1329.0
316.10	668.0
321.10	268.0
323.00	3338.0
324.00	463.0
327.10	651.0
327.90	363.0
331.90	234.0
333.10	391.0
334.00	2133.0
335.10	477.0
340.90	382.0
342.00	152.0
346.00	765.0
347.10	172.0
352.00	1051.0
353.00	582.0
353.90	959.0
365.00	4641.0
366.00	688.0
371.00	276.0
372.00	1804.0
373.20	368.0
383.00	691.0
383.90	192.0
390.00	252.0
391.00	244.0
402.00	772.0
403.00	1029.0
403.80	373.0
421.00	1114.0
421.90	779.0
423.00	5017.0
424.00	1266.0
425.30	220.0
441.00	15611.0
442.00	98528.0
443.00	18240.0
444.00	1850.0

Instrument :
BNA_G
ClientSampleId :
DFTPP574

m/z	Abundance
38.10	415.0
39.10	1551.0
40.00	156.0
44.00	752.0
49.00	181.0
50.00	4318.0
51.00	20272.0
52.00	832.0
56.00	584.0
57.00	1371.0
61.00	175.0
62.00	395.0
63.10	642.0
63.80	245.0
65.00	227.0
69.00	14568.0
74.00	1658.0
75.00	2132.0
76.20	790.0
77.10	16440.0
78.10	1237.0
79.00	938.0
80.00	1008.0
81.00	1437.0
81.90	413.0
84.90	312.0
86.00	426.0
87.00	155.0
90.90	333.0
92.00	354.0
92.90	2377.0
94.10	210.0
96.10	177.0
98.00	1670.0
99.00	1122.0
101.00	847.0
103.00	263.0
104.00	329.0
105.00	414.0
105.90	291.0
107.00	5686.0
108.10	721.0
110.00	9371.0
111.00	1633.0
116.10	481.0
117.00	4671.0
118.00	296.0
121.80	345.0
123.00	606.0
124.00	219.0
125.00	391.0
127.00	18744.0
128.00	1587.0
129.00	8964.0
130.00	845.0
131.00	223.0
133.90	472.0
135.00	464.0
136.00	353.0
137.00	365.0
139.90	154.0
141.00	1120.0
142.10	351.0
143.10	247.0
147.00	756.0
148.10	984.0
149.00	329.0
149.80	154.0
153.00	427.0
154.10	368.0
155.00	610.0
156.00	715.0
157.10	288.0
158.00	277.0
159.00	212.0
160.00	432.0
161.00	453.0
161.80	159.0
164.00	180.0
165.10	465.0
166.00	462.0
167.00	2571.0
168.00	1117.0
169.10	158.0
172.00	379.0
172.90	473.0
174.10	641.0
175.00	1207.0
176.00	349.0
177.00	465.0
178.10	250.0
179.00	2429.0

Instrument :
BNA_G
ClientSampleId :
DFTPP574

180.00	1342.0
181.10	411.0
182.00	246.0
183.80	247.0
185.10	1264.0
186.00	8600.0
187.00	2311.0
188.00	274.0
189.00	614.0
191.10	351.0
192.00	725.0
193.00	930.0
194.00	173.0
196.10	1713.0
198.00	56408.0
199.00	3848.0
199.90	332.0
201.30	271.0
201.50	263.0
203.10	435.0
204.00	2423.0
205.10	4224.0
206.10	17544.0
207.10	2288.0
208.00	937.0
209.00	208.0
210.20	298.0
211.00	433.0
212.90	182.0
215.90	501.0
217.00	5022.0
218.00	530.0
221.00	2389.0
222.00	818.0
222.90	1107.0
224.10	11150.0
225.00	2732.0
227.00	5133.0
228.00	739.0
229.00	1270.0
231.10	390.0
233.00	185.0
234.10	441.0
234.90	296.0
236.00	224.0
237.10	208.0
238.90	306.0
240.00	319.0
240.80	226.0
242.10	659.0
243.10	751.0
244.10	8184.0
245.10	1398.0
246.00	1831.0
246.90	609.0
249.00	296.0
251.10	183.0
251.90	162.0
253.10	232.0
255.00	48168.0
256.00	6866.0
257.00	667.0
258.00	2756.0
258.90	501.0
260.70	188.0
265.00	1237.0
266.10	224.0
272.00	226.0
273.00	1496.0
274.00	3560.0
275.00	21288.0
276.10	2535.0
277.00	2335.0
278.00	198.0
283.10	249.0
283.80	170.0
285.10	434.0
288.80	156.0
293.00	497.0
294.00	153.0
294.90	267.0
296.00	6602.0
297.00	921.0
303.00	850.0
304.20	189.0
309.00	176.0
313.90	373.0
315.00	790.0
316.00	510.0
323.00	2099.0
324.00	346.0
327.00	453.0
332.10	185.0
333.30	199.0
334.10	1393.0
334.90	287.0

Instrument :
BNA_G
ClientSampleId :
DFTPP574

341.10	256.0
345.90	340.0
352.00	791.0
353.20	390.0
354.00	879.0
355.00	288.0
359.10	203.0
365.00	3222.0
366.00	520.0
371.10	269.0
371.90	1006.0
372.10	1011.0
373.10	471.0
382.90	267.0
389.90	269.0
402.00	500.0
402.90	669.0
403.90	442.0
421.10	625.0
422.00	656.0
423.10	3867.0
424.00	1137.0
441.00	12309.0
442.00	70064.0
443.00	12810.0
444.00	1340.0

Instrument :
BNA_G
ClientSampleId :
DFTPP574