

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG053116\
 Data File : BG022121.D
 Acq On : 31 May 2016 20:16
 Operator : UM/SJ
 Sample : H3305-02
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BCZK8

Quant Time: Jun 01 01:08:44 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG052116.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jun 01 01:07:08 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.14	152	38002	20.00	ng/ul	0.00
18) Naphthalene-d8	10.95	136	208247	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.76	164	133424	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.51	188	295979	20.00	ng/ul	0.00
75) Chrysene-d12	21.79	240	269001	20.00	ng/ul	0.00
83) Perylene-d12	25.10	264	259201	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.50	96	300	0.41	ng/uL	0.00
5) Phenol-d5	7.30	99	16944	4.93	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.45	67	34854	19.36	ng/ul	0.00
9) 2-Chlorophenol-d4	7.67	132	51408	17.91	ng/ul	0.00
13) 4-Methylphenol-d8	8.85	113	37535	12.89	ng/ul	0.00
19) Nitrobenzene-d5	9.31	128	34041	22.16	ng/ul	0.00
22) 2-Nitrophenol-d4	10.03	143	41352	24.86	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.58	165	72936	24.85	ng/ul	0.00
29) 4-Chloroaniline-d4	11.11	131	930	0.29	ng/ul	0.02
43) Dimethylphthalate-d6	14.16	166	322260	32.16	ng/ul	0.00
46) Acenaphthylene-d8	14.46	160	384143	27.45	ng/ul	0.00
51) 4-Nitrophenol-d4	14.99	143	3000	1.74	ng/ul	0.01
57) Fluorene-d10	15.75	176	274460	29.24	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.87	200	47692	30.83	ng/ul	0.00
70) Anthracene-d10	17.61	188	415674	29.26	ng/ul	0.00
76) Pyrene-d10	19.89	212	451562	29.77	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.88	264	371375	30.88	ng/ul	0.00


Target Compounds						Qvalue
44) Dimethylphthalate	14.21	163	10113	1.00	ng/ul	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG053116\
Data File : BG022121.D
Acq On : 31 May 2016 20:16
Operator : UM/SJ
Sample : H3305-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BCZK8

Quant Time: Jun 01 01:08:44 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG052116.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jun 01 01:07:08 2016
Response via : Initial Calibration

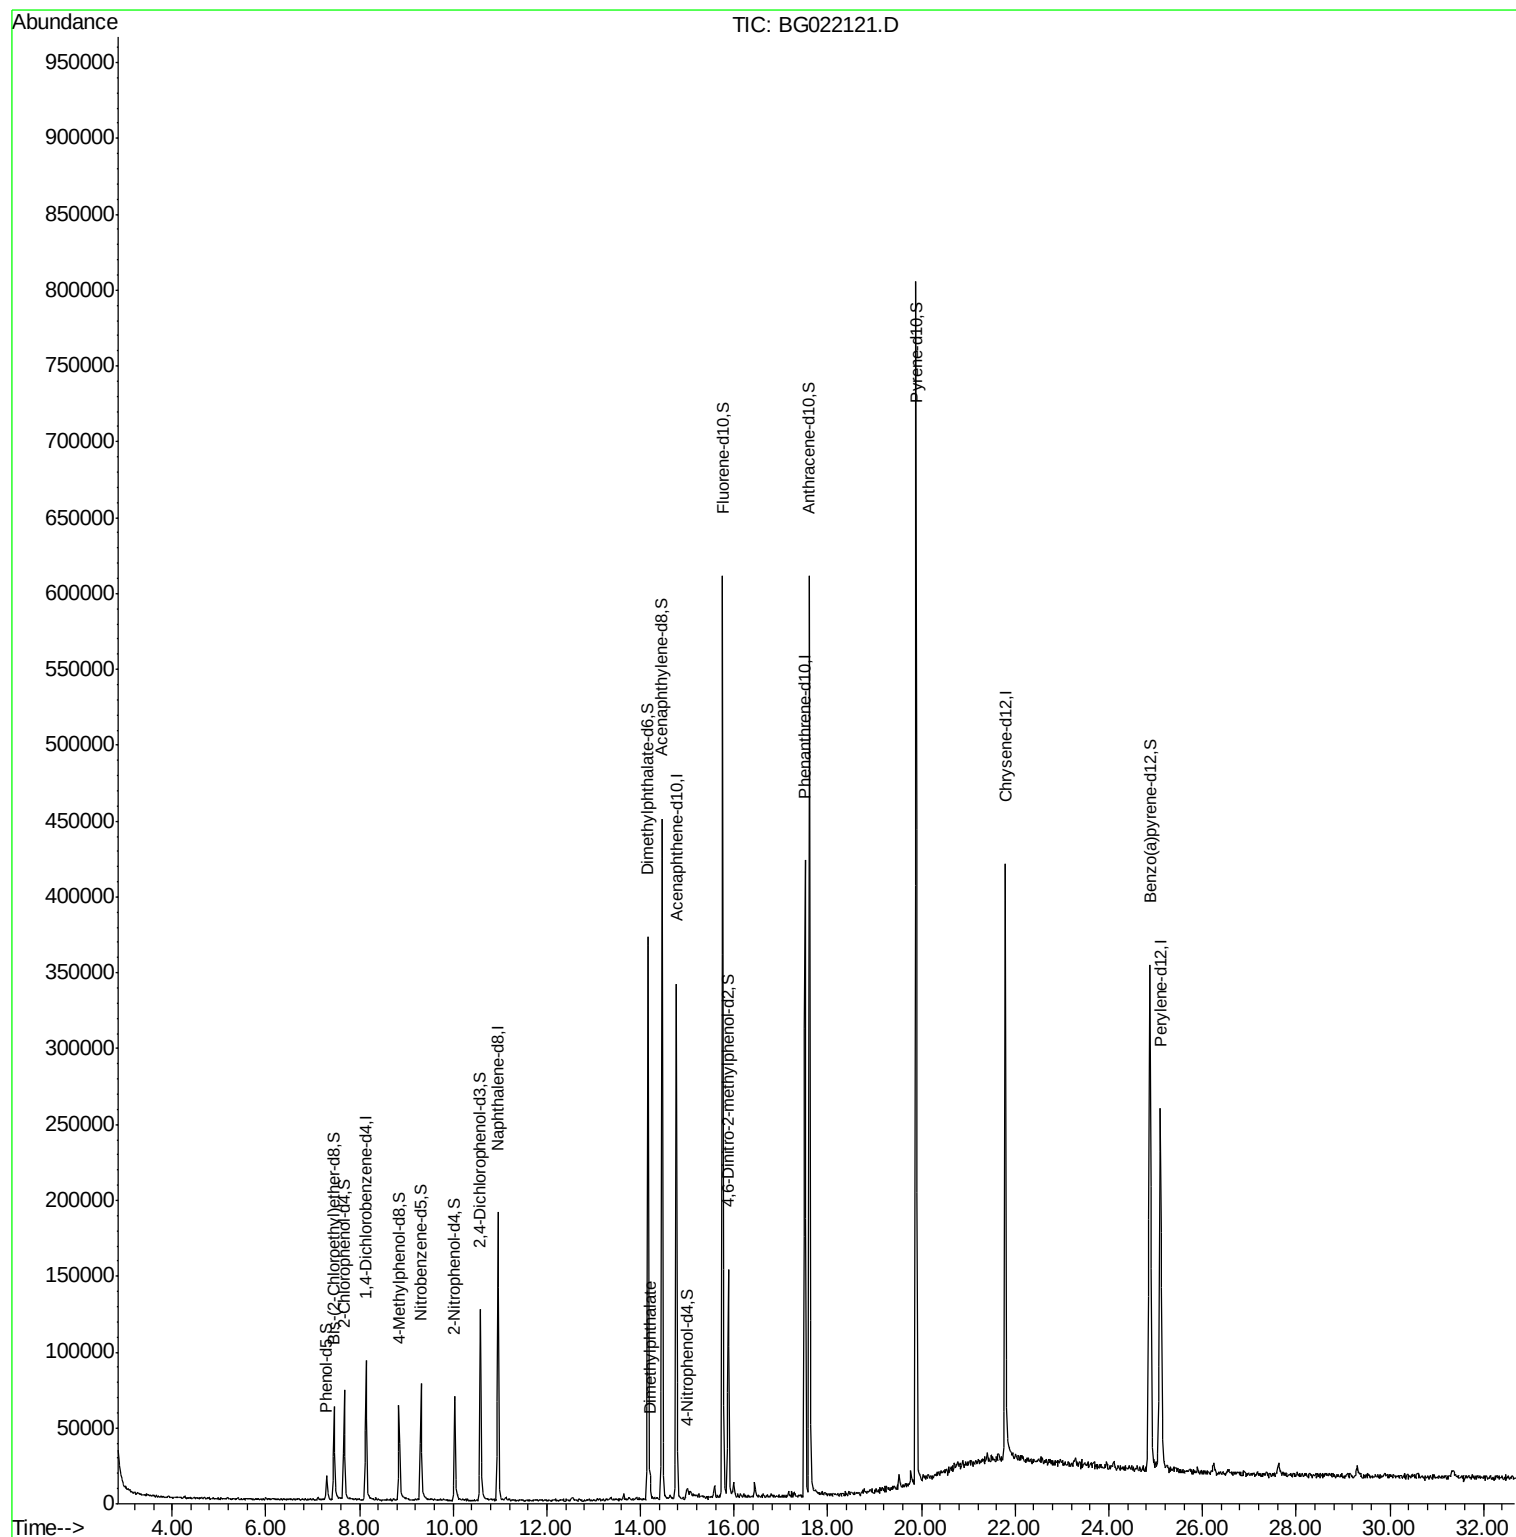

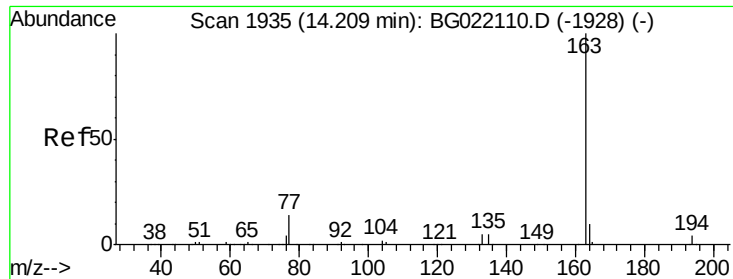

#44

Dimethylphthalate

Concen: 1.00 ng/ul

RT: 14.21 min Scan# 1935

Delta R.T. 0.00 min

Lab File: BG022121.D


Acq: 31 May 2016 20:16

Instrument :

BNA_G

ClientSampleId :

BCZK8

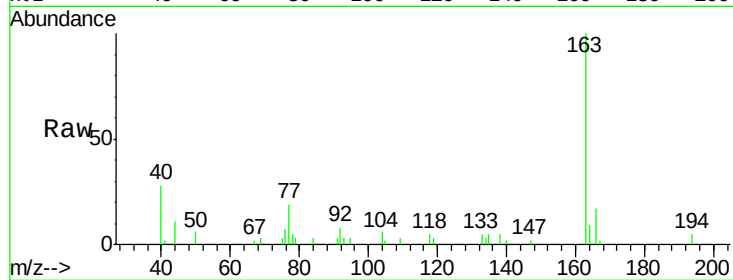


Tgt Ion:163 Resp: 10113

Ion Ratio Lower Upper

163 100

194 5.2 3.4 5.2

164 9.5 8.8 13.2

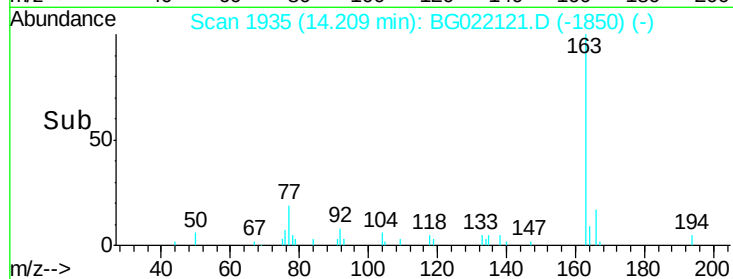

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

