

Data Path : Z:\HPCHEM1\BNA_G\Data\BG053116\
 Data File : BG022111.D
 Acq On : 31 May 2016 11:54
 Operator : UM/SJ
 Sample : PB90612BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK12

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG052116.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.502	110	113	117	rVB2	3640	3965	0.33%	0.037%
2	3.814	164	166	171	rVB5	1169	1530	0.13%	0.014%
3	4.266	239	243	244	rBV4	1453	1428	0.12%	0.013%
4	4.278	244	245	249	rVB3	2121	1773	0.15%	0.017%
5	5.482	445	450	452	rVB5	747	1277	0.11%	0.012%
6	5.776	497	500	504	rVB4	841	1398	0.12%	0.013%
7	7.298	751	759	769	rBV	87760	180304	15.00%	1.697%
8	7.363	769	770	772	rBV2	2000	1284	0.11%	0.012%
9	7.451	778	785	795	rBV	86308	167166	13.91%	1.573%
10	7.668	814	822	831	rBV	103094	207001	17.22%	1.948%
11	7.774	835	840	841	rVB3	1083	1525	0.13%	0.014%
12	7.897	860	861	866	rBV5	1142	1648	0.14%	0.016%
13	8.138	895	902	916	rBV	75879	151249	12.58%	1.423%
14	8.491	957	962	963	rBV2	1036	1416	0.12%	0.013%
15	8.849	1015	1023	1035	rBV	135865	271969	22.62%	2.559%
16	9.102	1064	1066	1069	rVB2	1208	1209	0.10%	0.011%
17	9.125	1069	1070	1075	rBV4	1187	1482	0.12%	0.014%
18	9.254	1087	1092	1094	rBV4	1001	1685	0.14%	0.016%
19	9.307	1094	1101	1111	rVV	95898	198955	16.55%	1.872%
20	9.407	1116	1118	1121	rVV3	1853	2080	0.17%	0.020%
21	9.437	1121	1123	1127	rVV5	1143	1586	0.13%	0.015%
22	9.689	1164	1166	1172	rVB4	743	1348	0.11%	0.013%
23	10.030	1218	1224	1238	rVV	81672	171941	14.30%	1.618%
24	10.171	1247	1248	1254	rVB3	1507	1448	0.12%	0.014%
25	10.576	1309	1317	1329	rBV	126813	265207	22.06%	2.496%
26	10.958	1373	1382	1393	rBV	140603	280084	23.30%	2.636%
27	11.093	1395	1405	1418	rBV	131451	297752	24.77%	2.802%
28	11.358	1446	1450	1454	rBV3	1150	2127	0.18%	0.020%
29	12.527	1645	1649	1658	rVB4	2723	5020	0.42%	0.047%
30	13.044	1732	1737	1742	rVB5	911	2057	0.17%	0.019%
31	13.779	1856	1862	1865	rVB4	856	1207	0.10%	0.011%
32	14.160	1920	1927	1936	rBV	358864	576433	47.95%	5.424%
33	14.460	1970	1978	1990	rBV	419835	710264	59.08%	6.684%
34	14.766	2023	2030	2040	rBV2	257708	456211	37.95%	4.293%

Data Path : Z:\HPCHEM1\BNA_G\Data\BG053116\
 Data File : BG022111.D
 Acq On : 31 May 2016 11:54
 Operator : UM/SJ
 Sample : PB90612BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK12

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG052116.M
 Title : SVOA CALIBRATION

35	14.977	2059	2066	2085	rBV2	72642	200758	16.70%	1.889%
36	15.159	2095	2097	2101	rVB4	1655	1761	0.15%	0.017%
37	15.189	2101	2102	2105	rVV3	1584	1317	0.11%	0.012%
38	15.224	2105	2108	2109	rVB3	1422	1413	0.12%	0.013%
39	15.242	2109	2111	2114	rBV3	1358	1256	0.10%	0.012%
40	15.518	2154	2158	2160	rVB3	1197	1595	0.13%	0.015%
41	15.753	2191	2198	2210	rBV	576005	923395	76.81%	8.689%
42	15.876	2213	2219	2232	rVV	135069	234351	19.49%	2.205%
43	15.958	2232	2233	2235	rVV2	1851	1752	0.15%	0.016%
44	15.988	2235	2238	2243	rVB4	5730	9341	0.78%	0.088%
45	16.428	2310	2313	2316	rBV5	1312	1450	0.12%	0.014%
46	16.757	2364	2369	2370	rBV4	1048	1758	0.15%	0.017%
47	17.128	2428	2432	2434	rBV4	1641	2493	0.21%	0.023%
48	17.169	2434	2439	2441	rVB5	1330	1804	0.15%	0.017%
49	17.251	2451	2453	2456	rVB2	2085	1795	0.15%	0.017%
50	17.298	2456	2461	2463	rBV4	2133	3360	0.28%	0.032%
51	17.363	2470	2472	2475	rVB3	1759	1598	0.13%	0.015%
52	17.509	2490	2497	2506	rBV2	339777	584105	48.59%	5.497%
53	17.603	2507	2513	2524	rVV2	587353	1005924	83.68%	9.466%
54	18.026	2583	2585	2588	rVB3	1374	1515	0.13%	0.014%
55	18.073	2588	2593	2594	rBV5	1497	1970	0.16%	0.019%
56	18.185	2609	2612	2614	rBV3	1594	1675	0.14%	0.016%
57	18.450	2654	2657	2661	rVB5	1698	2063	0.17%	0.019%
58	18.579	2676	2679	2681	rBV4	1662	2500	0.21%	0.024%
59	18.732	2703	2705	2707	rVB3	1454	1281	0.11%	0.012%
60	18.931	2737	2739	2741	rVB3	2039	1243	0.10%	0.012%
61	19.037	2753	2757	2760	rBV6	1057	1832	0.15%	0.017%
62	19.108	2767	2769	2772	rBV4	1216	1287	0.11%	0.012%
63	19.213	2784	2787	2790	rBV5	1266	1674	0.14%	0.016%
64	19.266	2794	2796	2797	rBV	1844	1379	0.11%	0.013%
65	19.360	2809	2812	2815	rBV5	2530	3378	0.28%	0.032%
66	19.401	2817	2819	2821	rBV3	1098	1265	0.11%	0.012%
67	19.448	2826	2827	2829	rVB2	2131	1216	0.10%	0.011%
68	19.490	2832	2834	2835	rBV2	1834	1566	0.13%	0.015%
69	19.525	2835	2840	2844	rVV2	6837	11188	0.93%	0.105%
70	19.619	2854	2856	2857	rBV2	2666	1318	0.11%	0.012%
71	19.636	2857	2859	2863	rVV5	1455	1545	0.13%	0.015%

Data Path : Z:\HPCHEM1\BNA_G\Data\BG053116\
Data File : BG022111.D
Acq On : 31 May 2016 11:54
Operator : UM/SJ
Sample : PB90612BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK12

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG052116.M
Title : SVOA CALIBRATION

72	19.772	2878	2882	2888	rBV2	5566	9760	0.81%	0.092%
73	19.883	2894	2901	2910	rBV2	740755	1202167	100.00%	11.313%
74	20.012	2921	2923	2926	rBV3	2601	3051	0.25%	0.029%
75	20.101	2936	2938	2941	rBV4	1532	2035	0.17%	0.019%
76	20.130	2941	2943	2944	rBV2	2400	1552	0.13%	0.015%
77	20.383	2983	2986	2989	rBV5	4591	4905	0.41%	0.046%
78	20.618	3024	3026	3028	rBV3	2279	2570	0.21%	0.024%
79	20.665	3032	3034	3036	rVB3	3251	1962	0.16%	0.018%
80	20.694	3036	3039	3040	rBV3	3460	3842	0.32%	0.036%
81	20.882	3067	3071	3074	rVB6	5627	8559	0.71%	0.081%
82	21.787	3218	3225	3236	rBV	314942	621832	51.73%	5.852%
83	22.028	3265	3266	3267	rBV	3483	1411	0.12%	0.013%
84	23.837	3572	3574	3575	rBV2	3711	2649	0.22%	0.025%
85	24.871	3738	3750	3765	rBV	335058	1101742	91.65%	10.368%
86	25.095	3778	3788	3804	rVB2	197759	654171	54.42%	6.156%
87	26.616	4045	4047	4048	rBV2	3769	1806	0.15%	0.017%
88	28.121	4301	4303	4304	rBV2	4250	2413	0.20%	0.023%
89	29.260	4495	4497	4499	rBV3	4306	4635	0.39%	0.044%
90	31.052	4800	4802	4803	rBV2	3620	1556	0.13%	0.015%


Sum of corrected areas: 10626768

Data Path : Z:\HPCHEM1\BNA_G\Data\BG053116\
Data File : BG022111.D
Acq On : 31 May 2016 11:54
Operator : UM/SJ
Sample : PB90612BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK12

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG052116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

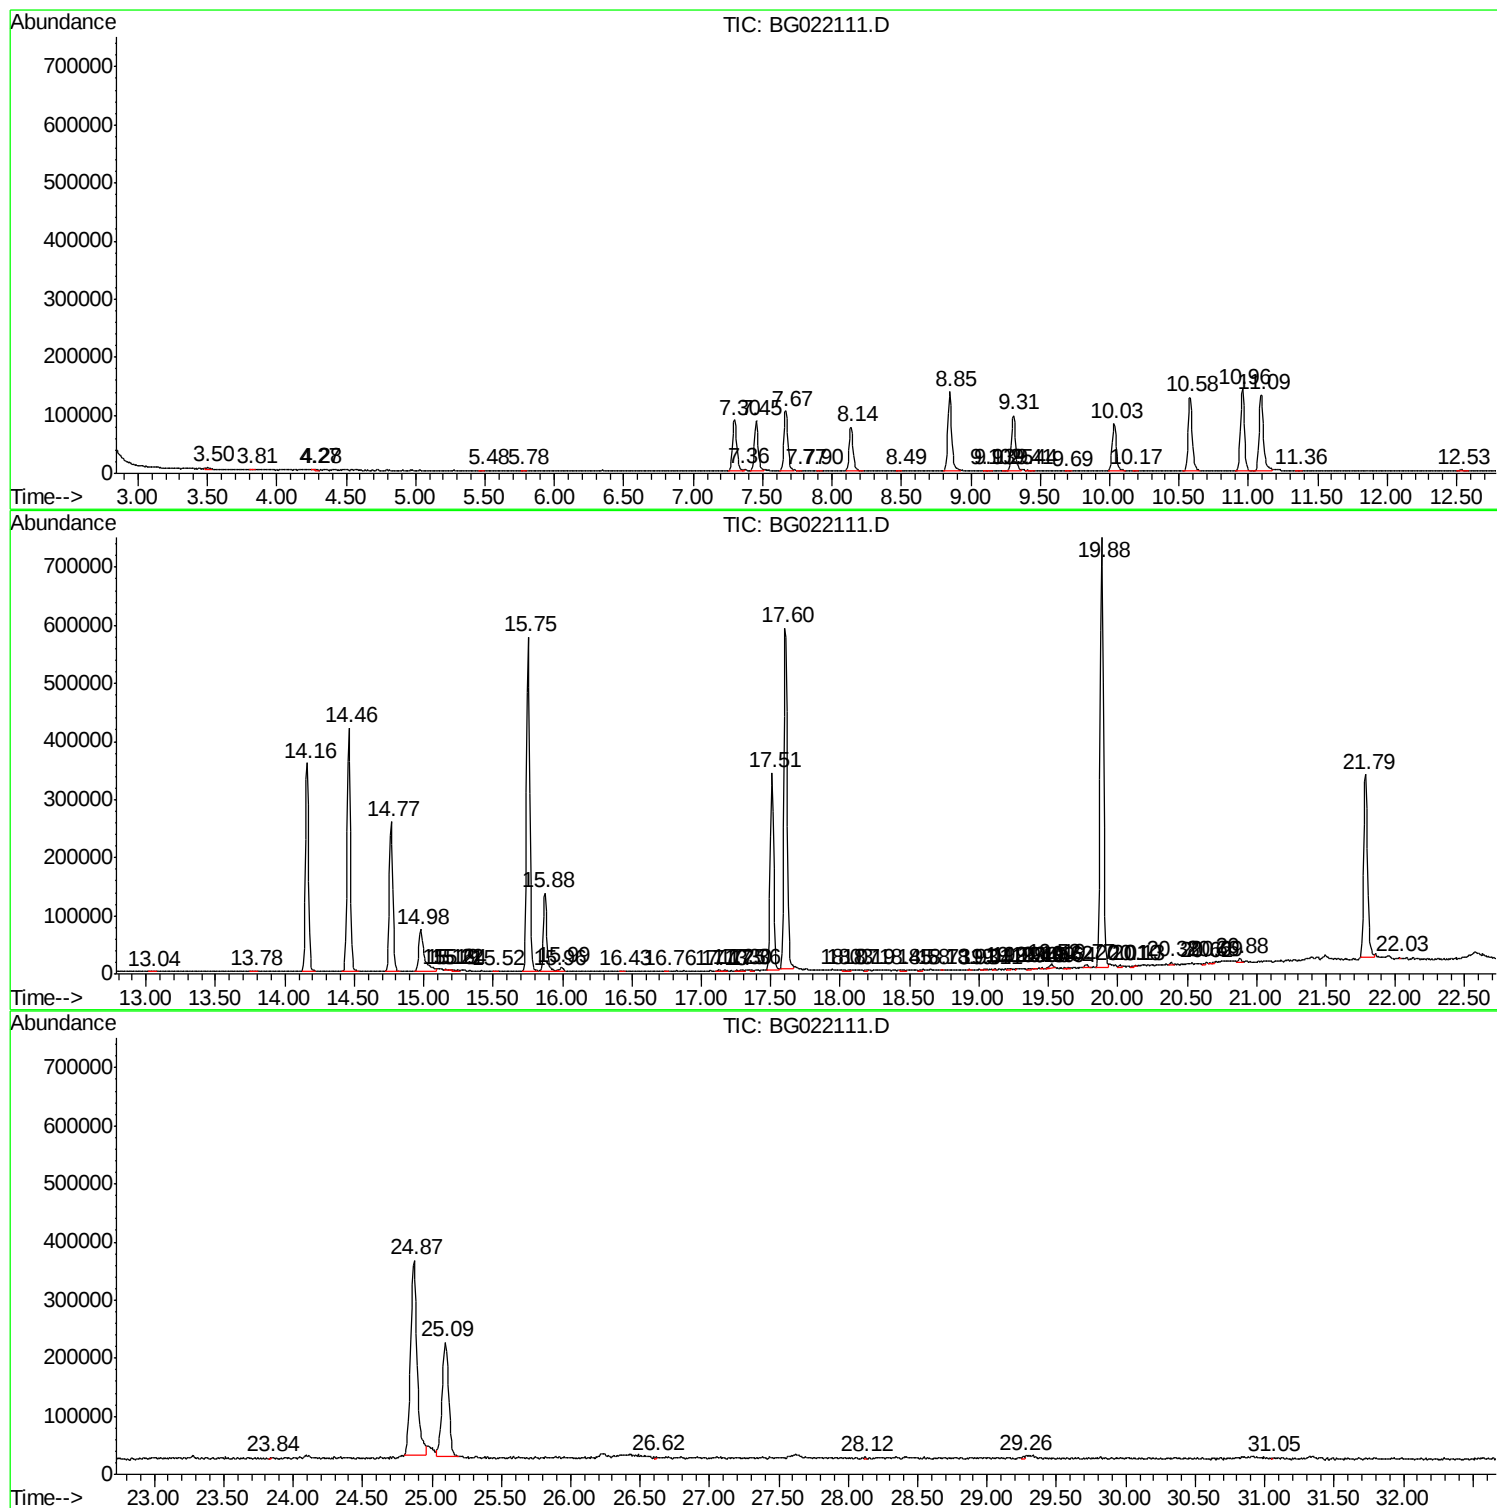

Data Path : Z:\HPCHEM1\BNA_G\Data\BG053116\
Data File : BG022111.D
Acq On : 31 May 2016 11:54
Operator : UM/SJ
Sample : PB90612BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK12

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG052116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_G\Data\BG053116\
Data File : BG022111.D
Acq On : 31 May 2016 11:54
Operator : UM/SJ
Sample : PB90612BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK12

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG052116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc