

Data Path : Z:\HPCHEM1\BNA G\DATA\BG053116\
 Data File : BG022112.D
 Acq On : 31 May 2016 12:46
 Operator : UM/SJ
 Sample : PB90901BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG052116.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.248	68	70	72	rBV3	1266	1292	0.12%	0.013%
2	3.501	107	113	119	rBV6	3292	6958	0.62%	0.071%
3	3.565	122	124	128	rVB4	1364	1481	0.13%	0.015%
4	4.276	242	245	249	rVB4	1841	2723	0.24%	0.028%
5	4.805	332	335	339	rVV4	716	1227	0.11%	0.012%
6	5.845	510	512	516	rBV3	745	1150	0.10%	0.012%
7	6.039	543	545	548	rBV3	1131	1327	0.12%	0.014%
8	7.191	738	741	744	rBV3	1211	1615	0.14%	0.016%
9	7.296	752	759	777	rVV	83809	176140	15.79%	1.793%
10	7.455	777	786	795	rBV	79352	160020	14.35%	1.629%
11	7.667	815	822	842	rVB	101193	205721	18.45%	2.094%
12	7.990	876	877	880	rBV3	1172	1199	0.11%	0.012%
13	8.137	894	902	915	rBV	74849	152841	13.70%	1.556%
14	8.848	1015	1023	1038	rBV	124742	256576	23.01%	2.611%
15	9.306	1093	1101	1114	rBV	89205	193820	17.38%	1.973%
16	9.735	1169	1174	1176	rVV4	929	1395	0.13%	0.014%
17	9.776	1178	1181	1186	rBV4	836	1270	0.11%	0.013%
18	10.034	1217	1225	1235	rBV2	73669	159865	14.33%	1.627%
19	10.581	1310	1318	1334	rBV	119854	253707	22.75%	2.582%
20	10.875	1364	1368	1369	rBV3	997	1210	0.11%	0.012%
21	10.957	1374	1382	1394	rBV	129703	268775	24.10%	2.736%
22	11.092	1398	1405	1419	rBV	115513	266420	23.89%	2.712%
23	11.727	1511	1513	1516	rVV4	1149	1264	0.11%	0.013%
24	11.768	1516	1520	1523	rVB4	1101	1469	0.13%	0.015%
25	12.531	1644	1650	1651	rBV3	2374	2377	0.21%	0.024%
26	14.159	1920	1927	1938	rBV	323842	519854	46.61%	5.291%
27	14.459	1971	1978	1989	rBV	366662	644958	57.83%	6.564%
28	14.570	1995	1997	2001	rVB3	1470	1177	0.11%	0.012%
29	14.764	2022	2030	2040	rBV2	236681	421795	37.82%	4.293%
30	14.982	2059	2067	2086	rBV	57345	169228	15.17%	1.722%
31	15.158	2096	2097	2102	rVB3	2234	2166	0.19%	0.022%
32	15.205	2103	2105	2108	rVV4	1638	1770	0.16%	0.018%
33	15.234	2108	2110	2115	rVB3	1516	1558	0.14%	0.016%
34	15.504	2152	2156	2159	rBV4	774	1288	0.12%	0.013%

Data Path : Z:\HPCHEM1\BNA G\DATA\BG053116\
 Data File : BG022112.D
 Acq On : 31 May 2016 12:46
 Operator : UM/SJ
 Sample : PB90901BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG052116.M
 Title : SVOA CALIBRATION

35	15.757	2190	2199	2211	rBV	492857	832409	74.64%	8.472%
36	15.875	2213	2219	2231	rVV	114484	202035	18.12%	2.056%
37	15.992	2234	2239	2244	rVV2	5540	8356	0.75%	0.085%
38	16.039	2246	2247	2251	rBV3	1045	1188	0.11%	0.012%
39	16.944	2394	2401	2402	rBV3	849	1686	0.15%	0.017%
40	17.161	2435	2438	2440	rBV3	1219	1388	0.12%	0.014%
41	17.308	2461	2463	2470	rVB4	1690	3002	0.27%	0.031%
42	17.449	2482	2487	2490	rBV4	610	1224	0.11%	0.012%
43	17.508	2490	2497	2506	rBV2	315883	528657	47.40%	5.381%
44	17.608	2506	2514	2526	rVV	535090	922355	82.70%	9.388%
45	17.714	2530	2532	2535	rVB3	1358	1614	0.14%	0.016%
46	17.855	2552	2556	2560	rBV5	1578	2073	0.19%	0.021%
47	18.648	2687	2691	2692	rBV3	1518	1661	0.15%	0.017%
48	19.106	2767	2769	2771	rBV3	1214	1265	0.11%	0.013%
49	19.353	2809	2811	2815	rBV5	1453	1695	0.15%	0.017%
50	19.429	2821	2824	2825	rBV3	1911	1481	0.13%	0.015%
51	19.523	2834	2840	2847	rBV	7233	13191	1.18%	0.134%
52	19.623	2855	2857	2859	rBV3	1132	1158	0.10%	0.012%
53	19.676	2863	2866	2868	rBV4	1125	1387	0.12%	0.014%
54	19.782	2878	2884	2886	rBV2	6404	9184	0.82%	0.093%
55	19.835	2890	2893	2894	rBV2	1400	1459	0.13%	0.015%
56	19.888	2894	2902	2912	rBV	708042	1115243	100.00%	11.351%
57	20.023	2924	2925	2928	rBV3	1744	1288	0.12%	0.013%
58	20.305	2969	2973	2974	rBV4	2967	3241	0.29%	0.033%
59	20.528	3009	3011	3012	rBV2	1900	1135	0.10%	0.012%
60	20.657	3031	3033	3040	rBV8	2593	4955	0.44%	0.050%
61	20.880	3068	3071	3074	rBV3	4884	5651	0.51%	0.058%
62	21.233	3129	3131	3133	rVB3	3600	2366	0.21%	0.024%
63	21.497	3172	3176	3180	rBV3	6848	12553	1.13%	0.128%
64	21.785	3219	3225	3235	rBV	302442	593036	53.18%	6.036%
65	22.302	3311	3313	3314	rBV2	2678	1411	0.13%	0.014%
66	22.573	3354	3359	3364	rBV8	6171	11807	1.06%	0.120%
67	22.725	3383	3385	3386	rBV2	2909	2662	0.24%	0.027%
68	23.519	3518	3520	3521	rBV2	3132	2084	0.19%	0.021%
69	24.206	3636	3637	3639	rBV2	3554	2423	0.22%	0.025%
70	24.294	3650	3652	3655	rBV4	3841	5211	0.47%	0.053%
71	24.876	3737	3751	3769	rBV2	305615	985358	88.35%	10.029%

Data Path : Z:\HPCHEM1\BNA G\DATA\BG053116\
Data File : BG022112.D
Acq On : 31 May 2016 12:46
Operator : UM/SJ
Sample : PB90901BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG052116.M
Title : SVOA CALIBRATION

72	25.099	3779	3789	3806	rVB2	191450	617919	55.41%	6.289%
73	25.698	3889	3891	3894	rBV4	3205	2412	0.22%	0.025%
74	26.233	3977	3982	3985	rBV7	6406	11937	1.07%	0.121%
75	26.973	4106	4108	4109	rBV2	3203	2019	0.18%	0.021%
76	28.454	4359	4360	4361	rBV	4014	2064	0.19%	0.021%
77	29.917	4607	4609	4611	rBV3	4396	4833	0.43%	0.049%
78	30.463	4700	4702	4703	rBV2	3159	1482	0.13%	0.015%
79	31.339	4847	4851	4854	rBV6	4262	6305	0.57%	0.064%
80	31.997	4961	4963	4964	rBV2	3247	1554	0.14%	0.016%


Sum of corrected areas: 9825053

Data Path : Z:\HPCHEM1\BNA G\DATA\BG053116\
Data File : BG022112.D
Acq On : 31 May 2016 12:46
Operator : UM/SJ
Sample : PB90901BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK01

Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG052116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

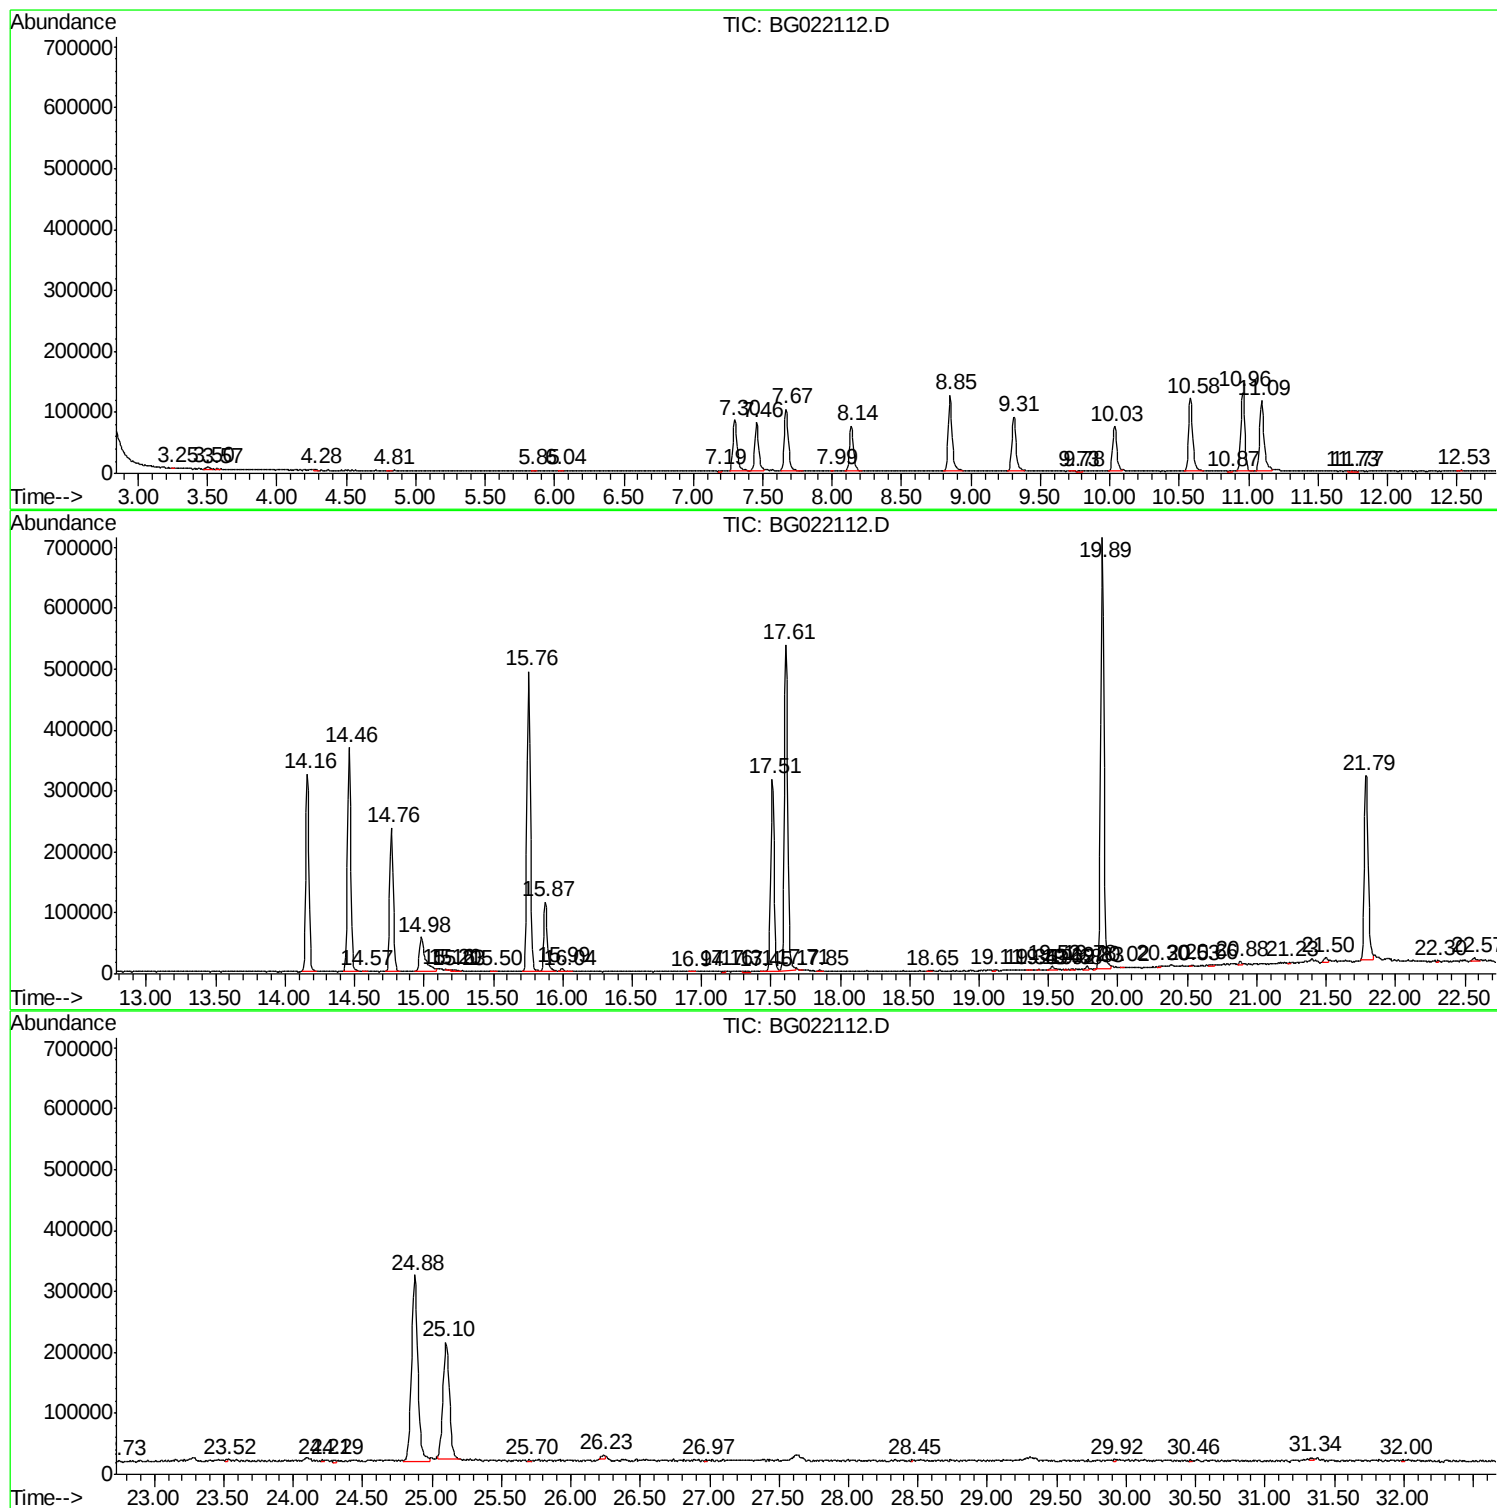

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG053116\
Data File : BG022112.D
Acq On : 31 May 2016 12:46
Operator : UM/SJ
Sample : PB90901BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK01

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG052116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG053116\
Data File : BG022112.D
Acq On : 31 May 2016 12:46
Operator : UM/SJ
Sample : PB90901BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK01

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG052116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc