

Data Path : Z:\HPCHEM1\BNA G\DATA\BG053116\
 Data File : BG022114.D
 Acq On : 31 May 2016 15:02
 Operator : UM/SJ
 Sample : PB90955BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK55

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG052116.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.502	108	113	118	rVB5	3414	5505	0.47%	0.056%
2	4.419	265	269	272	rBV4	1073	1639	0.14%	0.017%
3	5.330	422	424	428	rBV3	1086	1257	0.11%	0.013%
4	5.911	520	523	529	rVB3	780	1248	0.11%	0.013%
5	6.534	626	629	636	rVB5	738	1334	0.11%	0.014%
6	7.298	751	759	770	rBV	81098	159175	13.71%	1.612%
7	7.451	778	785	797	rBV	74030	145262	12.51%	1.471%
8	7.668	815	822	833	rVV	94495	184173	15.86%	1.865%
9	8.138	895	902	913	rBV	67713	131447	11.32%	1.331%
10	8.849	1015	1023	1037	rBV	116183	238535	20.54%	2.416%
11	9.307	1092	1101	1110	rBV	82958	172012	14.81%	1.742%
12	10.036	1217	1225	1235	rBV	66961	146836	12.64%	1.487%
13	10.582	1309	1318	1331	rBV	107554	233539	20.11%	2.365%
14	10.958	1374	1382	1391	rBV	125135	251412	21.65%	2.546%
15	11.094	1397	1405	1423	rBV	110234	257919	22.21%	2.612%
16	12.539	1647	1651	1655	rBV3	2085	3846	0.33%	0.039%
17	12.750	1683	1687	1691	rVB5	712	1246	0.11%	0.013%
18	13.303	1778	1781	1787	rVB3	744	1257	0.11%	0.013%
19	14.161	1920	1927	1935	rBV	342976	538707	46.38%	5.456%
20	14.460	1971	1978	1991	rBV	373609	661085	56.92%	6.696%
21	14.766	2021	2030	2040	rBV2	243561	426860	36.75%	4.323%
22	14.983	2061	2067	2078	rBV2	57315	156119	13.44%	1.581%
23	15.171	2098	2099	2104	rVB4	1564	1350	0.12%	0.014%
24	15.248	2110	2112	2116	rVB2	1024	1311	0.11%	0.013%
25	15.753	2191	2198	2212	rBV	508744	857239	73.81%	8.683%
26	15.876	2214	2219	2230	rVV	118258	204052	17.57%	2.067%
27	15.994	2234	2239	2243	rBV2	4822	7239	0.62%	0.073%
28	16.193	2269	2273	2275	rVB2	1151	1728	0.15%	0.018%
29	16.223	2275	2278	2280	rBV2	1250	1566	0.13%	0.016%
30	17.175	2436	2440	2442	rBV3	950	1342	0.12%	0.014%
31	17.304	2458	2462	2469	rVV4	1380	2973	0.26%	0.030%
32	17.510	2490	2497	2506	rBV2	333946	559993	48.22%	5.672%
33	17.609	2506	2514	2525	rBV2	545432	949178	81.73%	9.614%
34	18.978	2745	2747	2749	rBV3	1418	1300	0.11%	0.013%

Data Path : Z:\HPCHEM1\BNA G\DATA\BG053116\
 Data File : BG022114.D
 Acq On : 31 May 2016 15:02
 Operator : UM/SJ
 Sample : PB90955BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK55

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG052116.M
 Title : SVOA CALIBRATION

35	19.213	2784	2787	2795	rVV5	1818	3400	0.29%	0.034%
36	19.319	2802	2805	2807	rBV4	1123	1204	0.10%	0.012%
37	19.525	2836	2840	2844	rBV2	7075	9120	0.79%	0.092%
38	19.783	2878	2884	2887	rBV3	6867	10730	0.92%	0.109%
39	19.889	2894	2902	2912	rBV	748755	1161400	100.00%	11.763%
40	20.060	2929	2931	2934	rVB4	1960	1658	0.14%	0.017%
41	20.107	2936	2939	2941	rBV4	1439	1638	0.14%	0.017%
42	20.242	2959	2962	2963	rBV3	1398	1447	0.12%	0.015%
43	20.406	2989	2990	2996	rBV6	2077	2644	0.23%	0.027%
44	20.547	3012	3014	3017	rBV4	2432	3166	0.27%	0.032%
45	20.812	3057	3059	3063	rVB5	3466	3350	0.29%	0.034%
46	20.882	3068	3071	3075	rVV5	4513	4837	0.42%	0.049%
47	21.094	3105	3107	3109	rVB3	1957	1377	0.12%	0.014%
48	21.258	3134	3135	3138	rBV3	2380	2445	0.21%	0.025%
49	21.393	3156	3158	3161	rVB4	4671	4636	0.40%	0.047%
50	21.499	3171	3176	3183	rBV2	8437	18418	1.59%	0.187%
51	21.787	3218	3225	3237	rBV	314291	622171	53.57%	6.302%
52	21.951	3251	3253	3257	rVB4	6012	5747	0.49%	0.058%
53	22.069	3272	3273	3277	rBV2	2176	1326	0.11%	0.013%
54	22.568	3356	3358	3365	rVB8	5901	9022	0.78%	0.091%
55	22.768	3389	3392	3394	rBV4	3178	4135	0.36%	0.042%
56	22.839	3402	3404	3407	rBV4	2417	3874	0.33%	0.039%
57	22.880	3409	3411	3412	rBV2	2116	1452	0.13%	0.015%
58	23.015	3432	3434	3435	rVB2	2644	1364	0.12%	0.014%
59	23.115	3450	3451	3452	rBV	2596	1700	0.15%	0.017%
60	23.273	3476	3478	3479	rBV2	4621	3160	0.27%	0.032%
61	23.526	3519	3521	3525	rVB5	3331	3392	0.29%	0.034%
62	23.714	3551	3553	3554	rBV2	2805	1790	0.15%	0.018%
63	24.096	3613	3618	3627	rBV9	8267	20769	1.79%	0.210%
64	24.548	3693	3695	3697	rBV3	2456	2117	0.18%	0.021%
65	24.877	3739	3751	3763	rBV2	304885	955363	82.26%	9.676%
66	25.101	3779	3789	3804	rVB2	193121	613734	52.84%	6.216%
67	25.377	3835	3836	3837	rBV	3155	1682	0.14%	0.017%
68	25.923	3927	3929	3932	rVB3	2856	2002	0.17%	0.020%
69	26.241	3976	3983	3992	rVB3	11588	35137	3.03%	0.356%
70	26.299	3992	3993	3995	rVB2	3342	1455	0.13%	0.015%
71	26.752	4068	4070	4075	rBV6	2640	4138	0.36%	0.042%

Data Path : Z:\HPCHEM1\BNA G\DATA\BG053116\
Data File : BG022114.D
Acq On : 31 May 2016 15:02
Operator : UM/SJ
Sample : PB90955BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK55

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG052116.M
Title : SVOA CALIBRATION

72	26.887	4091	4093	4096	rBV4	3029	1964	0.17%	0.020%
73	27.627	4212	4219	4220	rBV6	10682	16789	1.45%	0.170%
74	28.285	4329	4331	4332	rBV2	2316	2134	0.18%	0.022%
75	28.726	4404	4406	4408	rBV3	2352	2238	0.19%	0.023%
76	29.055	4460	4462	4466	rBV5	2739	2632	0.23%	0.027%
77	29.601	4553	4555	4558	rVB3	3012	2072	0.18%	0.021%
78	29.872	4599	4601	4602	rBV2	2237	1441	0.12%	0.015%
79	30.248	4663	4665	4668	rVB4	2920	2494	0.21%	0.025%
80	30.453	4698	4700	4703	rVB4	3081	2810	0.24%	0.028%
81	31.152	4818	4819	4821	rBV2	2646	1901	0.16%	0.019%


Sum of corrected areas: 9873159

Data Path : Z:\HPCHEM1\BNA G\DATA\BG053116\
Data File : BG022114.D
Acq On : 31 May 2016 15:02
Operator : UM/SJ
Sample : PB90955BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK55

Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG052116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

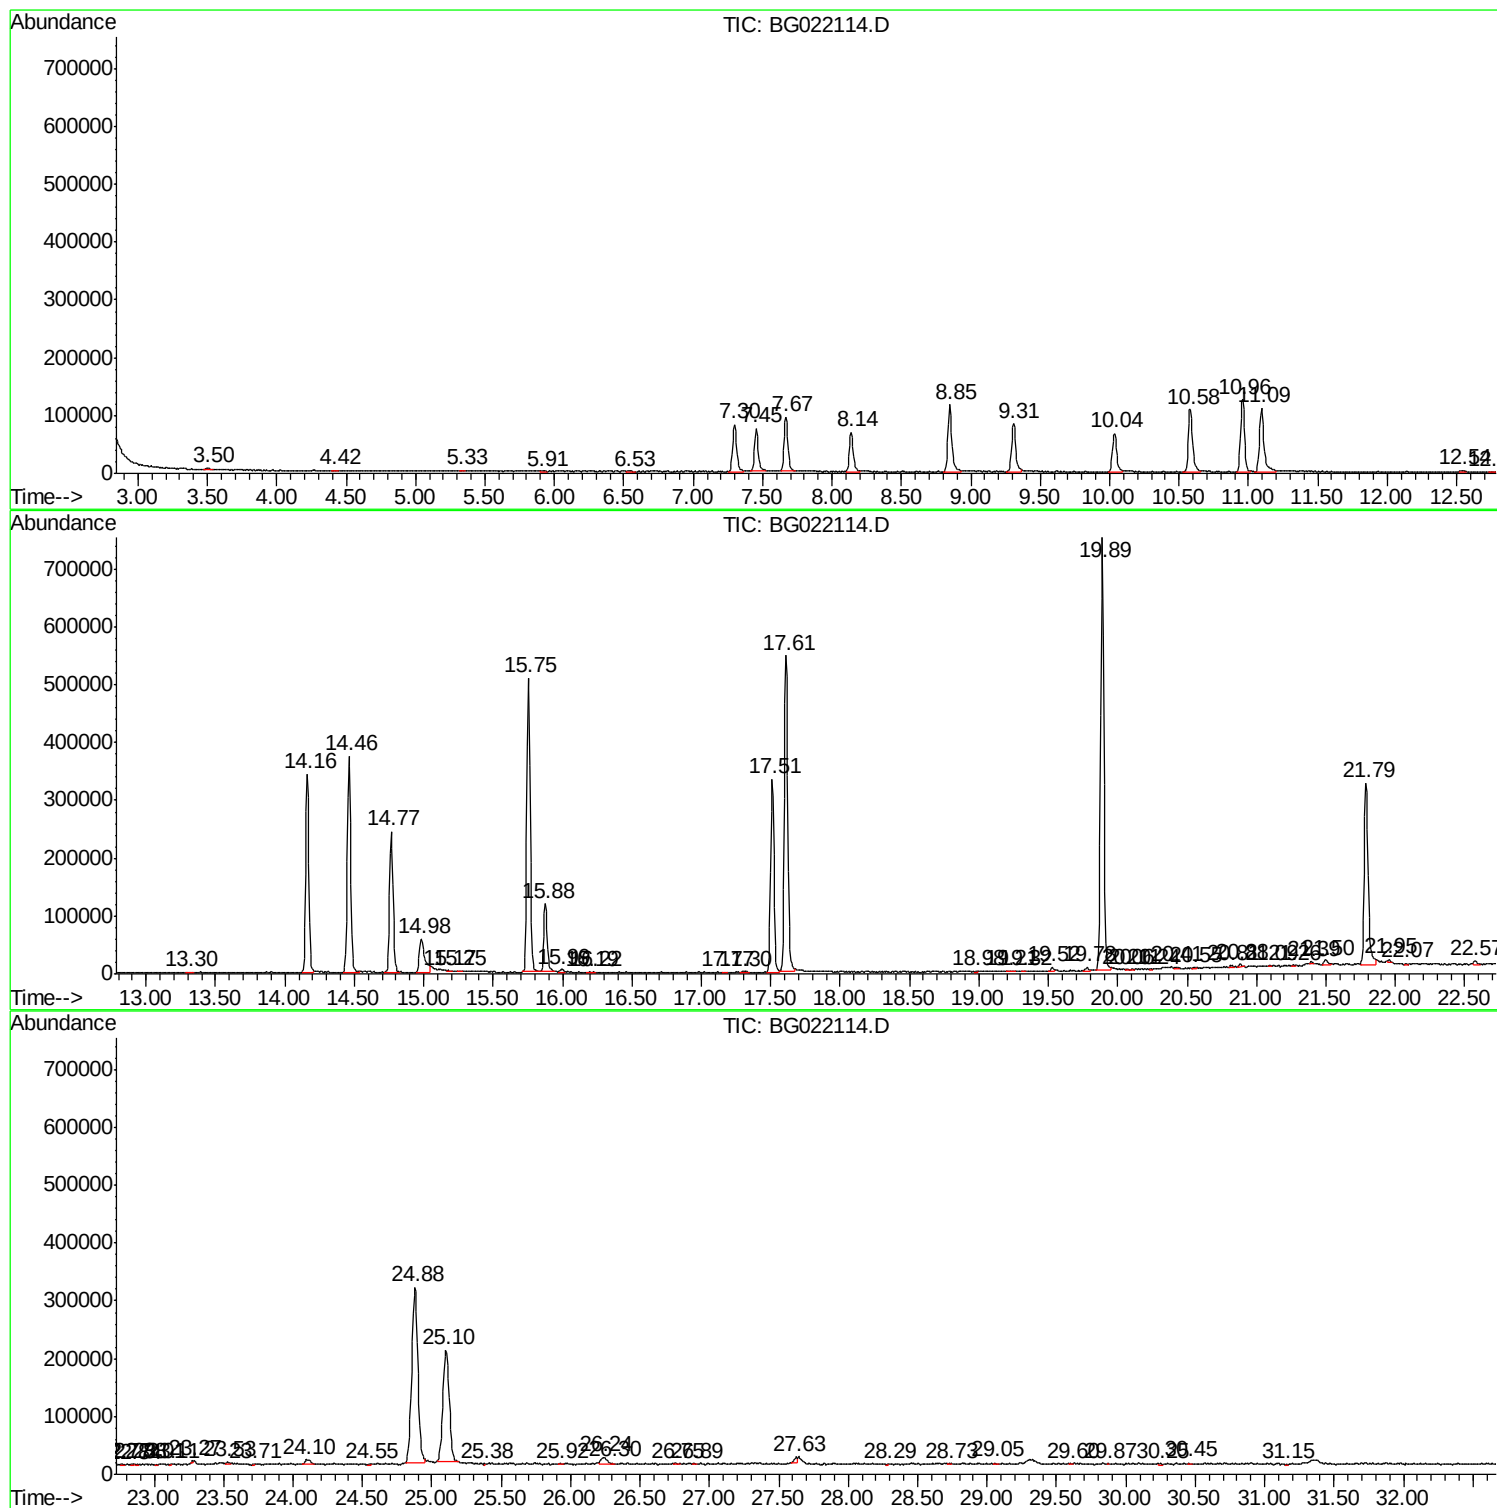

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG053116\
Data File : BG022114.D
Acq On : 31 May 2016 15:02
Operator : UM/SJ
Sample : PB90955BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK55

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG052116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG053116\
Data File : BG022114.D
Acq On : 31 May 2016 15:02
Operator : UM/SJ
Sample : PB90955BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK55

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG052116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc