

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG053122\
 Data File : BG053765.D
 Acq On : 31 May 2022 17:56
 Operator : CG/JU
 Sample : SSTD01022
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SSTD010422

Quant Time: May 31 23:15:19 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG053122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 31 23:09:35 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.104	152	21712	20.000	ng/u1	0.00
20) Naphthalene-d8	10.913	136	84769	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.726	164	57397	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.470	188	140496	20.000	ng/u1	0.00
79) Chrysene-d12	21.747	240	159091	20.000	ng/u1	0.00
88) Perylene-d12	25.026	264	157817	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.533	96	2565	4.173	ng/uL	0.00
4) Pyridine-d5	3.956	84	10382	6.766	ng/u1	0.00
7) Phenol-d5	7.247	99	15197	7.815	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.423	67	9843	8.287	ng/u1	0.00
11) 2-Chlorophenol-d4	7.634	132	12586	9.532	ng/u1	0.00
15) 4-Methylphenol-d8	8.792	113	13042	9.258	ng/u1	0.00
21) Nitrobenzene-d5	9.256	128	4562	7.476	ng/u1	0.00
24) 2-Nitrophenol-d4	9.985	143	4334	6.734	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.525	165	12721	9.085	ng/u1	0.00
31) 4-Chloroaniline-d4	11.036	131	17608	9.515	ng/u1	0.00
46) Dimethylphthalate-d6	14.127	166	41652	9.446	ng/u1	0.00
49) Acenaphthylene-d8	14.415	160	47670	8.897	ng/u1	0.00
54) 4-Nitrophenol-d4	14.891	143	4503	6.074	ng/u1	0.00
60) Fluorene-d10	15.713	176	37108	9.584	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.819	200	4178	5.843	ng/u1	0.00
73) Anthracene-d10	17.564	188	60869	9.304	ng/u1	0.00
81) Pyrene-d10	19.850	212	77379	8.694	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.797	264	74274	9.108	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.569	88	2397	3.183	ng/uL#	60
5) Pyridine	3.974	79	12091	7.292	ng/u1	94
6) Benzaldehyde	7.235	77	10778	8.337	ng/u1	95
8) Phenol	7.276	94	16582	8.847	ng/u1	98
10) Bis(2-Chloroethyl)ether	7.517	93	12883	9.112	ng/u1	92
12) 2-Chlorophenol	7.664	128	13109	9.717	ng/u1	94
13) 2-Methylphenol	8.533	108	12772	8.768	ng/u1	100
14) 2,2'-oxybis(1-Chloropr...	8.633	45	21939	9.546	ng/u1	98
16) Acetophenone	8.921	105	20492	9.325	ng/u1	95
17) N-Nitroso-di-n-propyla...	8.909	70	11568	9.029	ng/u1	90
18) 4-Methylphenol	8.857	108	13601	8.962	ng/u1	98
19) Hexachloroethane	9.197	117	5779	9.654	ng/u1	84
22) Nitrobenzene	9.303	77	12409	6.960	ng/u1	99
23) Isophorone	9.832	82	29479	8.650	ng/u1	97
25) 2-Nitrophenol	10.020	139	4369	6.546	ng/u1	91
26) 2,4-Dimethylphenol	10.073	107	15541	9.397	ng/u1	98
27) Bis(2-Chloroethoxy)met...	10.314	93	17433	9.198	ng/u1#	96
29) 2,4-Dichlorophenol	10.549	162	12748	9.364	ng/u1	99
30) Naphthalene	10.966	128	41455	9.450	ng/u1	99
32) 4-Chloroaniline	11.060	127	17241	9.481	ng/u1	99
33) Hexachlorobutadiene	11.260	225	10879	9.785	ng/u1	97
34) Caprolactam	11.824	113	3090	7.536	ng/u1	89
35) 4-Chloro-3-methylphenol	12.170	107	13163	8.914	ng/u1	96
36) 2-Methylnaphthalene	12.564	142	29035	9.379	ng/u1	96

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG053122\
 Data File : BG053765.D
 Acq On : 31 May 2022 17:56
 Operator : CG/JU
 Sample : SSTD01022
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SSTD010422

Quant Time: May 31 23:15:19 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG053122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 31 23:09:35 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.781	142	28246	9.012	ng/ul	95
39) 1,2,4,5-Tetrachloroben...	12.928	216	19592	10.327	ng/ul	99
40) Hexachlorocyclopentadiene	12.916	237	12640	9.624	ng/ul#	87
41) 2,4,6-Trichlorophenol	13.157	196	10740	9.264	ng/ul	91
42) 2,4,5-Trichlorophenol	13.228	196	11827	9.447	ng/ul	96
43) 1,1'-Biphenyl	13.563	154	40252	9.814	ng/ul	99
44) 2-Chloronaphthalene	13.604	162	31870	9.704	ng/ul	99
45) 2-Nitroaniline	13.792	65	5588	5.804	ng/ul	98
47) Dimethylphthalate	14.174	163	40678	9.667	ng/ul	98
48) 2,6-Dinitrotoluene	14.285	165	5151	6.757	ng/ul	95
50) Acenaphthylene	14.450	152	51593	9.970	ng/ul	99
51) 3-Nitroaniline	14.615	138	4790	6.225	ng/ul#	94
52) Acenaphthene	14.791	153	33855	10.014	ng/ul	97
53) 2,4-Dinitrophenol	14.814	184	2047	4.323	ng/ul	91
55) 4-Nitrophenol	14.902	109	4379	5.612	ng/ul	95
56) Dibenzofuran	15.120	168	48830	9.743	ng/ul	99
57) 2,4-Dinitrotoluene	15.067	165	7051	6.519	ng/ul	95
58) 2,3,4,6-Tetrachlorophenol	15.343	232	9454	8.378	ng/ul#	91
59) Diethylphthalate	15.537	149	41923	9.837	ng/ul	98
61) Fluorene	15.772	166	40474	9.743	ng/ul	98
62) 4-Chlorophenyl-phenyle...	15.766	204	22526	10.190	ng/ul	96
63) 4-Nitroaniline	15.772	138	4929	6.514	ng/ul	95
66) 4,6-Dinitro-2-methylph...	15.831	198	3131	4.476	ng/ul#	93
67) N-Nitrosodiphenylamine	15.972	169	36890	9.711	ng/ul	98
68) 4-Bromophenyl-phenylether	16.659	248	14420	10.366	ng/ul	93
69) Hexachlorobenzene	16.777	284	16848	9.376	ng/ul	96
70) Atrazine	16.918	200	16200	10.406	ng/ul	97
71) Pentachlorophenol	17.117	266	7628	6.981	ng/ul	91
72) Phenanthrene	17.511	178	69476	9.422	ng/ul	98
74) Anthracene	17.605	178	71900	9.753	ng/ul	99
75) 1,2,3,4-Tetrachloroben...	13.528	216	21103	10.085	ng/ul	95
76) Pentachlorobenzene	15.043	250	18792	9.361	ng/ul	94
77) Carbazole	17.864	167	64649	9.923	ng/ul	100
78) Di-n-butylphthalate	18.434	149	77641	10.022	ng/ul	99
80) Fluoranthene	19.515	202	90881	8.665	ng/ul	99
82) Pyrene	19.879	202	91136	8.743	ng/ul	100
83) Butylbenzylphthalate	20.766	149	33016	9.109	ng/ul	99
84) 3,3'-Dichlorobenzidine	21.642	252	35524	9.963	ng/ul	98
85) Benzo(a)anthracene	21.730	228	96138	9.363	ng/ul	99
86) Bis(2-ethylhexyl)phtha...	21.653	149	48543	9.670	ng/ul	99
87) Chrysene	21.794	228	92016	9.395	ng/ul	99
89) Di-n-octyl phthalate	22.887	149	83187	10.120	ng/ul	100
90) Benzo(b)fluoranthene	23.980	252	92769	9.103	ng/ul	97
91) Benzo(k)fluoranthene	24.051	252	90727	9.647	ng/ul	99
93) Benzo(a)pyrene	24.867	252	91079	9.467	ng/ul	99
94) Indeno(1,2,3-cd)pyrene	28.763	276	103956	9.554	ng/ul	99
95) Dibenzo(a,h)anthracene	28.839	278	89656	9.694	ng/ul	99
96) Benzo(g,h,i)perylene	29.926	276	87269	9.488	ng/ul	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG053122\
 Data File : BG053765.D
 Acq On : 31 May 2022 17:56
 Operator : CG/JU
 Sample : SST01022
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SST010422

Quant Time: May 31 23:15:19 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG053122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 31 23:09:35 2022
 Response via : Initial Calibration




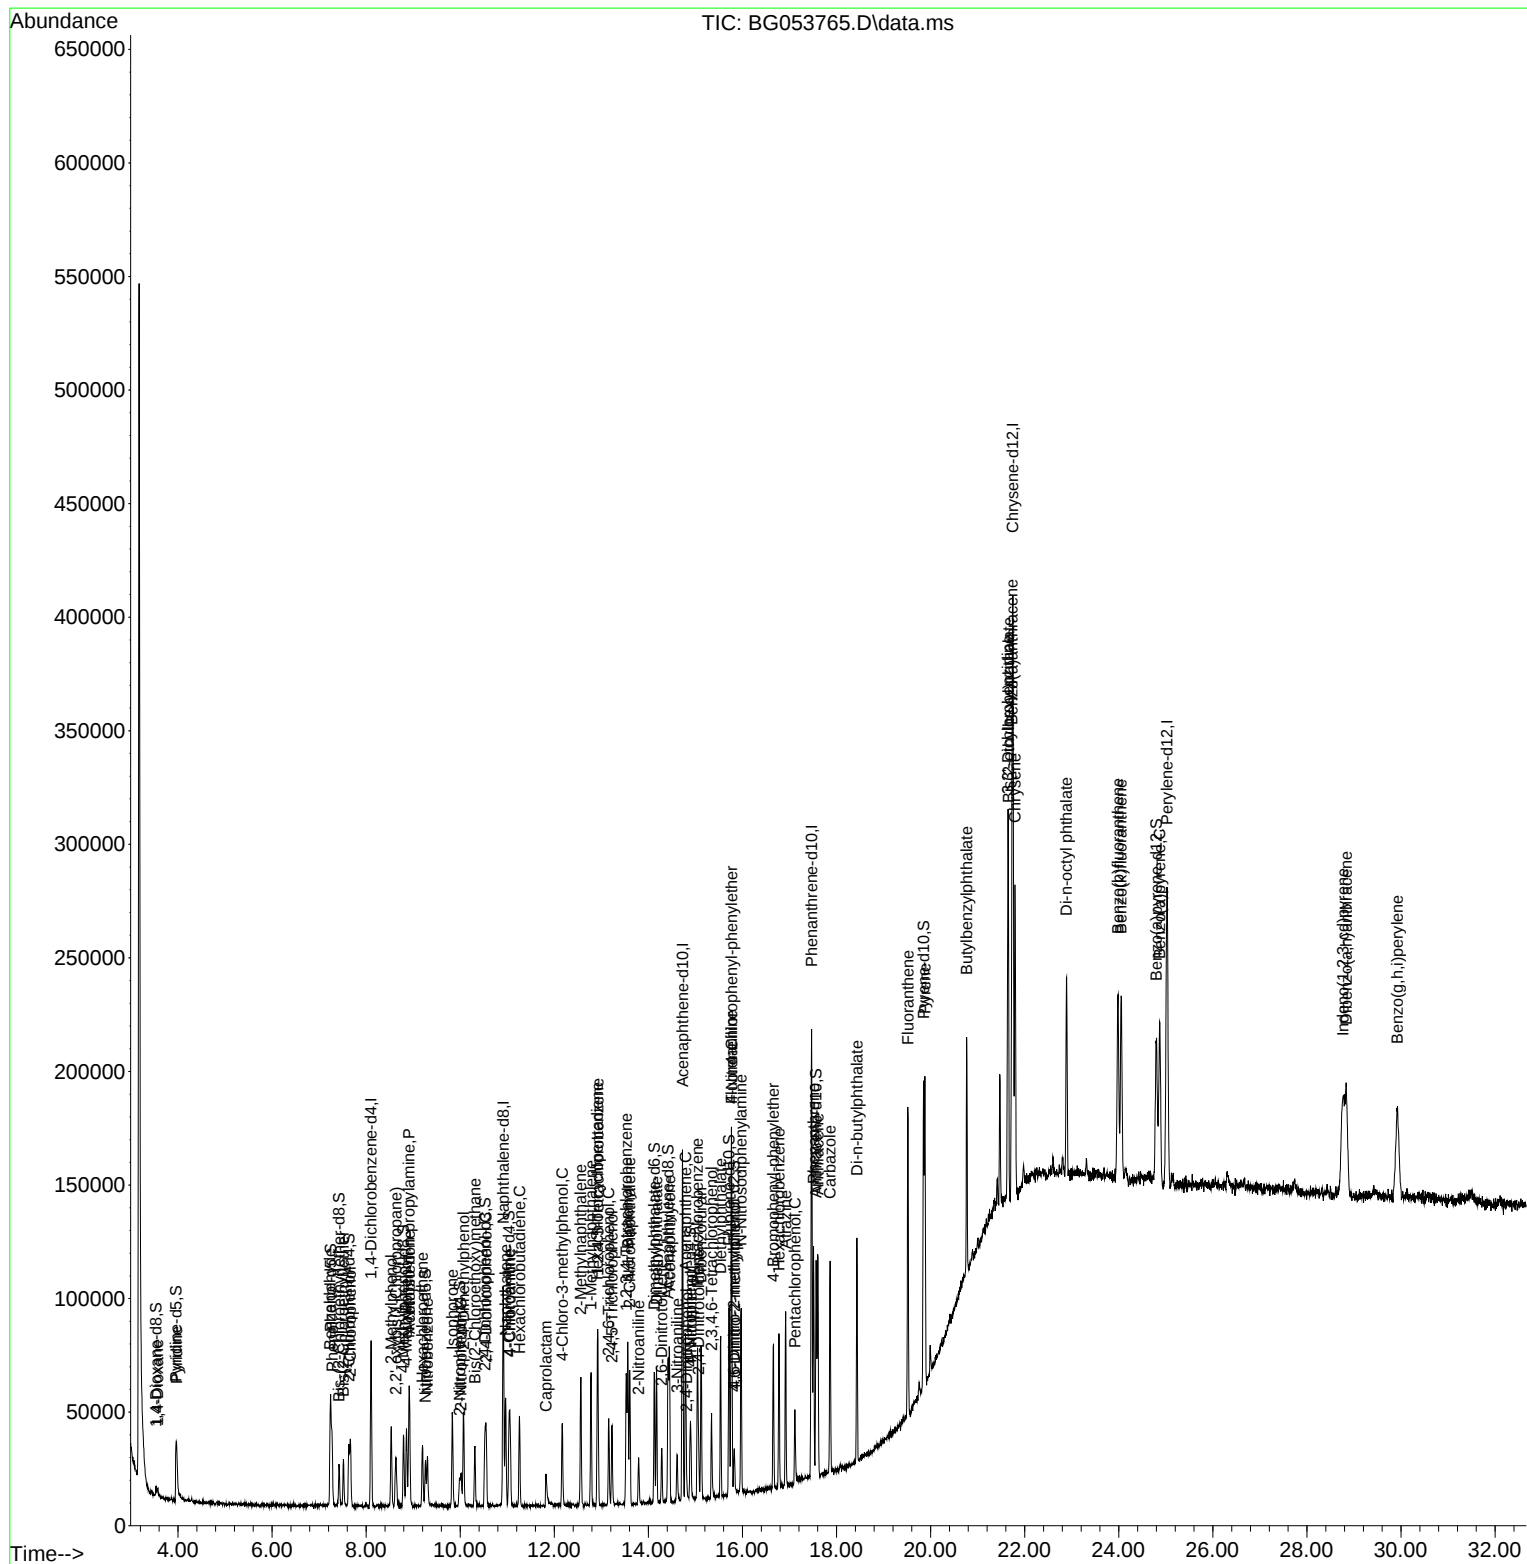




#2
1,4-Dioxane
Concen: 3.183 ng/uL
RT: 3.569 min Scan# 91
Delta R.T. 0.005 min
Lab File: BG053765.D
Acq: 31 May 2022 17:56




Instrument :
BNA_G
ClientSampleId :
SSTD010422


Tgt Ion: 88 Resp: 2397
Ion Ratio Lower Upper
88 100
43 100.7 48.1 72.1#
58 99.0 59.8 89.6#

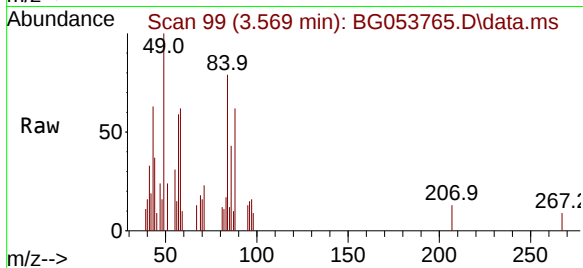

#5
Pyridine
Concen: 7.292 ng/uL
RT: 3.974 min Scan# 168
Delta R.T. 0.005 min
Lab File: BG053765.D
Acq: 31 May 2022 17:56

Tgt Ion: 79 Resp: 12091
Ion Ratio Lower Upper
79 100
52 87.1 75.4 113.2
51 46.0 35.2 52.8




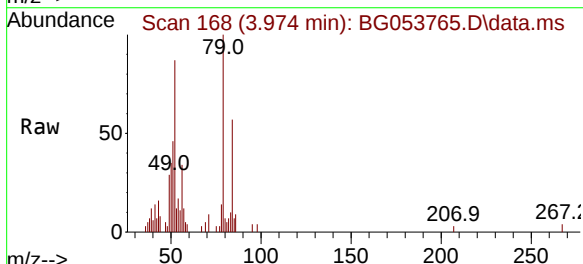


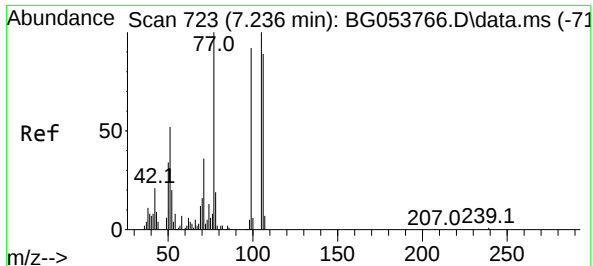

#6
Benzaldehyde
Concen: 8.337 ng/ul
RT: 7.235 min Scan# 71
Delta R.T. -0.001 min
Lab File: BG053765.D
Acq: 31 May 2022 17:56




Instrument :
BNA_G
ClientSampleId :
SSTD010422


Tgt Ion: 77 Resp: 10778
Ion Ratio Lower Upper
77 100
105 92.2 79.7 119.5
106 91.2 71.0 106.4

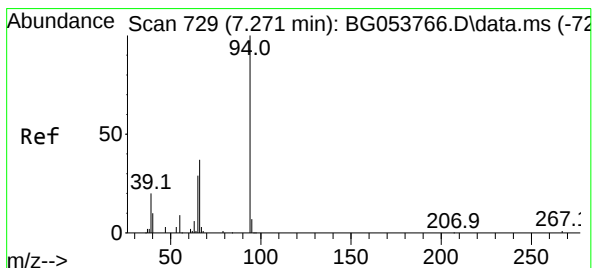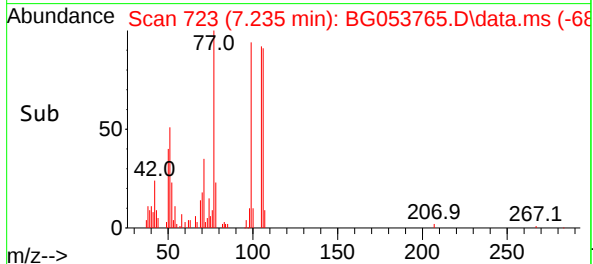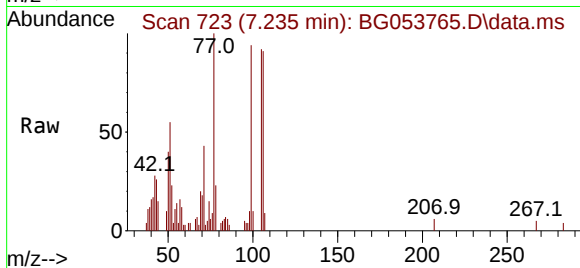

#8
Phenol
Concen: 8.847 ng/ul
RT: 7.276 min Scan# 730
Delta R.T. 0.005 min
Lab File: BG053765.D
Acq: 31 May 2022 17:56

Tgt Ion: 94 Resp: 16582
Ion Ratio Lower Upper
94 100
65 28.8 24.1 36.1
66 40.0 32.5 48.7


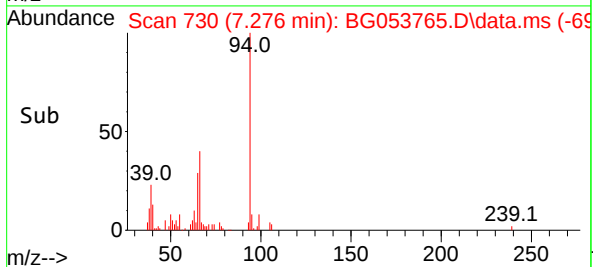

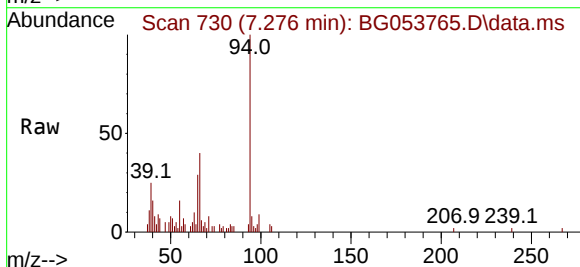




#10
Bis(2-Chloroethyl)ether
Concen: 9.112 ng/ul
RT: 7.517 min Scan# 771
Delta R.T. -0.001 min
Lab File: BG053765.D
Acq: 31 May 2022 17:56




Instrument :
BNA_G
ClientSampleId :
SSTD010422


Tgt Ion: 93 Resp: 12883
Ion Ratio Lower Upper
93 100
63 81.3 72.3 108.5
95 35.1 29.4 44.0



#12
2-Chlorophenol
Concen: 9.717 ng/ul
RT: 7.664 min Scan# 796
Delta R.T. -0.001 min
Lab File: BG053765.D
Acq: 31 May 2022 17:56

Tgt Ion:128 Resp: 13109
Ion Ratio Lower Upper
128 100
64 55.5 41.4 62.2
130 29.1 27.0 40.6









#13
2-Methylphenol
Concen: 8.768 ng/ul
RT: 8.533 min Scan# 944
Delta R.T. -0.001 min
Lab File: BG053765.D
Acq: 31 May 2022 17:56




Instrument :
BNA_G
ClientSampleId :
SSTD010422


Tgt Ion:108 Resp: 12772
Ion Ratio Lower Upper
108 100
107 95.0 75.8 113.8



#14
2,2'-oxybis(1-Chloropropane)
Concen: 9.546 ng/ul
RT: 8.633 min Scan# 961
Delta R.T. 0.005 min
Lab File: BG053765.D
Acq: 31 May 2022 17:56

Tgt Ion: 45 Resp: 21939
Ion Ratio Lower Upper
45 100
77 11.8 10.2 15.4
79 10.7 8.1 12.1







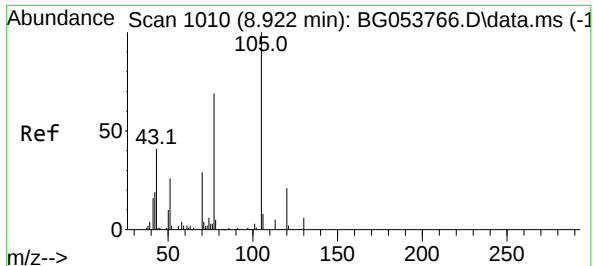

#16
Acetophenone
Concen: 9.325 ng/ul
RT: 8.921 min Scan# 1010
Delta R.T. -0.001 min
Lab File: BG053765.D
Acq: 31 May 2022 17:56




Instrument :
BNA_G
ClientSampleId :
SSTD010422


Tgt Ion:105 Resp: 20492
Ion Ratio Lower Upper
105 100
77 81.3 61.0 91.6
51 30.5 22.8 34.2

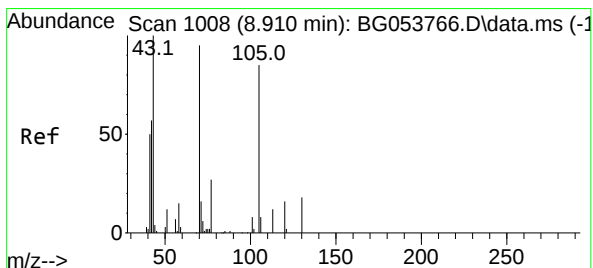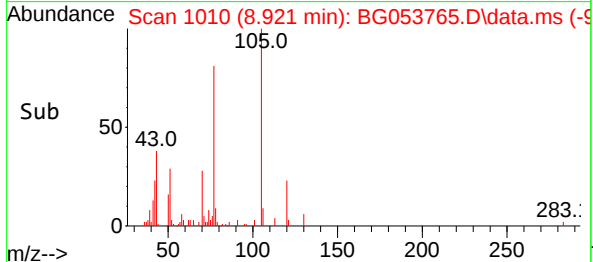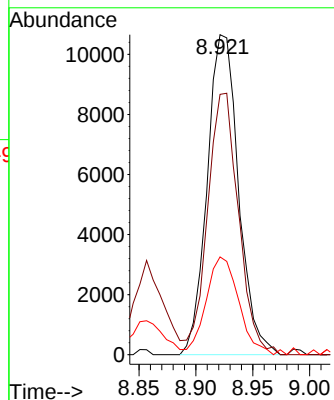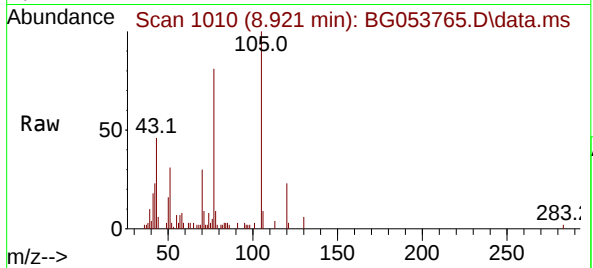

#17
N-Nitroso-di-n-propylamine
Concen: 9.029 ng/ul
RT: 8.909 min Scan# 1008
Delta R.T. -0.001 min
Lab File: BG053765.D
Acq: 31 May 2022 17:56

Tgt Ion: 70 Resp: 11568
Ion Ratio Lower Upper
70 100
42 73.7 50.2 75.4
101 9.7 7.1 10.7
130 20.3 15.5 23.3

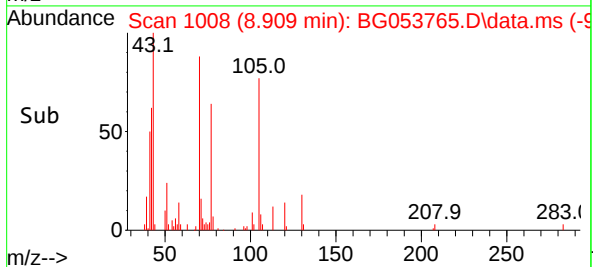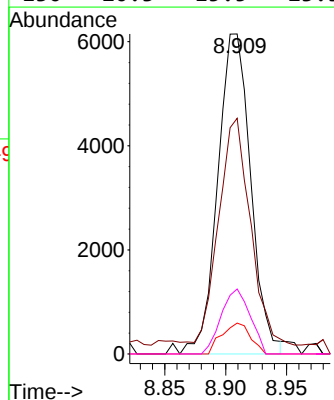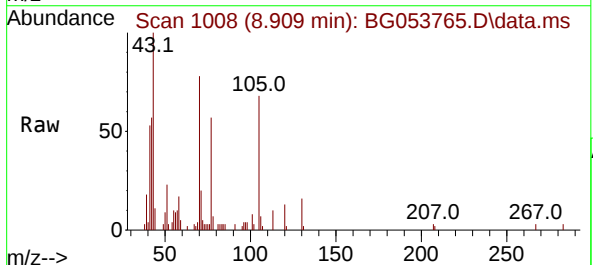



#18

4-Methylphenol

Concen: 8.962 ng/ul

RT: 8.857 min Scan# 999

Delta R.T. -0.001 min

Lab File: BG053765.D

Acq: 31 May 2022 17:56

Instrument :

BNA_G

ClientSampleId :





SSTD010422

Tgt Ion:108 Resp: 13601

Ion Ratio Lower Upper

108 100

107 115.9 90.7 136.1



#19

Hexachloroethane

Concen: 9.654 ng/ul

RT: 9.197 min Scan# 1057

Delta R.T. -0.001 min

Lab File: BG053765.D

Acq: 31 May 2022 17:56




Tgt Ion:117 Resp: 5779


Ion Ratio Lower Upper

117 100

201 126.8 117.4 176.0

199 66.7 64.0 96.0





#22

Nitrobenzene

Concen: 6.960 ng/ul

RT: 9.303 min Scan# 1107

Delta R.T. -0.001 min

Lab File: BG053765.D

Acq: 31 May 2022 17:56

Instrument :

BNA_G

ClientSampleId :

SSTD010422





Tgt Ion: 77 Resp: 12409

Ion Ratio Lower Upper

77 100

123 39.0 31.2 46.8

65 13.9 10.5 15.7

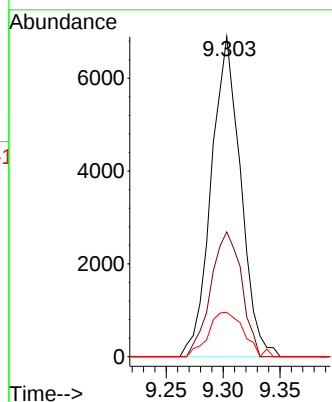

#23

Isophorone

Concen: 8.650 ng/ul

RT: 9.832 min Scan# 1165

Delta R.T. -0.001 min

Lab File: BG053765.D

Acq: 31 May 2022 17:56




Tgt Ion: 82 Resp: 29479


Ion Ratio Lower Upper

82 100

95 8.2 6.1 9.1

138 15.7 13.6 20.4









#25
2-Nitrophenol
Concen: 6.546 ng/ul
RT: 10.020 min Scan# 1197
Delta R.T. 0.005 min
Lab File: BG053765.D
Acq: 31 May 2022 17:56




Instrument :
BNA_G
ClientSampleId :
SSTD010422


Tgt Ion	Ratio	Lower	Upper
139	100		
65	52.9	47.7	71.5
109	38.9	27.1	40.7



#26
2,4-Dimethylphenol
Concen: 9.397 ng/ul
RT: 10.073 min Scan# 1206
Delta R.T. -0.001 min
Lab File: BG053765.D
Acq: 31 May 2022 17:56

Tgt Ion	Ratio	Lower	Upper
107	100		
121	48.5	39.9	59.9
122	85.0	66.7	100.1





#27

Bis(2-Chloroethoxy)methane

Concen: 9.198 ng/ul

RT: 10.314 min Scan# 1247

Delta R.T. -0.001 min

Lab File: BG053765.D

Acq: 31 May 2022 17:56





Instrument :

BNA_G

ClientSampleId :

SSTD010422

Tgt Ion: 93	Resp:	17433
Ion Ratio	Lower	Upper
93	100	
95	31.4	26.5 39.7
123	8.8	8.8 13.2#

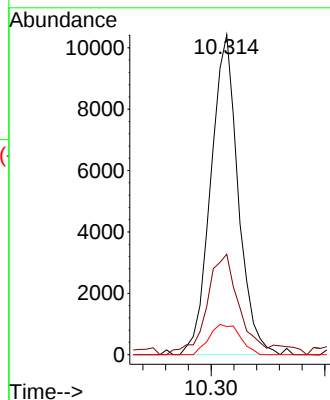

#29

2,4-Dichlorophenol

Concen: 9.364 ng/ul




RT: 10.549 min Scan# 1287


Delta R.T. -0.001 min

Lab File: BG053765.D

Acq: 31 May 2022 17:56

Tgt Ion: 162	Resp:	12748
Ion Ratio	Lower	Upper
162	100	
164	63.3	50.9 76.3
98	36.4	28.5 42.7



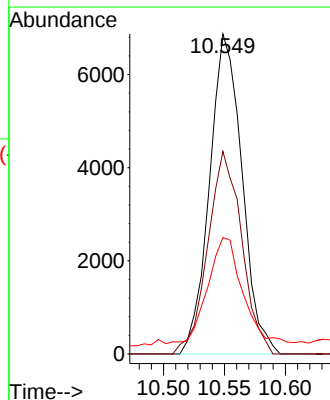





#30
Naphthalene
Concen: 9.450 ng/ul
RT: 10.966 min Scan# 1358
Delta R.T. -0.001 min
Lab File: BG053765.D
Acq: 31 May 2022 17:56




Instrument :
BNA_G
ClientSampleId :
SSTD010422


Tgt Ion:128 Resp: 41455
Ion Ratio Lower Upper
128 100
129 11.1 9.0 13.6
127 14.4 11.1 16.7

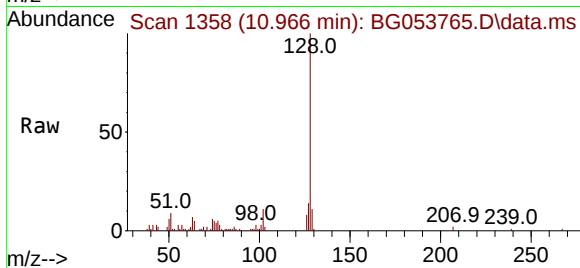

#32
4-Chloroaniline
Concen: 9.481 ng/ul
RT: 11.060 min Scan# 1374
Delta R.T. -0.001 min
Lab File: BG053765.D
Acq: 31 May 2022 17:56

Tgt Ion:127 Resp: 17241
Ion Ratio Lower Upper
127 100
129 31.5 25.4 38.2




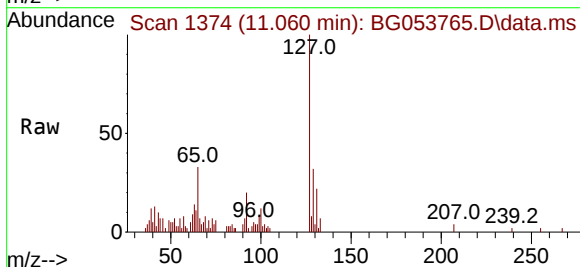




#33
Hexachlorobutadiene
Concen: 9.785 ng/ul
RT: 11.260 min Scan# 1408
Delta R.T. -0.001 min
Lab File: BG053765.D
Acq: 31 May 2022 17:56




Instrument :
BNA_G
ClientSampleId :
SSTD010422


Tgt Ion:225 Resp: 10879
Ion Ratio Lower Upper
225 100
223 60.6 50.2 75.2
227 67.1 51.8 77.6



#34
Caprolactam
Concen: 7.536 ng/ul
RT: 11.824 min Scan# 1504
Delta R.T. -0.007 min
Lab File: BG053765.D
Acq: 31 May 2022 17:56

Tgt Ion:113 Resp: 3090
Ion Ratio Lower Upper
113 100
55 204.0 167.8 251.6
56 132.0 127.6 191.4









#35
 4-Chloro-3-methylphenol
 Concen: 8.914 ng/ul
 RT: 12.170 min Scan# 1563
 Delta R.T. -0.001 min
 Lab File: BG053765.D
 Acq: 31 May 2022 17:56




Instrument :
 BNA_G
 ClientSampleId :
 SSTD010422


Tgt Ion:	107	Resp:	13163
Ion	Ratio	Lower	Upper
107	100		
144	31.3	21.3	31.9
142	83.5	65.0	97.4

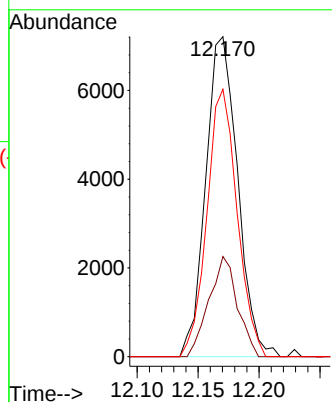

#36
 2-Methylnaphthalene
 Concen: 9.379 ng/ul
 RT: 12.564 min Scan# 1630
 Delta R.T. -0.001 min
 Lab File: BG053765.D
 Acq: 31 May 2022 17:56

Tgt Ion:	142	Resp:	29035
Ion	Ratio	Lower	Upper
142	100		
141	91.7	76.3	114.5



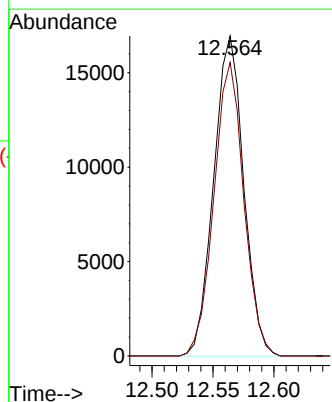



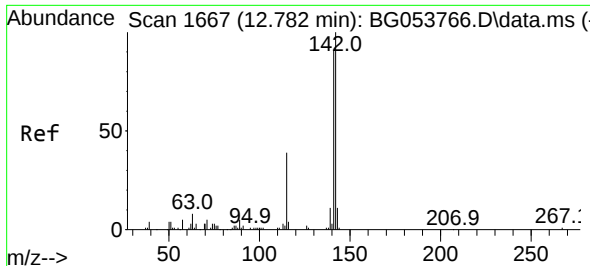

#37
 1-Methylnaphthalene
 Concen: 9.012 ng/ul
 RT: 12.781 min Scan# 1667
 Delta R.T. -0.001 min
 Lab File: BG053765.D
 Acq: 31 May 2022 17:56




Instrument :
 BNA_G
 ClientSampleId :
 SSTD010422


Tgt Ion:142 Resp: 28246
 Ion Ratio Lower Upper
 142 100
 141 97.1 73.4 110.2
 116 4.3 3.2 4.8

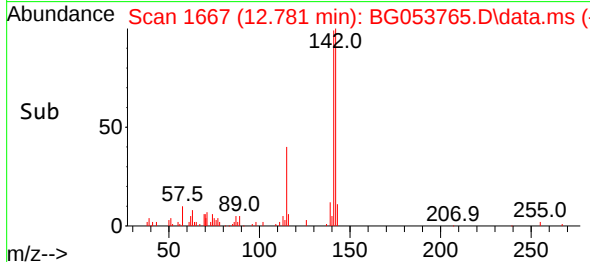

#39
 1,2,4,5-Tetrachlorobenzene
 Concen: 10.327 ng/ul
 RT: 12.928 min Scan# 1692
 Delta R.T. -0.001 min
 Lab File: BG053765.D
 Acq: 31 May 2022 17:56

Tgt Ion:216 Resp: 19592
 Ion Ratio Lower Upper
 216 100
 214 73.6 58.1 87.1
 179 18.4 14.8 22.2
 108 12.4 10.4 15.6


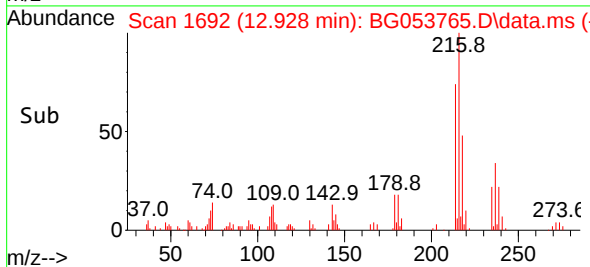

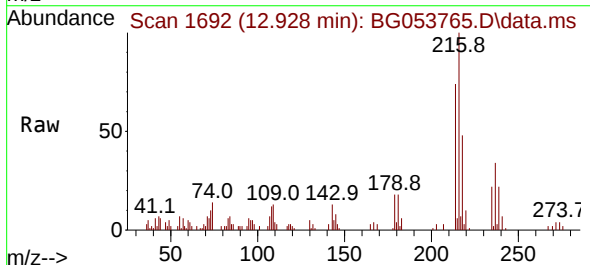




#40
Hexachlorocyclopentadiene
Concen: 9.624 ng/ul
RT: 12.916 min Scan# 1689
Delta R.T. 0.005 min
Lab File: BG053765.D
Acq: 31 May 2022 17:56




Instrument :
BNA_G
ClientSampleId :
SSTD010422


Tgt Ion:237 Resp: 12640
Ion Ratio Lower Upper
237 100
235 66.3 47.0 70.6
272 0.0 8.6 12.8#



#41
2,4,6-Trichlorophenol
Concen: 9.264 ng/ul
RT: 13.157 min Scan# 1731
Delta R.T. -0.001 min
Lab File: BG053765.D
Acq: 31 May 2022 17:56

Tgt Ion:196 Resp: 10740
Ion Ratio Lower Upper
196 100
198 92.8 81.9 122.9
200 28.3 25.7 38.5









#42
2,4,5-Trichlorophenol
Concen: 9.447 ng/ul
RT: 13.228 min Scan# 11
Delta R.T. -0.001 min
Lab File: BG053765.D
Acq: 31 May 2022 17:56




Instrument :
BNA_G
ClientSampleId :
SSTD010422


Tgt Ion:196 Resp: 11827
Ion Ratio Lower Upper
196 100
198 91.5 76.3 114.5
200 30.7 25.5 38.3



#43
1,1'-Biphenyl
Concen: 9.814 ng/ul
RT: 13.563 min Scan# 1800
Delta R.T. -0.001 min
Lab File: BG053765.D
Acq: 31 May 2022 17:56

Tgt Ion:154 Resp: 40252
Ion Ratio Lower Upper
154 100
153 41.6 32.7 49.1
76 12.0 9.0 13.6









#44
2-Chloronaphthalene
Concen: 9.704 ng/ul
RT: 13.604 min Scan# 1807
Delta R.T. -0.001 min
Lab File: BG053765.D
Acq: 31 May 2022 17:56




Instrument :
BNA_G
ClientSampleId :
SSTD010422


Tgt Ion:	162	Resp:	31870
Ion	Ratio	Lower	Upper
162	100		
164	31.8	25.7	38.5
127	35.0	28.3	42.5



#45
2-Nitroaniline
Concen: 5.804 ng/ul
RT: 13.792 min Scan# 1839
Delta R.T. -0.007 min
Lab File: BG053765.D
Acq: 31 May 2022 17:56

Tgt Ion:	65	Resp:	5588
Ion	Ratio	Lower	Upper
65	100		
92	67.1	52.2	78.4
138	99.8	79.0	118.4





#47

Dimethylphthalate

Concen: 9.667 ng/ul

RT: 14.174 min Scan# 1904

Delta R.T. -0.001 min

Lab File: BG053765.D

Acq: 31 May 2022 17:56

Instrument :

BNA_G

ClientSampleId :

SSTD010422





Tgt Ion:163 Resp: 40678

Ion Ratio Lower Upper

163 100

194 4.4 3.7 5.5

164 11.1 7.9 11.9



#48

2,6-Dinitrotoluene

Concen: 6.757 ng/ul

RT: 14.285 min Scan# 1923

Delta R.T. -0.001 min

Lab File: BG053765.D

Acq: 31 May 2022 17:56




Tgt Ion:165 Resp: 5151


Ion Ratio Lower Upper

165 100

89 52.2 44.7 67.1

121 19.1 16.9 25.3









#50
Acenaphthylene
Concen: 9.970 ng/ul
RT: 14.450 min Scan# 1951
Delta R.T. -0.001 min
Lab File: BG053765.D
Acq: 31 May 2022 17:56




Instrument :
BNA_G
ClientSampleId :
SSTD010422


Tgt Ion:152	Resp:	51593
Ion Ratio	Lower	Upper
152	100	
151	20.6	16.2 24.2
153	13.8	10.5 15.7

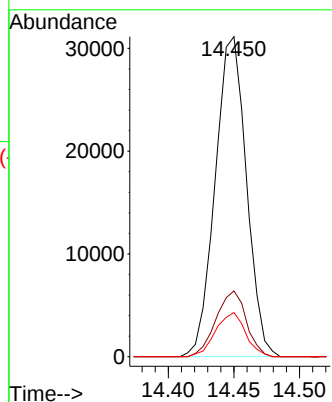

#51
3-Nitroaniline
Concen: 6.225 ng/ul
RT: 14.615 min Scan# 1979
Delta R.T. 0.005 min
Lab File: BG053765.D
Acq: 31 May 2022 17:56

Tgt Ion:138	Resp:	4790
Ion Ratio	Lower	Upper
138	100	
108	36.4	17.8 26.6#
92	115.7	94.2 141.4







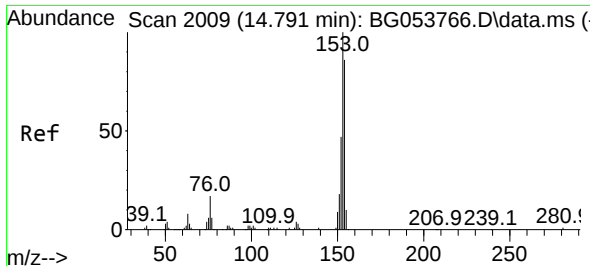

#52
Acenaphthene
Concen: 10.014 ng/ul
RT: 14.791 min Scan# 2009
Delta R.T. -0.001 min
Lab File: BG053765.D
Acq: 31 May 2022 17:56




Instrument :
BNA_G
ClientSampleId :
SSTD010422


Tgt Ion:153 Resp: 33855
Ion Ratio Lower Upper
153 100
152 48.9 37.5 56.3
154 88.5 68.8 103.2

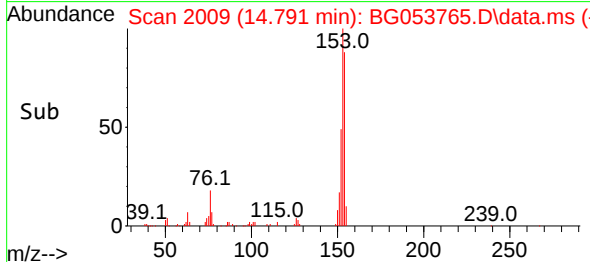

#53
2,4-Dinitrophenol
Concen: 4.323 ng/ul
RT: 14.814 min Scan# 2013
Delta R.T. -0.001 min
Lab File: BG053765.D
Acq: 31 May 2022 17:56

Tgt Ion:184 Resp: 2047
Ion Ratio Lower Upper
184 100
63 44.4 34.7 52.1
154 121.5 87.3 130.9


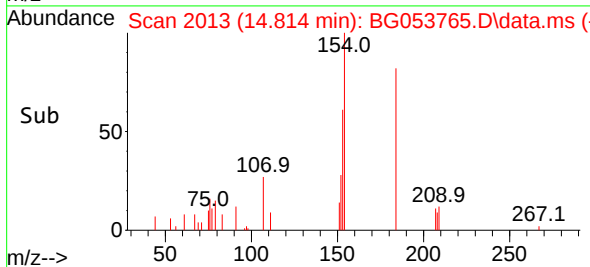

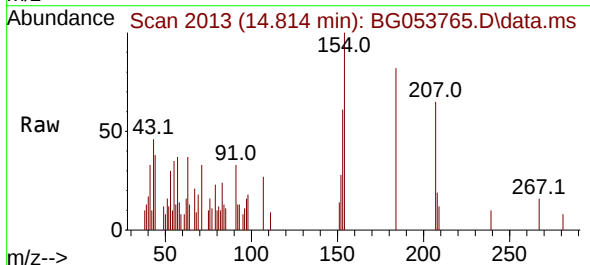


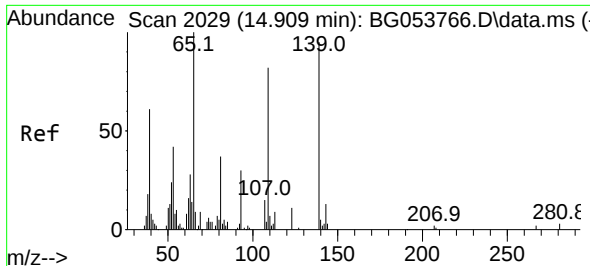

#55
4-Nitrophenol
Concen: 5.612 ng/ul
RT: 14.902 min Scan# 2029
Delta R.T. -0.007 min
Lab File: BG053765.D
Acq: 31 May 2022 17:56




Instrument :
BNA_G
ClientSampleId :
SSTD010422


Tgt Ion:109 Resp: 4379
Ion Ratio Lower Upper
109 100
139 122.5 92.9 139.3
65 126.7 97.8 146.6

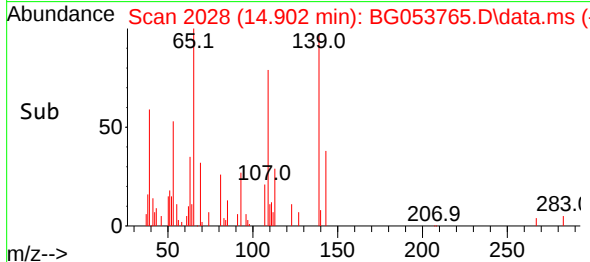

#56
Dibenzofuran
Concen: 9.743 ng/ul
RT: 15.120 min Scan# 2065
Delta R.T. -0.001 min
Lab File: BG053765.D
Acq: 31 May 2022 17:56

Tgt Ion:168 Resp: 48830
Ion Ratio Lower Upper
168 100
139 36.0 28.2 42.2


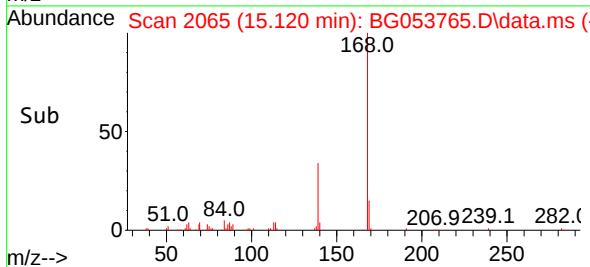

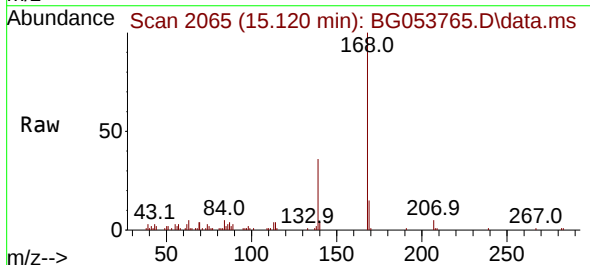




#57
2,4-Dinitrotoluene
Concen: 6.519 ng/ul
RT: 15.067 min Scan# 2056
Delta R.T. -0.001 min
Lab File: BG053765.D
Acq: 31 May 2022 17:56




Instrument :
BNA_G
ClientSampleId :
SSTD010422


Tgt Ion:165	Resp:	7051
Ion Ratio	Lower	Upper
165	100	
63	38.0	33.0 49.4
182	4.2	2.8 4.2

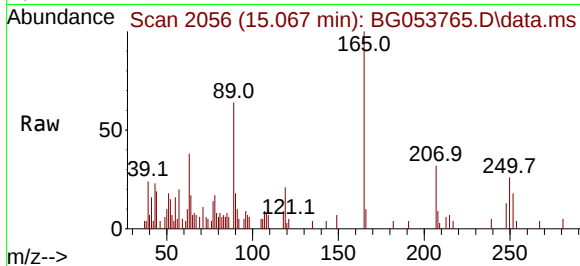

#58
2,3,4,6-Tetrachlorophenol
Concen: 8.378 ng/ul
RT: 15.343 min Scan# 2103
Delta R.T. -0.001 min
Lab File: BG053765.D
Acq: 31 May 2022 17:56

Tgt Ion:232	Resp:	9454
Ion Ratio	Lower	Upper
232	100	
131	29.1	27.5 41.3
130	2.2	1.8 2.8
166	20.5	20.7 31.1#




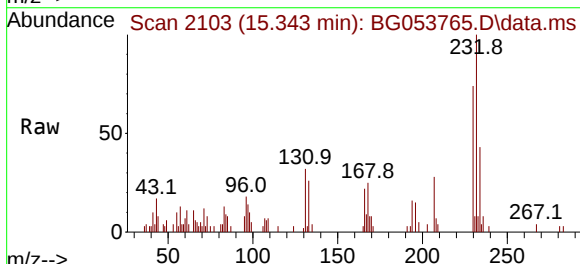




#59
Diethylphthalate
Concen: 9.837 ng/ul
RT: 15.537 min Scan# 2136
Delta R.T. -0.001 min
Lab File: BG053765.D
Acq: 31 May 2022 17:56




Instrument :
BNA_G
ClientSampleId :
SSTD010422


Tgt Ion:149 Resp: 41923
Ion Ratio Lower Upper
149 100
177 23.0 18.9 28.3
150 11.5 10.6 15.8

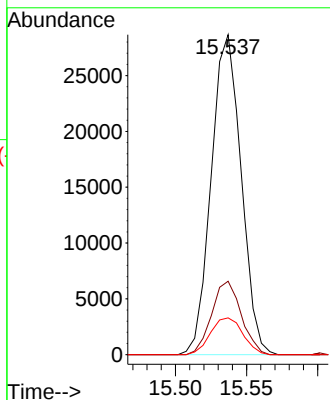

#61
Fluorene
Concen: 9.743 ng/ul
RT: 15.772 min Scan# 2176
Delta R.T. -0.001 min
Lab File: BG053765.D
Acq: 31 May 2022 17:56

Tgt Ion:166 Resp: 40474
Ion Ratio Lower Upper
166 100
165 100.3 81.7 122.5
167 14.0 11.0 16.4


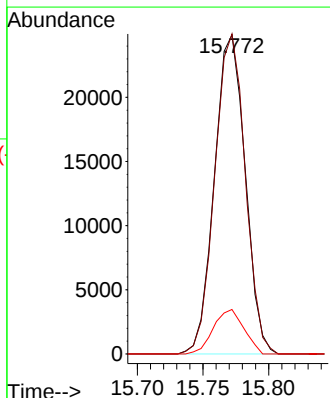






#62
4-Chlorophenyl-phenylether
Concen: 10.190 ng/ul
RT: 15.766 min Scan# 2175
Delta R.T. 0.005 min
Lab File: BG053765.D
Acq: 31 May 2022 17:56




Instrument :
BNA_G
ClientSampleId :
SSTD010422


Tgt Ion:204 Resp: 22526
Ion Ratio Lower Upper
204 100
206 31.0 27.1 40.7
141 48.4 40.7 61.1

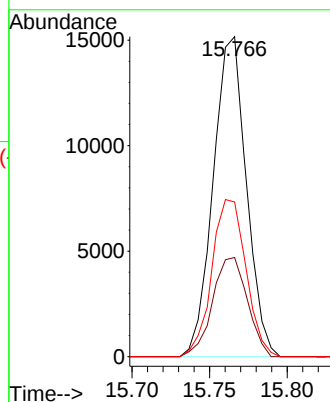

#63
4-Nitroaniline
Concen: 6.514 ng/ul
RT: 15.772 min Scan# 2176
Delta R.T. -0.001 min
Lab File: BG053765.D
Acq: 31 May 2022 17:56

Tgt Ion:138 Resp: 4929
Ion Ratio Lower Upper
138 100
92 48.6 42.0 63.0
108 104.1 79.0 118.6



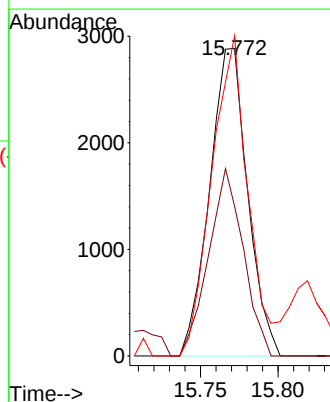





#66
4,6-Dinitro-2-methylphenol
Concen: 4.476 ng/ul
RT: 15.831 min Scan# 2186
Delta R.T. -0.001 min
Lab File: BG053765.D
Acq: 31 May 2022 17:56




Instrument :
BNA_G
ClientSampleId :
SSTD010422


Tgt Ion:198 Resp: 3131
Ion Ratio Lower Upper
198 100
182 0.0 3.4 5.0#
77 21.1 14.7 22.1

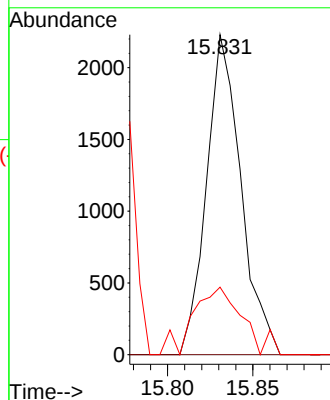

#67
N-Nitrosodiphenylamine
Concen: 9.711 ng/ul
RT: 15.972 min Scan# 2210
Delta R.T. -0.001 min
Lab File: BG053765.D
Acq: 31 May 2022 17:56

Tgt Ion:169 Resp: 36890
Ion Ratio Lower Upper
169 100
168 62.1 51.0 76.4
167 34.5 28.7 43.1



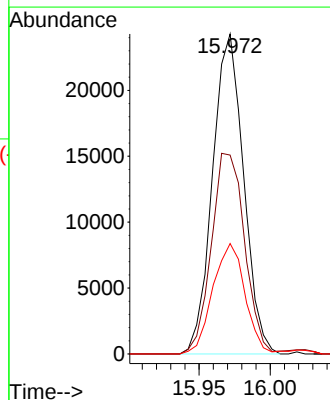





#68
4-Bromophenyl-phenylether
Concen: 10.366 ng/ul
RT: 16.659 min Scan# 21
Delta R.T. -0.001 min
Lab File: BG053765.D
Acq: 31 May 2022 17:56




Instrument :
BNA_G
ClientSampleId :
SSTD010422


Tgt Ion	Ratio	Lower	Upper
248	100		
250	106.2	78.2	117.2
141	60.7	46.7	70.1

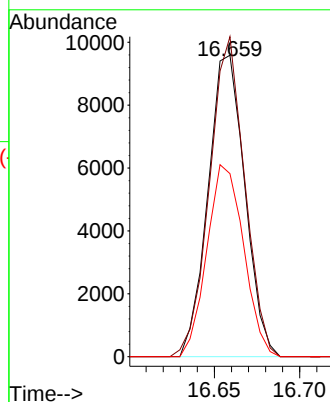

#69
Hexachlorobenzene
Concen: 9.376 ng/ul
RT: 16.777 min Scan# 2347
Delta R.T. -0.001 min
Lab File: BG053765.D
Acq: 31 May 2022 17:56

Tgt Ion	Ratio	Lower	Upper
284	100		
142	25.5	20.8	31.2
249	30.5	27.4	41.0



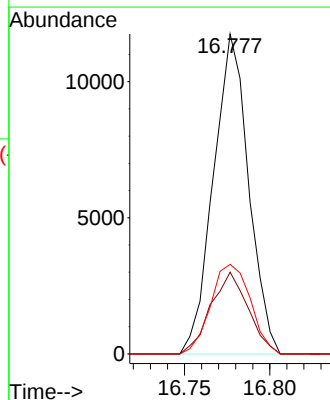





#70
Atrazine
Concen: 10.406 ng/ul
RT: 16.918 min Scan# 21
Delta R.T. -0.001 min
Lab File: BG053765.D
Acq: 31 May 2022 17:56




Instrument :
BNA_G
ClientSampleId :
SSTD010422


Tgt Ion:200 Resp: 16200
Ion Ratio Lower Upper
200 100
173 21.2 19.8 29.6
215 47.9 38.8 58.2



#71
Pentachlorophenol
Concen: 6.981 ng/ul
RT: 17.117 min Scan# 2405
Delta R.T. 0.005 min
Lab File: BG053765.D
Acq: 31 May 2022 17:56

Tgt Ion:266 Resp: 7628
Ion Ratio Lower Upper
266 100
264 58.3 56.8 85.2
268 61.4 48.0 72.0



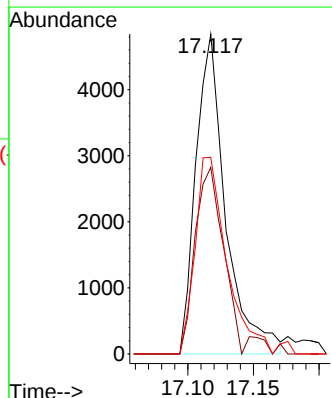



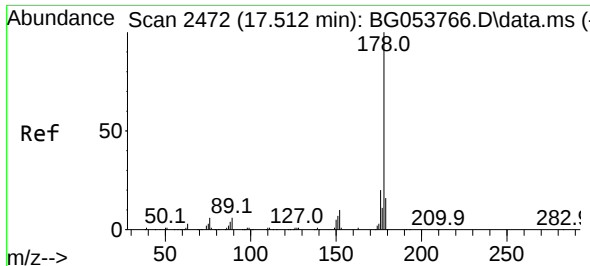

#72
Phenanthrene
Concen: 9.422 ng/ul
RT: 17.511 min Scan# 2472
Delta R.T. -0.001 min
Lab File: BG053765.D
Acq: 31 May 2022 17:56




Instrument :
BNA_G
ClientSampleId :
SSTD010422


Tgt Ion:178 Resp: 69476
Ion Ratio Lower Upper
178 100
179 15.6 12.6 19.0
176 18.5 15.7 23.5

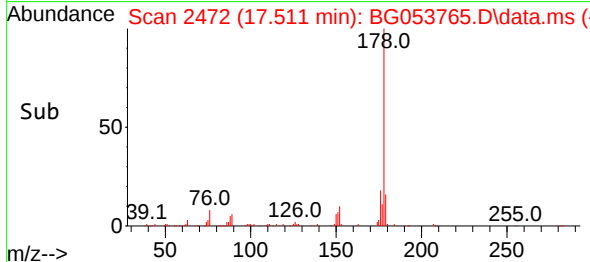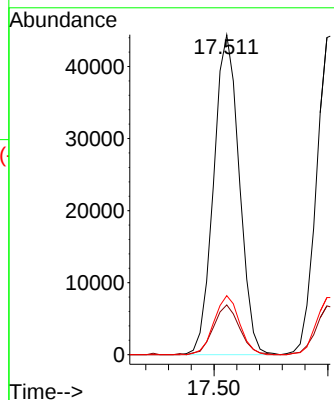

#74
Anthracene
Concen: 9.753 ng/ul
RT: 17.605 min Scan# 2488
Delta R.T. 0.005 min
Lab File: BG053765.D
Acq: 31 May 2022 17:56

Tgt Ion:178 Resp: 71900
Ion Ratio Lower Upper
178 100
179 14.7 12.4 18.6
176 17.9 14.6 22.0


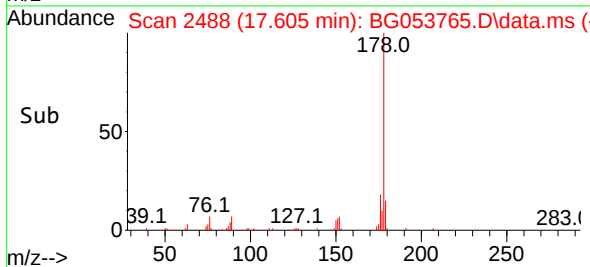
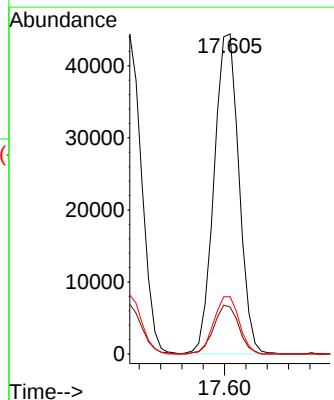
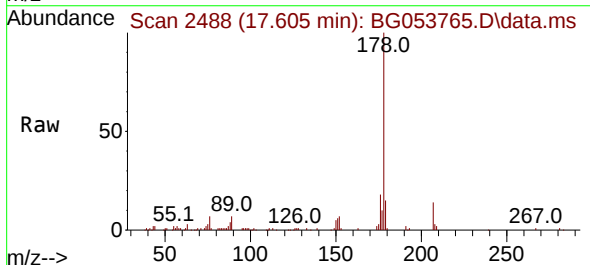




#75
1,2,3,4-Tetrachlorobenzene
Concen: 10.085 ng/uL
RT: 13.528 min Scan# 11
Delta R.T. -0.001 min
Lab File: BG053765.D
Acq: 31 May 2022 17:56




Instrument :
BNA_G
ClientSampleId :
SSTD010422


Tgt Ion:	216	Resp:	21103
Ion Ratio	Lower	Upper	
216	100		
214	75.2	64.2	96.4
218	51.3	39.0	58.4



#76
Pentachlorobenzene
Concen: 9.361 ng/uL
RT: 15.043 min Scan# 2052
Delta R.T. -0.001 min
Lab File: BG053765.D
Acq: 31 May 2022 17:56

Tgt Ion:	250	Resp:	18792
Ion Ratio	Lower	Upper	
250	100		
248	64.7	47.7	71.5
252	66.8	50.0	75.0







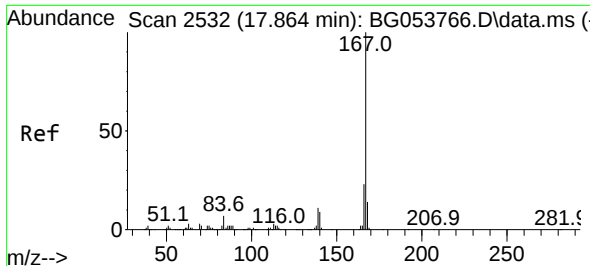

#77
 Carbazole
 Concen: 9.923 ng/ul
 RT: 17.864 min Scan# 2532
 Delta R.T. -0.001 min
 Lab File: BG053765.D
 Acq: 31 May 2022 17:56




Instrument :
 BNA_G
 ClientSampleId :
 SST010422


Tgt Ion:167 Resp: 64649
 Ion Ratio Lower Upper
 167 100
 166 22.5 18.2 27.2
 139 11.2 9.0 13.6

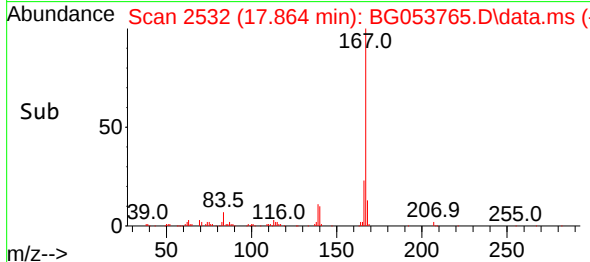

#78
 Di-n-butylphthalate
 Concen: 10.022 ng/ul
 RT: 18.434 min Scan# 2629
 Delta R.T. -0.001 min
 Lab File: BG053765.D
 Acq: 31 May 2022 17:56

Tgt Ion:149 Resp: 77641
 Ion Ratio Lower Upper
 149 100
 150 9.1 7.1 10.7
 104 6.0 4.2 6.2


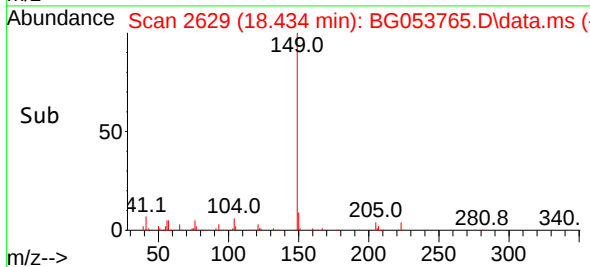

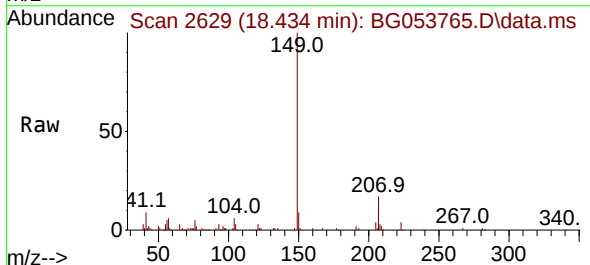




#80
Fluoranthene
Concen: 8.665 ng/ul
RT: 19.515 min Scan# 2813
Delta R.T. -0.001 min
Lab File: BG053765.D
Acq: 31 May 2022 17:56




Instrument :
BNA_G
ClientSampleId :
SSTD010422


Tgt Ion:202 Resp: 90881
Ion Ratio Lower Upper
202 100
101 8.2 6.6 9.8
100 6.3 5.8 8.8

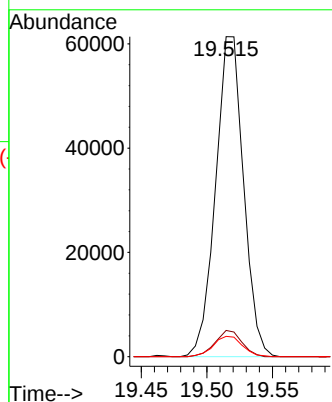

#82
Pyrene
Concen: 8.743 ng/ul
RT: 19.879 min Scan# 2875
Delta R.T. -0.001 min
Lab File: BG053765.D
Acq: 31 May 2022 17:56

Tgt Ion:202 Resp: 91136
Ion Ratio Lower Upper
202 100
101 8.9 7.3 10.9
100 7.7 6.2 9.4







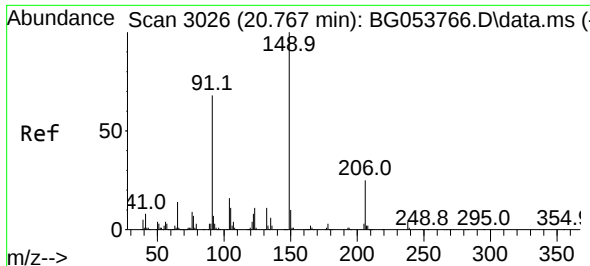

#83
Butylbenzylphthalate
Concen: 9.109 ng/ul
RT: 20.766 min Scan# 3026
Delta R.T. -0.001 min
Lab File: BG053765.D
Acq: 31 May 2022 17:56




Instrument :
BNA_G
ClientSampleId :
SSTD010422


Tgt Ion:	149	Resp:	33016
Ion Ratio	Lower	Upper	
149	100		
91	67.6	54.0	81.0
206	25.9	19.5	29.3

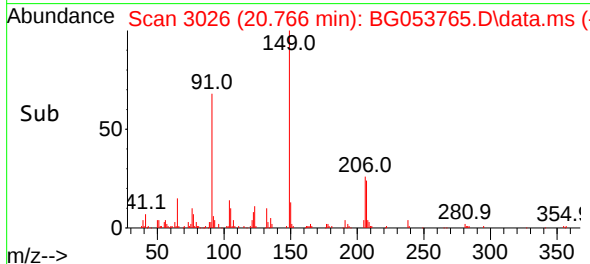

#84
3,3'-Dichlorobenzidine
Concen: 9.963 ng/ul
RT: 21.642 min Scan# 3175
Delta R.T. 0.005 min
Lab File: BG053765.D
Acq: 31 May 2022 17:56

Tgt Ion:	252	Resp:	35524
Ion Ratio	Lower	Upper	
252	100		
254	63.8	49.6	74.4
126	7.3	6.0	9.0


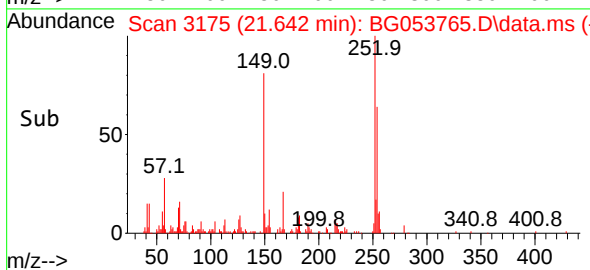

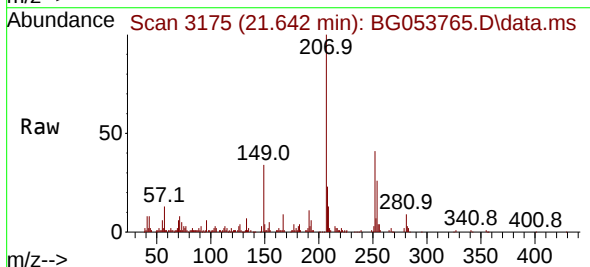




#85
Benzo(a)anthracene
Concen: 9.363 ng/ul
RT: 21.730 min Scan# 3190
Delta R.T. -0.001 min
Lab File: BG053765.D
Acq: 31 May 2022 17:56




Instrument :
BNA_G
ClientSampleId :
SSTD010422


Tgt Ion:228 Resp: 96138
Ion Ratio Lower Upper
228 100
229 20.0 16.5 24.7
226 28.0 22.1 33.1

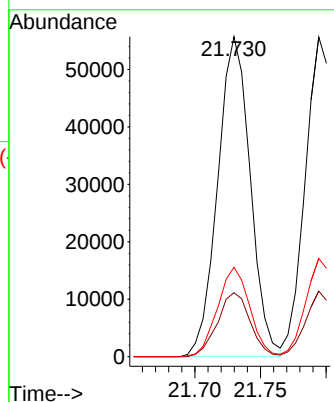

#86
Bis(2-ethylhexyl)phthalate
Concen: 9.670 ng/ul
RT: 21.653 min Scan# 3177
Delta R.T. -0.001 min
Lab File: BG053765.D
Acq: 31 May 2022 17:56

Tgt Ion:149 Resp: 48543
Ion Ratio Lower Upper
149 100
167 26.6 21.7 32.5
279 5.5 3.9 5.9

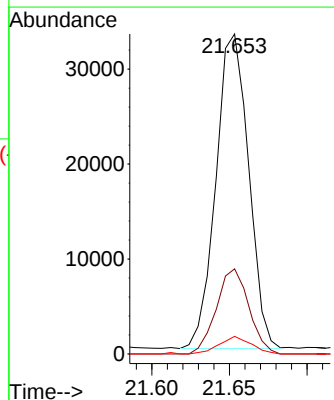



#87

Chrysene

Concen: 9.395 ng/ul

RT: 21.794 min Scan# 31

Delta R.T. -0.001 min

Lab File: BG053765.D

Acq: 31 May 2022 17:56

Instrument :

BNA_G

ClientSampleId :

SSTD010422





Tgt Ion:228 Resp: 92016

Ion Ratio Lower Upper

228 100

226 30.7 24.2 36.4

229 20.5 16.3 24.5



#89

Di-n-octyl phthalate

Concen: 10.120 ng/ul




RT: 22.887 min Scan# 3387


Delta R.T. -0.001 min

Lab File: BG053765.D

Acq: 31 May 2022 17:56

Tgt Ion:149 Resp: 83187









#90
Benzo(b)fluoranthene
Concen: 9.103 ng/ul
RT: 23.980 min Scan# 31
Delta R.T. -0.007 min
Lab File: BG053765.D
Acq: 31 May 2022 17:56




Instrument :
BNA_G
ClientSampleId :
SSTD010422


Tgt Ion:252 Resp: 92769
Ion Ratio Lower Upper
252 100
253 21.3 18.2 27.4
125 7.1 6.1 9.1

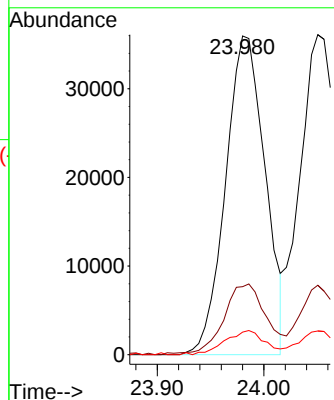

#91
Benzo(k)fluoranthene
Concen: 9.647 ng/ul
RT: 24.051 min Scan# 3585
Delta R.T. -0.001 min
Lab File: BG053765.D
Acq: 31 May 2022 17:56

Tgt Ion:252 Resp: 90727
Ion Ratio Lower Upper
252 100
253 21.7 17.4 26.2
125 7.4 5.4 8.0



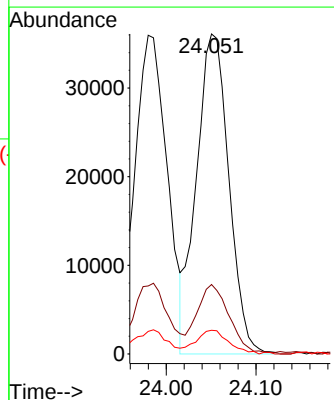





#93
Benzo(a)pyrene
Concen: 9.467 ng/ul
RT: 24.867 min Scan# 31
Delta R.T. -0.007 min
Lab File: BG053765.D
Acq: 31 May 2022 17:56




Instrument :
BNA_G
ClientSampleId :
SSTD010422


Tgt Ion:252 Resp: 91079
Ion Ratio Lower Upper
252 100
253 21.6 17.6 26.4
125 7.9 6.8 10.2



#94
Indeno(1,2,3-cd)pyrene
Concen: 9.554 ng/ul
RT: 28.763 min Scan# 4387
Delta R.T. -0.007 min
Lab File: BG053765.D
Acq: 31 May 2022 17:56

Tgt Ion:276 Resp: 103956
Ion Ratio Lower Upper
276 100
138 13.6 10.1 15.1
277 24.9 19.9 29.9









#95
 Dibenzo(a,h)anthracene
 Concen: 9.694 ng/ul
 RT: 28.839 min Scan# 4400
 Delta R.T. -0.001 min
 Lab File: BG053765.D
 Acq: 31 May 2022 17:56

Instrument :
 BNA_G
 ClientSampleId :
 SSTD010422

Tgt Ion:278 Resp: 89656
 Ion Ratio Lower Upper
 278 100
 139 10.0 8.6 13.0
 279 23.9 19.4 29.0



#96
 Benzo(g,h,i)perylene
 Concen: 9.488 ng/ul
 RT: 29.926 min Scan# 4585
 Delta R.T. -0.001 min
 Lab File: BG053765.D
 Acq: 31 May 2022 17:56

Tgt Ion:276 Resp: 87269
 Ion Ratio Lower Upper
 276 100
 138 15.2 11.3 16.9
 277 25.7 18.6 27.8

