
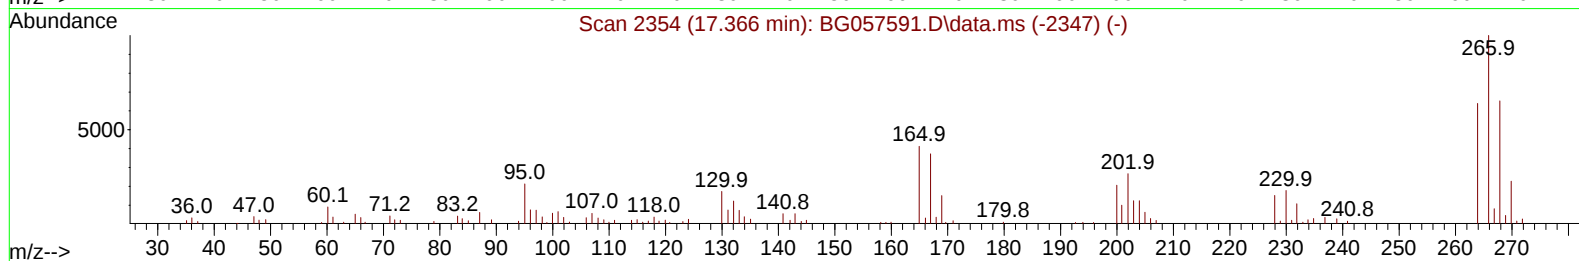
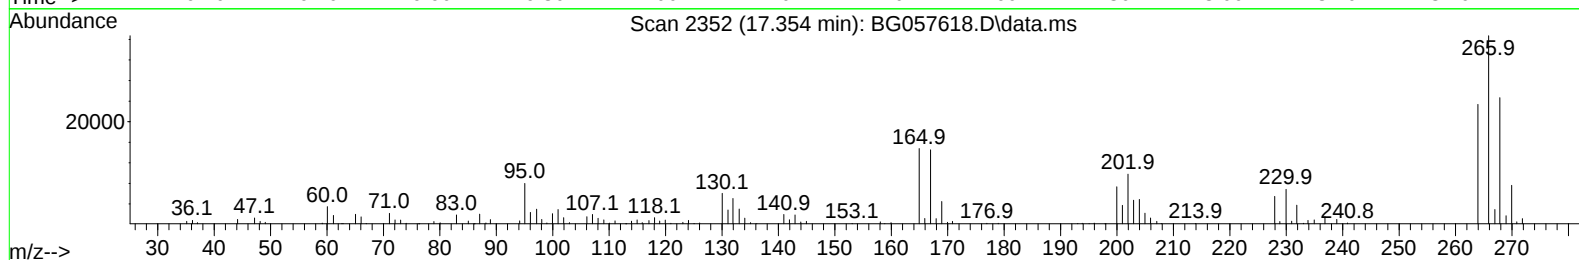


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG053123\
Data File : BG057618.D
Acq On : 31 May 2023 11:39
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 01 05:23:57 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG052723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 01 03:51:58 2023
Response via : Initial Calibration

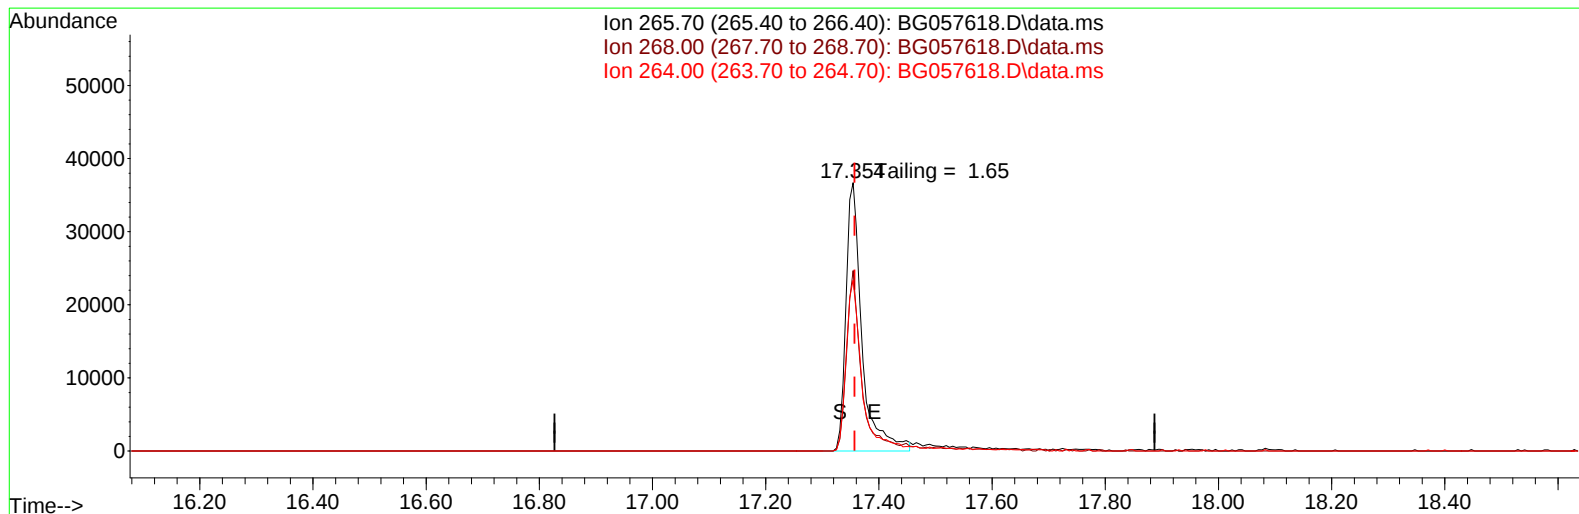

TIC: BG057618.D\data.ms

(70) Pentachlorophenol (C)




17.354min (-0.002) 56482.28 ng

response 71214

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	67.20
264.00	64.00	63.63
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG053123\
Data File : BG057618.D
Acq On : 31 May 2023 11:39
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 01 05:23:57 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG052723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 01 03:51:58 2023
Response via : Initial Calibration

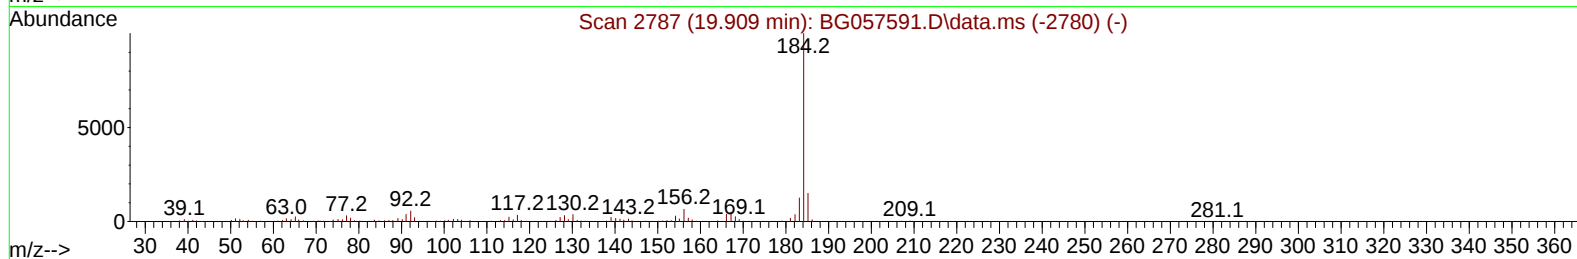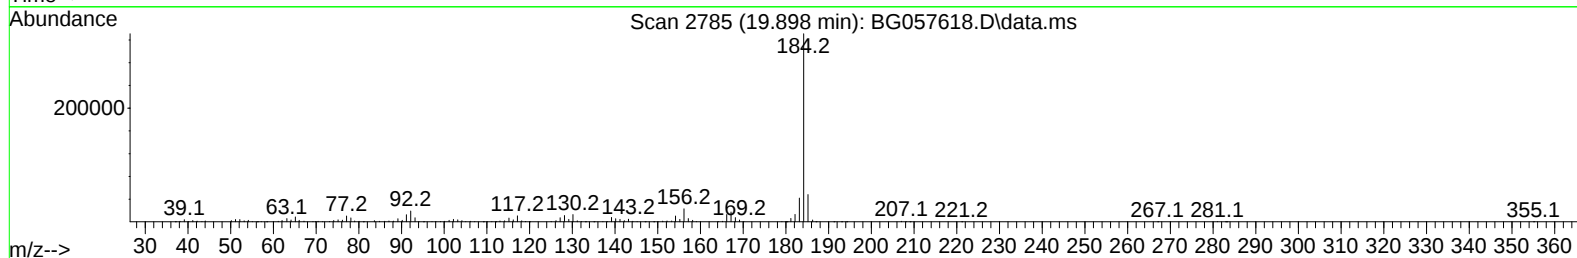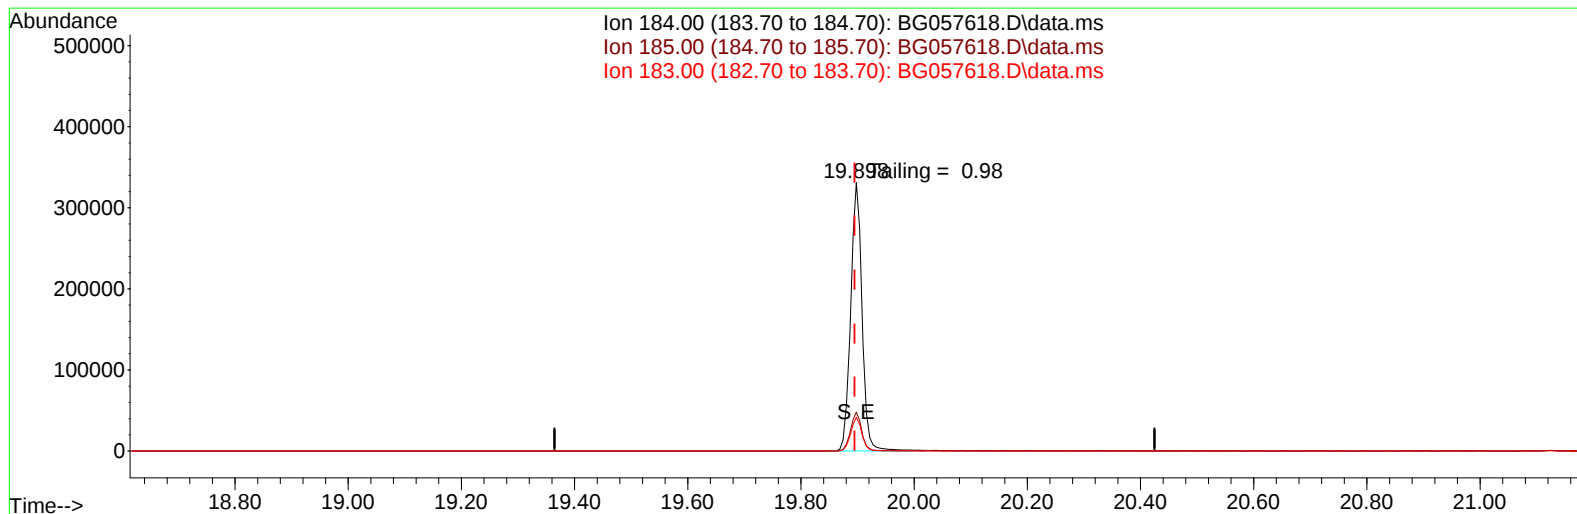

TIC: BG057618.D\data.ms

(77) Benzidine**19.898min (+ 0.003) 279840.02 ng****response 465740**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.49
183.00	12.50	12.62
0.00	0.00	0.00