
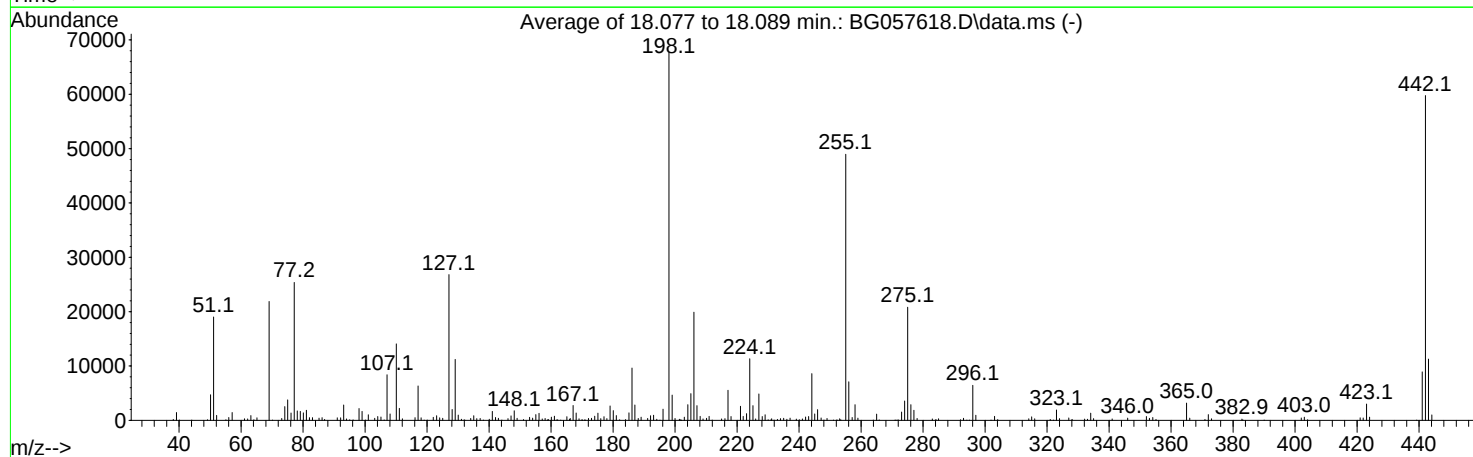


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG053123\
Data File : BG057618.D
Acq On : 31 May 2023 11:39
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG052723.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jun 01 03:51:58 2023

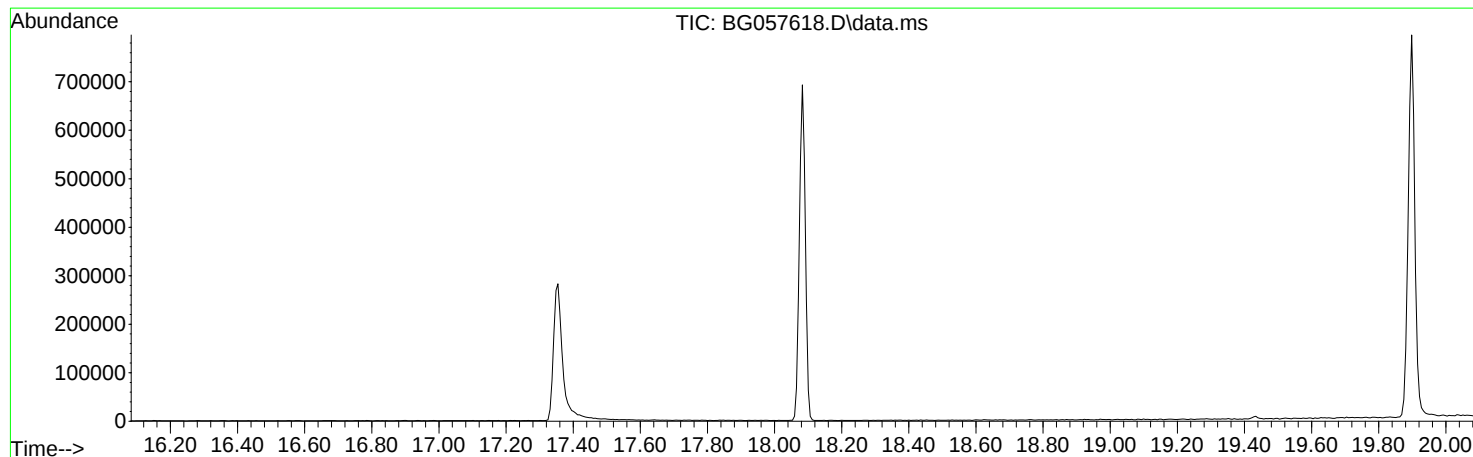

AutoFind: Scans 2475, 2476, 2477; Background Corrected with Scan 2469

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.1	19031	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	32.3	21867	PASS
70	69	0.00	2	0.3	62	PASS
127	198	10	80	39.6	26824	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	67688	PASS
199	198	5	9	6.9	4661	PASS
275	198	10	60	30.7	20808	PASS
365	198	1	100	4.7	3191	PASS
441	198	0.01	100	13.2	8926	PASS
442	442	50	100	100.0	59763	PASS
443	442	15	24	18.9	11291	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/31/2023	BNA_G	<u>BG057618.D</u>
Compound Name	Response	Retention Time
DDT	206739	21.126
DDD	5732	20.72
DDE	312	20.168
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6044	212783	2.84

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG053123\
Data File : BG057618.D
Acq On : 31 May 2023 11:39
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jun 01 05:23:57 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG052723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 01 03:51:58 2023
Response via : Initial Calibration

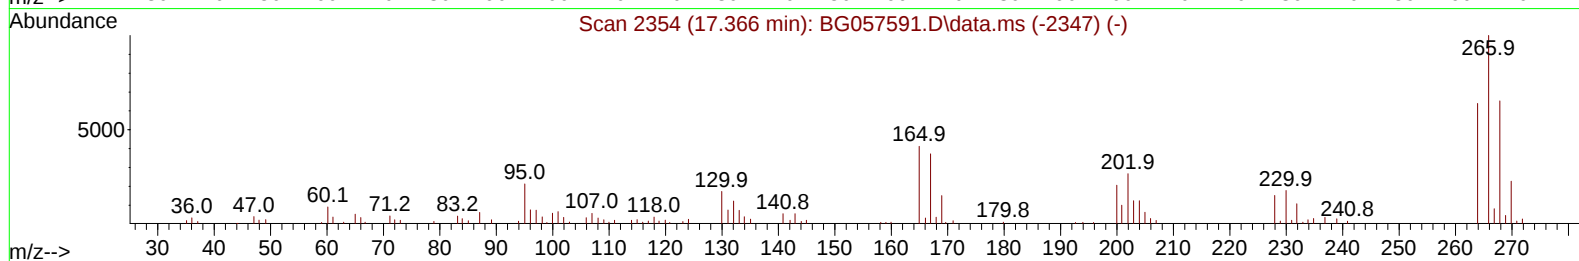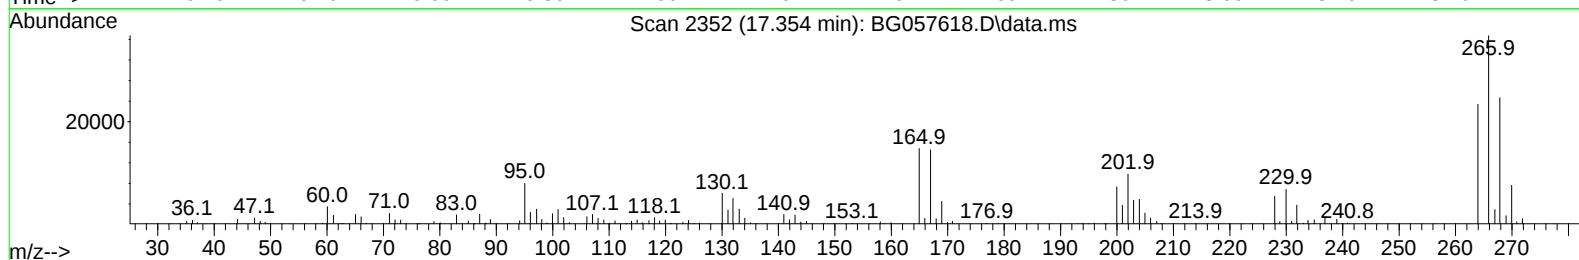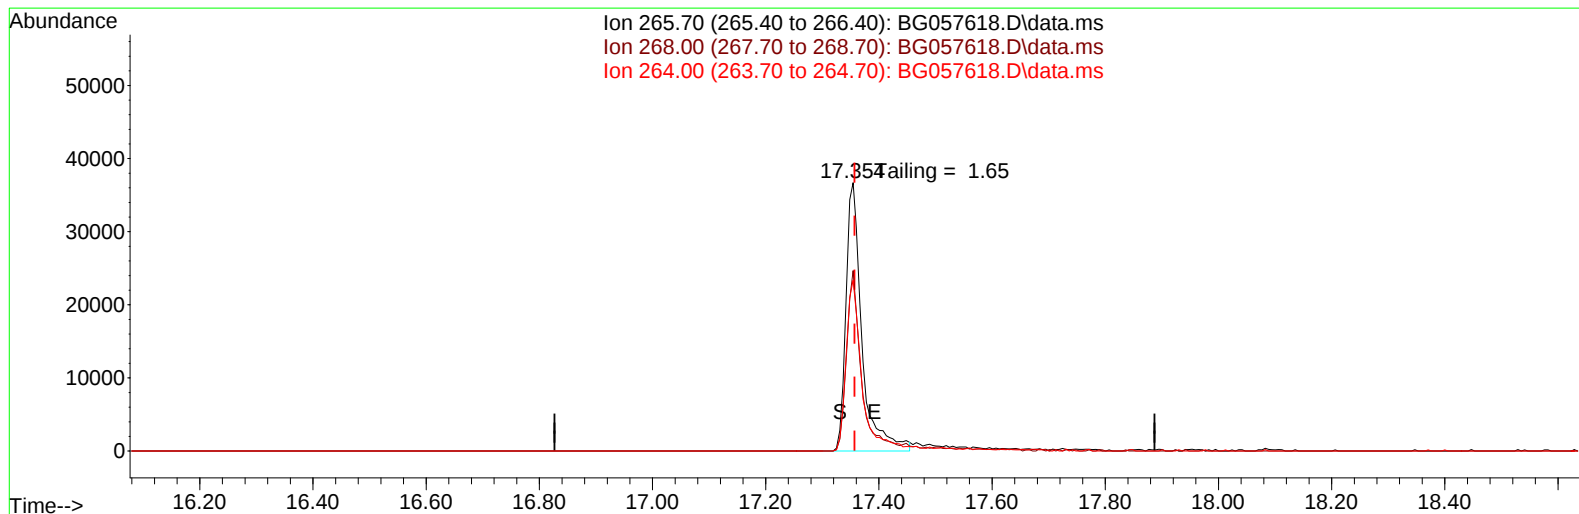

TIC: BG057618.D\data.ms

(70) Pentachlorophenol (C)

17.354min (-0.002) 56482.28 ng




response 71214

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	67.20
264.00	64.00	63.63
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG053123\
Data File : BG057618.D
Acq On : 31 May 2023 11:39
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jun 01 05:23:57 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG052723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 01 03:51:58 2023
Response via : Initial Calibration

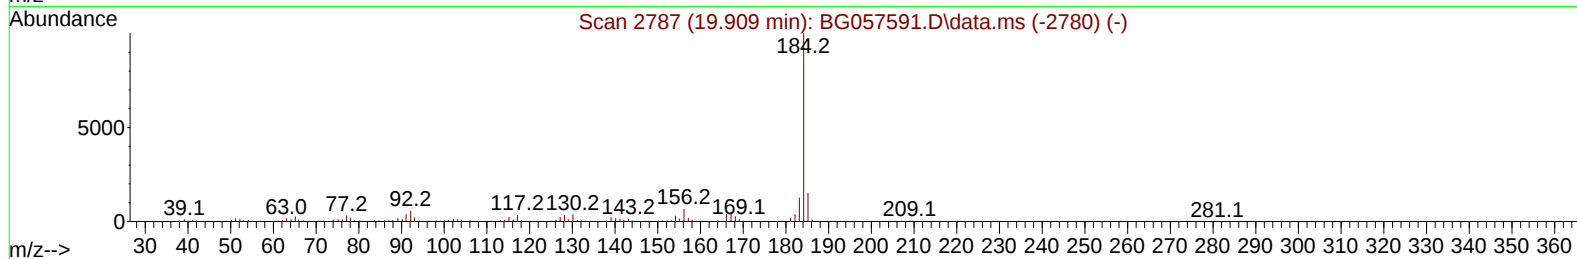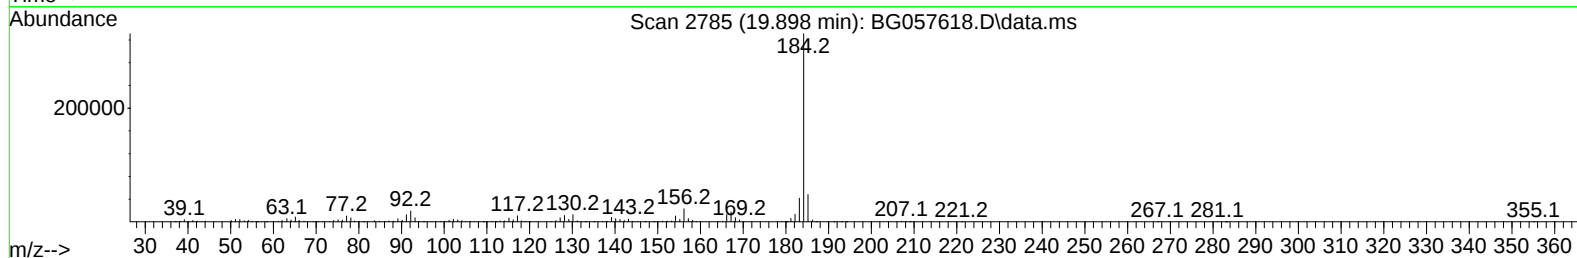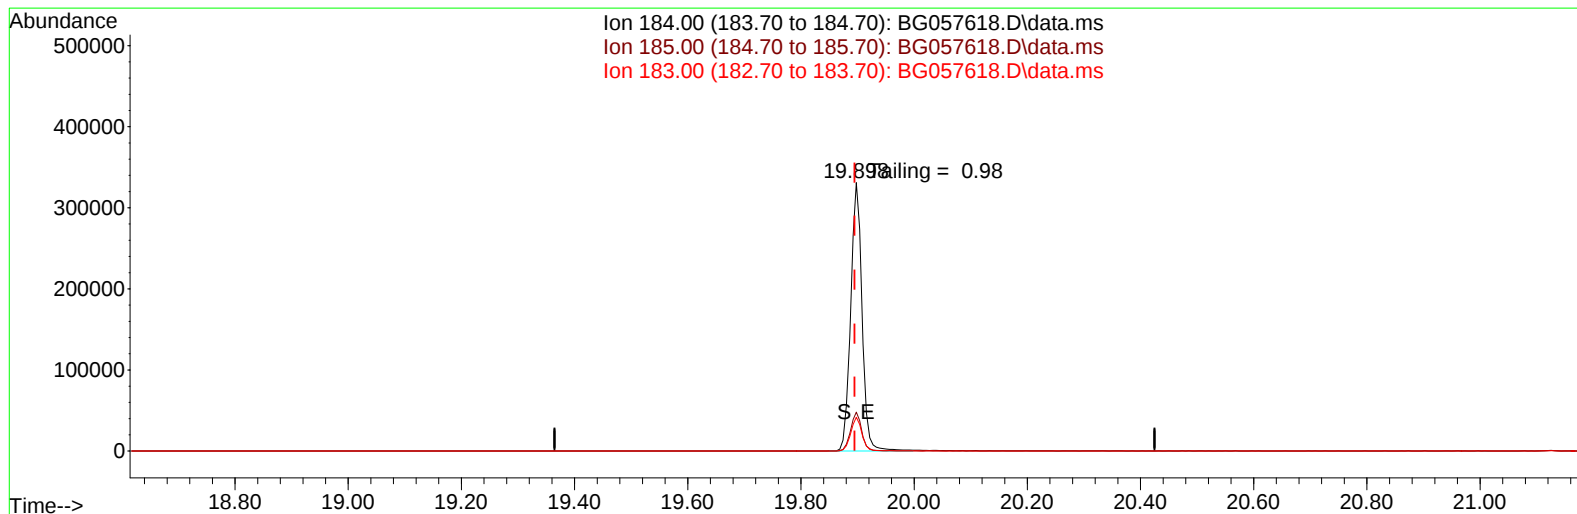

TIC: BG057618.D\data.ms

(77) Benzidine

19.898min (+ 0.003) 279840.02 ng

response 465740

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.49
183.00	12.50	12.62
0.00	0.00	0.00