




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG053124\
 Data File : BG061411.D
 Acq On : 1 Jun 2024 3:47
 Operator : MA/JU
 Sample : P2588-18
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BH6E3

Manual IntegrationsAPPROVED

Quant Time: Jun 01 04:27:54 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG052124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 30 22:54:48 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/03/2024
 Supervised By :mohammad ahmed 06/04/2024

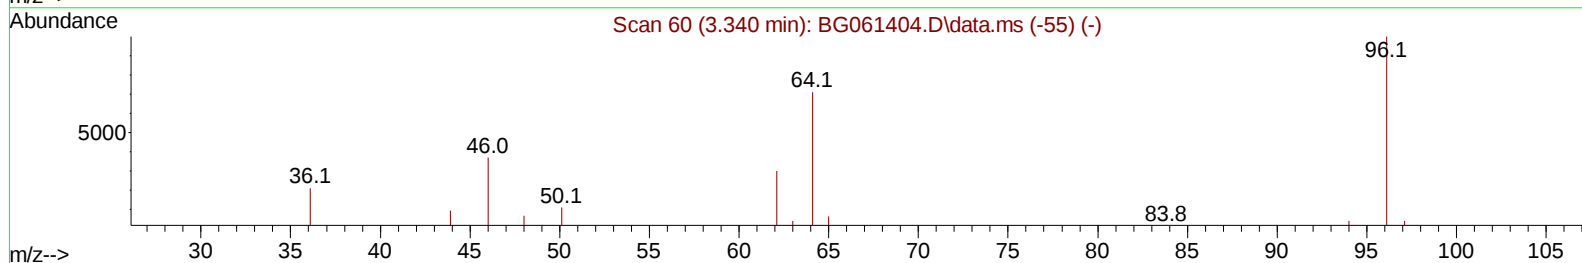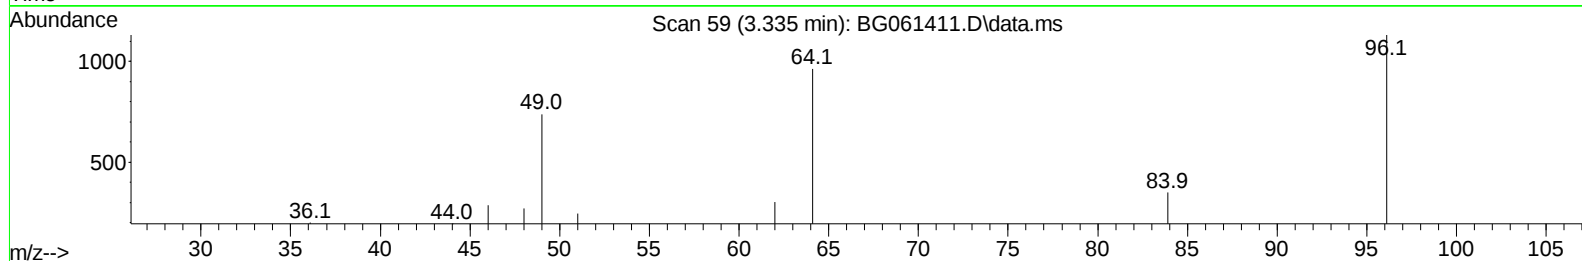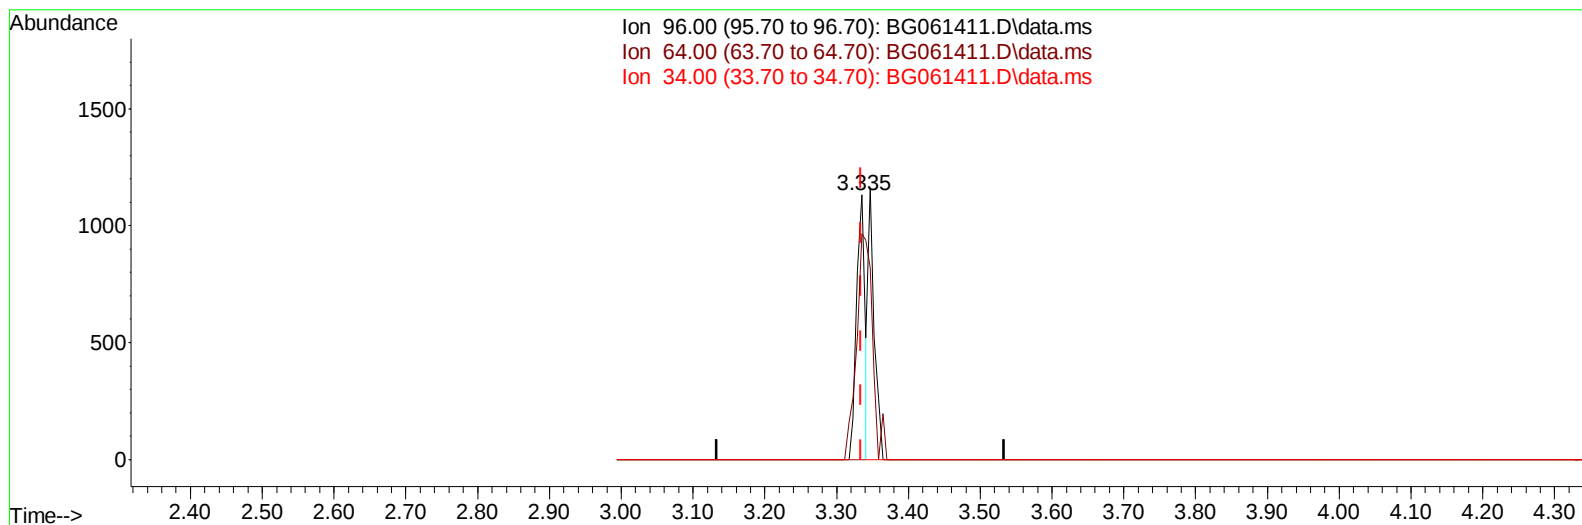

TIC: BG061411.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.335min (+ 0.001) 1.87 ng/uL

response 929

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	91.80	85.23
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG053124\
Data File : BG061411.D
Acq On : 1 Jun 2024 3:47
Operator : MA/JU
Sample : P2588-18
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BH6E3

Manual IntegrationsAPPROVED

Quant Time: Jun 01 04:27:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG052124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu May 30 22:54:48 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/03/2024
Supervised By :mohammad ahmed 06/04/2024

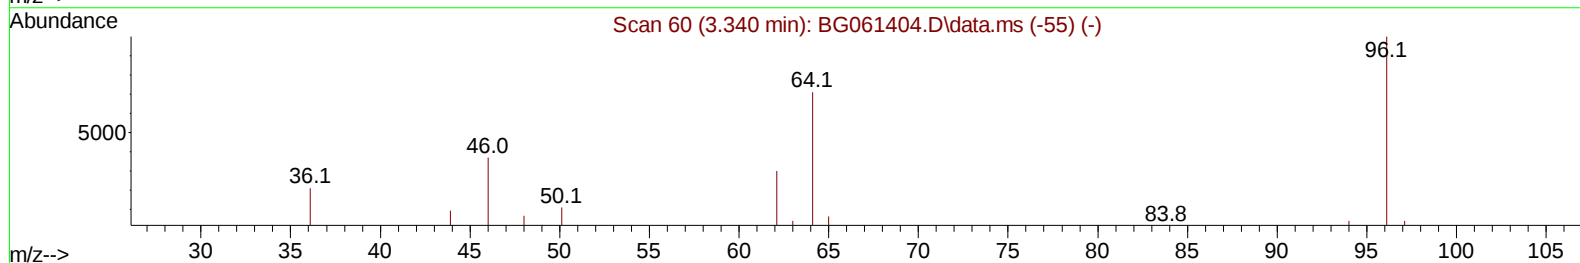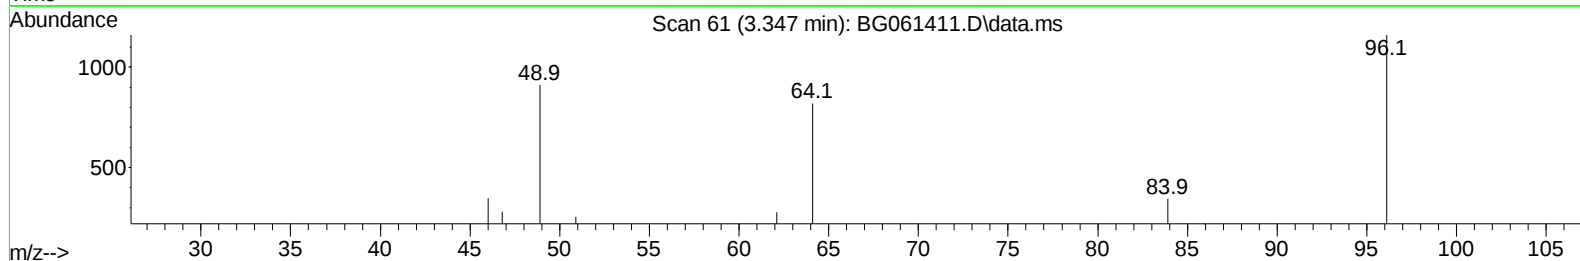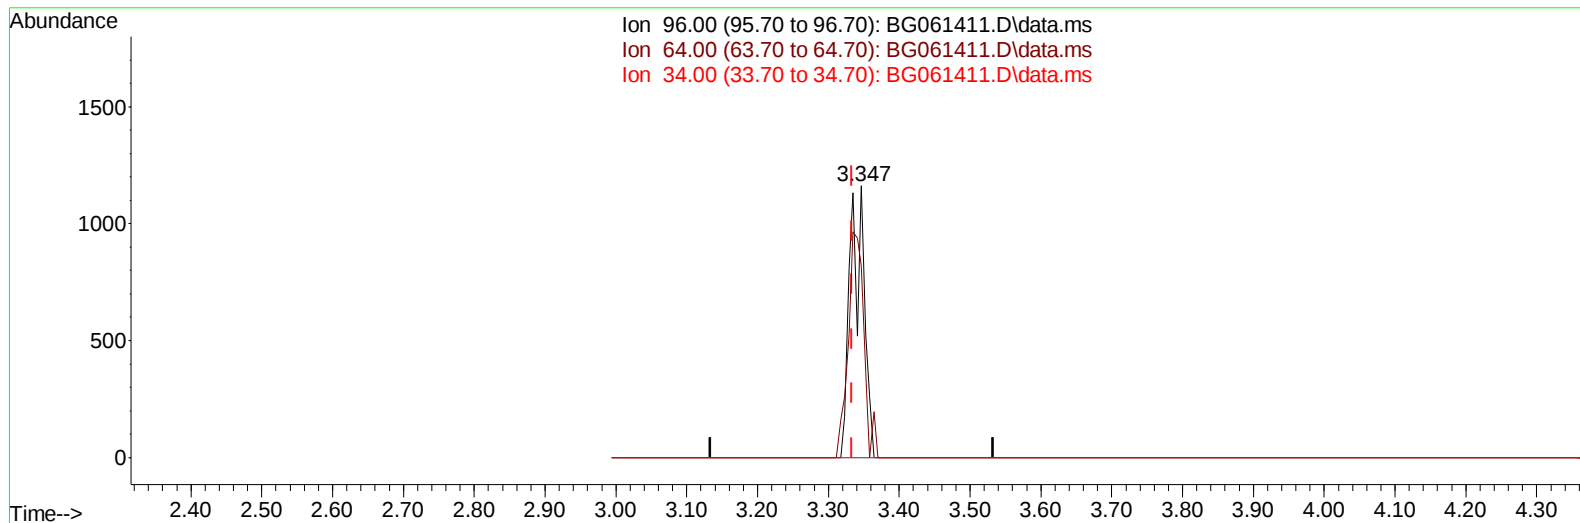

TIC: BG061411.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.347min (+ 0.013) 3.25 ng/uL m

response 1615

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	91.80	70.63#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG053124\
Data File : BG061411.D
Acq On : 1 Jun 2024 3:47
Operator : MA/JU
Sample : P2588-18
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BH6E3

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 06/03/2024
Supervised By :mohammad ahmed 06/04/2024

Quant Time: Jun 01 04:27:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG052124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu May 30 22:54:48 2024
Response via : Initial Calibration

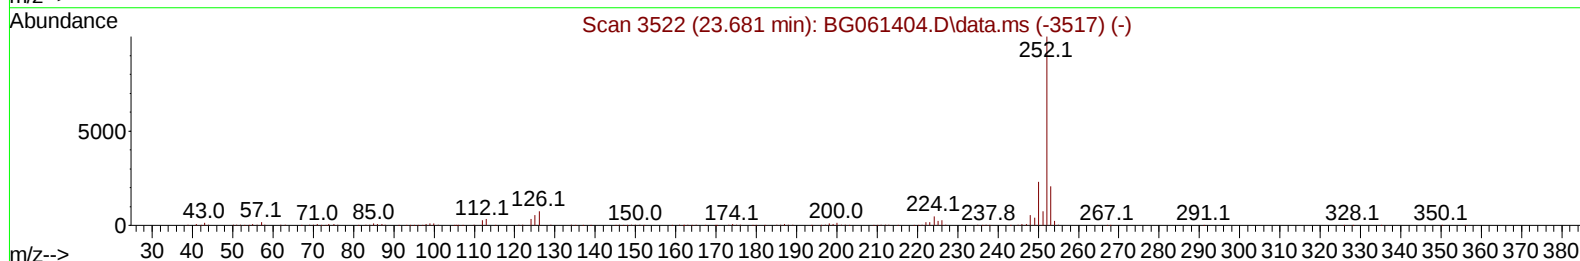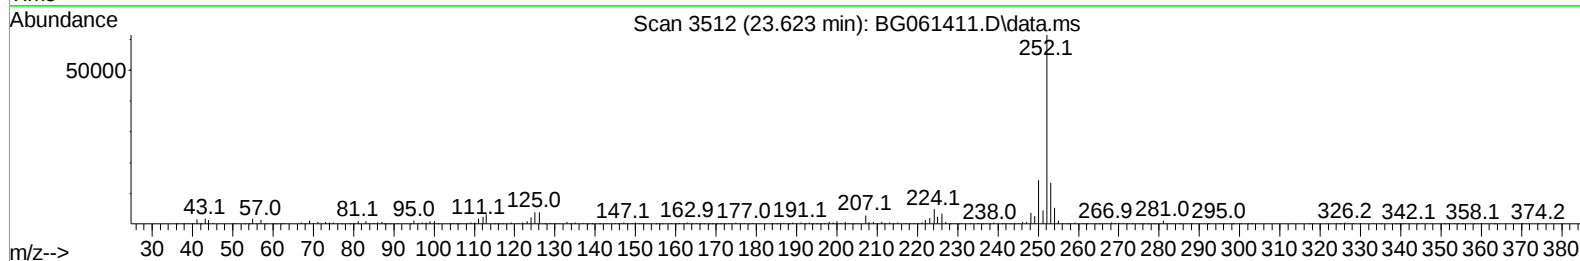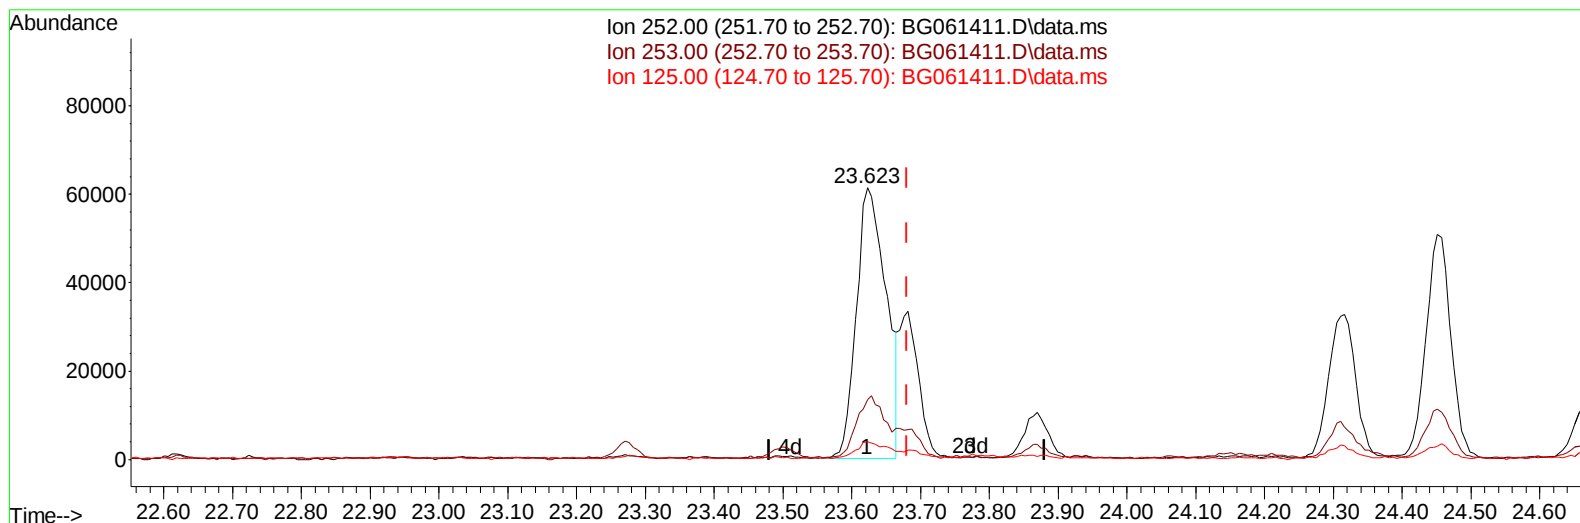

TIC: BG061411.D\data.ms

(91) Benzo(k)fluoranthene

23.623min (-0.057) 13.67 ng/u1

response 184554

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	20.00	22.05
125.00	5.40	6.45
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG053124\
Data File : BG061411.D
Acq On : 1 Jun 2024 3:47
Operator : MA/JU
Sample : P2588-18
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BH6E3

Manual IntegrationsAPPROVED

Quant Time: Jun 01 04:27:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG052124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu May 30 22:54:48 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/03/2024
Supervised By :mohammad ahmed 06/04/2024

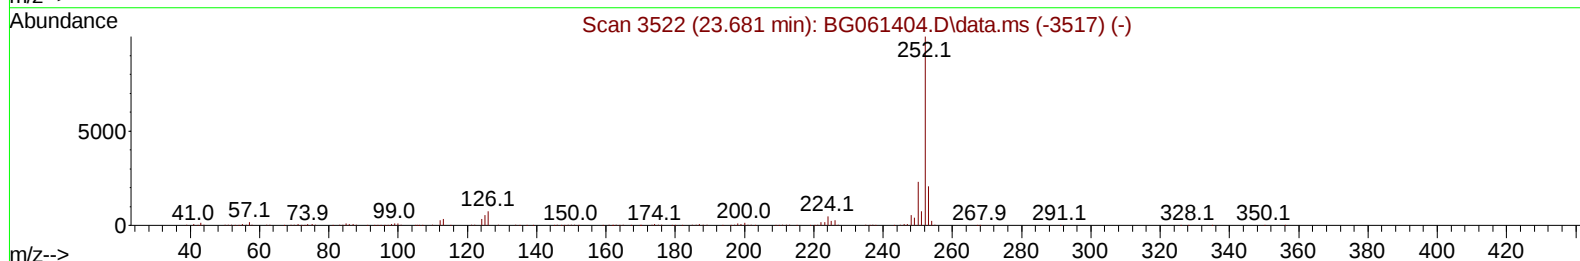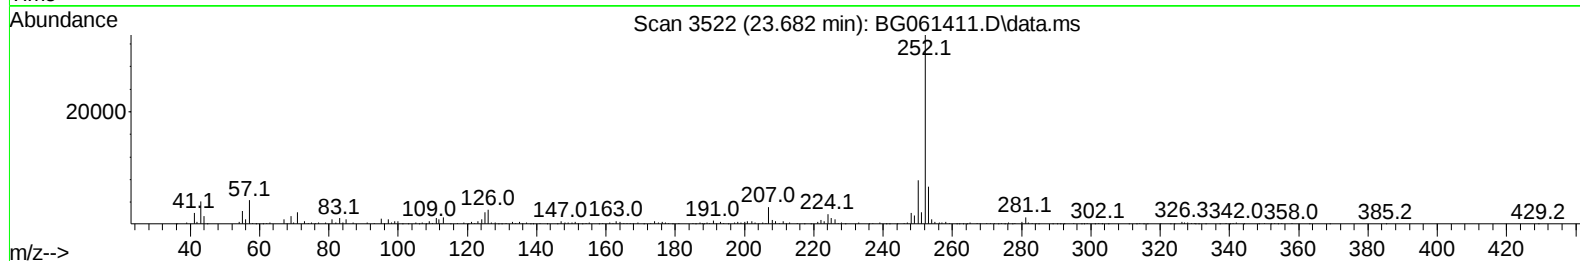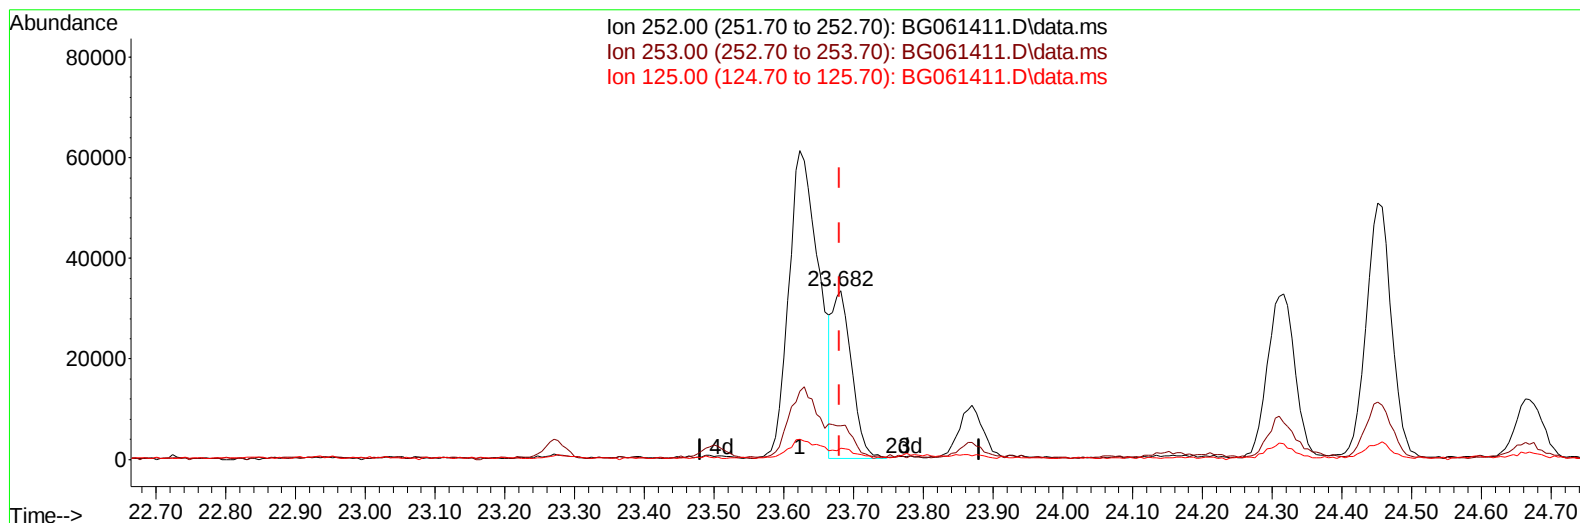

TIC: BG061411.D\data.ms

(91) Benzo(k)fluoranthene

23.682min (+ 0.001) 4.75 ng/u1 m

response 64092

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	20.00	20.09
125.00	5.40	6.49#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG053124\
 Data File : BG061411.D
 Acq On : 1 Jun 2024 3:47
 Operator : MA/JU
 Sample : P2588-18
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BH6E3

Manual IntegrationsAPPROVED

Quant Time: Jun 01 04:29:21 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG052124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 30 22:54:48 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/03/2024
 Supervised By :mohammad ahmed 06/04/2024

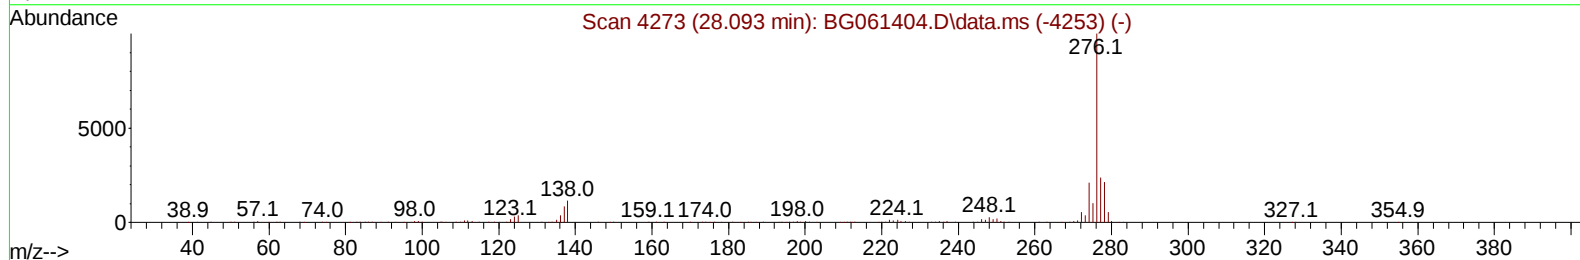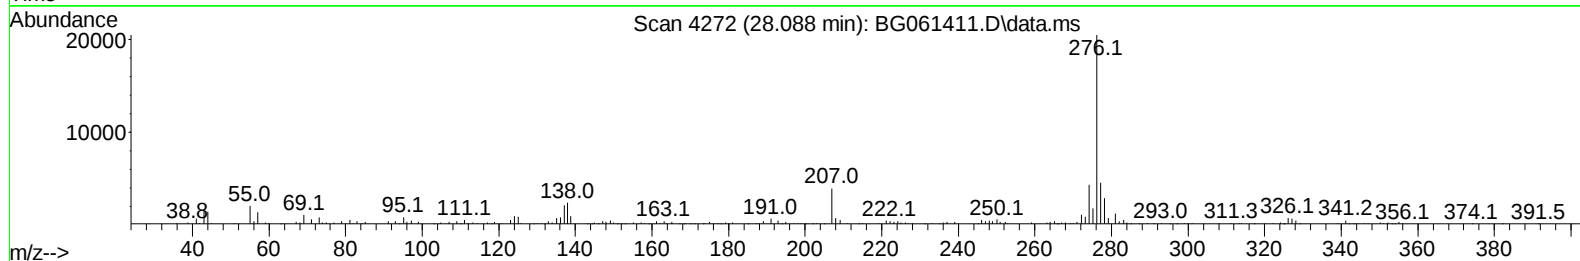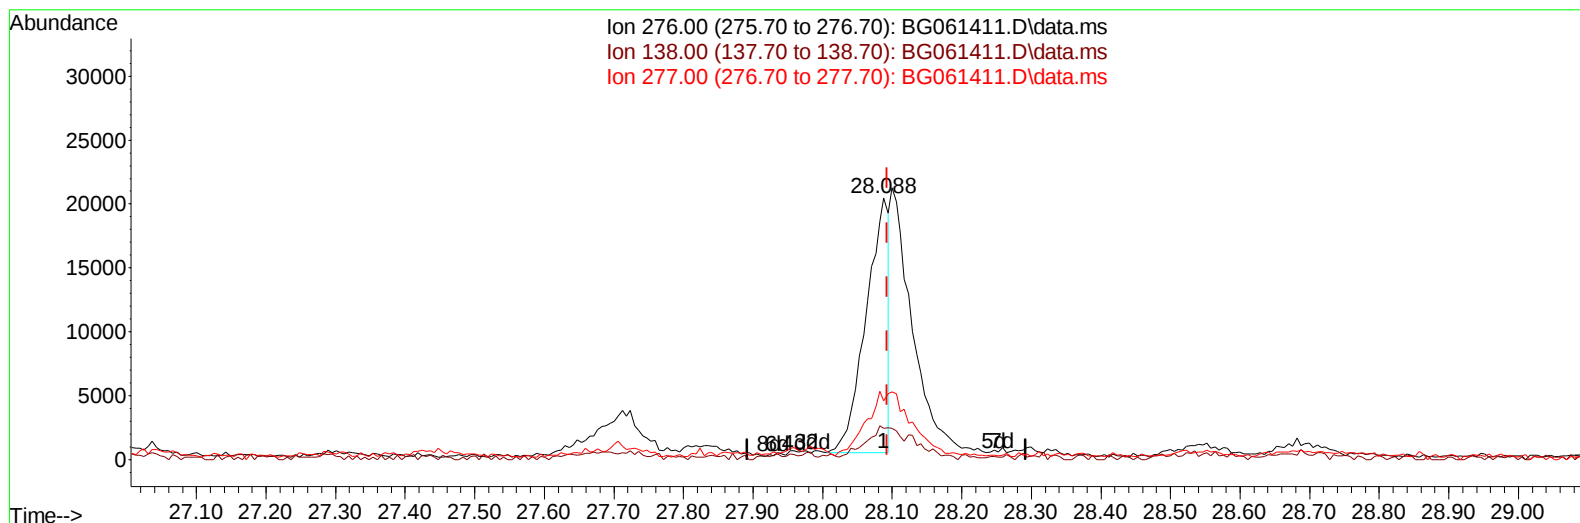

TIC: BG061411.D\data.ms

(94) Indeno(1,2,3-cd)pyrene

28.088min (-0.004) 2.97 ng/u1

response 45291

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	10.80	16.66#
277.00	24.60	22.44
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG053124\
Data File : BG061411.D
Acq On : 1 Jun 2024 3:47
Operator : MA/JU
Sample : P2588-18
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BH6E3

Manual IntegrationsAPPROVED

Quant Time: Jun 01 04:29:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG052124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu May 30 22:54:48 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/03/2024
Supervised By :mohammad ahmed 06/04/2024

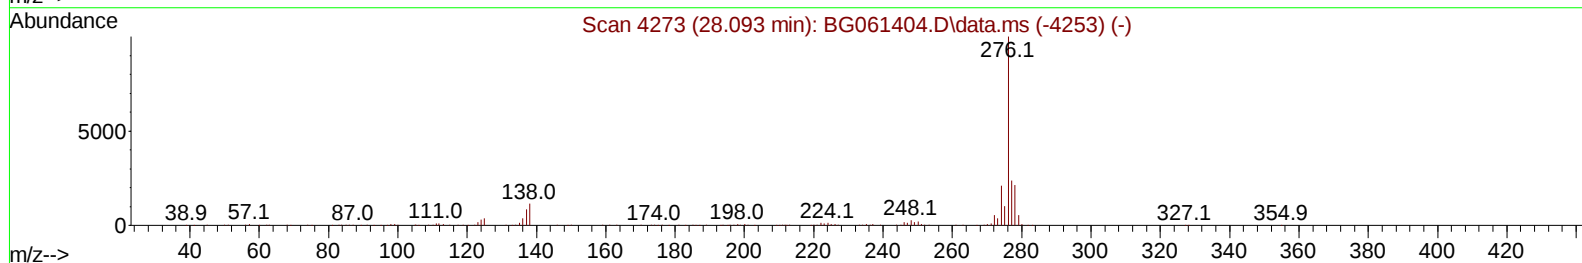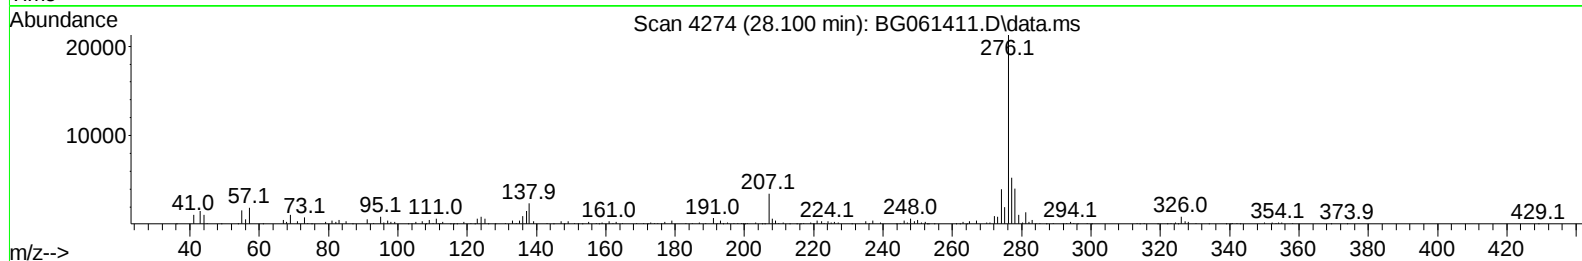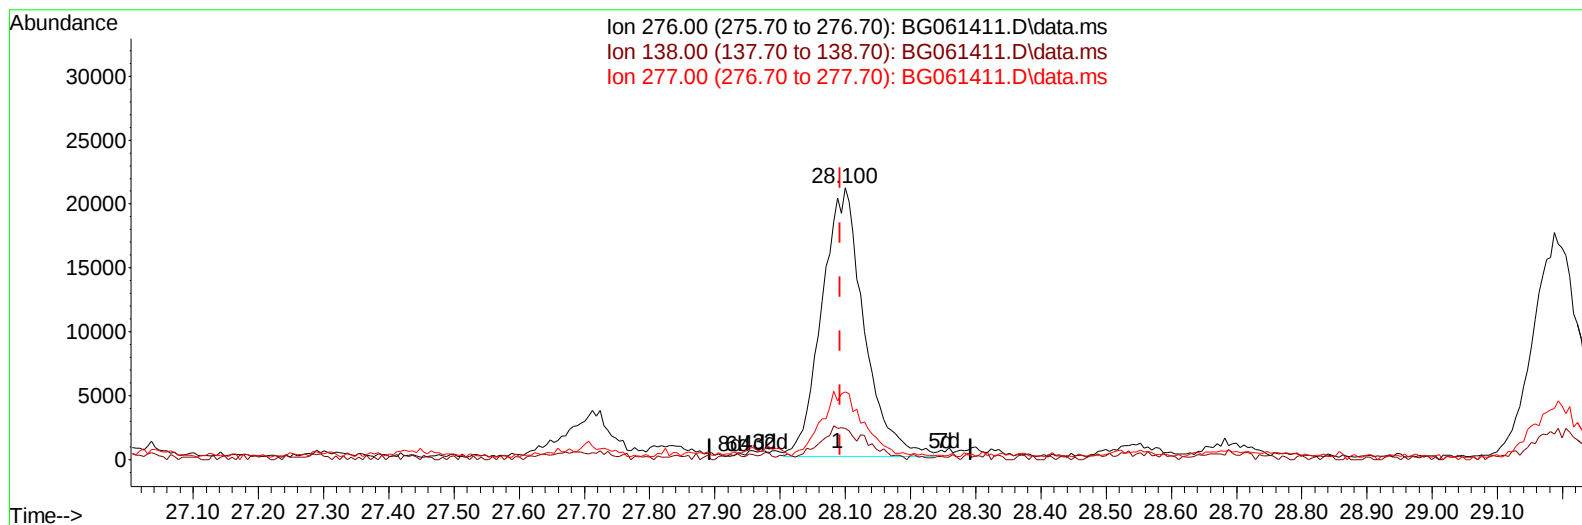

TIC: BG061411.D\data.ms

(94) Indeno(1,2,3-cd)pyrene

28.100min (+ 0.007) 6.15 ng/u1 m

response 93930

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	10.80	11.39
277.00	24.60	24.86
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG053124\
 Data File : BG061411.D
 Acq On : 1 Jun 2024 3:47
 Operator : MA/JU
 Sample : P2588-18
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BH6E3

Manual IntegrationsAPPROVED

Quant Time: Jun 01 04:29:48 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG052124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 30 22:54:48 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/03/2024
 Supervised By :mohammad ahmed 06/04/2024

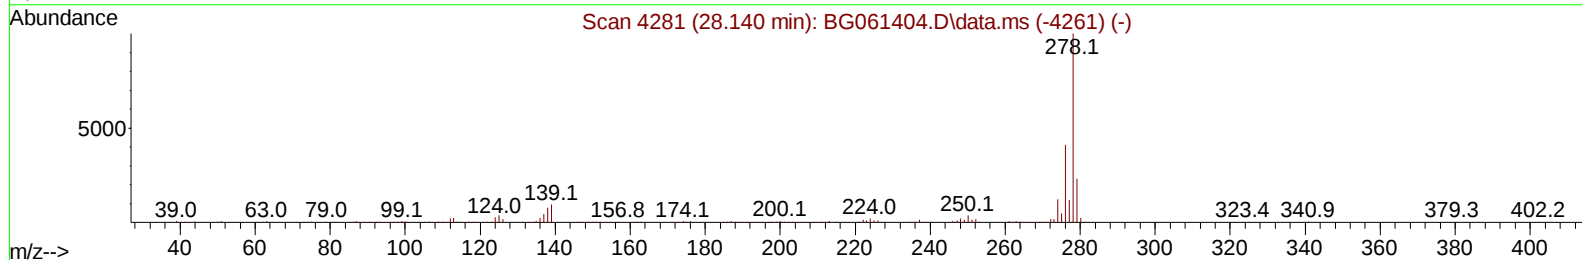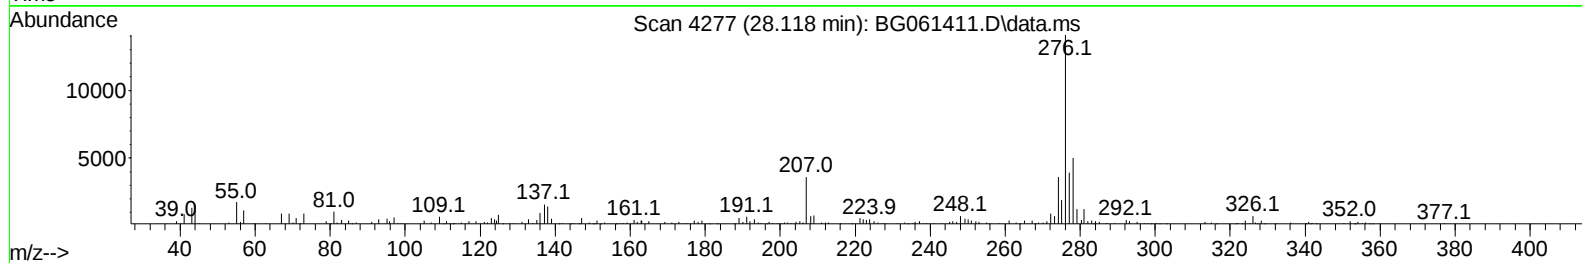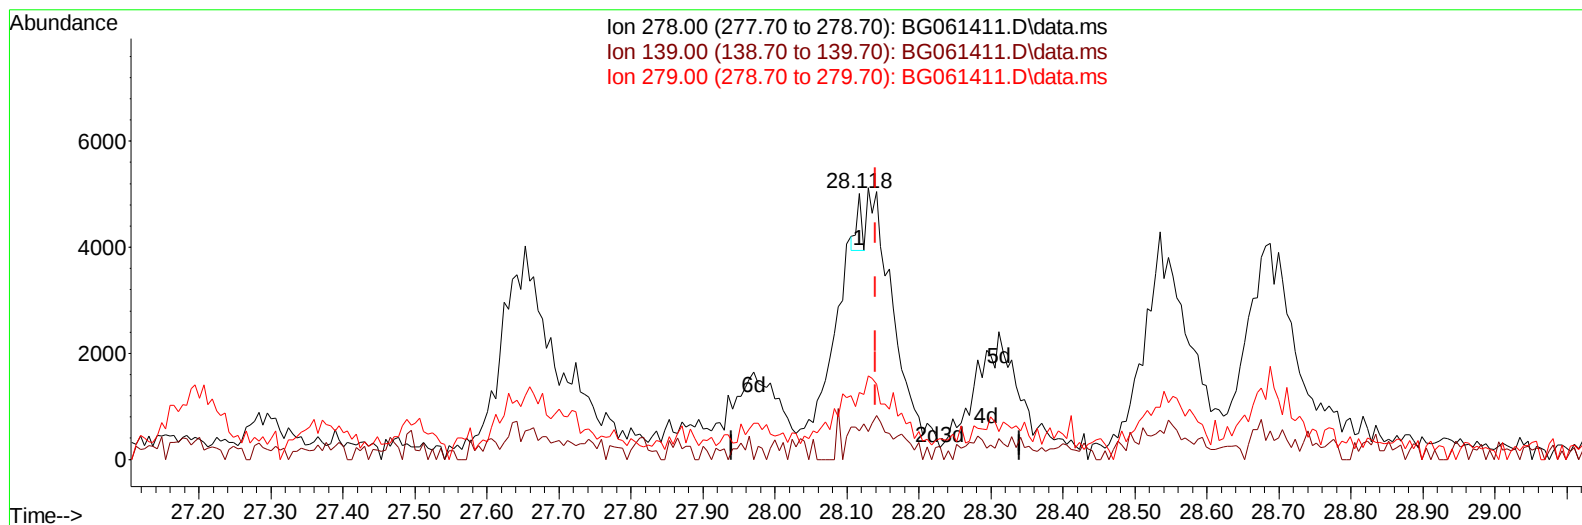

TIC: BG061411.D\data.ms

(95) Dibenzo(a,h)anthracene

28.118min (-0.022) 0.04 ng/u1

response 482

Ion	Exp%	Act%
278.00	100.00	100.00
139.00	8.00	10.82#
279.00	24.90	25.10
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG053124\
Data File : BG061411.D
Acq On : 1 Jun 2024 3:47
Operator : MA/JU
Sample : P2588-18
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BH6E3

Manual IntegrationsAPPROVED

Quant Time: Jun 01 04:29:48 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG052124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu May 30 22:54:48 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/03/2024
Supervised By :mohammad ahmed 06/04/2024

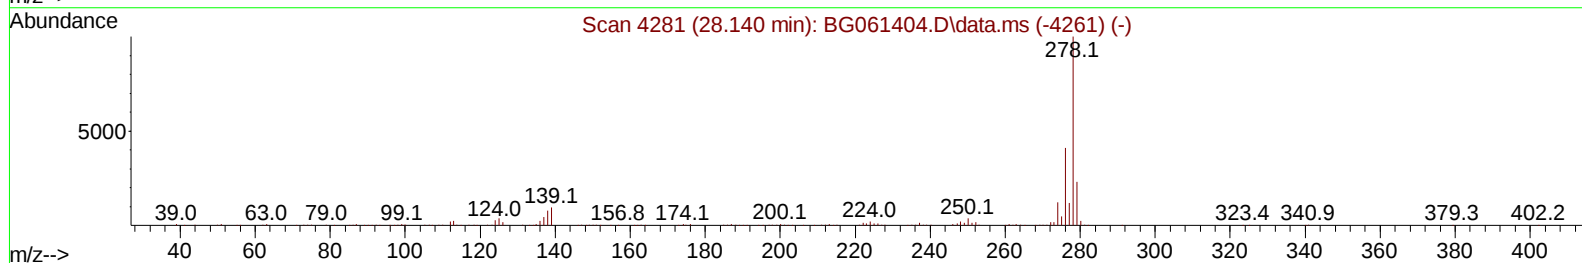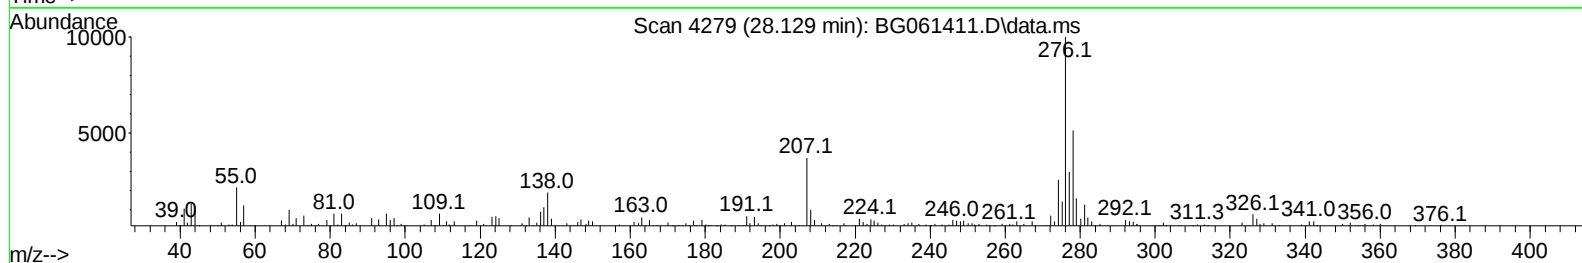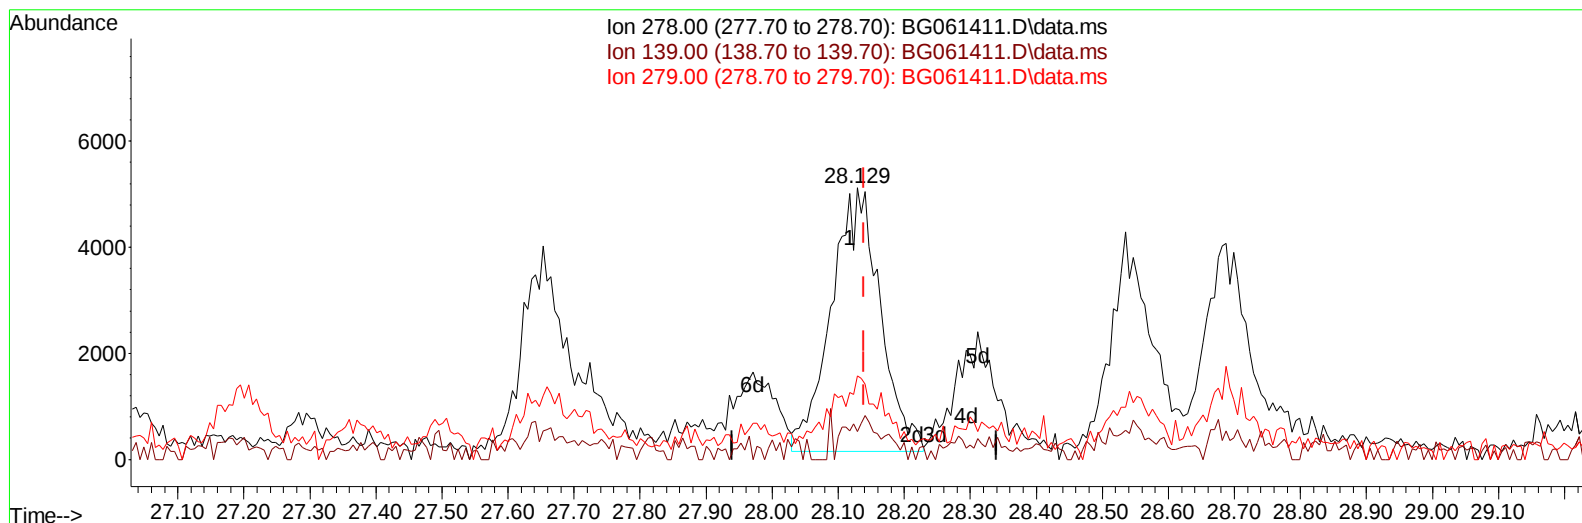

TIC: BG061411.D\data.ms

(95) Dibenzo(a,h)anthracene

28.129min (-0.010) 2.02 ng/u1 m

response 25443

Ion	Exp%	Act%
278.00	100.00	100.00
139.00	8.00	10.18#
279.00	24.90	30.79#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG053124\
 Data File : BG061411.D
 Acq On : 1 Jun 2024 3:47
 Operator : MA/JU
 Sample : P2588-18
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BH6E3

Manual IntegrationsAPPROVED

Quant Time: Jun 01 04:30:17 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG052124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 30 22:54:48 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/03/2024
 Supervised By :mohammad ahmed 06/04/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.877	152		27827	20.000	ng/ul	0.00
20) Naphthalene-d8	10.667	136		108959	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.510	164		81737	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.260	188		192422	20.000	ng/ul	0.00
79) Chrysene-d12	21.514	240		195884	20.000	ng/ul	0.00
88) Perylene-d12	24.598	264		223292	20.000	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.347	96		1615m	3.248	ng/uL	0.01
4) Pyridine-d5	3.746	84		21930	12.397	ng/ul	0.00
7) Phenol-d5	7.060	99		37186	16.273	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.201	67		23293	16.217	ng/ul	0.00
11) 2-Chlorophenol-d4	7.412	132		30406	17.979	ng/ul	0.00
15) 4-Methylphenol-d8	8.593	113		30500	15.653	ng/ul	0.00
21) Nitrobenzene-d5	9.022	128		15598	18.593	ng/ul	0.00
24) 2-Nitrophenol-d4	9.757	143		17963	18.296	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.303	165		35711	18.657	ng/ul	0.00
31) 4-Chloroaniline-d4	10.808	131		34800	13.897	ng/ul	0.00
46) Dimethylphthalate-d6	13.917	166		119698	18.882	ng/ul	0.00
49) Acenaphthylene-d8	14.199	160		131127	19.896	ng/ul	0.00
54) 4-Nitrophenol-d4	14.757	143		11045	14.093	ng/ul	0.02
60) Fluorene-d10	15.503	176		112073	20.477	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.644	200		13805	11.862	ng/ul	0.00
73) Anthracene-d10	17.360	188		188747	22.249	ng/ul	0.00
81) Pyrene-d10	19.651	212		227371	22.607	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.387	264		244049	22.734	ng/ul	0.00
Target Compounds							
						Qvalue	
6) Benzaldehyde	7.019	77		1649	1.380	ng/ul#	87
72) Phenanthrene	17.301	178		91154	9.760	ng/ul	98
74) Anthracene	17.389	178		13617	1.410	ng/ul	99
77) Carbazole	17.665	167		9714	1.237	ng/ul#	93
80) Fluoranthene	19.316	202		244799	20.289	ng/ul	99
82) Pyrene	19.680	202		226257	18.066	ng/ul	99
85) Benzo(a)anthracene	21.496	228		128686	9.521	ng/ul	98
86) Bis(2-ethylhexyl)phtha...	21.402	149		25184	3.954	ng/ul#	94
87) Chrysene	21.555	228		135306	10.872	ng/ul	98
90) Benzo(b)fluoranthene	23.623	252		184554	13.882	ng/ul	99
91) Benzo(k)fluoranthene	23.682	252		64092m	4.749	ng/ul	
93) Benzo(a)pyrene	24.451	252		127131	10.070	ng/ul	97
94) Indeno(1,2,3-cd)pyrene	28.100	276		93930m	6.153	ng/ul	
95) Dibenzo(a,h)anthracene	28.129	278		25443m	2.021	ng/ul	
96) Benzo(g,h,i)perylene	29.187	276		88784	7.310	ng/ul	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed

