

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG053124\
 Data File : BG061406.D
 Acq On : 1 Jun 2024 00:21
 Operator : MA/JU
 Sample : P2588-04
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BH5S5

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 06/03/2024
 Supervised By :mohammad ahmed 06/04/2024

Quant Time: Jun 01 01:34:00 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG052124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 30 22:54:48 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.876	152	29174	20.000	ng/ul	0.00
20) Naphthalene-d8	10.667	136	112834	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.510	164	87015	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.259	188	214470	20.000	ng/ul	0.00
79) Chrysene-d12	21.507	240	221304	20.000	ng/ul	0.00
88) Perylene-d12	24.592	264	254016	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.340	96	1465	2.810	ng/uL	0.00
4) Pyridine-d5	3.740	84	21638	11.667	ng/ul	0.00
7) Phenol-d5	7.060	99	33122	13.825	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.201	67	19839	13.175	ng/ul	0.00
11) 2-Chlorophenol-d4	7.412	132	26726	15.073	ng/ul	0.00
15) 4-Methylphenol-d8	8.593	113	25056	12.265	ng/ul	0.00
21) Nitrobenzene-d5	9.028	128	13232	15.231	ng/ul	0.00
24) 2-Nitrophenol-d4	9.750	143	15172	14.922	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.303	165	33171	16.735	ng/ul	0.00
31) 4-Chloroaniline-d4	10.802	131	33527	12.929	ng/ul	0.00
46) Dimethylphthalate-d6	13.910	166	114592	16.980	ng/ul	0.00
49) Acenaphthylene-d8	14.198	160	123362	17.582	ng/ul	0.00
54) 4-Nitrophenol-d4	14.745	143	13351	16.002	ng/ul	0.00
60) Fluorene-d10	15.503	176	106695	18.312	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.638	200	18238	14.060	ng/ul	0.00
73) Anthracene-d10	17.353	188	199496	21.099	ng/ul	0.00
81) Pyrene-d10	19.651	212	242809	21.368	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.380	264	261358	21.402	ng/ul	0.00
Target Compounds						
					Qvalue	
72) Phenanthrene	17.300	178	49946	4.798	ng/ul	97
80) Fluoranthene	19.316	202	112116	8.225	ng/ul	98
82) Pyrene	19.680	202	103542	7.318	ng/ul	97
85) Benzo(a)anthracene	21.490	228	58172	3.810	ng/ul	99
87) Chrysene	21.554	228	58146	4.135	ng/ul	96
90) Benzo(b)fluoranthene	23.617	252	74971	4.957	ng/ul#	94
91) Benzo(k)fluoranthene	23.675	252	27173m	1.770	ng/ul	
93) Benzo(a)pyrene	24.445	252	53930	3.755	ng/ul#	91
94) Indeno(1,2,3-cd)pyrene	28.088	276	39416m	2.270	ng/ul	
96) Benzo(g,h,i)perylene	29.175	276	38789m	2.808	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG053124\
Data File : BG061406.D
Acq On : 1 Jun 2024 00:21
Operator : MA/JU
Sample : P2588-04
Misc :
ALS Vial : 17 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
BH5S5

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 06/03/2024
Supervised By :mohammad ahmed 06/04/2024


Quant Time: Jun 01 01:34:00 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG052124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu May 30 22:54:48 2024
Response via : Initial Calibration

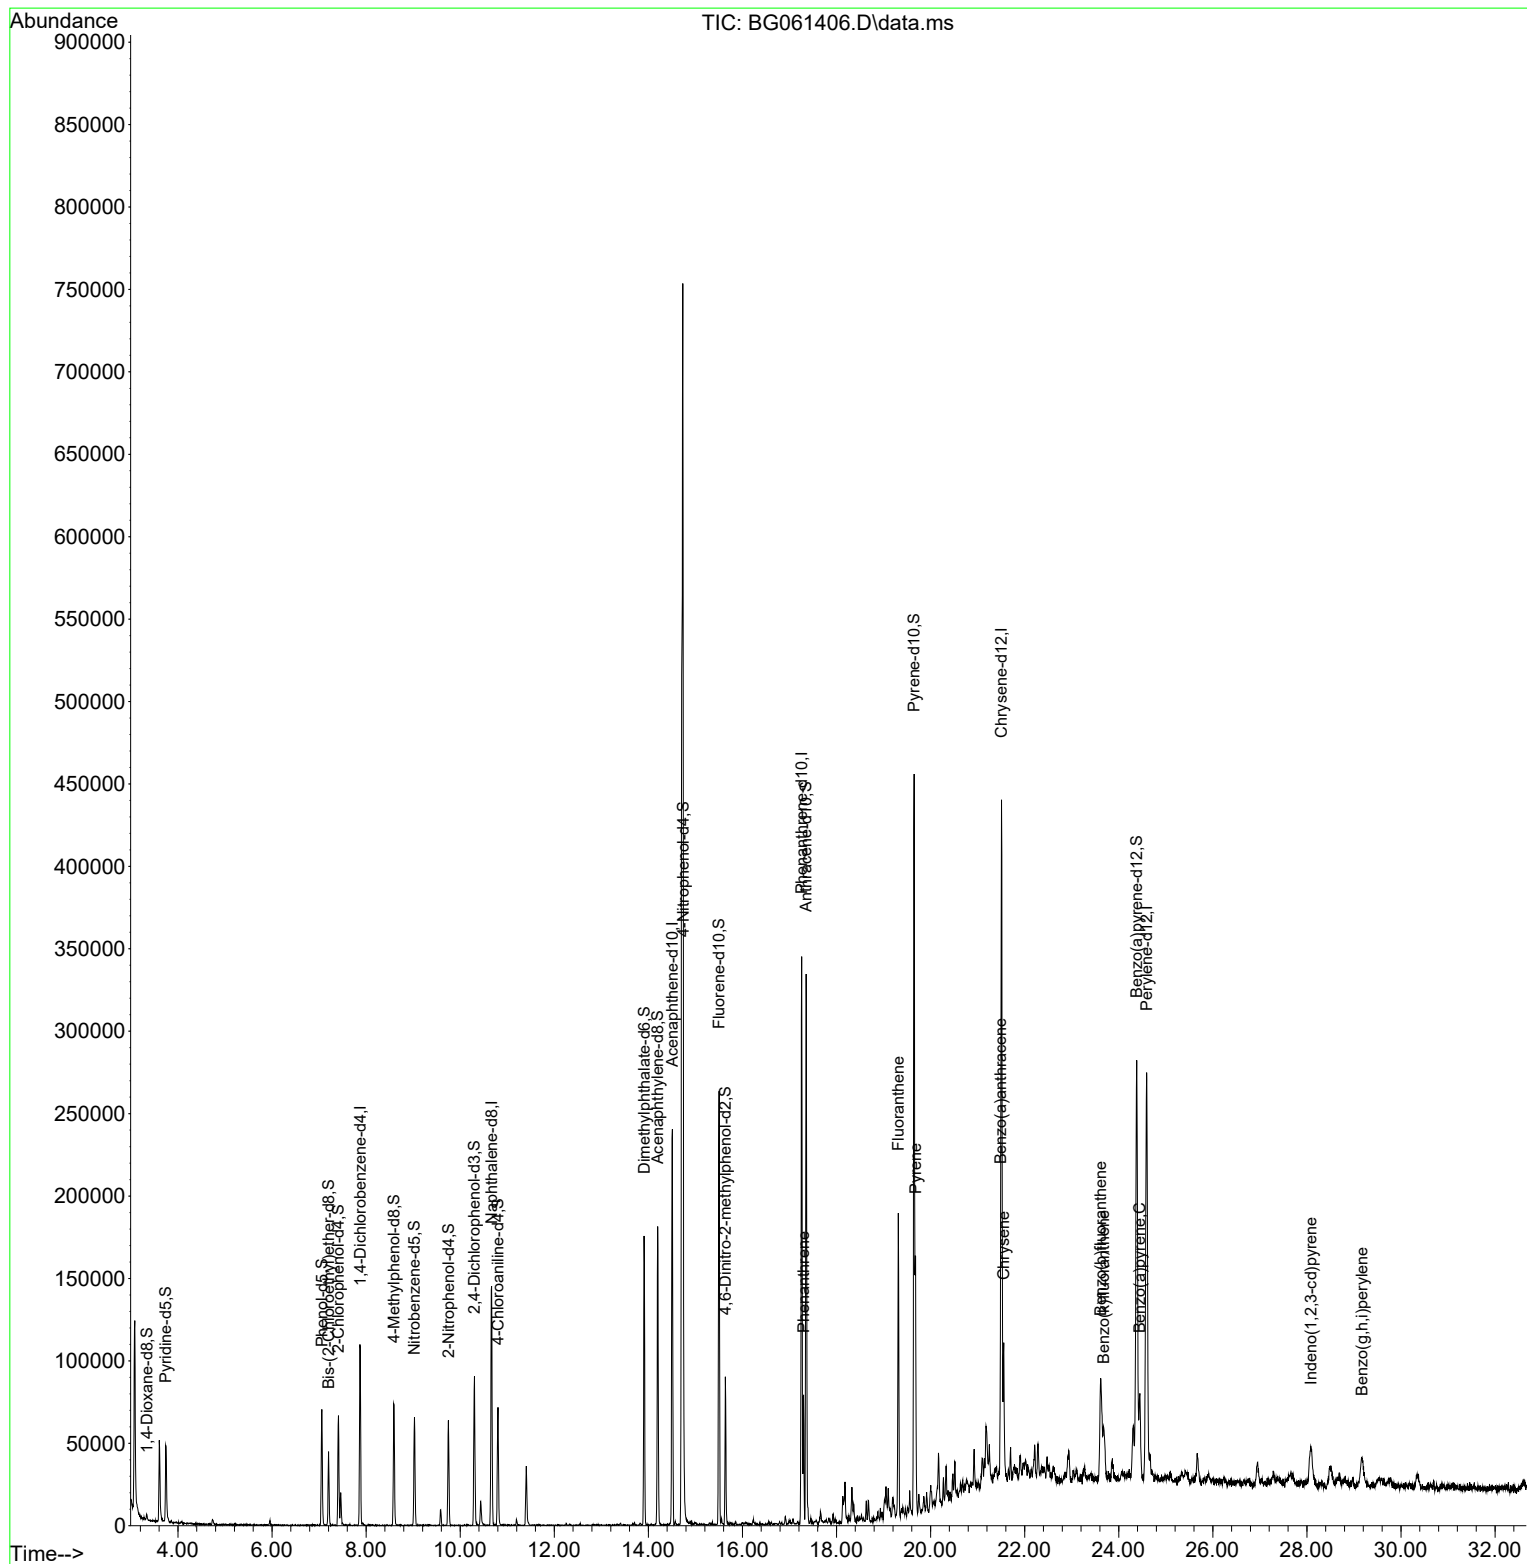

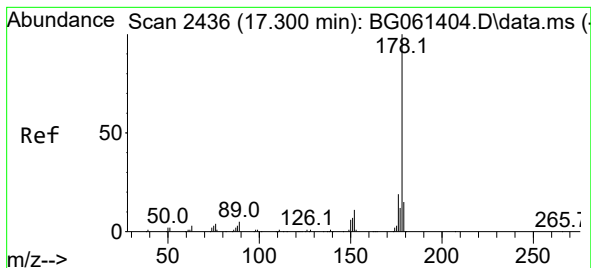

#72
Phenanthrene
Concen: 4.798 ng/ul
RT: 17.300 min Scan# 2436
Delta R.T. 0.001 min
Lab File: BG061406.D
Acq: 1 Jun 2024 00:21




Instrument :
BNA_G
ClientSampleId :
BH5S5

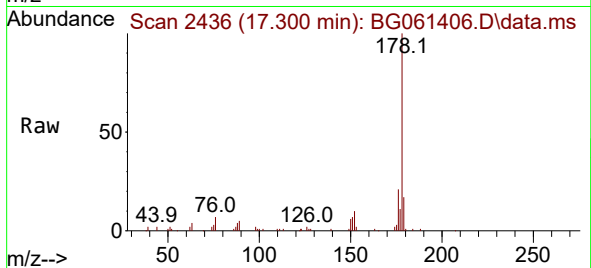


Tgt Ion:178 Resp: 49940
Ion Ratio Lower Upper
178 100
179 16.9 12.7 19.1
176 20.7 15.5 23.3

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 06/03/2024
Supervised By :mohammad ahmed 06/04/2024

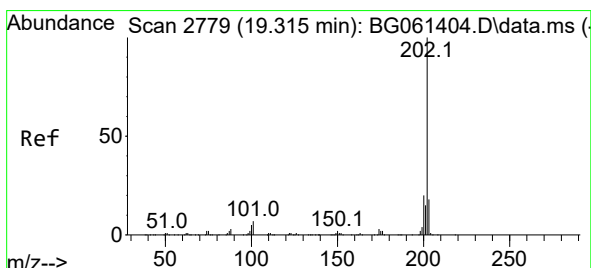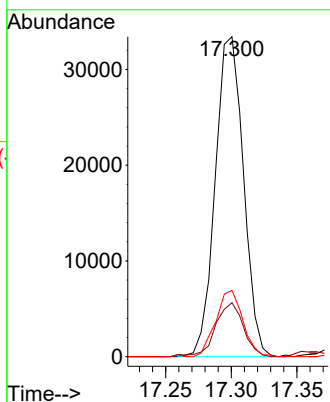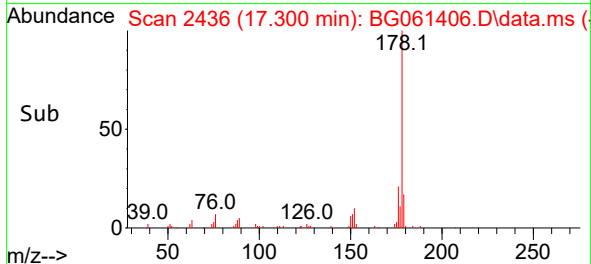


#80
Fluoranthene
Concen: 8.225 ng/ul
RT: 19.316 min Scan# 2779
Delta R.T. 0.001 min
Lab File: BG061406.D
Acq: 1 Jun 2024 00:21

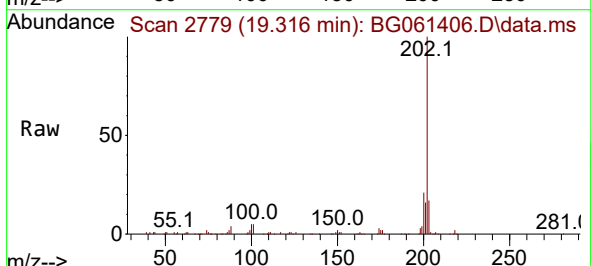


Tgt Ion:202 Resp: 112116
Ion Ratio Lower Upper
202 100
101 5.2 4.8 7.2
100 4.9 4.1 6.1

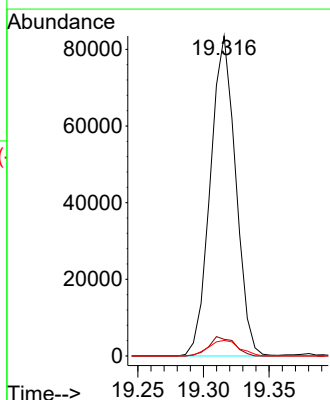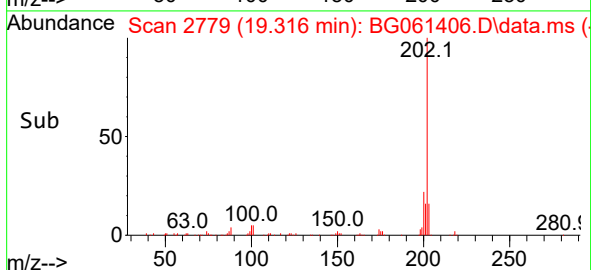

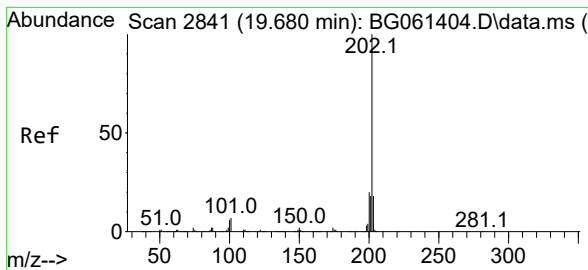

#82
 Pyrene
 Concen: 7.318 ng/ul
 RT: 19.680 min Scan# 2149
 Delta R.T. 0.001 min
 Lab File: BG061406.D
 Acq: 1 Jun 2024 00:21




Instrument :
 BNA_G
 ClientSampleId :
 BH5S5

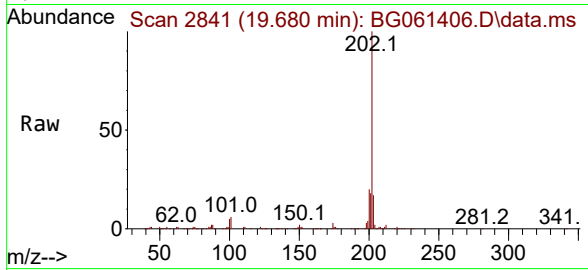


Tgt Ion:202 Resp: 10354
 Ion Ratio Lower Upper
 202 100
 101 6.2 5.7 8.5
 100 5.1 5.1 7.7

Manual Integrations
 APPROVED



Reviewed By :Jagrut Upadhyay 06/03/2024
 Supervised By :mohammad ahmed 06/04/2024

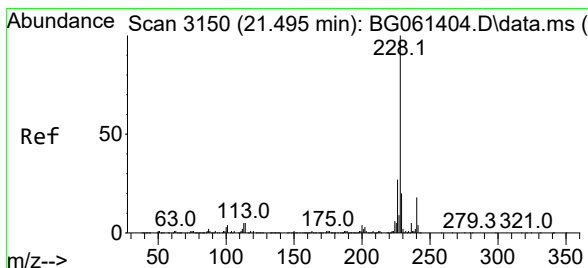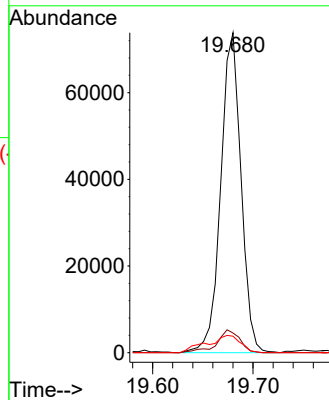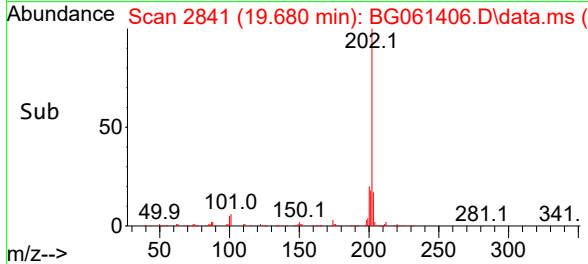


#85
 Benzo(a)anthracene
 Concen: 3.810 ng/ul
 RT: 21.490 min Scan# 3149
 Delta R.T. -0.005 min
 Lab File: BG061406.D
 Acq: 1 Jun 2024 00:21

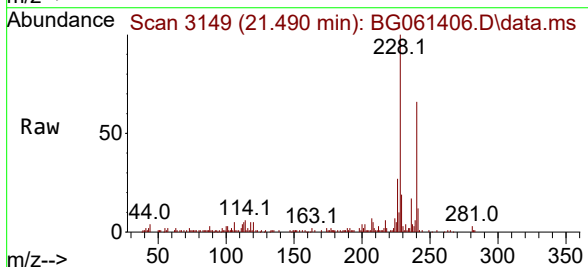

Tgt Ion:228 Resp: 58172
 Ion Ratio Lower Upper
 228 100
 229 19.0 15.2 22.8
 226 27.4 21.4 32.2

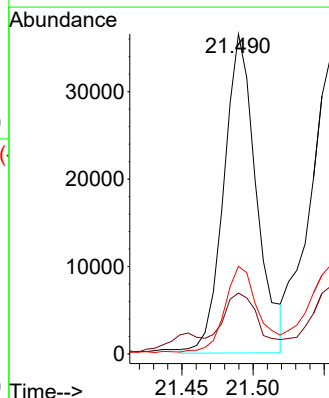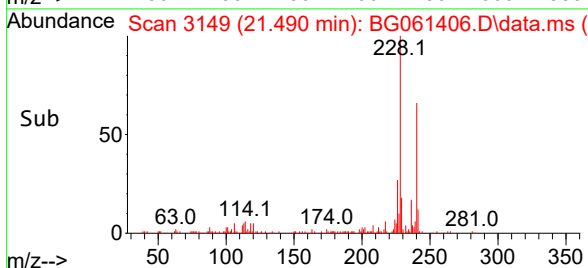

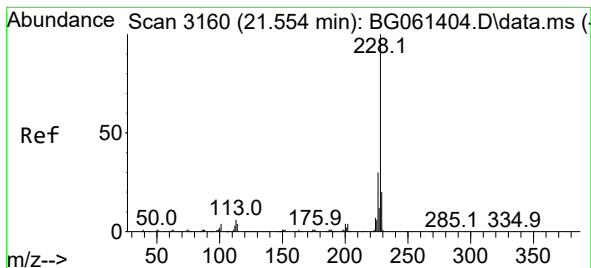

#87

Chrysene

Concen: 4.135 ng/ul

RT: 21.554 min Scan# 3160

Delta R.T. 0.001 min

Lab File: BG061406.D

Acq: 1 Jun 2024 00:21

Instrument :

BNA_G

ClientSampleId :





BH5S5

Tgt Ion:	228	Resp:	58140
Ion Ratio	Lower	Upper	
228	100		
226	29.8	23.4	35.0
229	22.7	15.4	23.2

Manual Integrations

APPROVED

Reviewed By :Jagrut Upadhyay 06/03/2024
Supervised By :mohammad ahmed 06/04/2024

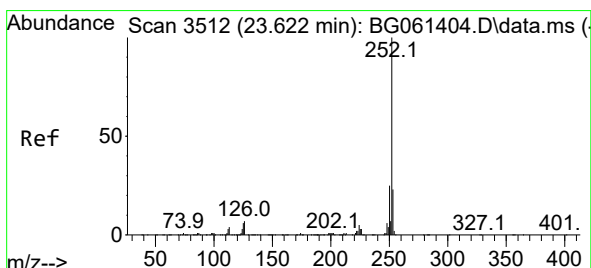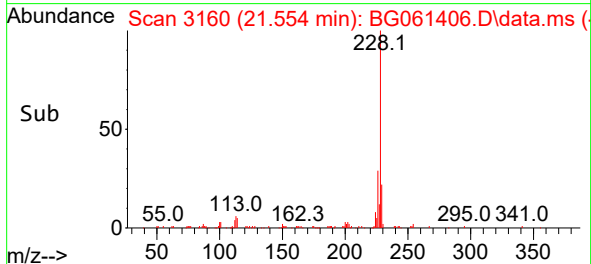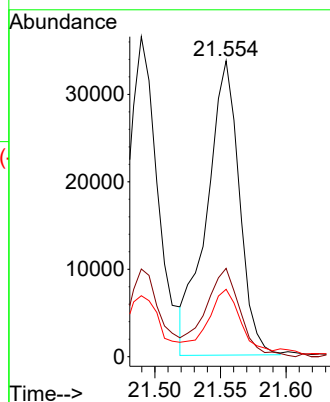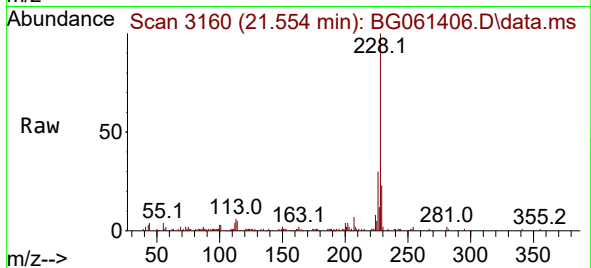

#90

Benzo(b)fluoranthene

Concen: 4.957 ng/ul




RT: 23.617 min Scan# 3511


Delta R.T. 0.001 min

Lab File: BG061406.D

Acq: 1 Jun 2024 00:21


Tgt Ion:	252	Resp:	74971
Ion Ratio	Lower	Upper	
252	100		
253	19.8	17.8	26.8
125	8.4	4.6	6.8

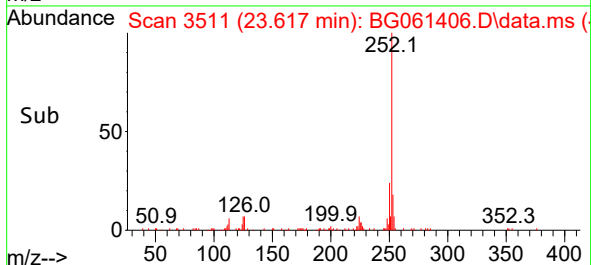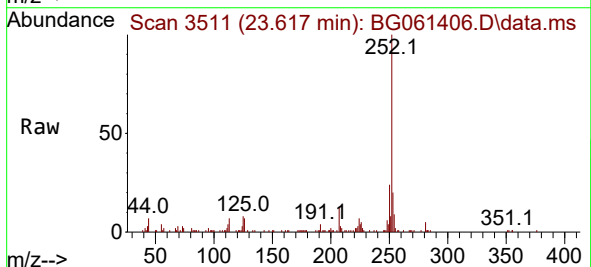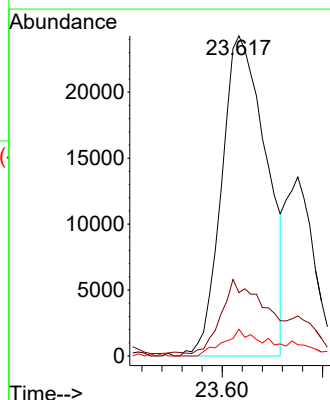

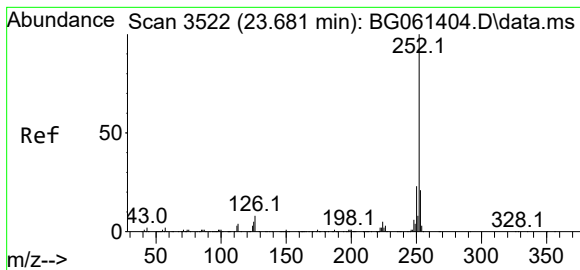

#91
Benzo(k)fluoranthene
Concen: 1.770 ng/ul m
RT: 23.675 min Scan# 3521
Delta R.T. -0.005 min
Lab File: BG061406.D
Acq: 1 Jun 2024 00:21




Instrument :
BNA_G
ClientSampleId :
BH5S5

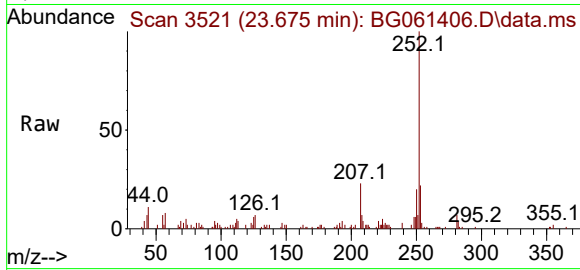


Tgt Ion:252 Resp: 2717
Ion Ratio Lower Upper
252 100
253 22.4 16.0 24.0
125 6.3 4.3 6.5

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 06/03/2024
Supervised By :mohammad ahmed 06/04/2024

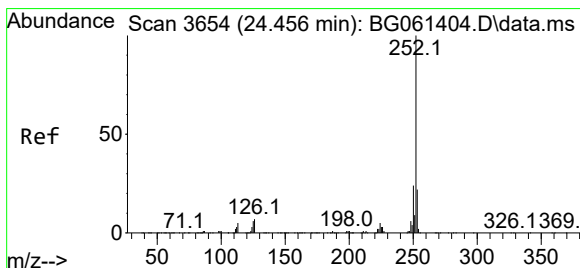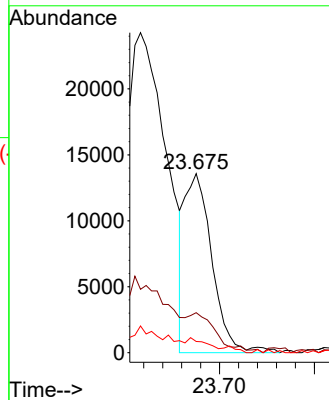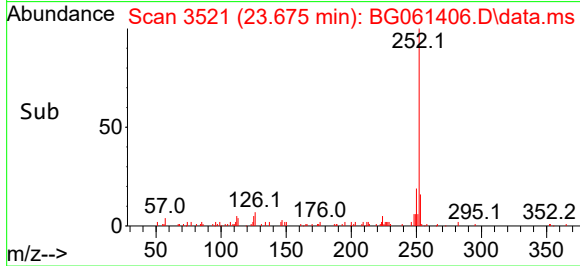


#93
Benzo(a)pyrene
Concen: 3.755 ng/ul
RT: 24.445 min Scan# 3652
Delta R.T. -0.005 min
Lab File: BG061406.D
Acq: 1 Jun 2024 00:21

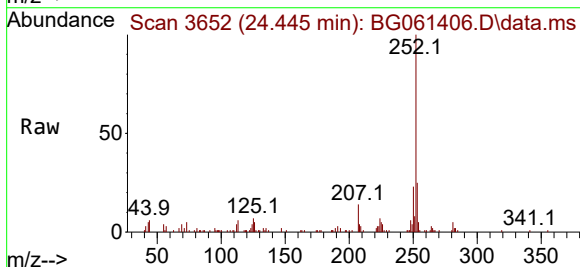

Tgt Ion:252 Resp: 53930
Ion Ratio Lower Upper
252 100
253 25.4 16.4 24.6#
125 7.1 4.3 6.5#

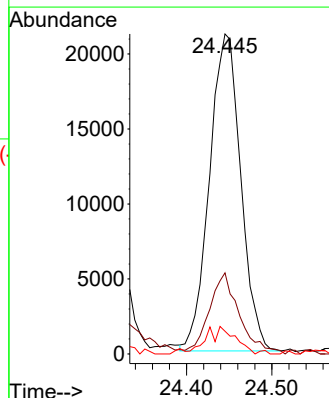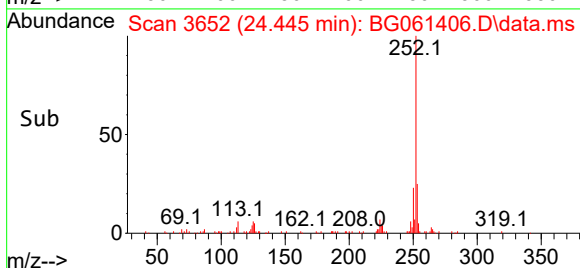

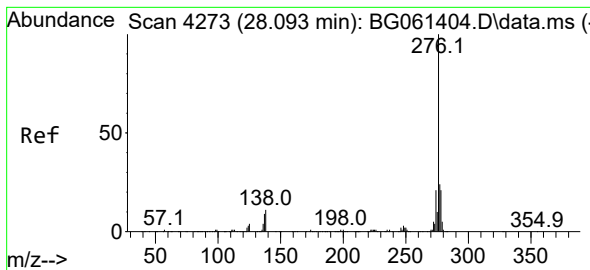

#94

Indeno(1,2,3-cd)pyrene

Concen: 2.270 ng/ul m

RT: 28.088 min Scan# 441

Delta R.T. -0.005 min

Lab File: BG061406.D

Acq: 1 Jun 2024 00:21

Instrument :

BNA_G

ClientSampleId :





BH5S5

Tgt Ion:	276	Resp:	39410
Ion Ratio	Lower	Upper	
276	100		
138	13.3	8.6	13.0
277	18.4	19.7	29.5

Manual Integrations

APPROVED

Reviewed By :Jagrut Upadhyay 06/03/2024
Supervised By :mohammad ahmed 06/04/2024

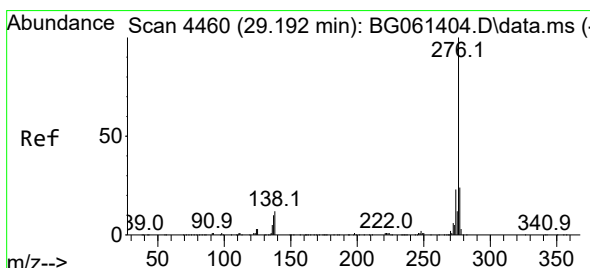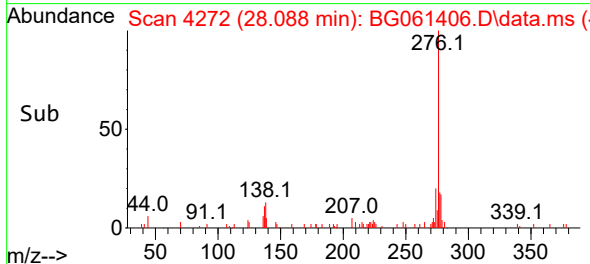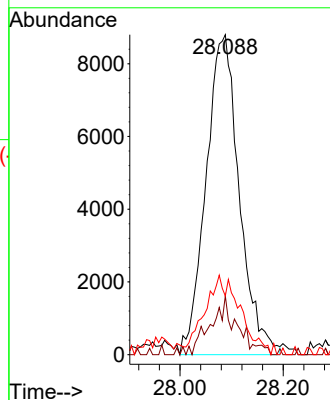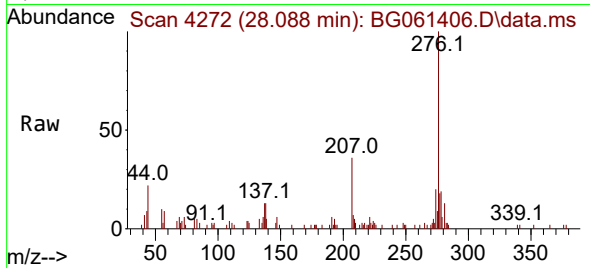

#96

Benzo(g,h,i)perylene

Concen: 2.808 ng/ul m

RT: 29.175 min Scan# 4457

Delta R.T. 0.001 min

Lab File: BG061406.D

Acq: 1 Jun 2024 00:21

Tgt Ion:	276	Resp:	38789
Ion Ratio	Lower	Upper	
276	100		
138	10.4	8.7	13.1
277	24.2	18.2	27.2

