
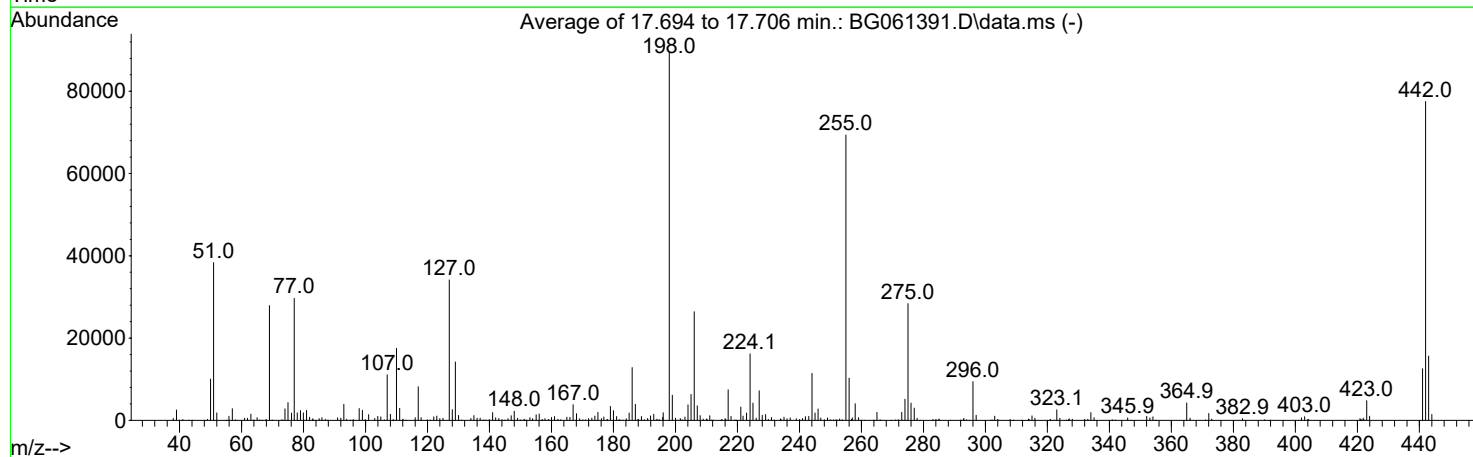


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG053124\
Data File : BG061391.D
Acq On : 31 May 2024 13:27
Operator : MA/JU
Sample : DFTPP575
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP575

Integration File: LSCINT.P

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG052124.MA.M
Title : SVOA CALIBRATION
Last Update : Thu May 30 22:54:48 2024

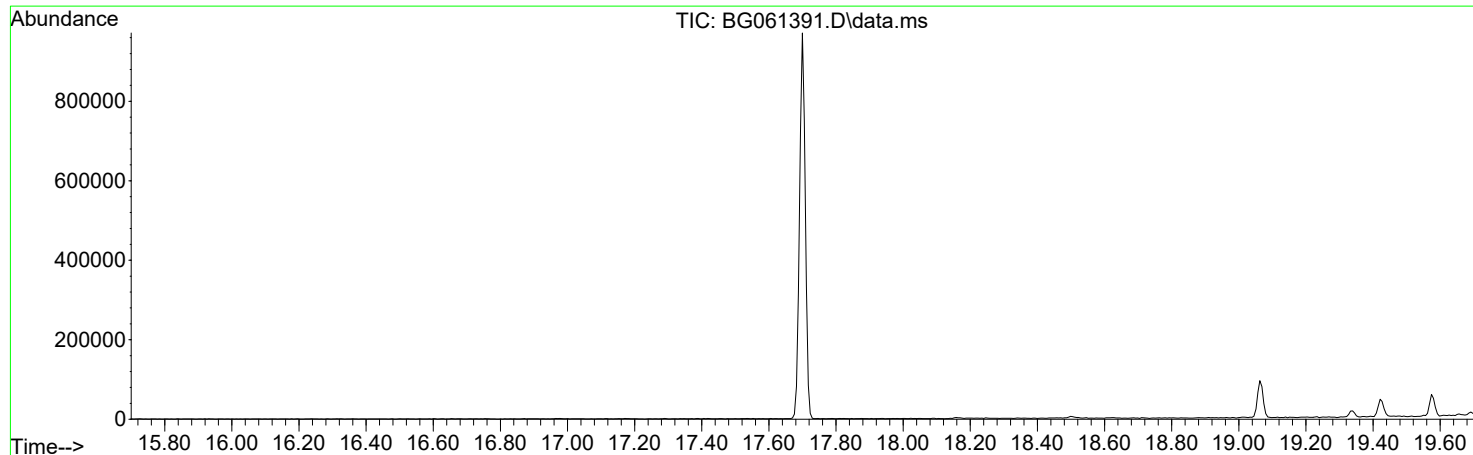

AutoFind: Scans 2503, 2504, 2505; Background Corrected with Scan 2497

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.9	38347	PASS
68	69	0.00	2	0.8	231	PASS
69	198	0.00	100	31.2	27901	PASS
70	69	0.00	2	0.4	122	PASS
127	198	10	80	38.2	34136	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	89427	PASS
199	198	5	9	6.9	6127	PASS
275	198	10	60	31.8	28397	PASS
365	198	1	100	4.7	4239	PASS
441	198	0.01	100	14.0	12551	PASS
442	198	50	100	86.7	77520	PASS
443	442	15	24	20.2	15625	PASS

Scan 2497 (17.659 min): BG061391.D\data.ms
DFTPP575

m/z	Abundance
43.10	214.0
44.00	814.0
55.00	318.0
207.10	242.0

Instrument :
BNA_G
ClientSampleId :
DFTPP575

m/z	Abundance
38.00	561.0
39.00	2723.0
41.00	209.0
43.10	256.0
44.00	812.0
49.00	328.0
50.00	10012.0
51.00	39096.0
52.00	2357.0
55.20	170.0
55.90	1067.0
57.00	2677.0
58.00	195.0
61.00	562.0
61.90	480.0
63.00	1454.0
63.80	274.0
65.00	820.0
66.90	165.0
67.90	694.0
69.00	28624.0
73.10	241.0
74.00	2606.0
75.00	4466.0
76.10	1829.0
77.00	29688.0
78.00	1938.0
79.00	2631.0
80.00	1948.0
81.00	2559.0
82.00	908.0
82.90	586.0
85.00	379.0
85.90	521.0
87.00	241.0
91.00	674.0
92.00	637.0
93.00	4162.0
94.00	325.0
95.10	198.0
96.10	201.0
98.00	2555.0
99.00	2549.0
99.90	314.0
101.00	1449.0
102.90	500.0
104.00	988.0
104.90	805.0
106.10	384.0
107.00	11204.0
108.00	1519.0
108.90	405.0
110.00	16744.0
111.00	2928.0
111.90	338.0
116.00	733.0
117.00	8001.0
117.90	723.0
119.90	199.0
120.90	193.0
122.00	813.0
123.00	966.0
124.00	552.0
125.10	445.0
127.00	31552.0
128.00	2484.0
129.00	13243.0
130.10	1116.0
134.10	594.0
134.90	971.0
135.90	360.0
137.00	787.0
138.20	204.0
139.90	251.0
141.00	1782.0
142.00	546.0
143.10	453.0
144.80	158.0
145.90	396.0
147.00	1291.0
148.00	2080.0
149.00	465.0
149.90	194.0
151.20	256.0
153.00	844.0
153.90	427.0
155.10	1370.0
156.00	1536.0
156.90	250.0
157.90	288.0
159.00	371.0
160.10	651.0

Instrument :
BNA_G
ClientSampleId :
DFTPP575

161.00	888.0
162.10	339.0
163.10	182.0
165.00	877.0
166.00	774.0
167.00	3717.0
168.00	1657.0
169.10	368.0
170.20	160.0
170.90	193.0
172.00	567.0
173.00	515.0
174.00	878.0
175.00	2061.0
176.10	543.0
176.90	557.0
177.90	296.0
179.00	3164.0
180.00	2287.0
181.00	895.0
181.80	271.0
183.10	222.0
184.10	335.0
185.10	1481.0
186.00	10928.0
187.10	3579.0
187.90	544.0
189.00	910.0
191.00	522.0
191.90	752.0
193.00	1291.0
193.70	169.0
194.60	203.0
195.90	2186.0
198.00	79536.0
199.00	5682.0
200.00	363.0
201.70	493.0
202.20	187.0
203.10	922.0
204.00	3517.0
205.00	5893.0
206.00	23144.0
207.00	3513.0
208.00	1042.0
209.00	284.0
209.90	413.0
211.00	931.0
212.20	243.0
214.80	244.0
216.10	680.0
217.00	6403.0
217.90	858.0
219.20	178.0
219.60	161.0
219.80	161.0
221.00	2824.0
221.80	933.0
222.90	1349.0
224.10	13330.0
225.00	3877.0
227.00	6229.0
228.00	1092.0
229.10	1193.0
230.10	167.0
231.00	640.0
233.90	522.0
235.10	770.0
235.90	290.0
237.00	472.0
239.00	270.0
240.10	224.0
241.00	421.0
242.00	943.0
243.00	892.0
244.10	9616.0
245.00	1635.0
246.00	2132.0
246.80	510.0
248.10	180.0
249.00	549.0
249.90	167.0
251.00	180.0
251.80	179.0
253.00	439.0
253.80	437.0
255.00	59288.0
256.00	8810.0
257.10	915.0
258.00	3543.0
259.10	506.0
265.00	1700.0
273.00	1305.0
274.00	3991.0
275.00	23256.0
276.00	3686.0

Instrument :
BNA_G
ClientSampleId :
DFTPP575

277.00	2509.0
278.00	379.0
278.90	158.0
283.00	202.0
284.00	310.0
284.90	464.0
288.80	165.0
292.90	477.0
293.10	500.0
294.00	265.0
296.00	7601.0
297.00	942.0
303.00	838.0
303.80	190.0
307.90	167.0
309.10	262.0
313.90	400.0
315.00	974.0
316.00	517.0
320.80	251.0
323.00	1801.0
324.00	474.0
327.00	527.0
328.10	227.0
332.10	160.0
333.10	228.0
334.10	1491.0
335.00	396.0
340.90	319.0
346.00	534.0
352.00	730.0
353.00	351.0
354.10	806.0
354.80	156.0
365.00	3265.0
366.20	328.0
372.10	1235.0
373.20	220.0
382.90	330.0
401.90	431.0
403.00	761.0
404.20	366.0
420.90	593.0
421.90	743.0
423.00	3040.0
423.90	909.0
441.10	9054.0
442.00	54080.0
443.00	11306.0
444.00	1238.0

Instrument :
BNA_G
ClientSampleId :
DFTPP575

m/z	Abundance
37.90	424.0
39.00	3002.0
40.00	186.0
41.10	151.0
43.00	164.0
44.00	906.0
49.00	380.0
50.00	11748.0
51.00	44824.0
52.00	1869.0
55.00	579.0
56.00	1036.0
57.00	3558.0
58.00	172.0
61.00	640.0
61.90	580.0
63.00	1708.0
64.00	270.0
65.00	521.0
69.00	32688.0
69.90	173.0
74.00	3274.0
75.00	4991.0
76.10	2316.0
77.00	35784.0
78.00	2392.0
79.00	2625.0
79.90	2221.0
81.00	2727.0
81.90	789.0
83.10	715.0
85.10	362.0
86.00	899.0
87.00	329.0
87.90	182.0
91.00	460.0
92.00	659.0
93.00	4591.0
93.90	277.0
96.00	186.0
98.00	3888.0
99.00	3066.0
99.80	314.0
101.00	1770.0
103.00	513.0
103.90	1031.0
105.00	1057.0
107.00	12732.0
108.00	1686.0
110.00	20984.0
111.00	3360.0
112.10	552.0
116.00	846.0
117.00	9528.0
118.00	723.0
120.00	209.0
122.00	1066.0
123.00	1281.0
124.00	462.0
125.00	743.0
127.00	42392.0
128.00	3254.0
129.00	17456.0
129.90	1451.0
131.00	272.0
134.00	455.0
135.00	1767.0
136.00	709.0
137.10	553.0
137.90	194.0
138.90	187.0
140.10	254.0
141.00	2194.0
142.00	738.0
143.00	646.0
144.00	336.0
145.00	169.0
146.00	542.0
147.00	1227.0
148.00	2747.0
149.00	619.0
150.10	268.0
151.20	385.0
152.00	185.0
153.10	529.0
153.80	421.0
155.00	1557.0
156.00	1935.0
157.10	345.0
157.80	617.0
159.20	351.0
160.00	686.0

Instrument :
BNA_G
ClientSampleId :
DFTPP575

161.00	1083.0
162.00	256.0
163.00	224.0
165.00	822.0
165.90	801.0
167.00	4368.0
168.10	1661.0
169.10	466.0
172.00	581.0
173.10	717.0
174.00	1360.0
175.00	1889.0
176.10	463.0
176.90	1182.0
178.10	551.0
179.00	3825.0
180.00	2731.0
181.00	1094.0
182.00	359.0
184.10	547.0
185.00	2089.0
186.00	16448.0
187.00	4569.0
188.10	538.0
189.00	1091.0
190.00	242.0
191.10	314.0
192.00	1487.0
193.00	1893.0
194.00	555.0
194.90	247.0
196.10	3527.0
198.00	108144.0
199.00	7358.0
200.00	711.0
201.50	457.0
202.20	234.0
203.00	751.0
204.10	4377.0
205.00	7505.0
206.10	32688.0
207.10	4542.0
208.00	1532.0
208.90	216.0
210.00	636.0
211.00	1369.0
215.00	393.0
215.90	575.0
217.00	8863.0
218.00	913.0
219.10	230.0
221.10	4059.0
221.80	1348.0
223.00	2109.0
224.00	20168.0
225.00	4902.0
226.10	935.0
227.00	8754.0
228.00	1495.0
229.00	1650.0
229.90	253.0
231.10	695.0
234.10	644.0
234.90	528.0
236.00	412.0
237.00	528.0
239.00	489.0
240.00	261.0
241.00	525.0
241.90	875.0
243.00	1152.0
244.10	13152.0
245.10	2342.0
246.00	3391.0
246.90	650.0
249.10	616.0
249.90	158.0
250.90	180.0
251.80	150.0
252.90	242.0
255.00	81256.0
256.00	12710.0
257.00	937.0
258.00	4732.0
259.00	913.0
260.90	163.0
265.00	2469.0
266.00	206.0
269.80	175.0
271.10	182.0
272.10	309.0
273.00	2760.0
274.00	6644.0
275.00	33920.0
276.00	4820.0
277.10	3376.0

Instrument :
BNA_G
ClientSampleId :
DFTPP575

278.00	739.0
283.10	287.0
284.10	356.0
285.10	510.0
292.30	177.0
293.00	493.0
294.90	175.0
296.00	11174.0
297.00	1517.0
301.80	206.0
303.00	1243.0
304.10	375.0
308.00	263.0
311.70	163.0
314.10	667.0
315.00	1232.0
316.00	685.0
321.00	386.0
322.10	199.0
323.00	3208.0
323.90	454.0
327.10	571.0
328.00	252.0
332.00	381.0
333.10	378.0
333.90	2279.0
335.00	874.0
341.10	281.0
345.90	676.0
347.00	175.0
352.00	1337.0
353.00	799.0
354.00	889.0
365.00	4988.0
366.00	694.0
371.00	173.0
372.00	2101.0
373.00	305.0
383.00	460.0
390.00	418.0
391.90	187.0
402.00	852.0
403.00	1009.0
403.90	302.0
420.80	667.0
421.40	446.0
422.10	880.0
423.00	5993.0
423.90	1202.0
441.00	14752.0
442.00	92984.0
443.00	18280.0
443.90	1375.0

Instrument :
BNA_G
ClientSampleId :
DFTPP575

m/z	Abundance
38.00	464.0
39.10	1842.0
41.00	262.0
43.00	329.0
44.00	767.0
50.00	8403.0
51.00	31120.0
52.00	1292.0
55.00	239.0
56.00	954.0
57.00	2342.0
61.00	375.0
62.00	468.0
63.00	1353.0
65.00	612.0
65.90	344.0
69.00	22392.0
69.90	194.0
73.10	295.0
74.00	2573.0
75.00	3517.0
76.10	1102.0
77.00	23488.0
78.00	1194.0
79.00	1878.0
80.00	1308.0
81.00	2013.0
82.00	614.0
83.00	466.0
84.00	174.0
85.00	502.0
86.00	552.0
87.00	290.0
91.00	742.0
92.00	348.0
93.00	2926.0
94.00	181.0
96.10	180.0
97.90	2188.0
99.00	1724.0
101.00	1000.0
103.00	414.0
104.00	937.0
105.00	737.0
107.00	9361.0
108.00	1236.0
109.00	292.0
110.00	14833.0
111.00	2418.0
112.10	416.0
113.10	183.0
116.10	469.0
117.00	6997.0
117.90	525.0
122.00	684.0
123.00	883.0
124.00	279.0
124.90	362.0
127.00	28464.0
128.00	2138.0
129.00	11933.0
130.00	1103.0
133.90	310.0
135.00	813.0
136.10	579.0
136.90	357.0
139.90	240.0
141.00	1797.0
142.00	566.0
142.90	311.0
144.10	188.0
146.00	358.0
147.00	912.0
148.00	1831.0
149.10	397.0
150.90	186.0
151.30	176.0
151.60	163.0
153.00	673.0
154.00	480.0
155.00	1165.0
156.10	1238.0
157.00	242.0
158.00	336.0
158.90	203.0
159.90	730.0
161.00	796.0
162.10	281.0
162.90	155.0
164.90	645.0
166.00	606.0
167.00	3308.0

Instrument :
BNA_G
ClientSampleId :
DFTPP575

168.00	1555.0
169.10	371.0
170.00	197.0
171.00	178.0
171.90	183.0
172.90	402.0
174.00	915.0
175.00	1907.0
176.20	300.0
176.90	751.0
177.90	281.0
179.00	3153.0
180.00	2163.0
181.00	797.0
182.10	186.0
184.00	270.0
185.10	1752.0
186.00	11099.0
187.00	3551.0
188.10	331.0
189.00	761.0
190.00	229.0
191.00	561.0
192.00	1047.0
193.00	1300.0
194.10	360.0
194.90	216.0
196.00	2128.0
198.00	80600.0
199.00	5340.0
200.00	540.0
200.80	165.0
201.40	362.0
203.00	789.0
204.10	3459.0
205.00	5550.0
206.10	23432.0
207.00	3348.0
207.90	909.0
209.00	408.0
210.30	520.0
211.10	1048.0
211.70	234.0
215.00	329.0
216.20	650.0
217.00	6996.0
218.00	1100.0
221.00	2840.0
221.80	919.0
223.00	1883.0
224.00	15059.0
225.00	3772.0
226.00	744.0
227.00	6571.0
228.00	1118.0
229.00	1354.0
229.90	311.0
230.90	741.0
231.90	181.0
233.90	496.0
234.80	499.0
235.10	497.0
236.10	415.0
237.00	807.0
239.00	370.0
240.10	234.0
241.00	495.0
242.00	857.0
243.00	942.0
244.00	11507.0
245.10	1451.0
246.00	2827.0
247.00	549.0
247.90	252.0
249.10	557.0
250.10	215.0
252.10	300.0
253.00	429.0
255.00	67656.0
256.00	9319.0
256.80	652.0
258.00	3814.0
259.00	566.0
259.90	207.0
264.00	206.0
265.00	1622.0
266.10	301.0
271.00	233.0
271.80	242.0
273.00	1788.0
274.10	4810.0
275.00	28016.0
276.00	4103.0
277.00	3060.0
277.90	444.0
283.10	255.0

Instrument :
BNA_G
ClientSampleId :
DFTPP575

283.80	178.0
285.10	459.0
292.00	233.0
293.00	538.0
293.80	246.0
296.00	9430.0
297.00	1291.0
302.20	188.0
303.00	970.0
304.00	388.0
308.00	250.0
313.90	505.0
315.00	1027.0
315.90	473.0
320.90	326.0
323.10	2649.0
324.10	542.0
326.10	186.0
326.80	539.0
328.10	296.0
332.00	250.0
332.90	187.0
334.00	1936.0
335.10	663.0
341.90	223.0
345.80	566.0
352.10	855.0
353.10	619.0
354.00	910.0
355.20	151.0
364.90	4463.0
365.90	645.0
371.00	235.0
372.00	1700.0
372.90	432.0
382.90	534.0
390.20	254.0
400.90	177.0
401.90	631.0
403.00	870.0
404.00	253.0
404.30	299.0
421.10	687.0
421.90	869.0
423.00	5357.0
424.00	898.0
441.00	13847.0
442.00	85496.0
443.00	17288.0
444.10	1694.0

Instrument :
BNA_G
ClientSampleId :
DFTPP575