

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG060115\
 Data File : BG017382.D
 Acq On : 1 Jun 2015 23:39
 Operator : TP/IZ
 Sample : G2430-03
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BCRD6

Quant Time: Jun 02 03:54:10 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG052915.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 02 03:15:26 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	26860	20.00	ng/ul	0.00
18) Naphthalene-d8	10.43	136	120914	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.31	164	85002	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.05	188	201696	20.00	ng/ul	0.00
75) Chrysene-d12	21.24	240	200300	20.00	ng/ul	0.00
83) Perylene-d12	23.48	264	195375	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.06	96	1794	3.17	ng/uL	0.00
5) Phenol-d5	6.84	99	42295	18.68	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.98	67	26527	19.60	ng/ul	0.00
9) 2-Chlorophenol-d4	7.18	132	35539	19.36	ng/ul	0.00
13) 4-Methylphenol-d8	8.38	113	35883	18.50	ng/ul	0.00
19) Nitrobenzene-d5	8.80	128	19097	20.39	ng/ul	0.00
22) 2-Nitrophenol-d4	9.52	143	21914	19.66	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.08	165	34497	17.60	ng/ul	0.00
29) 4-Chloroaniline-d4	10.58	131	45575	20.26	ng/ul	0.00
43) Dimethylphthalate-d6	13.72	166	111069	18.33	ng/ul	0.00
46) Acenaphthylene-d8	13.99	160	138665	17.67	ng/ul	0.00
51) 4-Nitrophenol-d4	14.56	143	19807	17.13	ng/ul	0.00
57) Fluorene-d10	15.30	176	99113	16.97	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.43	200	21611	15.31	ng/ul	0.00
70) Anthracene-d10	17.15	188	152921	16.18	ng/ul	0.00
76) Pyrene-d10	19.45	212	153296	15.81	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.34	264	110706	12.69	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.77	163	22395	3.33	ng/ul	99
81) Bis(2-ethylhexyl)phthalate	21.16	149	8736	1.08	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG060115\
Data File : BG017382.D
Acq On : 1 Jun 2015 23:39
Operator : TP/IZ
Sample : G2430-03
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BCRD6

Quant Time: Jun 02 03:54:10 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG052915.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jun 02 03:15:26 2015
Response via : Initial Calibration

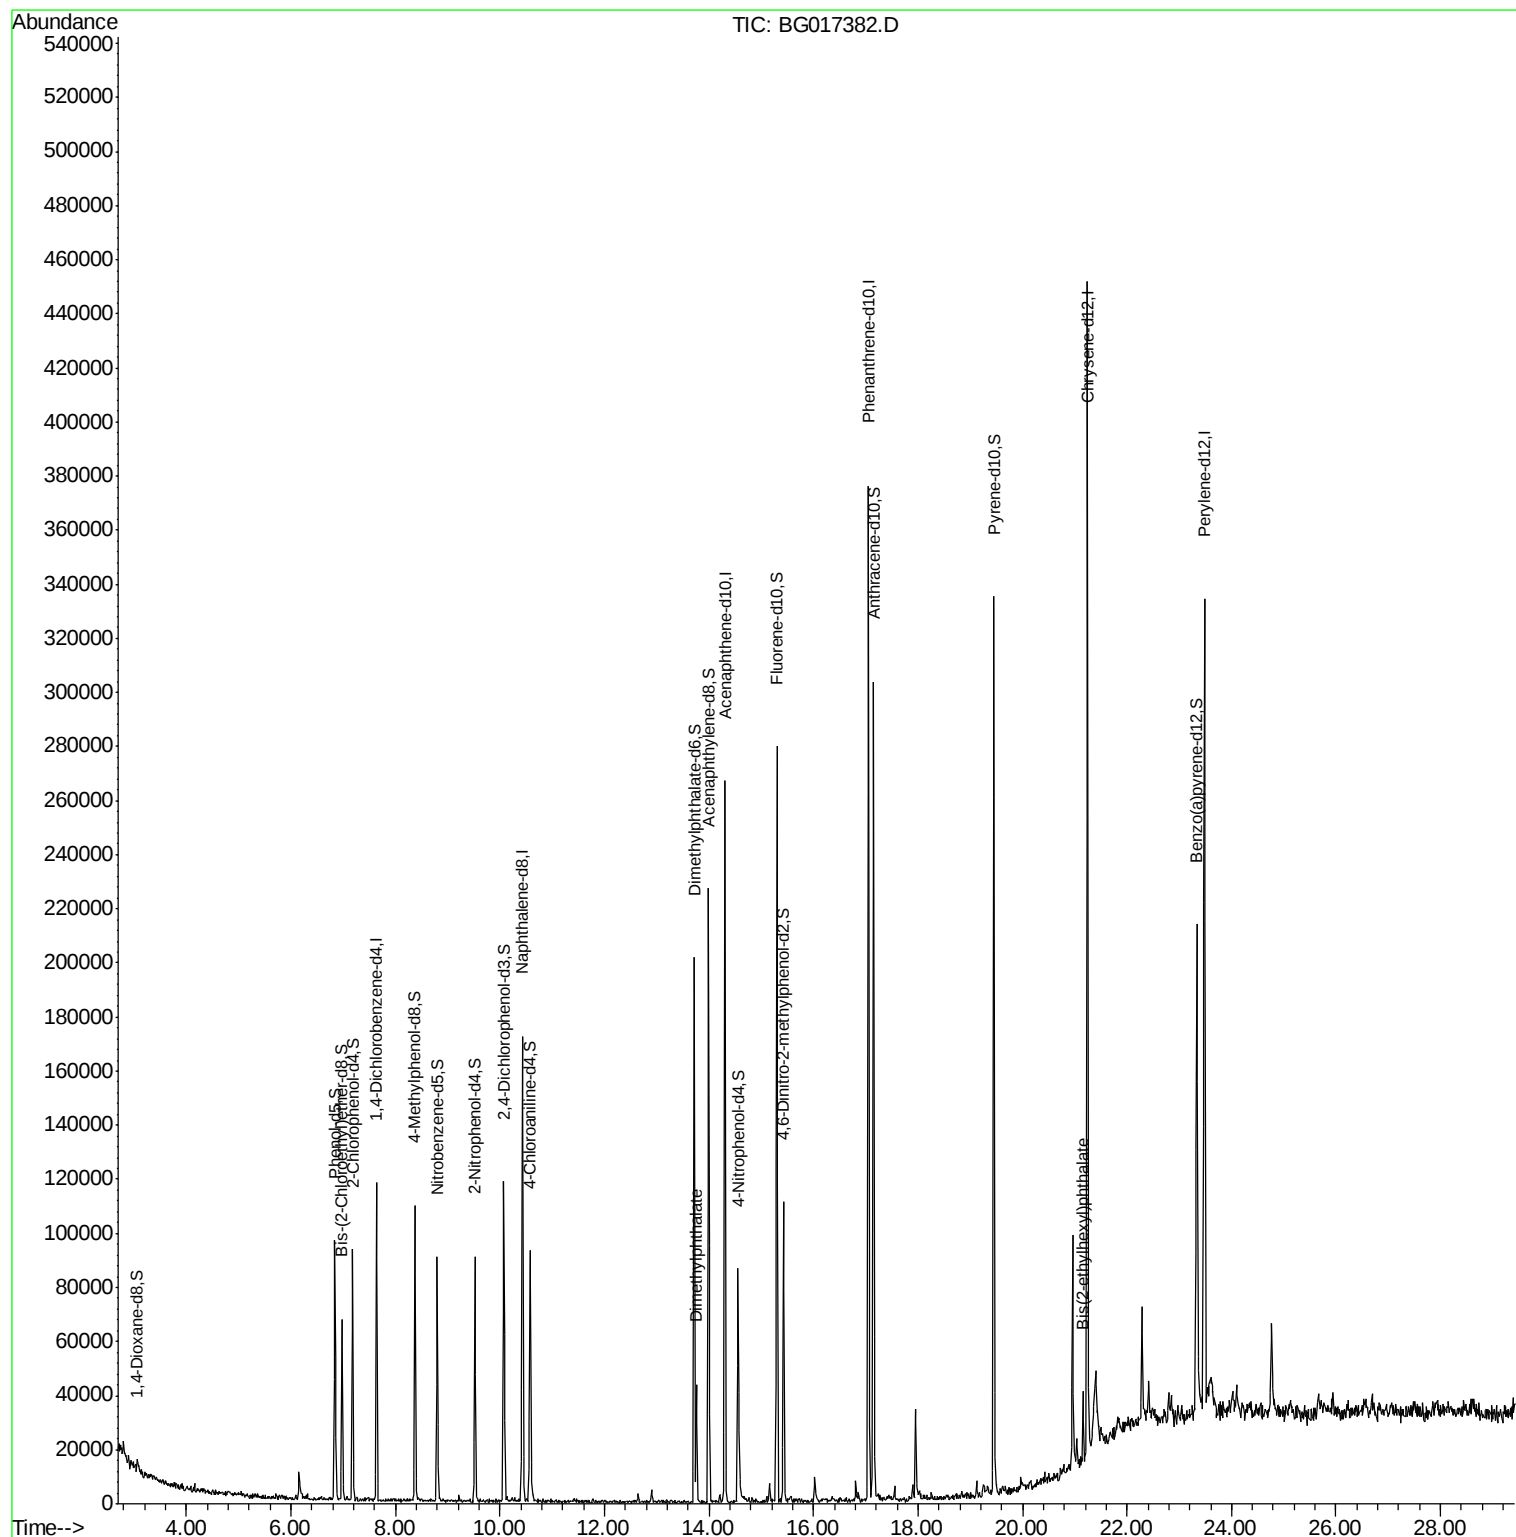

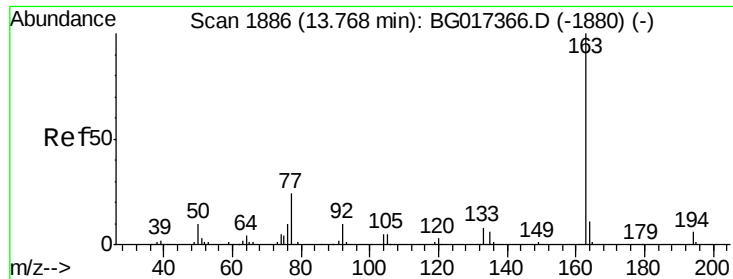

#44

Dimethylphthalate

Concen: 3.33 ng/ul

RT: 13.77 min Scan# 1885

Delta R.T. -0.00 min

Lab File: BG017382.D

Acq: 1 Jun 2015 23:39

Instrument :

BNA_G

ClientSampleId :

BCRD6


Tgt Ion:163 Resp: 22395

Ion Ratio Lower Upper

163 100

194 6.0 5.2 7.8




164 11.0 9.2 13.8

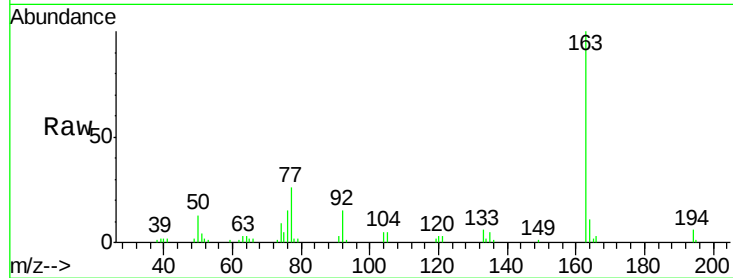

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

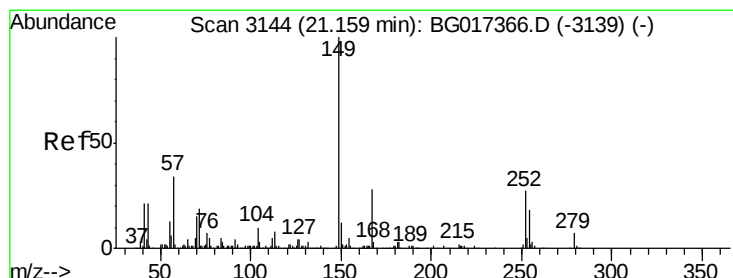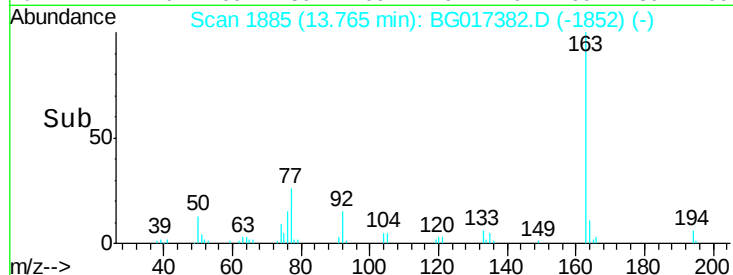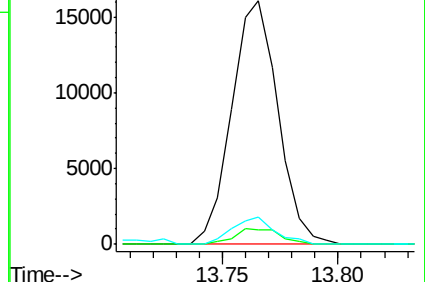

#81

Bis(2-ethylhexyl)phthalate

Concen: 1.08 ng/ul

RT: 21.16 min Scan# 3144

Delta R.T. -0.00 min

Lab File: BG017382.D

Acq: 1 Jun 2015 23:39


Tgt Ion:149 Resp: 8736

Ion Ratio Lower Upper

149 100

167 29.5 25.1 37.7

279 8.7 7.0 10.4

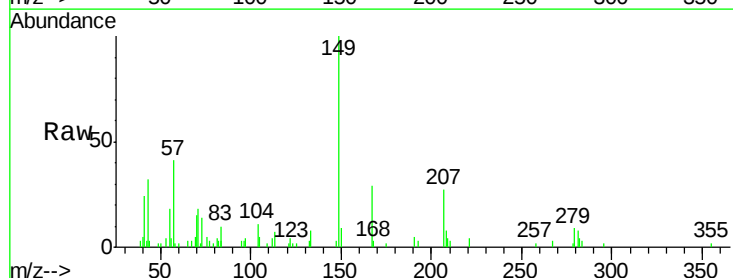

Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

