

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG060115\
 Data File : BG017383.D
 Acq On : 2 Jun 2015 00:13
 Operator : TP/IZ
 Sample : G2430-04
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BCRD7

Quant Time: Jun 02 03:58:41 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG052915.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 02 03:15:26 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	23646	20.00	ng/ul	0.00
18) Naphthalene-d8	10.43	136	107231	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.30	164	79098	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.05	188	184984	20.00	ng/ul	0.00
75) Chrysene-d12	21.24	240	186603	20.00	ng/ul	0.00
83) Perylene-d12	23.49	264	181294	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.06	96	2076	4.17	ng/uL	0.00
5) Phenol-d5	6.84	99	41737	20.94	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.98	67	26231	22.02	ng/ul	0.00
9) 2-Chlorophenol-d4	7.18	132	36153	22.38	ng/ul	0.00
13) 4-Methylphenol-d8	8.38	113	31622	18.52	ng/ul	0.00
19) Nitrobenzene-d5	8.80	128	17515	21.09	ng/ul	0.00
22) 2-Nitrophenol-d4	9.53	143	21057	21.30	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.07	165	35877	20.64	ng/ul	0.00
29) 4-Chloroaniline-d4	10.58	131	39422	19.76	ng/ul	0.00
43) Dimethylphthalate-d6	13.72	166	116871	20.72	ng/ul	0.00
46) Acenaphthylene-d8	14.00	160	134881	18.47	ng/ul	0.00
51) 4-Nitrophenol-d4	14.56	143	22073	20.52	ng/ul	0.00
57) Fluorene-d10	15.30	176	96053	17.67	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.43	200	23270	17.97	ng/ul	0.00
70) Anthracene-d10	17.15	188	140219	16.18	ng/ul	0.00
76) Pyrene-d10	19.45	212	141531	15.66	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.34	264	96046	11.87	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.76	163	27552	4.40	ng/ul#	95
81) Bis(2-ethylhexyl)phthalate	21.16	149	41476	5.49	ng/ul	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG060115\
Data File : BG017383.D
Acq On : 2 Jun 2015 00:13
Operator : TP/IZ
Sample : G2430-04
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BCRD7

Quant Time: Jun 02 03:58:41 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG052915.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jun 02 03:15:26 2015
Response via : Initial Calibration

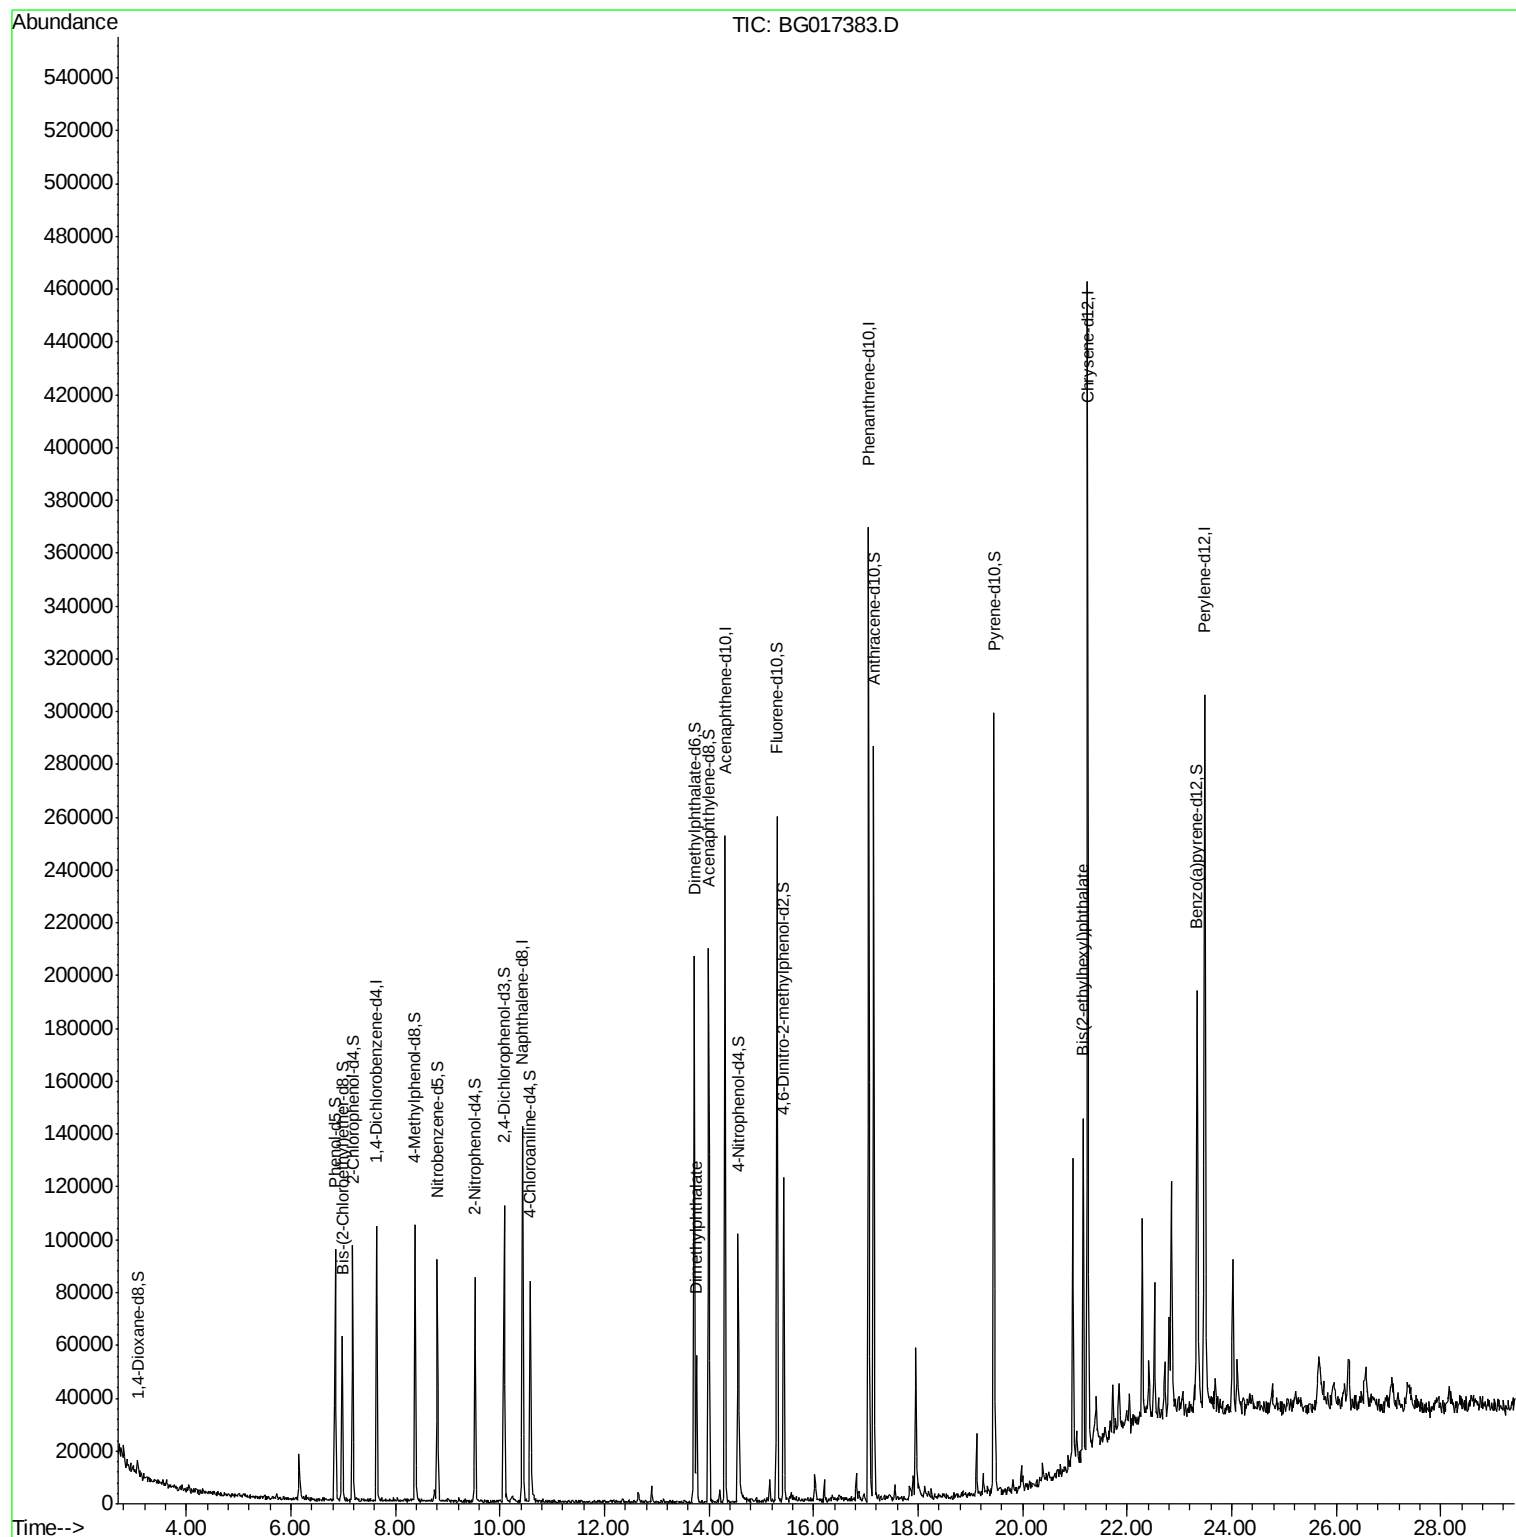

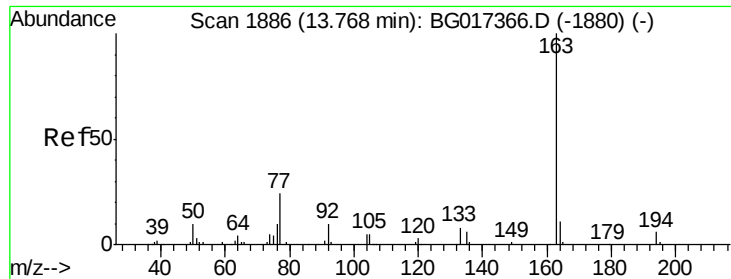

#44

Dimethylphthalate

Concen: 4.40 ng/ul

RT: 13.76 min Scan# 1885

Delta R.T. -0.01 min

Lab File: BG017383.D

Acq: 2 Jun 2015 00:13

Instrument :

BNA_G

ClientSampleId :

BCRD7


Tgt Ion:163 Resp: 27552

Ion Ratio Lower Upper

163 100

194 6.1 5.2 7.8




164 8.7 9.2 13.8#

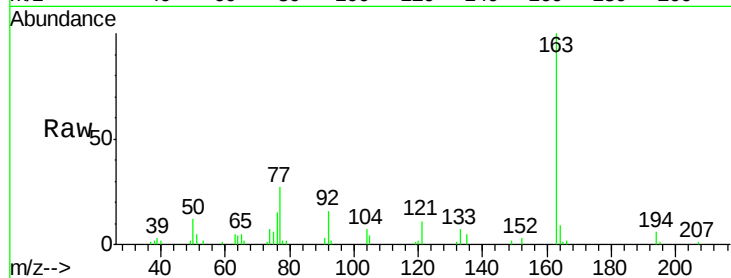

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

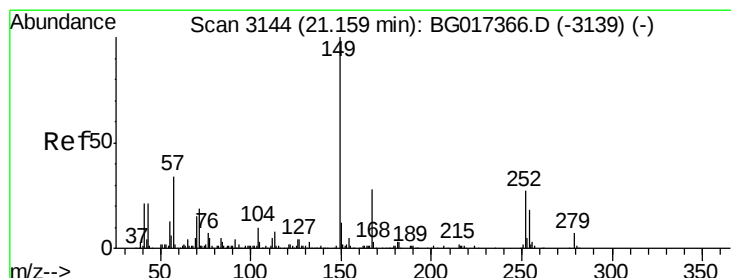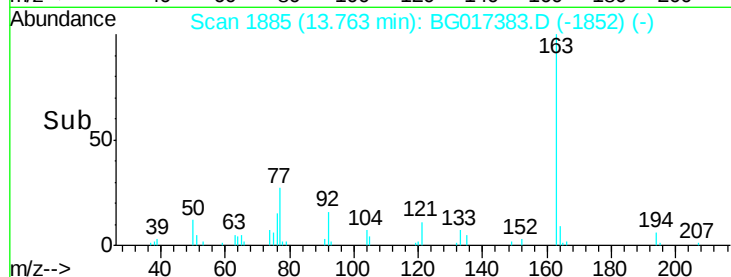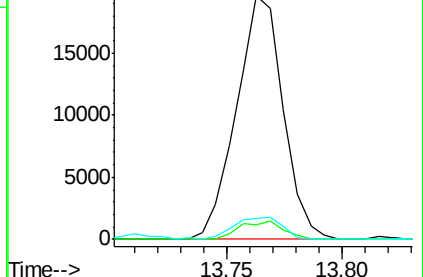

#81

Bis(2-ethylhexyl)phthalate

Concen: 5.49 ng/ul

RT: 21.16 min Scan# 3144

Delta R.T. -0.01 min

Lab File: BG017383.D

Acq: 2 Jun 2015 00:13


Tgt Ion:149 Resp: 41476

Ion Ratio Lower Upper

149 100

167 29.0 25.1 37.7

279 8.1 7.0 10.4

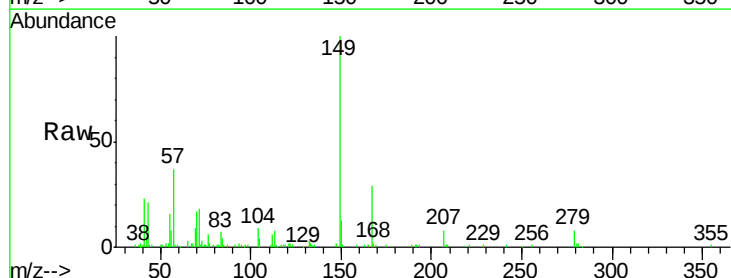

Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

