

Data Path : Z:\HPCHEM1\BNA G\DATA\BG060116\
 Data File : BG022140.D
 Acq On : 1 Jun 2016 13:56
 Operator : UM/SJ
 Sample : H3254-02
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BCZH8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG052116.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.884	176	178	181	rBV3	985	1118	0.16%	0.022%
2	4.054	205	207	210	rBV3	916	944	0.13%	0.019%
3	4.724	319	321	324	rBV4	1103	1127	0.16%	0.022%
4	4.859	342	344	347	rBV2	1228	1124	0.16%	0.022%
5	5.036	371	374	378	rBV3	898	1478	0.21%	0.029%
6	5.200	399	402	405	rVB4	1051	1254	0.18%	0.025%
7	5.987	534	536	538	rBV3	733	819	0.12%	0.016%
8	6.598	634	640	643	rBV4	781	1364	0.19%	0.027%
9	7.110	723	727	728	rBV4	772	986	0.14%	0.019%
10	7.133	730	731	737	rVB3	844	1114	0.16%	0.022%
11	7.303	753	760	774	rBV2	14167	34908	4.95%	0.685%
12	7.462	780	787	796	rBV	16411	36668	5.20%	0.719%
13	7.668	817	822	833	rVV2	21765	43046	6.11%	0.845%
14	7.756	835	837	840	rVV4	1342	1152	0.16%	0.023%
15	7.785	840	842	845	rVV	1057	1028	0.15%	0.020%
16	7.815	845	847	850	rVB2	977	1005	0.14%	0.020%
17	8.003	877	879	881	rBV2	1071	973	0.14%	0.019%
18	8.067	888	890	892	rBV3	1004	1145	0.16%	0.022%
19	8.091	892	894	895	rVV2	1487	1009	0.14%	0.020%
20	8.138	895	902	916	rVV	78519	168425	23.89%	3.305%
21	8.343	935	937	939	rBV2	878	834	0.12%	0.016%
22	8.461	954	957	960	rVB2	758	918	0.13%	0.018%
23	8.584	975	978	980	rBV	940	1078	0.15%	0.021%
24	8.684	993	995	998	rVB3	888	828	0.12%	0.016%
25	8.714	998	1000	1005	rBV2	745	1175	0.17%	0.023%
26	8.849	1017	1023	1035	rBV3	18287	45992	6.52%	0.902%
27	8.972	1043	1044	1046	rBV2	1256	961	0.14%	0.019%
28	9.237	1085	1089	1090	rBV2	927	1107	0.16%	0.022%
29	9.307	1095	1101	1117	rVV	18941	50416	7.15%	0.989%
30	9.530	1137	1139	1141	rVB	952	793	0.11%	0.016%
31	9.930	1202	1207	1210	rBV3	808	1076	0.15%	0.021%
32	10.041	1219	1226	1237	rBV4	9036	24754	3.51%	0.486%
33	10.135	1240	1242	1245	rVB	1491	1443	0.20%	0.028%
34	10.288	1265	1268	1270	rVB2	837	874	0.12%	0.017%

Data Path : Z:\HPCHEM1\BNA G\DATA\BG060116\
 Data File : BG022140.D
 Acq On : 1 Jun 2016 13:56
 Operator : UM/SJ
 Sample : H3254-02
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BCZH8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG052116.M
 Title : SVOA CALIBRATION

35	10.376	1278	1283	1284	rVB2	672	872	0.12%	0.017%
36	10.400	1284	1287	1289	rBV	756	876	0.12%	0.017%
37	10.435	1289	1293	1296	rVV3	614	1107	0.16%	0.022%
38	10.476	1298	1300	1303	rVB	818	819	0.12%	0.016%
39	10.512	1303	1306	1308	rBV2	752	886	0.13%	0.017%
40	10.582	1310	1318	1326	rBV	20938	44849	6.36%	0.880%
41	10.658	1329	1331	1337	rVB4	1474	2131	0.30%	0.042%
42	10.794	1350	1354	1357	rVB2	1210	1496	0.21%	0.029%
43	10.888	1365	1370	1371	rBV2	1026	1187	0.17%	0.023%
44	10.952	1373	1381	1396	rVV	150536	317752	45.08%	6.234%
45	11.111	1402	1408	1418	rBV4	2846	8474	1.20%	0.166%
46	11.875	1534	1538	1542	rBV2	991	1204	0.17%	0.024%
47	12.597	1658	1661	1666	rBV2	514	793	0.11%	0.016%
48	13.138	1750	1753	1759	rVB	948	1746	0.25%	0.034%
49	13.191	1759	1762	1764	rBV2	632	810	0.11%	0.016%
50	13.402	1795	1798	1800	rBV	788	798	0.11%	0.016%
51	13.637	1834	1838	1843	rVB4	1808	2533	0.36%	0.050%
52	14.154	1920	1926	1931	rBV	72306	121122	17.18%	2.376%
53	14.201	1931	1934	1941	rVV	13264	22710	3.22%	0.446%
54	14.254	1941	1943	1946	rVB	1143	798	0.11%	0.016%
55	14.460	1971	1978	1987	rBV	123750	216062	30.65%	4.239%
56	14.630	2005	2007	2013	rVB2	1755	1989	0.28%	0.039%
57	14.759	2021	2029	2043	rBV2	282546	518792	73.60%	10.179%
58	14.877	2047	2049	2052	rBV2	902	1031	0.15%	0.020%
59	15.582	2163	2169	2176	rBV4	3699	6393	0.91%	0.125%
60	15.635	2176	2178	2181	rBV2	667	761	0.11%	0.015%
61	15.752	2189	2198	2209	rBV	158294	280571	39.80%	5.505%
62	15.882	2216	2220	2225	rVB3	3268	4495	0.64%	0.088%
63	15.946	2230	2231	2234	rBV	795	827	0.12%	0.016%
64	15.982	2236	2237	2238	rBV	1602	1031	0.15%	0.020%
65	16.240	2278	2281	2284	rVB2	668	798	0.11%	0.016%
66	16.440	2309	2315	2317	rBV3	3120	4452	0.63%	0.087%
67	16.704	2355	2360	2364	rBV3	963	1596	0.23%	0.031%
68	17.233	2445	2450	2455	rVB6	2121	3742	0.53%	0.073%
69	17.286	2458	2459	2461	rBV2	1155	815	0.12%	0.016%
70	17.509	2490	2497	2506	rBV	361999	627488	89.02%	12.312%
71	17.603	2507	2513	2529	rVB2	158605	302013	42.84%	5.926%

Data Path : Z:\HPCHEM1\BNA G\DATA\BG060116\
 Data File : BG022140.D
 Acq On : 1 Jun 2016 13:56
 Operator : UM/SJ
 Sample : H3254-02
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BCZH8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG052116.M
 Title : SVOA CALIBRATION

72	17.862	2555	2557	2559	rVB2	1288	899	0.13%	0.018%
73	17.938	2567	2570	2573	rBV2	944	937	0.13%	0.018%
74	17.967	2573	2575	2578	rVV2	1034	1210	0.17%	0.024%
75	18.009	2580	2582	2585	rVB3	1114	997	0.14%	0.020%
76	18.079	2592	2594	2596	rVB2	869	763	0.11%	0.015%
77	18.103	2596	2598	2600	rBV2	697	835	0.12%	0.016%
78	18.167	2607	2609	2614	rVB3	624	1048	0.15%	0.021%
79	18.643	2686	2690	2693	rBV3	879	1022	0.14%	0.020%
80	19.002	2749	2751	2753	rVB2	960	817	0.12%	0.016%
81	19.172	2777	2780	2781	rBV2	811	835	0.12%	0.016%
82	19.231	2788	2790	2796	rVB3	771	1265	0.18%	0.025%
83	19.289	2798	2800	2802	rBV2	1856	1535	0.22%	0.030%
84	19.354	2809	2811	2813	rVB	1300	1005	0.14%	0.020%
85	19.383	2813	2816	2817	rBV2	1146	1219	0.17%	0.024%
86	19.519	2835	2839	2841	rBV2	2298	3488	0.49%	0.068%
87	19.554	2841	2845	2850	rVB3	5331	8559	1.21%	0.168%
88	19.730	2872	2875	2879	rBV3	1182	1625	0.23%	0.032%
89	19.765	2879	2881	2883	rBV3	2006	2027	0.29%	0.040%
90	19.883	2894	2901	2914	rBV	244023	409546	58.10%	8.036%
91	20.047	2927	2929	2933	rVB3	2288	2135	0.30%	0.042%
92	20.077	2933	2934	2936	rBV2	1545	907	0.13%	0.018%
93	20.230	2958	2960	2961	rBV2	1993	1120	0.16%	0.022%
94	20.359	2980	2982	2983	rBV2	2583	1860	0.26%	0.036%
95	20.653	3030	3032	3034	rBV3	2052	1841	0.26%	0.036%
96	20.705	3039	3041	3043	rVB3	2809	1710	0.24%	0.034%
97	21.399	3155	3159	3169	rVB9	9471	20287	2.88%	0.398%
98	21.787	3218	3225	3242	rBV	356155	704917	100.00%	13.831%
99	24.865	3740	3749	3766	rVB2	99426	307197	43.58%	6.027%
100	25.094	3778	3788	3804	rVB2	214145	676345	95.95%	13.270%


Sum of corrected areas: 5096706

Data Path : Z:\HPCHEM1\BNA G\DATA\BG060116\
Data File : BG022140.D
Acq On : 1 Jun 2016 13:56
Operator : UM/SJ
Sample : H3254-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BCZH8

Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG052116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

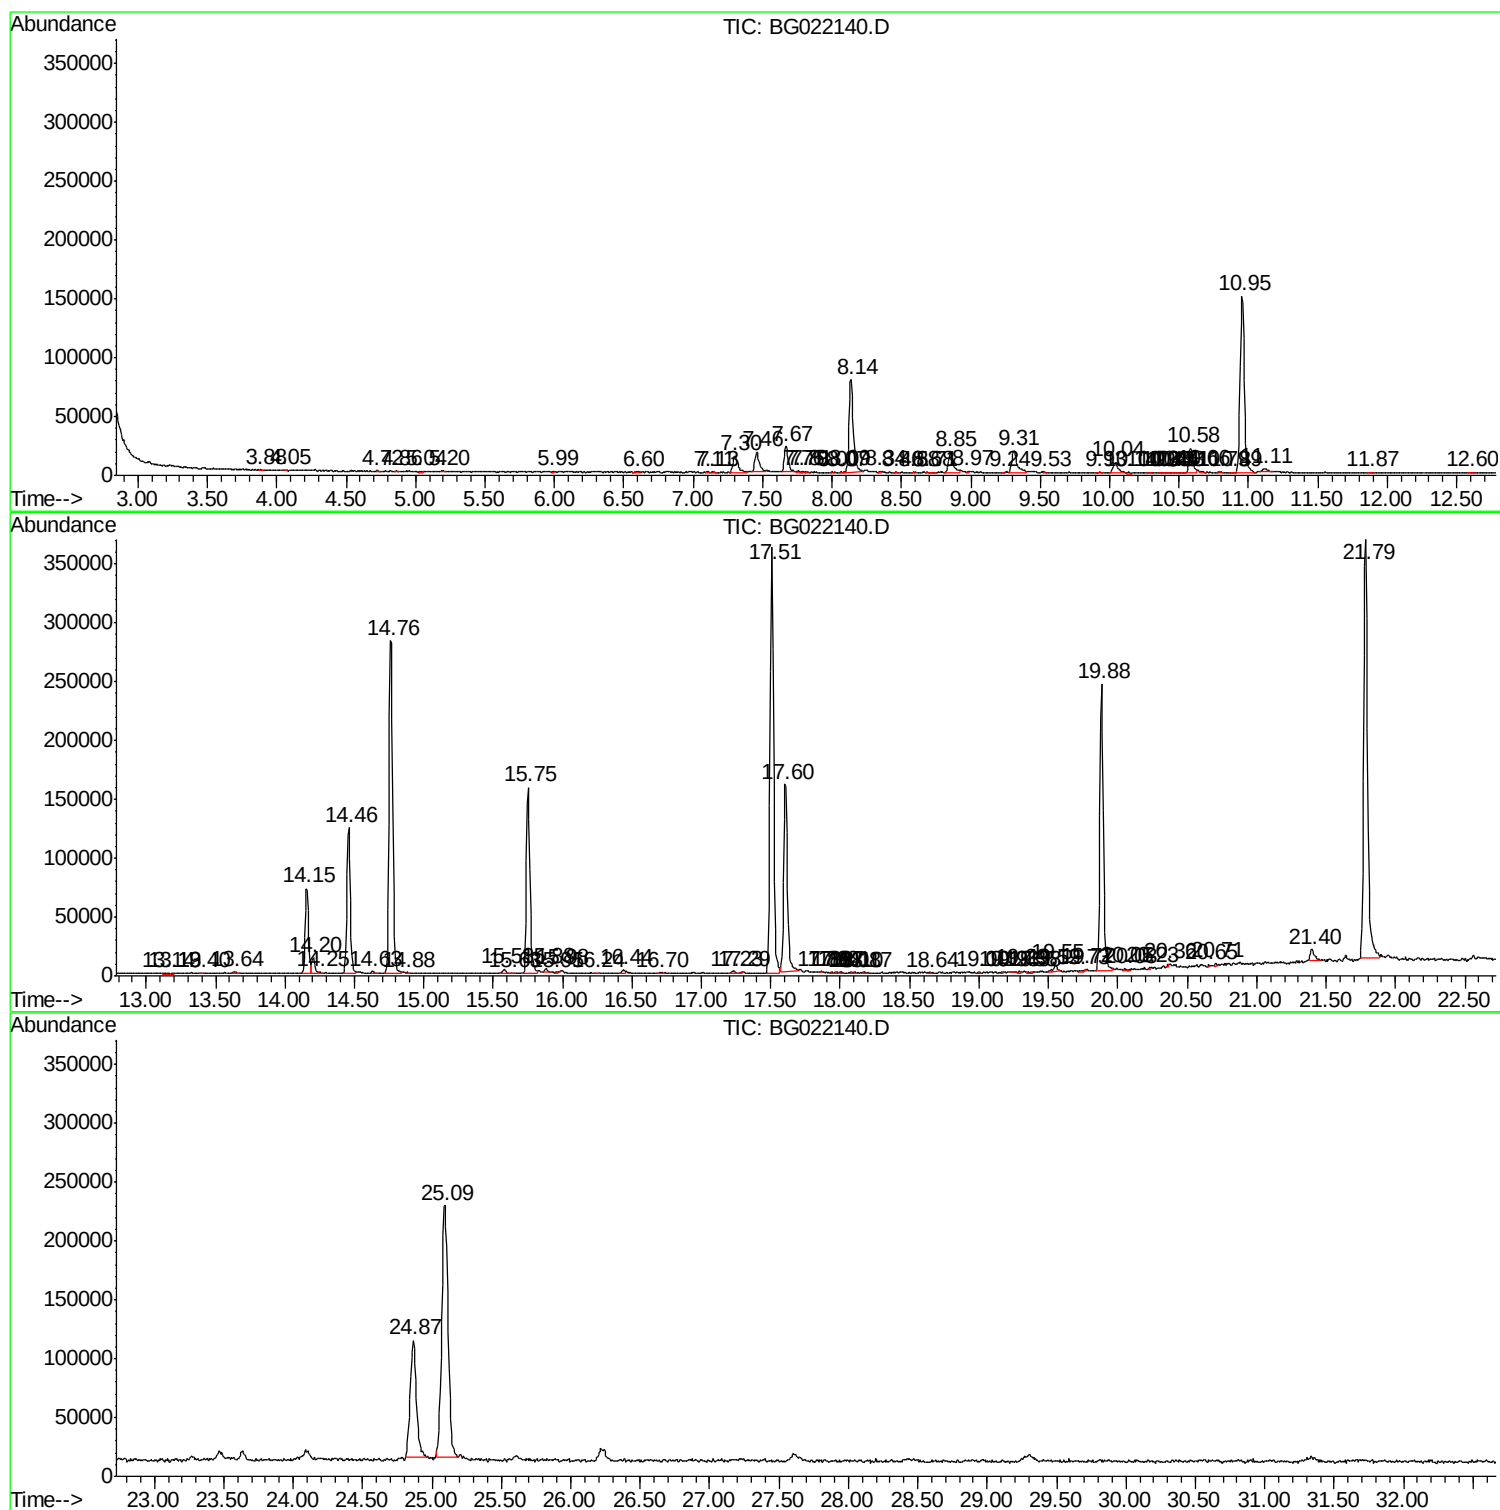

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG060116\
Data File : BG022140.D
Acq On : 1 Jun 2016 13:56
Operator : UM/SJ
Sample : H3254-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BCZH8

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG052116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG060116\
Data File : BG022140.D
Acq On : 1 Jun 2016 13:56
Operator : UM/SJ
Sample : H3254-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BCZH8

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG052116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc