

Data Path : Z:\HPCHEM1\BNA G\DATA\BG060116\
 Data File : BG022141.D
 Acq On : 1 Jun 2016 14:36
 Operator : UM/SJ
 Sample : H3254-05
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BCZM1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG052116.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.185	57	59	66	rVV6	3762	4981	0.43%	0.048%
2	3.502	109	113	117	rBV5	2966	4604	0.40%	0.044%
3	3.790	157	162	165	rBV3	2060	3289	0.29%	0.031%
4	4.266	240	243	248	rBV4	1598	2959	0.26%	0.028%
5	5.458	443	446	452	rVB2	772	1394	0.12%	0.013%
6	7.297	752	759	772	rBV	75541	163974	14.25%	1.570%
7	7.450	779	785	799	rBV	70732	141358	12.28%	1.353%
8	7.662	815	821	836	rVB	91583	188792	16.40%	1.807%
9	8.132	890	901	915	rBV	86075	183180	15.91%	1.754%
10	8.243	918	920	924	rVB4	1326	1557	0.14%	0.015%
11	8.355	932	939	942	rBV4	1682	2481	0.22%	0.024%
12	8.790	1010	1013	1015	rBV3	1528	1858	0.16%	0.018%
13	8.843	1015	1022	1041	rVV	117583	252939	21.98%	2.421%
14	9.307	1093	1101	1110	rBV	76797	170443	14.81%	1.632%
15	9.677	1160	1164	1166	rBV4	1117	1596	0.14%	0.015%
16	10.030	1217	1224	1233	rBV	61491	136991	11.90%	1.311%
17	10.576	1310	1317	1333	rBV	117700	254639	22.12%	2.438%
18	10.952	1371	1381	1394	rBV	169622	339701	29.51%	3.252%
19	11.093	1397	1405	1425	rBV	96900	246149	21.39%	2.356%
20	11.487	1467	1472	1475	rVV2	853	1513	0.13%	0.014%
21	12.538	1648	1651	1657	rBV4	1269	1928	0.17%	0.018%
22	13.567	1823	1826	1831	rVB4	1770	2926	0.25%	0.028%
23	13.643	1833	1839	1842	rBV3	1545	2603	0.23%	0.025%
24	14.154	1920	1926	1931	rBV	294912	482807	41.95%	4.622%
25	14.201	1931	1934	1942	rVV	50894	82989	7.21%	0.794%
26	14.460	1969	1978	1990	rBV	364274	645828	56.11%	6.183%
27	14.536	1990	1991	1994	rVV3	1585	1562	0.14%	0.015%
28	14.565	1994	1996	1999	rVV2	1402	1836	0.16%	0.018%
29	14.636	2003	2008	2012	rVB4	4109	6704	0.58%	0.064%
30	14.765	2022	2030	2039	rBV2	292080	523733	45.50%	5.014%
31	14.983	2060	2067	2081	rBV3	46155	137321	11.93%	1.315%
32	15.312	2121	2123	2128	rBV3	1613	2476	0.22%	0.024%
33	15.459	2145	2148	2150	rBV2	1014	1383	0.12%	0.013%
34	15.488	2150	2153	2156	rVB4	1030	1467	0.13%	0.014%

Data Path : Z:\HPCHEM1\BNA G\DATA\BG060116\
 Data File : BG022141.D
 Acq On : 1 Jun 2016 14:36
 Operator : UM/SJ
 Sample : H3254-05
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BCZM1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG052116.M
 Title : SVOA CALIBRATION

35	15.576	2164	2168	2173	rVB3	9142	13742	1.19%	0.132%
36	15.682	2185	2186	2188	rVV2	1867	1370	0.12%	0.013%
37	15.752	2191	2198	2211	rVV	507829	853401	74.14%	8.170%
38	15.870	2213	2218	2229	rVV	95401	172652	15.00%	1.653%
39	15.987	2231	2238	2248	rVB9	7732	18981	1.65%	0.182%
40	16.128	2258	2262	2268	rBV3	1709	2774	0.24%	0.027%
41	16.205	2273	2275	2277	rVB2	2270	1632	0.14%	0.016%
42	16.275	2281	2287	2293	rBV3	774	1884	0.16%	0.018%
43	16.440	2309	2315	2325	rVV3	9399	21606	1.88%	0.207%
44	16.780	2368	2373	2374	rBV4	1582	1702	0.15%	0.016%
45	17.015	2410	2413	2417	rVB3	1317	1958	0.17%	0.019%
46	17.057	2417	2420	2425	rVB2	1207	1918	0.17%	0.018%
47	17.233	2445	2450	2455	rBV3	5676	8849	0.77%	0.085%
48	17.292	2455	2460	2463	rVV5	2628	5520	0.48%	0.053%
49	17.315	2463	2464	2467	rVB	1671	1365	0.12%	0.013%
50	17.368	2470	2473	2475	rBV	1346	1868	0.16%	0.018%
51	17.509	2490	2497	2507	rBV2	382224	661127	57.44%	6.329%
52	17.603	2507	2513	2526	rVV	526715	911400	79.18%	8.725%
53	17.762	2539	2540	2545	rVB4	2122	1974	0.17%	0.019%
54	17.967	2573	2575	2579	rVB3	2005	2373	0.21%	0.023%
55	18.208	2612	2616	2618	rVB4	1615	1667	0.14%	0.016%
56	18.238	2618	2621	2623	rBV2	1188	1877	0.16%	0.018%
57	18.443	2651	2656	2660	rVB3	1538	2060	0.18%	0.020%
58	18.796	2714	2716	2719	rBV3	1460	1367	0.12%	0.013%
59	19.272	2794	2797	2798	rBV3	1552	1979	0.17%	0.019%
60	19.348	2808	2810	2814	rVB5	2479	2255	0.20%	0.022%
61	19.401	2814	2819	2820	rBV4	1922	2907	0.25%	0.028%
62	19.466	2828	2830	2833	rVB4	1926	2054	0.18%	0.020%
63	19.518	2835	2839	2842	rBV2	7442	11460	1.00%	0.110%
64	19.771	2878	2882	2886	rBV2	4625	7372	0.64%	0.071%
65	19.883	2891	2901	2914	rBV	713707	1151013	100.00%	11.019%
66	20.077	2932	2934	2935	rBV2	2220	1525	0.13%	0.015%
67	20.218	2956	2958	2960	rBV3	2023	1802	0.16%	0.017%
68	20.347	2978	2980	2981	rVB2	2206	1366	0.12%	0.013%
69	20.376	2984	2985	2987	rBV3	2692	1341	0.12%	0.013%
70	20.688	3036	3038	3039	rBV2	3018	2867	0.25%	0.027%
71	20.752	3046	3049	3052	rBV5	3403	4557	0.40%	0.044%

Data Path : Z:\HPCHEM1\BNA G\DATA\BG060116\
 Data File : BG022141.D
 Acq On : 1 Jun 2016 14:36
 Operator : UM/SJ
 Sample : H3254-05
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BCZM1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG052116.M
 Title : SVOA CALIBRATION

72	20.817	3058	3060	3063	rBV4	2374	3257	0.28%	0.031%
73	20.999	3088	3091	3094	rBV5	3854	5361	0.47%	0.051%
74	21.399	3154	3159	3168	rBV8	14706	37667	3.27%	0.361%
75	21.786	3217	3225	3238	rBV	393054	752184	65.35%	7.201%
76	23.255	3473	3475	3477	rBV3	4409	3518	0.31%	0.034%
77	24.536	3692	3693	3696	rBV3	3721	1968	0.17%	0.019%
78	24.865	3738	3749	3767	rBV3	286185	949510	82.49%	9.090%
79	25.100	3777	3789	3801	rVB2	222845	717065	62.30%	6.865%
80	26.851	4085	4087	4088	rBV2	2808	1792	0.16%	0.017%
81	26.869	4088	4090	4092	rBV3	2579	1994	0.17%	0.019%
82	28.314	4334	4336	4337	rBV2	2604	1932	0.17%	0.018%
83	28.555	4375	4377	4378	rBV3	2097	1381	0.12%	0.013%
84	28.602	4383	4385	4386	rBV2	2316	1576	0.14%	0.015%
85	28.661	4393	4395	4399	rVB5	2924	2344	0.20%	0.022%
86	29.031	4449	4458	4459	rBV8	22879	43721	3.80%	0.419%
87	29.248	4493	4495	4499	rBV4	3042	5473	0.48%	0.052%
88	30.077	4634	4636	4638	rVB3	3202	1970	0.17%	0.019%
89	30.112	4640	4642	4644	rBV3	2764	2924	0.25%	0.028%
90	30.482	4703	4705	4706	rBV2	2320	1807	0.16%	0.017%
91	30.535	4713	4714	4716	rBV2	2125	1873	0.16%	0.018%
92	31.246	4833	4835	4836	rBV2	2007	1692	0.15%	0.016%
93	31.446	4867	4869	4870	rBV	2845	1620	0.14%	0.016%
94	31.604	4892	4896	4897	rBV3	2901	3640	0.32%	0.035%
95	31.857	4937	4939	4940	rBV2	2714	1664	0.14%	0.016%
96	31.898	4944	4946	4948	rBV3	2223	1638	0.14%	0.016%
97	32.174	4992	4993	4995	rBV2	3098	2447	0.21%	0.023%
98	32.198	4995	4997	4999	rVB3	2331	2232	0.19%	0.021%
99	32.262	5007	5008	5010	rBV2	2497	2287	0.20%	0.022%
100	32.591	5062	5064	5067	rBV4	2102	1898	0.16%	0.018%


Sum of corrected areas: 10445961

Data Path : Z:\HPCHEM1\BNA G\DATA\BG060116\
Data File : BG022141.D
Acq On : 1 Jun 2016 14:36
Operator : UM/SJ
Sample : H3254-05
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BCZM1

Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG052116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

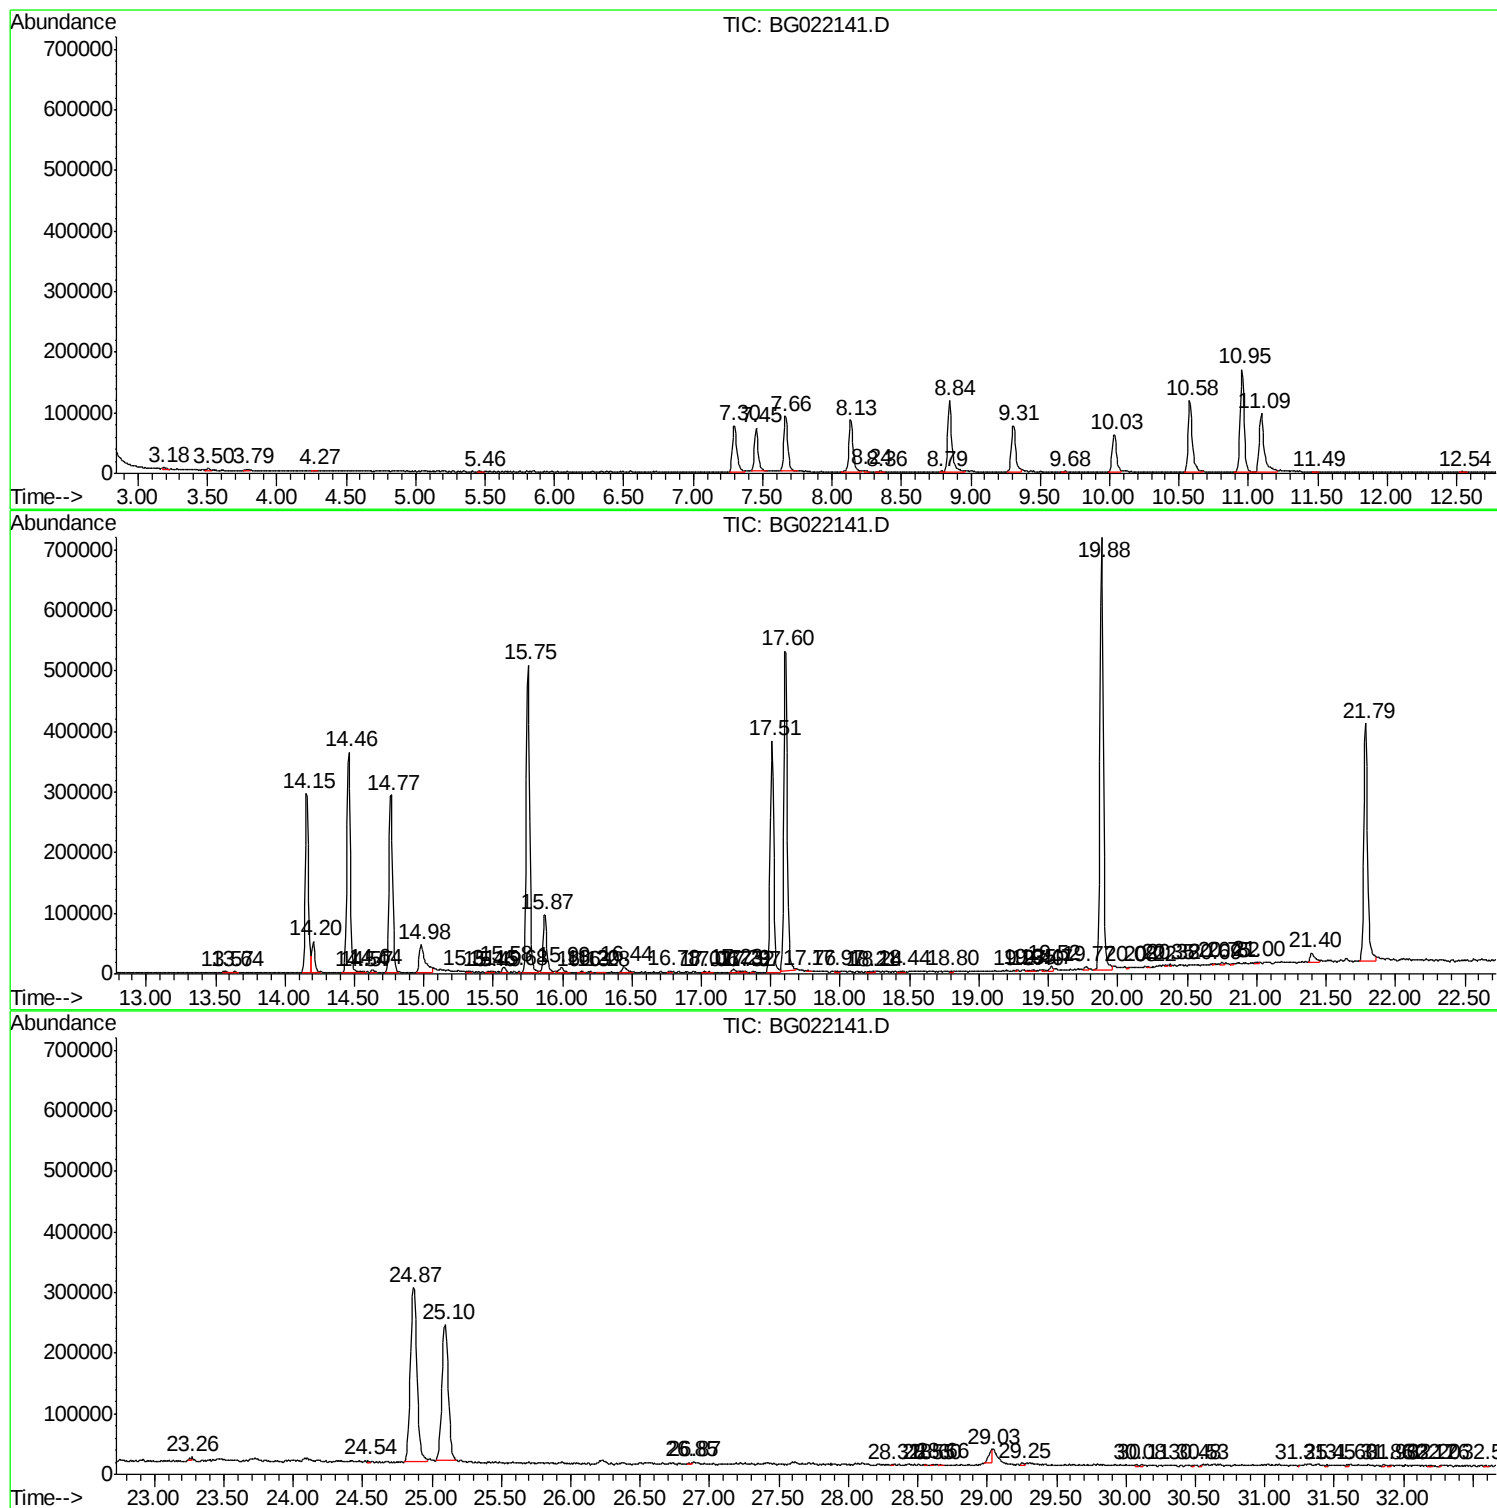

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG060116\
Data File : BG022141.D
Acq On : 1 Jun 2016 14:36
Operator : UM/SJ
Sample : H3254-05
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BCZM1

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG052116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG060116\
Data File : BG022141.D
Acq On : 1 Jun 2016 14:36
Operator : UM/SJ
Sample : H3254-05
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BCZM1

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG052116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc