
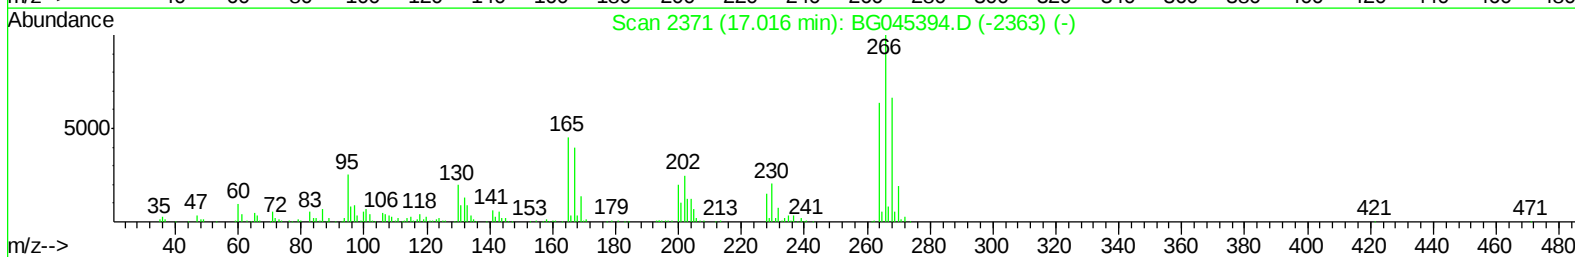
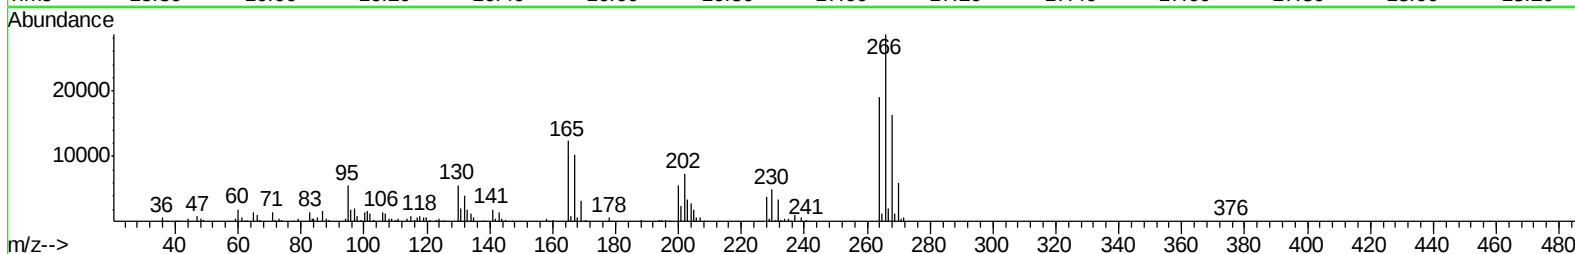


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG060120\
 Data File : BG045553.D
 Acq On : 1 Jun 2020 12:38
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 02 02:31:57 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG051520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 01 15:07:00 2020
 Response via : Initial Calibration

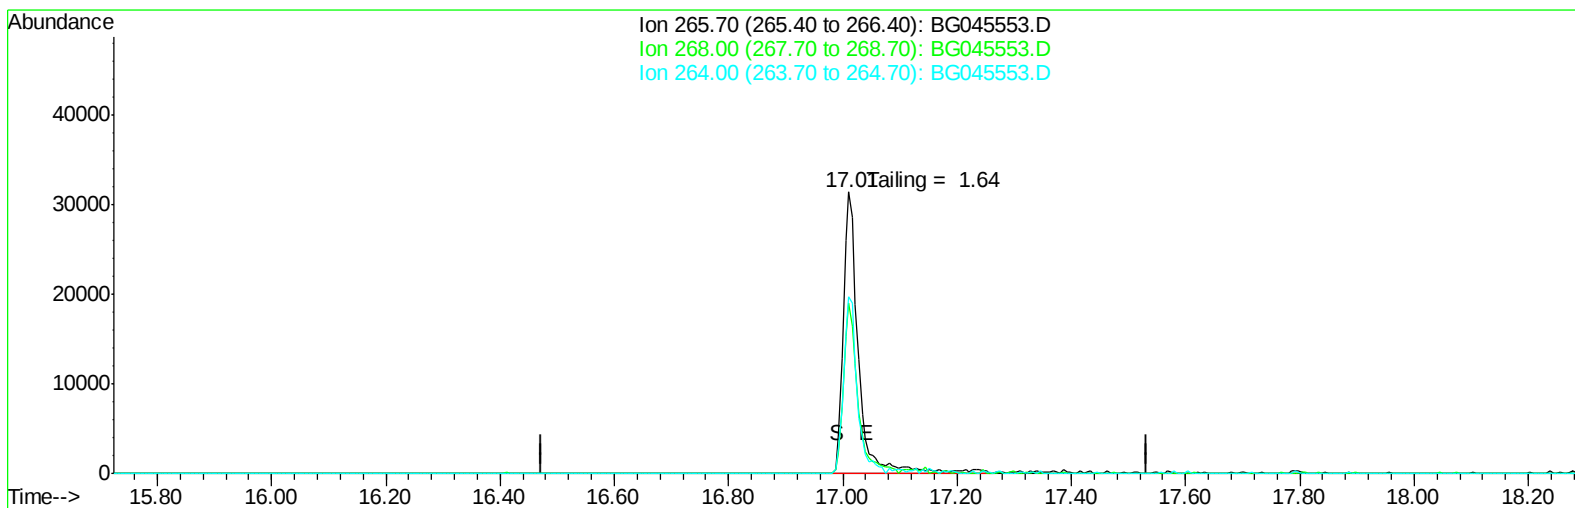

TIC: BG045553.D

(70) Pentachlorophenol (C)




17.004min (-17.004) 0.00ng

response 0

Ion	Exp%	Act%
265.70	100	0.00
268.00	66.50	0.00#
264.00	63.70	0.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG060120\
 Data File : BG045553.D
 Acq On : 1 Jun 2020 12:38
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 02 02:31:57 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG051520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 01 15:07:00 2020
 Response via : Initial Calibration

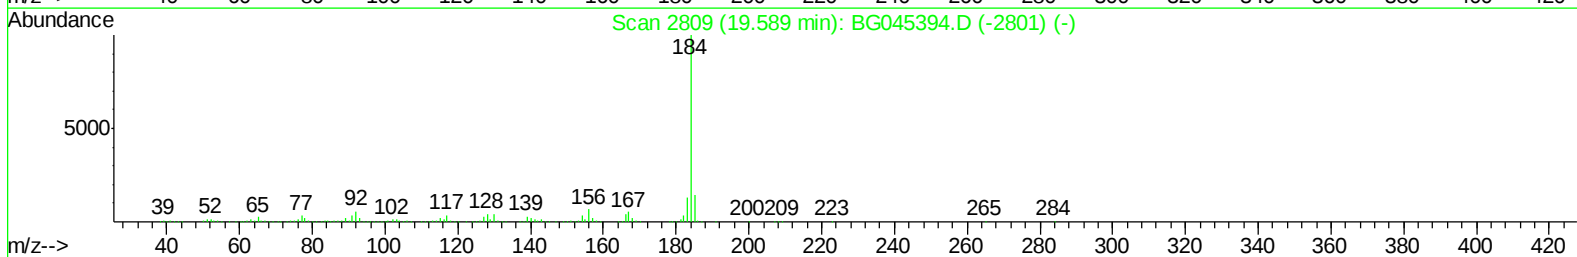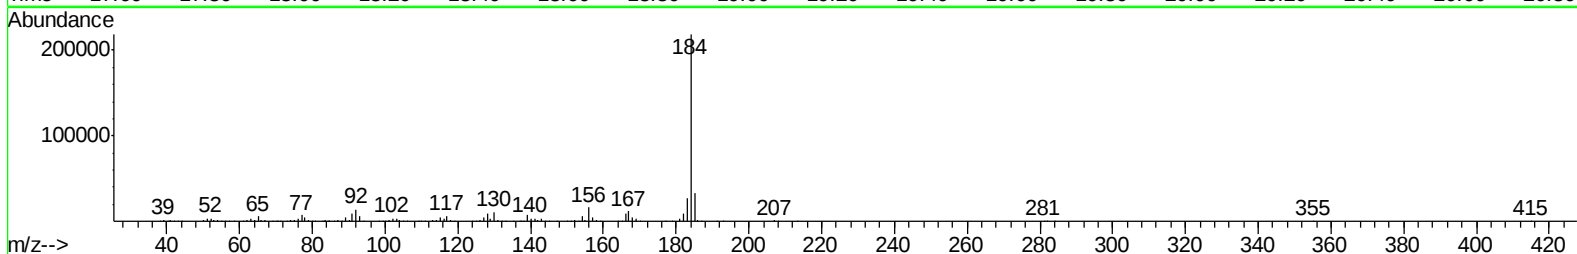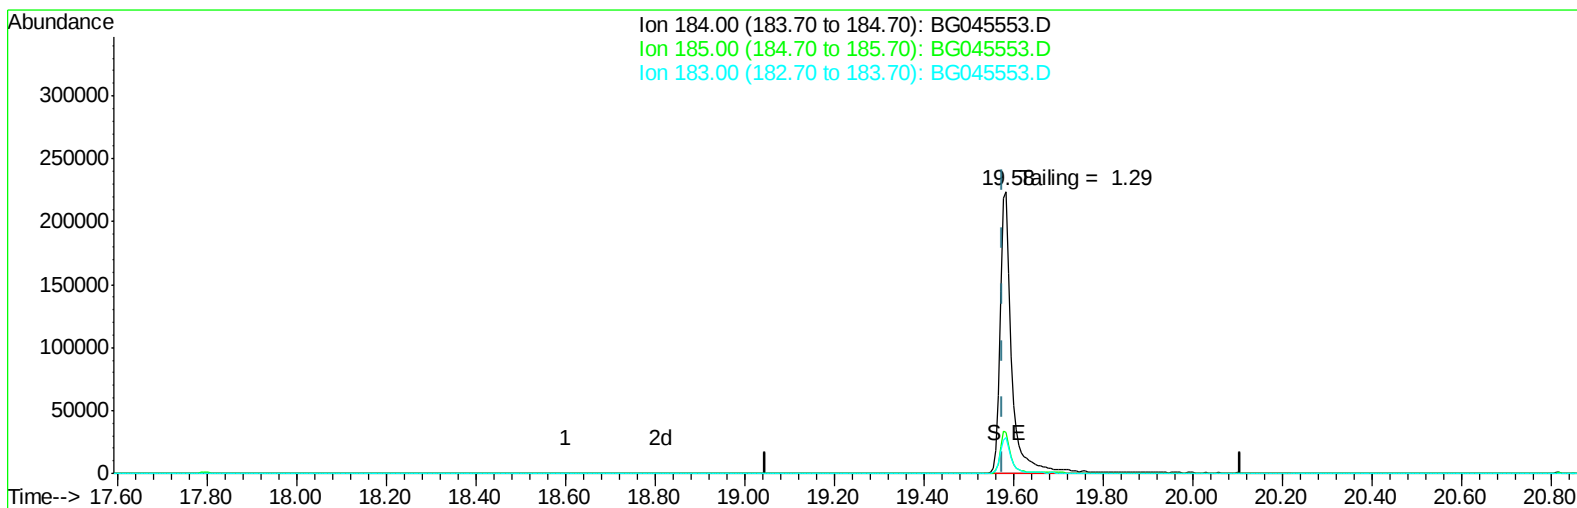

TIC: BG045553.D

(77) Benzidine

18.602min (-0.974) 5.99ng

response 57

Ion	Exp%	Act%
184.00	100	100
185.00	14.60	0.00#
183.00	12.80	0.00#
0.00	0.00	0.00