


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060120\
 Data File : BG045553.D
 Acq On : 1 Jun 2020 12:38
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG051520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 01 15:07:00 2020

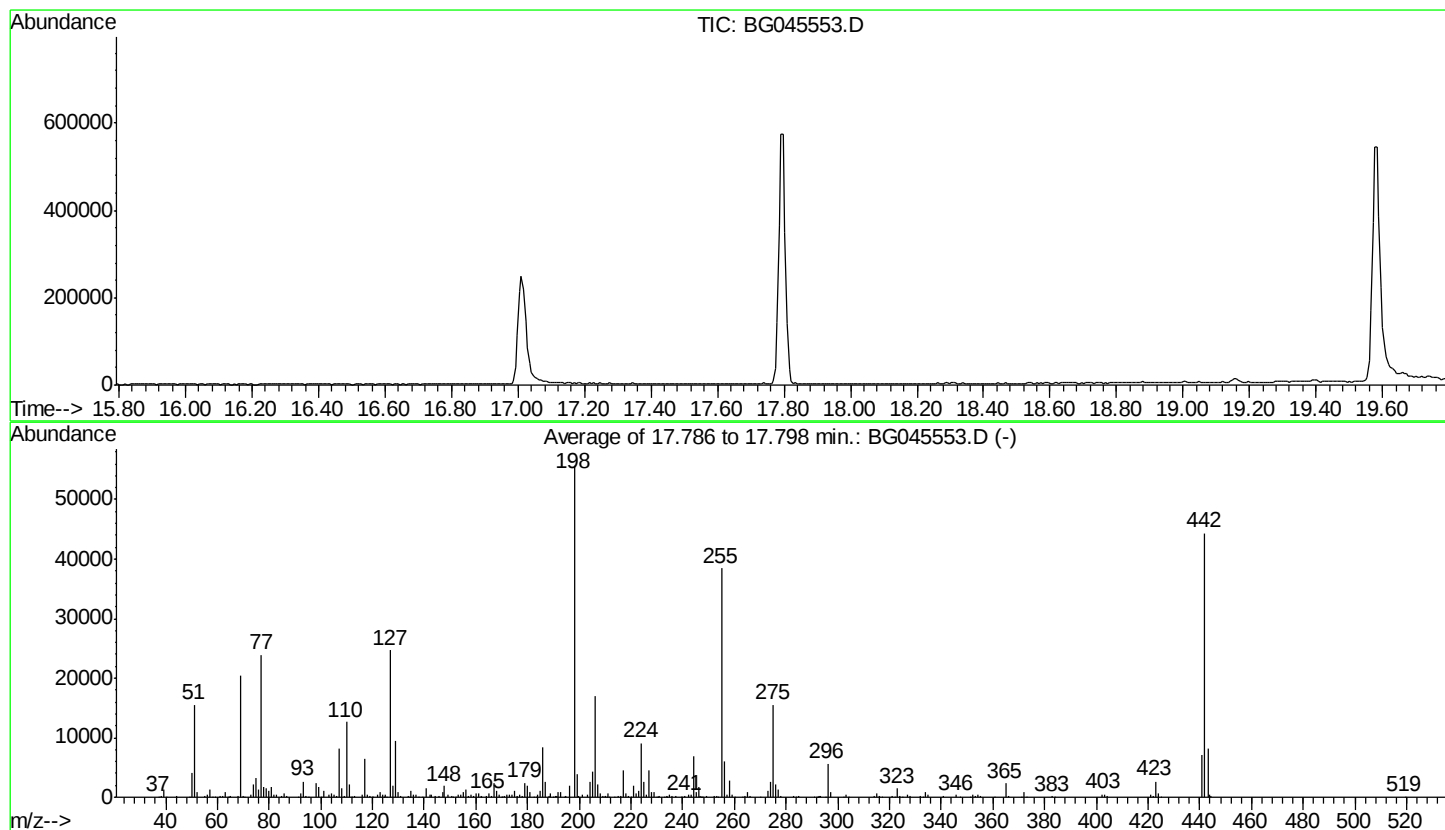

AutoFind: Scans 2502, 2503, 2504; Background Corrected with Scan 2496

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.9	15566	PASS
68	69	0.00	2	1.6	327	PASS
69	198	0.00	100	36.7	20424	PASS
70	69	0.00	2	0.7	133	PASS
127	198	10	80	44.3	24658	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	55698	PASS
199	198	5	9	6.9	3862	PASS
275	198	10	60	27.9	15544	PASS
365	198	1	100	4.2	2320	PASS
441	198	0.01	100	12.6	7041	PASS
442	198	50	100	79.6	44357	PASS
443	442	15	24	18.5	8227	PASS