

Data Path : Z:\HPCHEM1\BNA G\DATA\BG060216\
 Data File : BG022149.D
 Acq On : 2 Jun 2016 12:08
 Operator : UM/SJ
 Sample : H3302-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 CB199

Manual Integrations
 APPROVED

umangi
 6/3/2016 4:54:50 PM

Quant Time: Jun 03 11:03:39 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG052116.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 03 01:08:24 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.13	152	39488	20.00	ng/ul	0.00
18) Naphthalene-d8	10.95	136	219584	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.76	164	137157	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.51	188	286619	20.00	ng/ul	0.00
75) Chrysene-d12	21.78	240	267376	20.00	ng/ul	0.00
83) Perylene-d12	25.09	264	255132	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.50	96	725	0.96	ng/uL	0.00
5) Phenol-d5	7.29	99	33422	9.37	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.45	67	16890	9.03	ng/ul	0.00
9) 2-Chlorophenol-d4	7.66	132	31298	10.49	ng/ul	0.00
13) 4-Methylphenol-d8	8.84	113	24766	8.18	ng/ul	0.00
19) Nitrobenzene-d5	9.31	128	15136	9.35	ng/ul	0.00
22) 2-Nitrophenol-d4	10.04	143	15633	8.91	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.58	165	31171	10.07	ng/ul	0.00
29) 4-Chloroaniline-d4	11.10	131	21901	6.50	ng/ul	0.00
43) Dimethylphthalate-d6	14.16	166	122083	11.85	ng/ul	0.00
46) Acenaphthylene-d8	14.46	160	161567	11.23	ng/ul	0.00
51) 4-Nitrophenol-d4	15.01	143	6537m	3.68	ng/ul	0.03
57) Fluorene-d10	15.75	176	111337	11.54	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.87	200	6857	4.58	ng/ul	0.00
70) Anthracene-d10	17.61	188	151837	11.04	ng/ul	0.00
76) Pyrene-d10	19.88	212	163206	10.82	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.86	264	136442	11.53	ng/ul	0.00

Target Compounds

						Ovalue
44) Dimethylphthalate	14.20	163	26848	2.59	ng/ul	97
69) Phenanthrene	17.55	178	26334	1.65	ng/ul	98
74) Fluoranthene	19.55	202	103102	6.33	ng/ul	98
77) Pyrene	19.91	202	98070	5.21	ng/ul	99
80) Benzo(a)anthracene	21.77	228	64714	4.13	ng/ul	94
82) Chrysene	21.83	228	65271	4.34	ng/ul	96
85) Benzo(b)fluoranthene	24.04	252	110007	7.37	ng/ul	98
86) Benzo(k)fluoranthene	24.10	252	30868m	2.12	ng/ul	
88) Benzo(a)pyrene	24.93	252	66817	4.64	ng/ul	93
89) Indeno(1,2,3-cd)pyrene	28.88	276	57381m	3.47	ng/ul	
90) Dibenzo(a,h)anthracene	28.92	278	14960m	1.08	ng/ul	
91) Benzo(g,h,i)perylene	30.06	276	50746m	3.84	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA G\DATA\BG060216\
Data File : BG022149.D
Acq On : 2 Jun 2016 12:08
Operator : UM/SJ
Sample : H3302-01
Misc :
ALS Vial : 4 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampled :
CB199

Manual Integrations
APPROVED

umangi
6/3/2016 4:54:50 PM

Quant Time: Jun 03 11:03:39 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG052116.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 03 01:08:24 2016
Response via : Initial Calibration

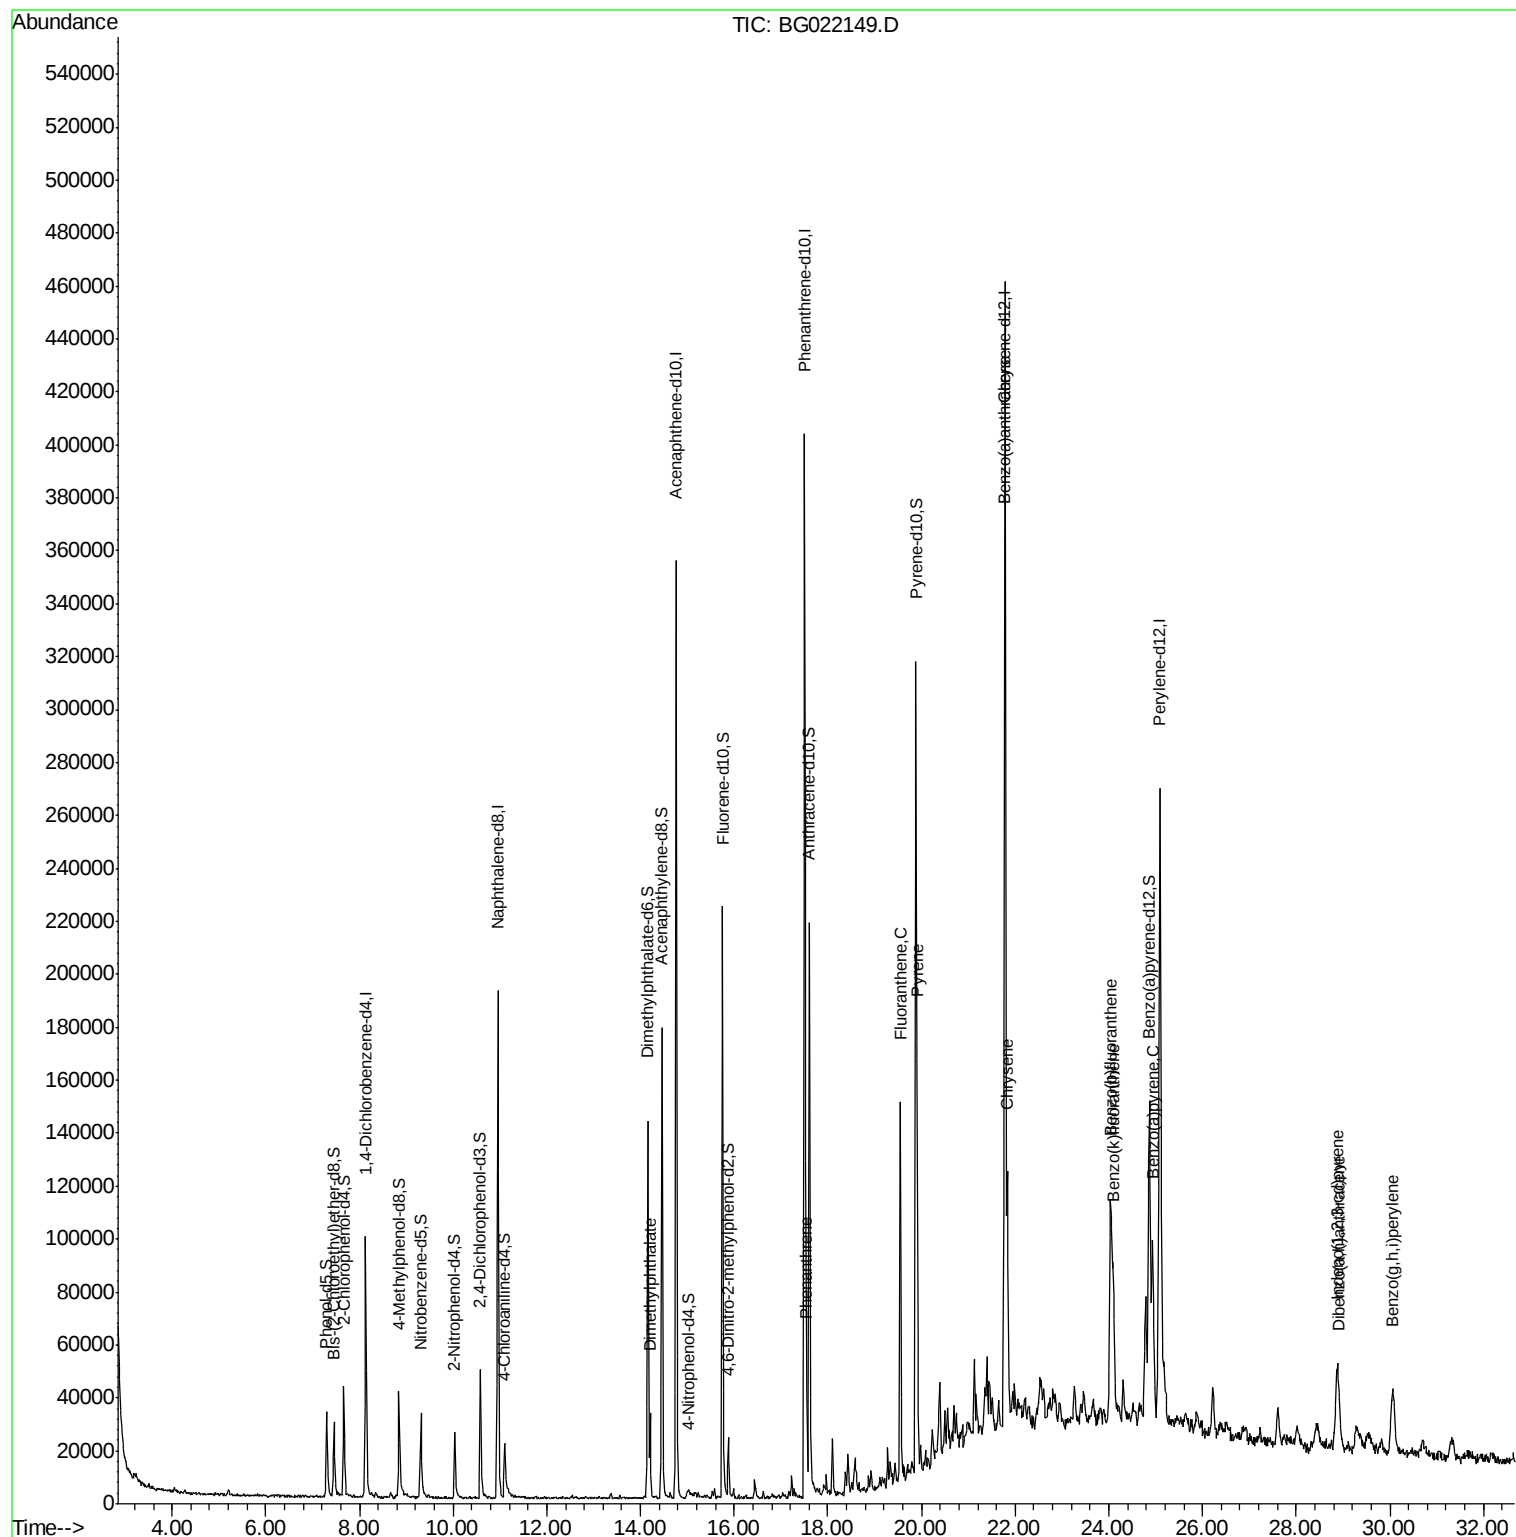

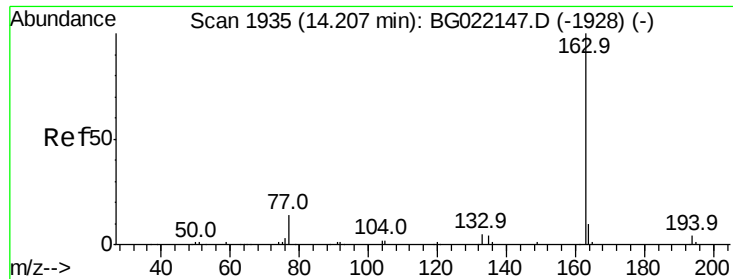

#44

Dimethylphthalate

Concen: 2.59 ng/ul

RT: 14.20 min Scan# 1934

Delta R.T. -0.00 min

Lab File: BG022149.D

Acq: 2 Jun 2016 12:08

Instrument :

BNA_G





ClientSampled :

CB199

Tot Ion:	163	Resp:	26848
Ion Ratio	Lower	Upper	
163	100		
194	4.6	3.4	5.2
164	9.8	8.8	13.2

Manual Integrations
APPROVED

umangi
6/3/2016 4:54:50 PM

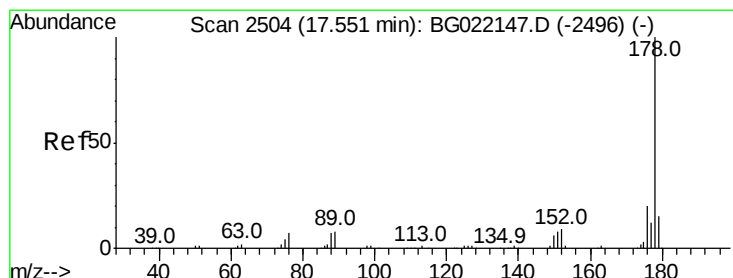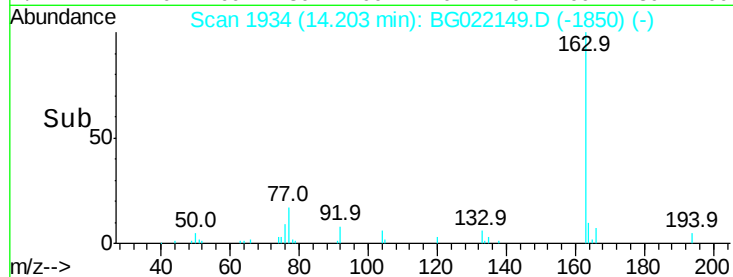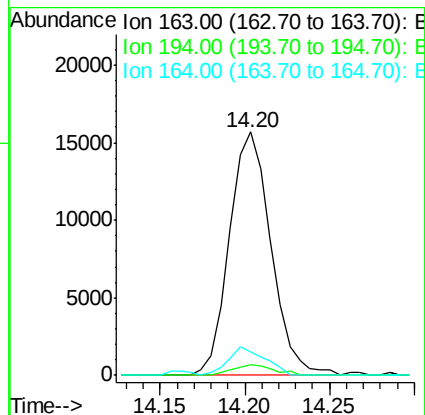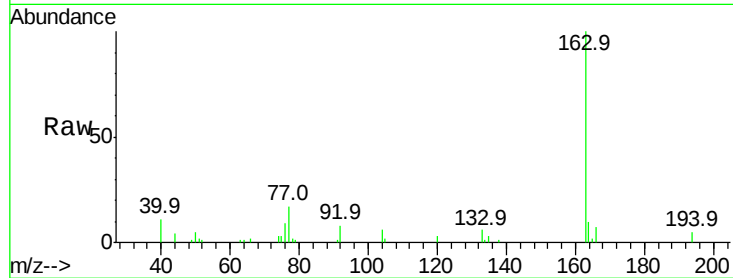

#69

Phenanthrene

Concen: 1.65 ng/ul




RT: 17.55 min Scan# 2503


Delta R.T. -0.00 min

Lab File: BG022149.D

Acq: 2 Jun 2016 12:08

Tgt Ion:	178	Resp:	26334
Ion Ratio	Lower	Upper	
178	100		
179	15.7	12.9	19.3
176	21.2	15.8	23.8

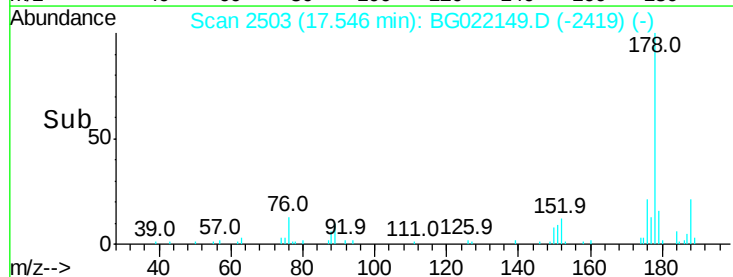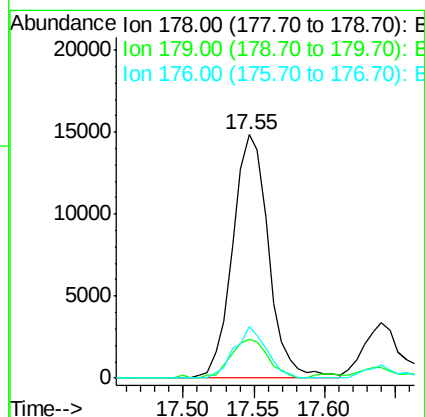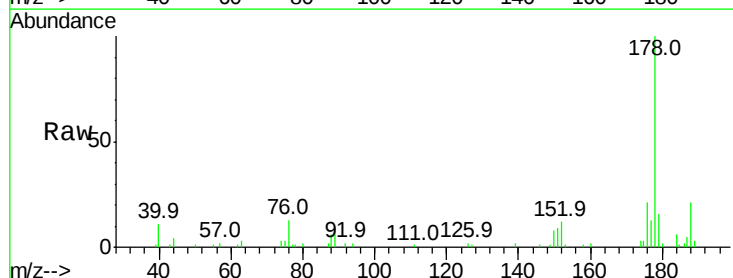

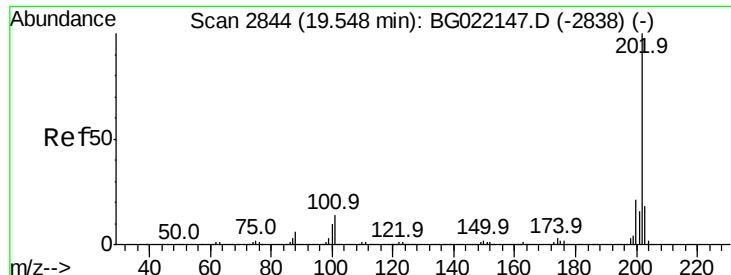

#74

Fluoranthene

Concen: 6.33 ng/ul

RT: 19.55 min Scan# 2844

Delta R.T. 0.00 min

Lab File: BG022149.D

Acq: 2 Jun 2016 12:08

Instrument :

BNA_G





ClientSampleId :

CB199

Tot Ion:	202	Resp:	103102
Ion Ratio	Lower	Upper	
202	100		
101	12.5	10.6	16.0
100	9.9	8.7	13.1

Manual Integrations
APPROVED

umangi
6/3/2016 4:54:50 PM

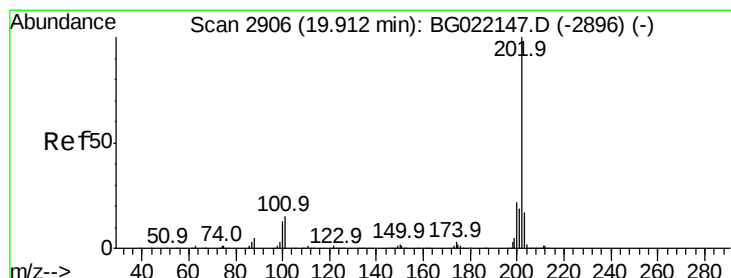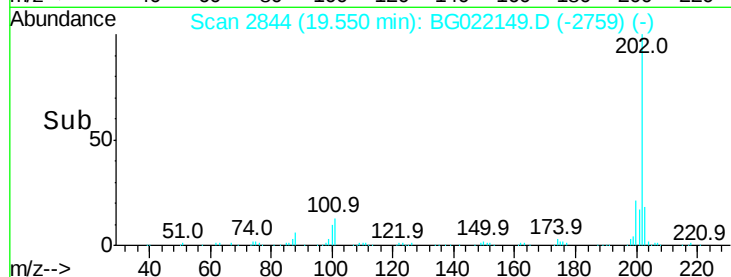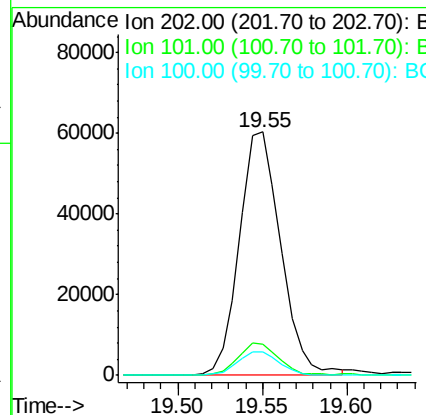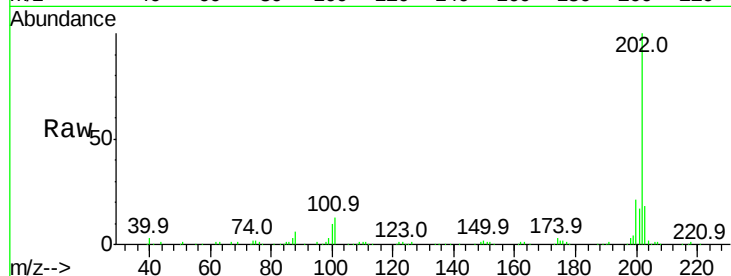

#77

Pyrene

Concen: 5.21 ng/ul




RT: 19.91 min Scan# 2905


Delta R.T. -0.00 min

Lab File: BG022149.D

Acq: 2 Jun 2016 12:08

Tgt Ion:	202	Resp:	98070
Ion Ratio	Lower	Upper	
202	100		
101	15.4	12.5	18.7
100	12.3	10.2	15.4

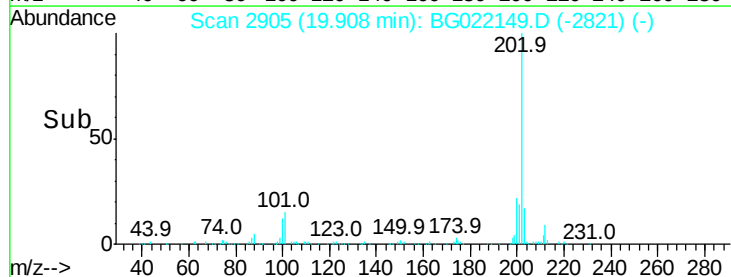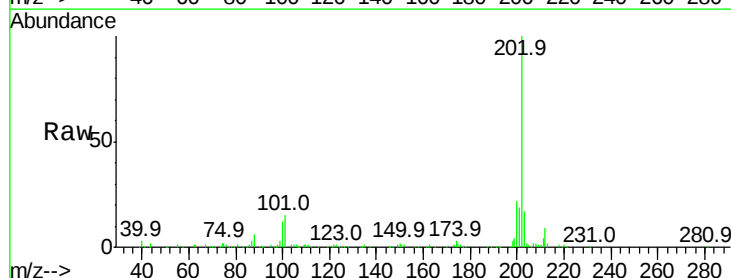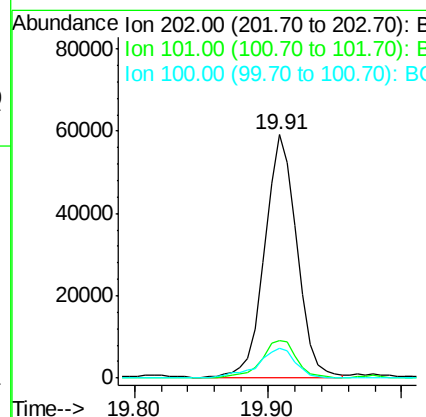

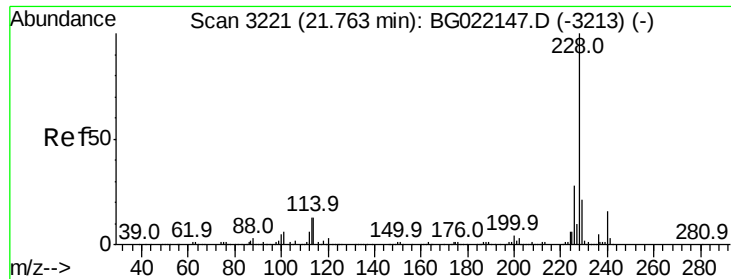





#80
Benzo(a)anthracene
Concen: 4.13 ng/ul
RT: 21.77 min Scan# 3221
Delta R.T. 0.00 min
Lab File: BG022149.D
Acq: 2 Jun 2016 12:08

Instrument :
BNA_G
ClientSampleId :
CB199

Tot Ion	Ratio	Lower	Upper
228	100		
229	23.0	15.4	23.2
226	30.9	22.8	34.2




Manual Integrations
APPROVED


umangi
6/3/2016 4:54:50 PM

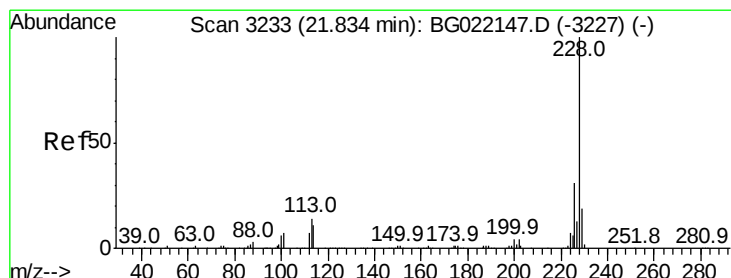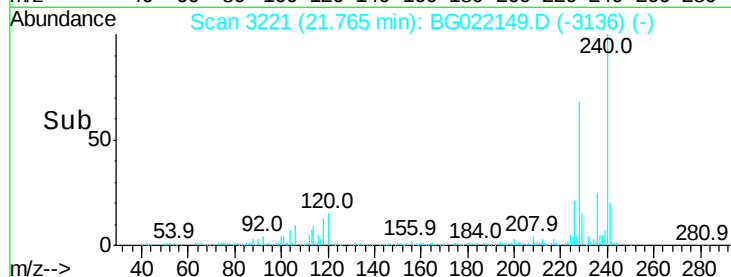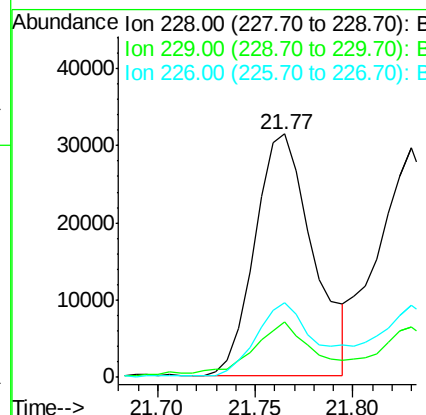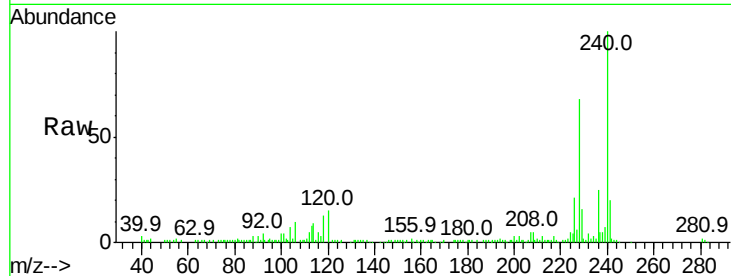

#82
Chrysene
Concen: 4.34 ng/ul
RT: 21.83 min Scan# 3232
Delta R.T. -0.00 min
Lab File: BG022149.D
Acq: 2 Jun 2016 12:08

Tgt Ion	Ratio	Lower	Upper
228	100		
226	31.1	24.2	36.4
229	22.1	15.0	22.6

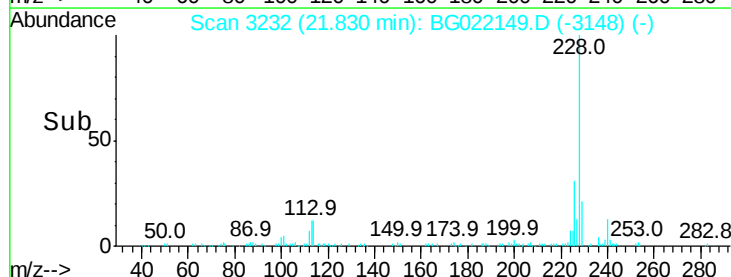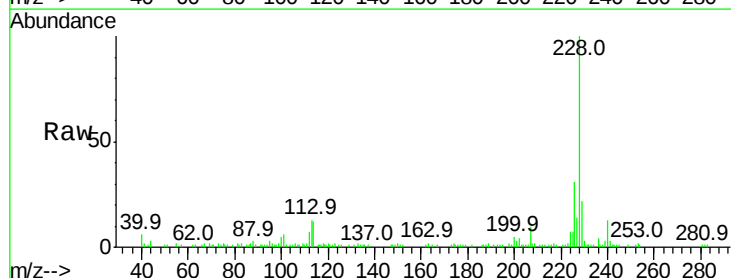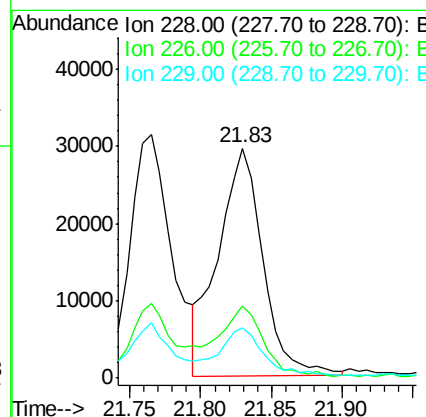

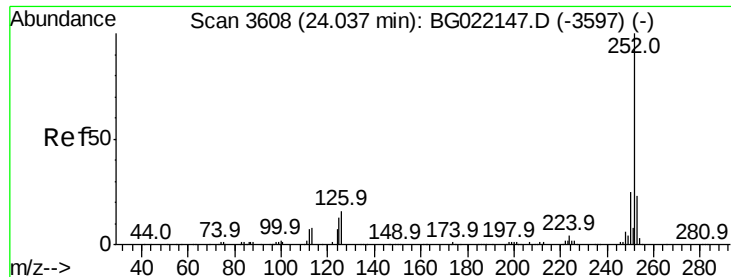

#85

Benzo(b)fluoranthene

Concen: 7.37 ng/ul

RT: 24.04 min Scan# 3608

Delta R.T. 0.00 min

Lab File: BG022149.D

Acq: 2 Jun 2016 12:08

Instrument :

BNA_G





ClientSampleId :

CB199

Tot Ion	Ratio	Lower	Upper
252	100		
253	22.1	18.2	27.2
125	15.3	10.8	16.2

Manual Integrations
APPROVED

umangi
6/3/2016 4:54:50 PM

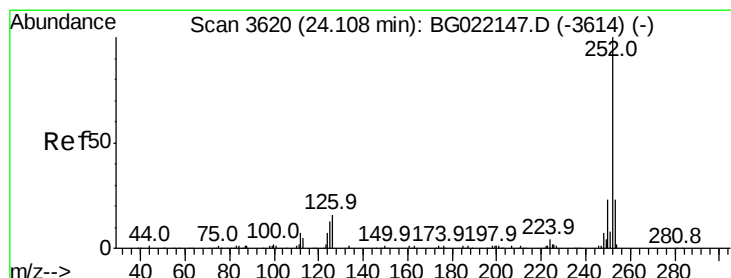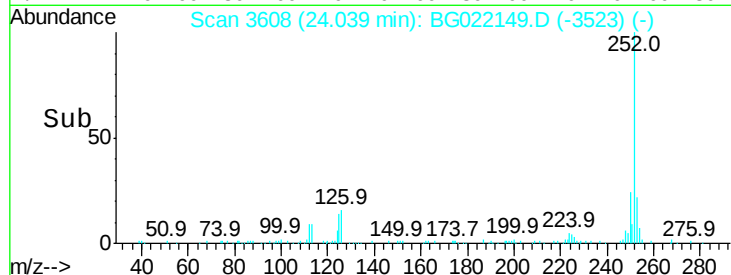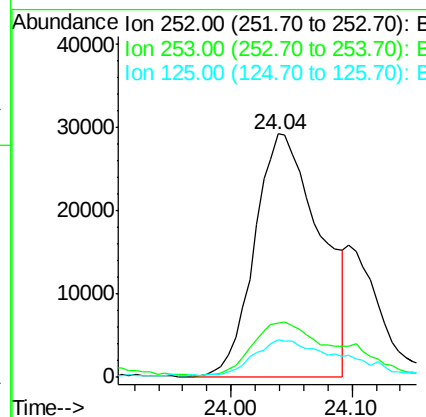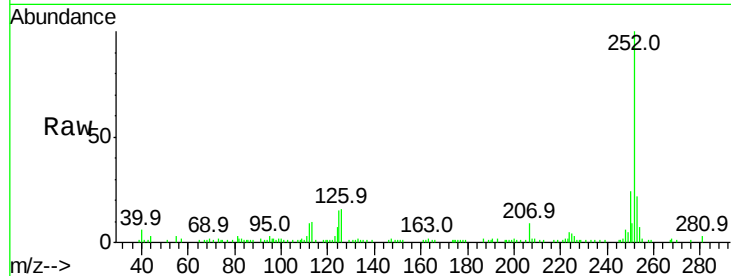

#86

Benzo(k)fluoranthene

Concen: 2.12 ng/ul m




RT: 24.10 min Scan# 3618


Delta R.T. -0.01 min

Lab File: BG022149.D

Acq: 2 Jun 2016 12:08

Tgt Ion	Ratio	Lower	Upper
252	100		
253	23.4	15.8	23.6
125	17.2	10.6	16.0#

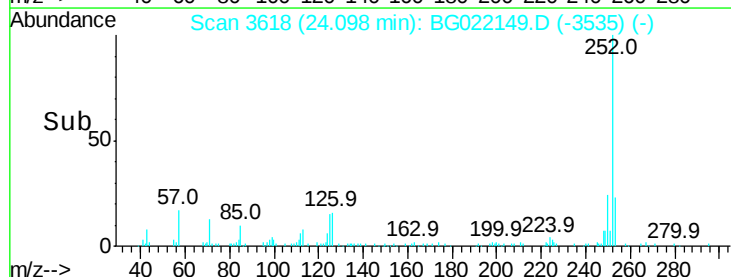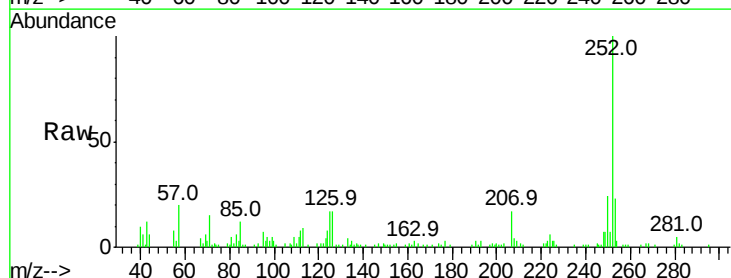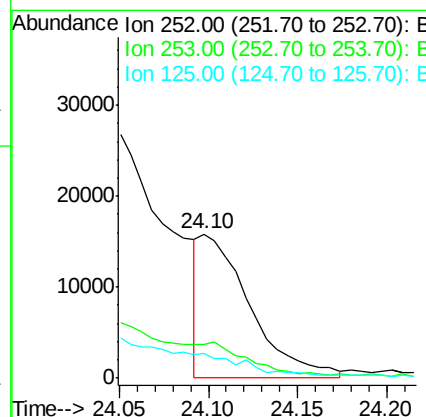

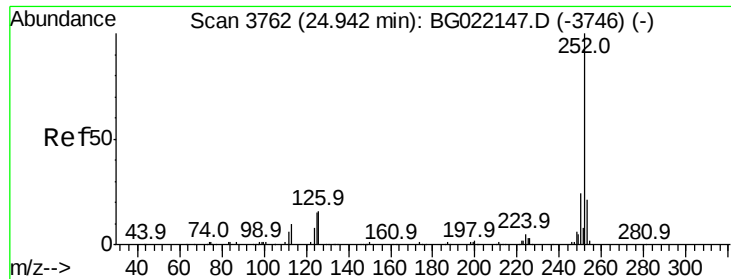





#88
Benzo(a)pyrene
Concen: 4.64 ng/ul
RT: 24.93 min Scan# 3760
Delta R.T. -0.01 min
Lab File: BG022149.D
Acq: 2 Jun 2016 12:08

Instrument :
BNA_G
ClientSampleId :
CB199

Tot Ion	Ratio	Lower	Upper
252	100		
253	19.3	19.0	28.4
125	16.2	12.0	18.0




Manual Integrations
APPROVED


umangi
6/3/2016 4:54:50 PM

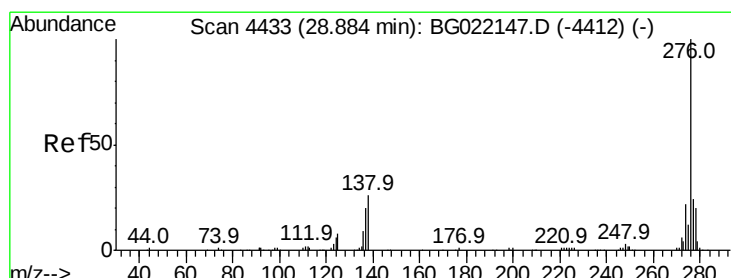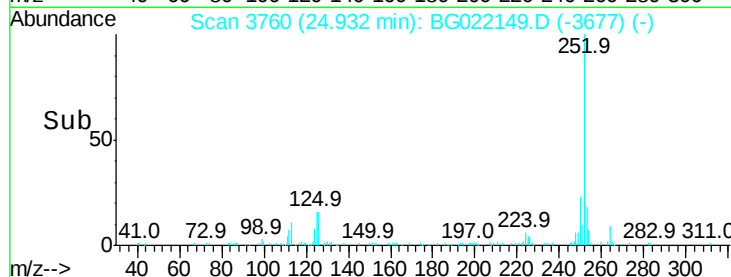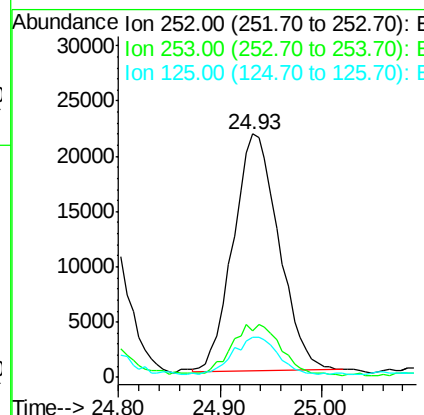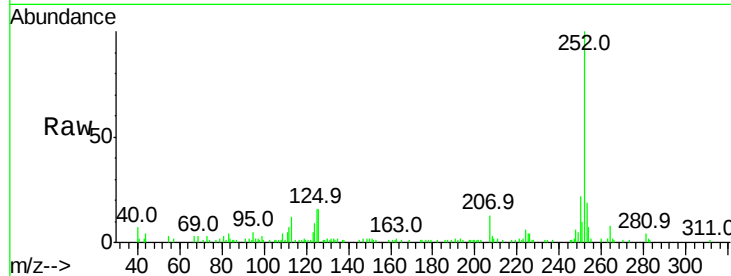

#89
Indeno(1,2,3-cd)pyrene
Concen: 3.47 ng/ul m
RT: 28.88 min Scan# 4432
Delta R.T. -0.00 min
Lab File: BG022149.D
Acq: 2 Jun 2016 12:08

Tgt Ion	Ratio	Lower	Upper
276	100		
138	24.8	20.8	31.2
277	26.1	17.6	26.4

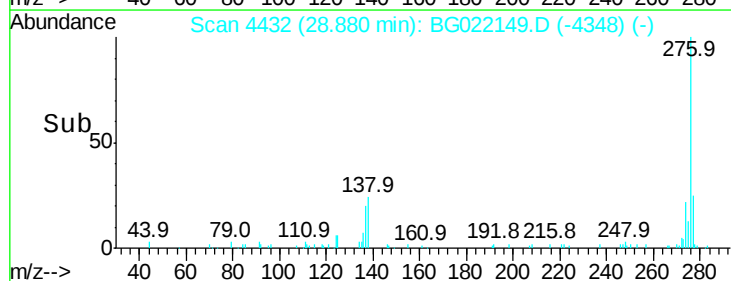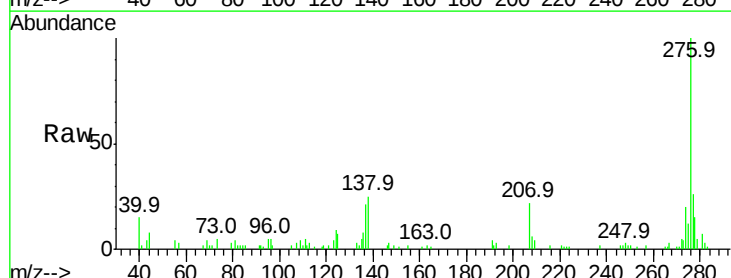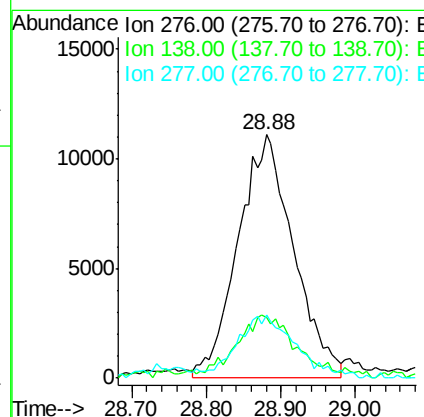

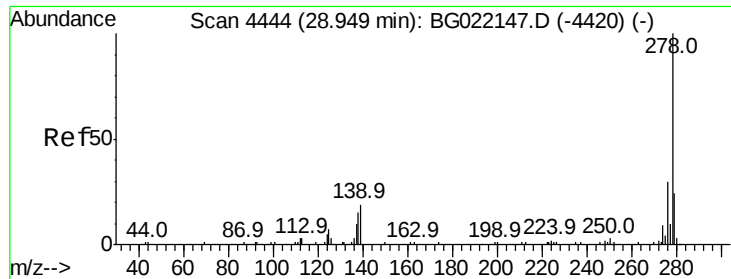





#90
Dibenzo(a,h)anthracene
Concen: 1.08 ng/ul m
RT: 28.92 min Scan# 4439
Delta R.T. -0.03 min
Lab File: BG022149.D
Acq: 2 Jun 2016 12:08

Instrument :
BNA_G
ClientSampleId :
CB199

Tot Ion	Ratio	Lower	Upper
278	100		
139	11.2	16.3	24.5#
279	36.2	19.1	28.7#

Manual Integrations
APPROVED

umangi
6/3/2016 4:54:50 PM

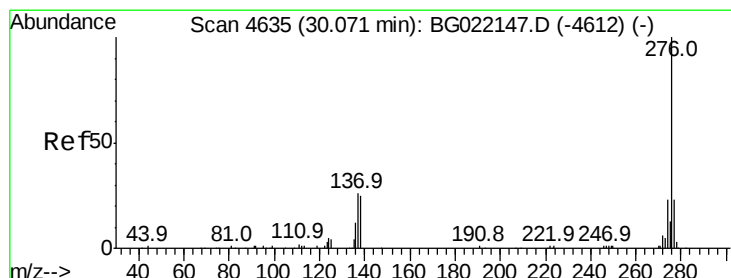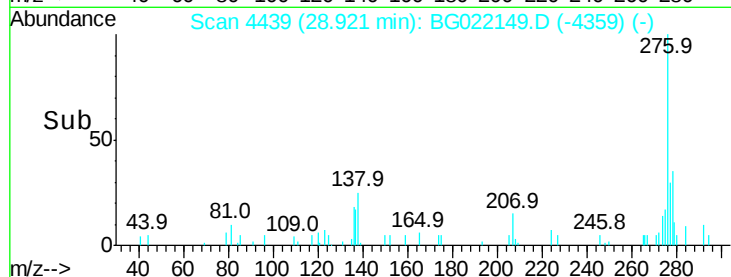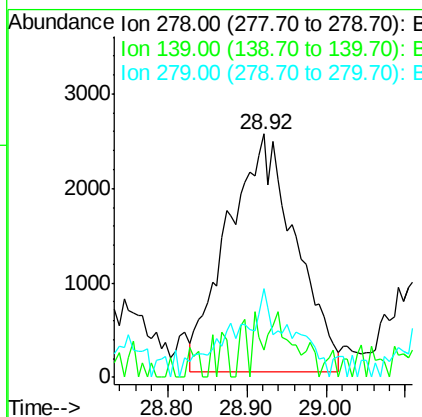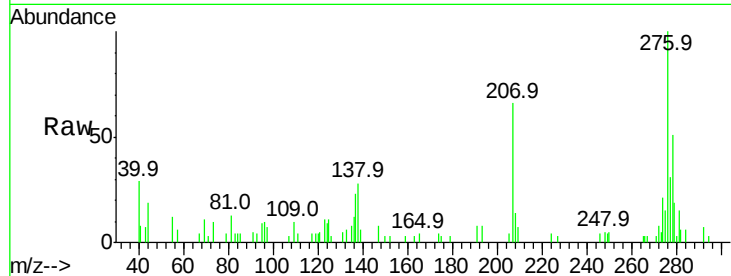

#91
Benzo(g,h,i)perylene
Concen: 3.84 ng/ul m
RT: 30.06 min Scan# 4633
Delta R.T. -0.01 min
Lab File: BG022149.D
Acq: 2 Jun 2016 12:08

Tgt Ion	Ratio	Lower	Upper
276	100		
138	28.6	22.1	33.1
277	28.0	17.0	25.4#

