

Data Path : Z:\HPCHEM1\BNA G\DATA\BG060216\
 Data File : BG022158.D
 Acq On : 2 Jun 2016 18:17
 Operator : UM/SJ
 Sample : H3302-12
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 CB208

Manual Integrations
 APPROVED

umangi
 6/3/2016 4:55:02 PM

Quant Time: Jun 03 02:10:11 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG052116.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 03 01:08:24 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.14	152	59228	20.00	ng/ul	0.00
18) Naphthalene-d8	10.96	136	310460	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.76	164	191244	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.51	188	398634	20.00	ng/ul	0.00
75) Chrysene-d12	21.79	240	360321	20.00	ng/ul	0.00
83) Perylene-d12	25.09	264	345724	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.50	96	1302	1.15	ng/uL	0.00
5) Phenol-d5	7.30	99	60716	11.34	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.45	67	31956	11.39	ng/ul	0.00
9) 2-Chlorophenol-d4	7.67	132	55579	12.42	ng/ul	0.00
13) 4-Methylphenol-d8	8.85	113	55259	12.18	ng/ul	0.00
19) Nitrobenzene-d5	9.31	128	29632	12.94	ng/ul	0.00
22) 2-Nitrophenol-d4	10.03	143	31542	12.72	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.58	165	55044	12.58	ng/ul	0.00
29) 4-Chloroaniline-d4	11.09	131	35521	7.45	ng/ul	0.00
43) Dimethylphthalate-d6	14.16	166	204115	14.21	ng/ul	0.00
46) Acenaphthylene-d8	14.46	160	283917	14.15	ng/ul	0.00
51) 4-Nitrophenol-d4	14.99	143	20318m	8.21	ng/ul	0.01
57) Fluorene-d10	15.75	176	201958	15.01	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.87	200	16510	7.92	ng/ul	0.00
70) Anthracene-d10	17.60	188	299781	15.67	ng/ul	0.00
76) Pyrene-d10	19.88	212	315625	15.53	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.86	264	268591	16.74	ng/ul	0.00

Target Compounds					Ovalue
44) Dimethylphthalate	14.20	163	41921	2.90 ng/ul	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA G\DATA\BG060216\
Data File : BG022158.D
Acq On : 2 Jun 2016 18:17
Operator : UM/SJ
Sample : H3302-12
Misc :
ALS Vial : 13 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
CB208

Manual Integrations
APPROVED

umangi
6/3/2016 4:55:02 PM

Quant Time: Jun 03 02:10:11 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG052116.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 03 01:08:24 2016
Response via : Initial Calibration

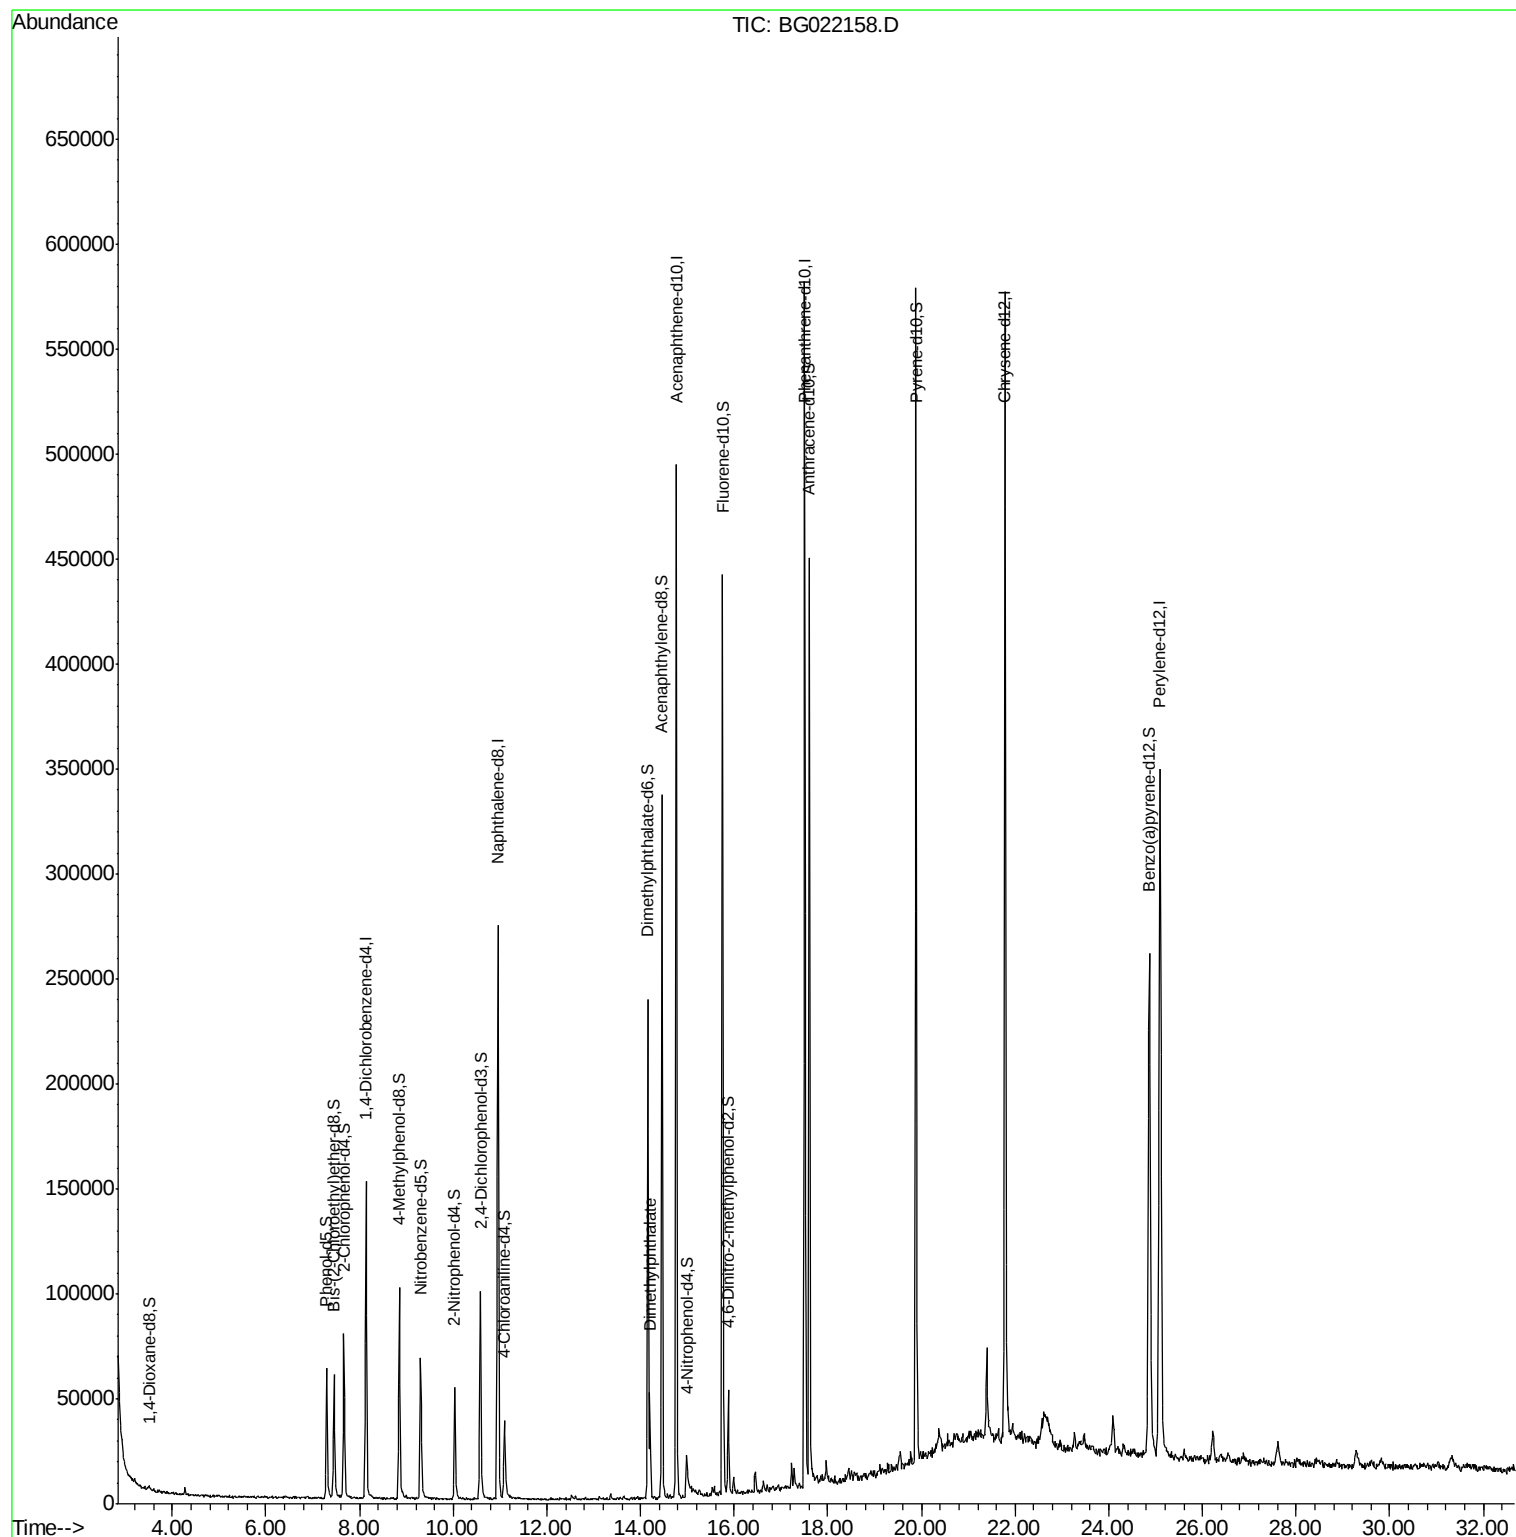

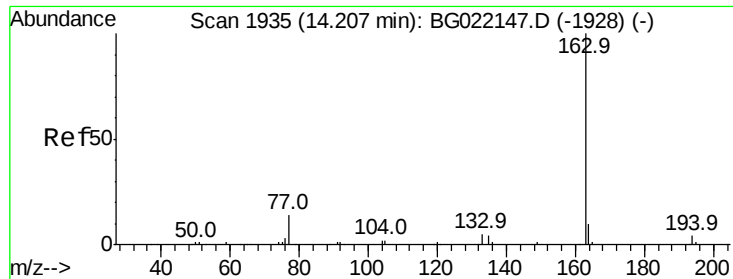

#44

Dimethylphthalate

Concen: 2.90 ng/ul

RT: 14.20 min Scan# 1934

Delta R.T. -0.01 min

Lab File: BG022158.D


Acq: 2 Jun 2016 18:17

Instrument :

BNA_G

ClientSampleId :

CB208

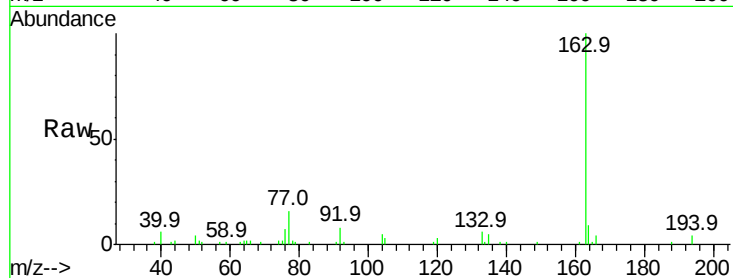

Tot Ion:	163	Resp:	41921
Ion Ratio	Lower	Upper	
163	100		
194	4.0	3.4	5.2
164	8.8	8.8	13.2

Manual Integrations
APPROVED

umangi
6/3/2016 4:55:02 PM

