

Data Path : Z:\HPCHEM1\BNA G\DATA\BG060216\
 Data File : BG022160.D
 Acq On : 2 Jun 2016 19:39
 Operator : UM/SJ
 Sample : H3302-14
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 CB210

Manual Integrations
 APPROVED

umangi
 6/3/2016 4:55:06 PM

Quant Time: Jun 03 02:25:46 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG052116.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 03 01:08:24 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.14	152	48257	20.00	ng/ul	0.00
18) Naphthalene-d8	10.95	136	252495	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.76	164	157178	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.50	188	329849	20.00	ng/ul	0.00
75) Chrysene-d12	21.79	240	290016	20.00	ng/ul	0.00
83) Perylene-d12	25.09	264	293879	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.50	96	941	1.02	ng/uL	0.00
5) Phenol-d5	7.29	99	52484	12.04	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.45	67	27668	12.10	ng/ul	0.00
9) 2-Chlorophenol-d4	7.67	132	49717	13.64	ng/ul	0.00
13) 4-Methylphenol-d8	8.84	113	47477	12.84	ng/ul	0.00
19) Nitrobenzene-d5	9.31	128	23225	12.47	ng/ul	0.00
22) 2-Nitrophenol-d4	10.03	143	26990	13.38	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.58	165	47167	13.25	ng/ul	0.00
29) 4-Chloroaniline-d4	11.09	131	54637	14.10	ng/ul	0.00
43) Dimethylphthalate-d6	14.16	166	172602	14.62	ng/ul	0.00
46) Acenaphthylene-d8	14.46	160	238547	14.47	ng/ul	0.00
51) 4-Nitrophenol-d4	14.98	143	16907m	8.32	ng/ul	0.00
57) Fluorene-d10	15.75	176	165470	14.97	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.88	200	11059	6.41	ng/ul	0.00
70) Anthracene-d10	17.60	188	241501	15.25	ng/ul	0.00
76) Pyrene-d10	19.88	212	239293	14.63	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.86	264	206509	15.14	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	14.20	163	30857	2.60	ng/ul	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA G\DATA\BG060216\
Data File : BG022160.D
Acq On : 2 Jun 2016 19:39
Operator : UM/SJ
Sample : H3302-14
Misc :
ALS Vial : 15 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
CB210

Manual Integrations
APPROVED

umangi
6/3/2016 4:55:06 PM

Quant Time: Jun 03 02:25:46 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG052116.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 03 01:08:24 2016
Response via : Initial Calibration

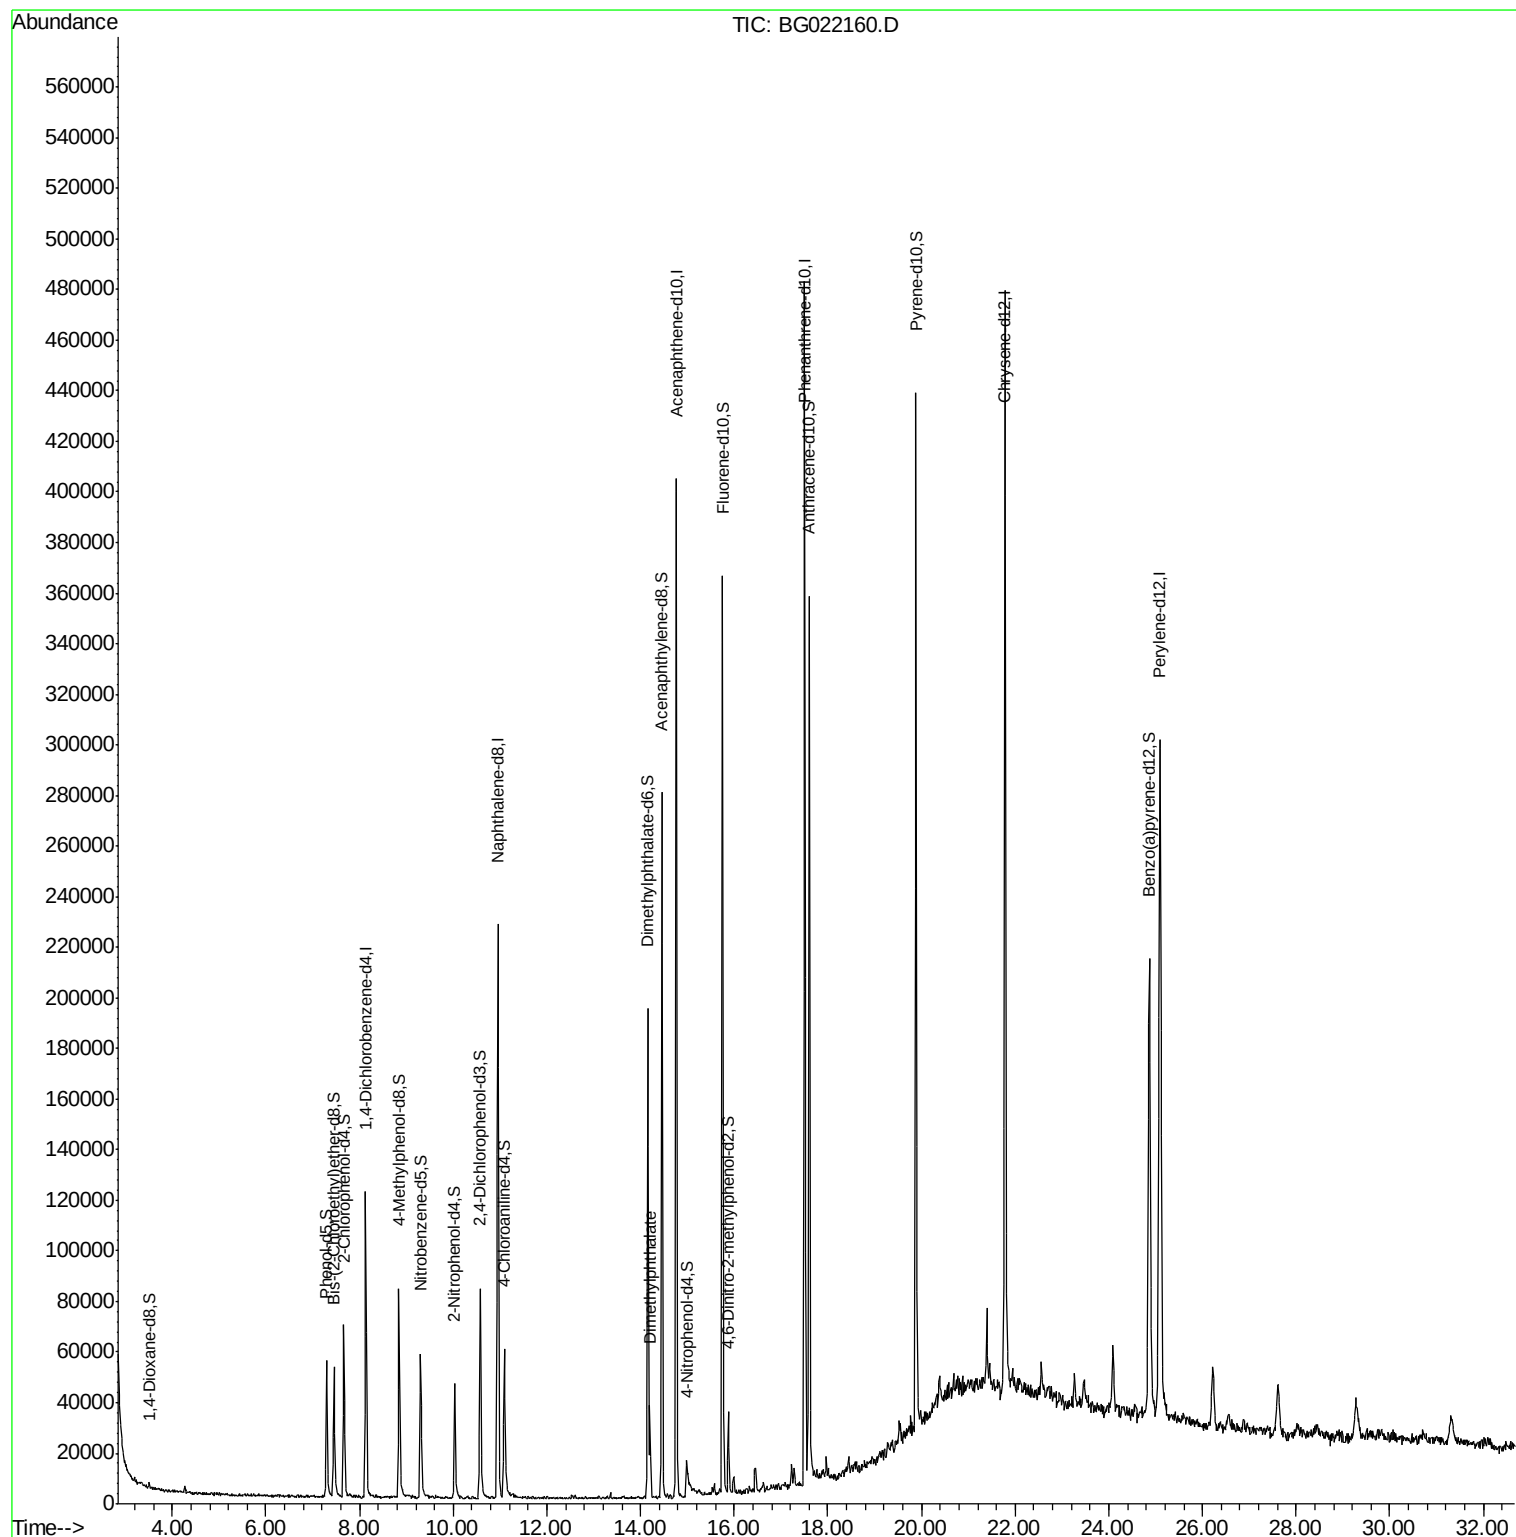

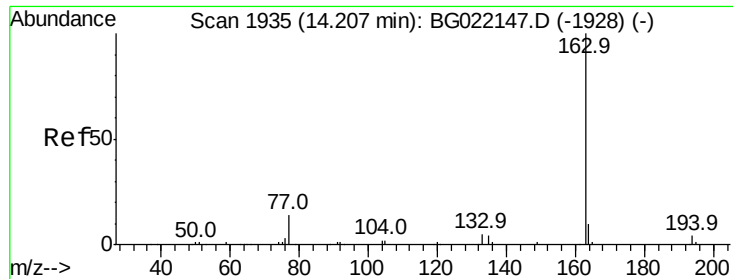


#44
 Dimethylphthalate
 Concen: 2.60 ng/ul
 RT: 14.20 min Scan# 1934
 Delta R.T. -0.01 min
 Lab File: BG022160.D
 Acq: 2 Jun 2016 19:39

Instrument :
 BNA_G
 ClientSampleId :
 CB210

Tot Ion	Ratio	Resp Lower	Resp Upper
163	100		
194	4.4	3.4	5.2
164	11.1	8.8	13.2

Manual Integrations
 APPROVED

umangi
 6/3/2016 4:55:06 PM

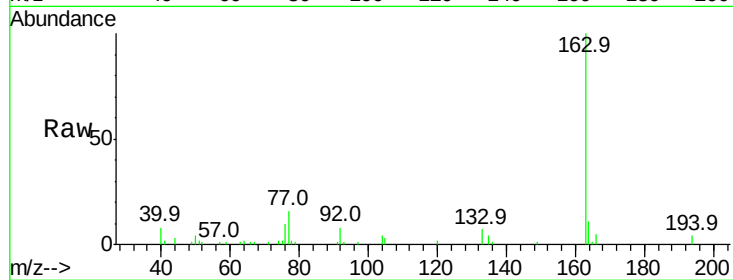

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

