

Data Path : Z:\HPCHEM1\BNA G\DATA\BG060216\
 Data File : BG022148.D
 Acq On : 2 Jun 2016 11:27
 Operator : UM/SJ
 Sample : PB90942BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK42

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG052116.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.498	109	112	117	rVB3	3613	4740	0.43%	0.043%
2	3.604	129	130	137	rVB4	1410	1564	0.14%	0.014%
3	4.057	202	207	210	rBV4	1100	1614	0.15%	0.015%
4	4.268	239	243	247	rVV4	1521	2678	0.24%	0.025%
5	7.171	733	737	741	rBV3	787	1280	0.12%	0.012%
6	7.294	751	758	768	rBV	81897	170337	15.31%	1.563%
7	7.453	778	785	796	rBV	74333	143828	12.93%	1.319%
8	7.664	814	821	831	rBV	99806	197959	17.79%	1.816%
9	8.134	892	901	913	rBV	93491	189597	17.04%	1.739%
10	8.845	1013	1022	1042	rBV	120789	266325	23.94%	2.443%
11	9.303	1091	1100	1111	rBV	84732	184649	16.60%	1.694%
12	10.032	1216	1224	1241	rBV	66171	148782	13.37%	1.365%
13	10.578	1308	1317	1334	rBV	118360	261192	23.48%	2.396%
14	10.954	1372	1381	1392	rBV	182111	369645	33.23%	3.391%
15	11.090	1395	1404	1418	rBV	112613	263020	23.64%	2.413%
16	12.541	1646	1651	1655	rBV3	1374	3059	0.27%	0.028%
17	14.157	1919	1926	1936	rBV	317386	508397	45.70%	4.664%
18	14.227	1936	1938	1941	rVV3	1710	2031	0.18%	0.019%
19	14.456	1969	1977	1990	rBV	383492	679295	61.06%	6.232%
20	14.762	2021	2029	2039	rBV2	340293	597797	53.73%	5.484%
21	14.979	2058	2066	2077	rBV2	43531	122333	11.00%	1.122%
22	15.132	2090	2092	2096	rVB5	1376	1533	0.14%	0.014%
23	15.749	2190	2197	2212	rBV	513193	877997	78.92%	8.055%
24	15.872	2212	2218	2231	rVV	85941	152144	13.68%	1.396%
25	15.990	2234	2238	2243	rVV2	5024	7718	0.69%	0.071%
26	17.506	2489	2496	2505	rBV2	449871	731017	65.71%	6.706%
27	17.605	2506	2513	2528	rVB2	530749	935292	84.07%	8.580%
28	18.011	2578	2582	2585	rVB4	1109	1499	0.13%	0.014%
29	18.452	2652	2657	2661	rVV3	1188	2111	0.19%	0.019%
30	19.527	2834	2840	2848	rVV4	5557	12622	1.13%	0.116%
31	19.603	2850	2853	2856	rBV2	1528	1889	0.17%	0.017%
32	19.773	2876	2882	2887	rVV3	4146	7065	0.64%	0.065%
33	19.885	2893	2901	2918	rBV	686431	1112505	100.00%	10.206%
34	20.249	2959	2963	2965	rBV2	1071	1439	0.13%	0.013%

Data Path : Z:\HPCHEM1\BNA G\DATA\BG060216\
 Data File : BG022148.D
 Acq On : 2 Jun 2016 11:27
 Operator : UM/SJ
 Sample : PB90942BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK42

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG052116.M
 Title : SVOA CALIBRATION

35	20.308	2972	2973	2977	rBV3	1445	1451	0.13%	0.013%
36	20.414	2988	2991	2995	rBV5	1721	2953	0.27%	0.027%
37	20.649	3030	3031	3033	rBV2	1432	1262	0.11%	0.012%
38	20.678	3035	3036	3039	rBV3	1687	1814	0.16%	0.017%
39	20.849	3063	3065	3070	rVB5	1228	1808	0.16%	0.017%
40	21.219	3126	3128	3131	rBV4	1680	1782	0.16%	0.016%
41	21.783	3216	3224	3236	rBV	456429	894846	80.44%	8.209%
42	22.018	3261	3264	3266	rBV3	1770	1858	0.17%	0.017%
43	22.335	3316	3318	3320	rVB2	1927	1488	0.13%	0.014%
44	22.829	3400	3402	3405	rVB4	1855	1490	0.13%	0.014%
45	22.940	3419	3421	3423	rVB3	2613	1531	0.14%	0.014%
46	23.123	3450	3452	3454	rBV3	2036	1408	0.13%	0.013%
47	23.264	3472	3476	3477	rBV4	4082	3969	0.36%	0.036%
48	23.916	3585	3587	3590	rBV4	2381	2822	0.25%	0.026%
49	24.151	3624	3627	3628	rBV3	1889	1488	0.13%	0.014%
50	24.791	3734	3736	3737	rBV	1595	1602	0.14%	0.015%
51	24.862	3737	3748	3762	rVV2	314239	967275	86.95%	8.874%
52	25.091	3775	3787	3804	rBV2	273479	913117	82.08%	8.377%
53	25.420	3841	3843	3844	rVB2	2326	1471	0.13%	0.013%
54	25.455	3847	3849	3851	rBV2	2089	2048	0.18%	0.019%
55	25.802	3907	3908	3911	rVB2	2063	1562	0.14%	0.014%
56	25.954	3932	3934	3936	rVB2	1830	1465	0.13%	0.013%
57	25.972	3936	3937	3940	rVB3	1884	1750	0.16%	0.016%
58	26.001	3940	3942	3944	rBV3	2718	2214	0.20%	0.020%
59	26.043	3947	3949	3951	rVB3	2263	1635	0.15%	0.015%
60	26.072	3951	3954	3955	rBV2	2584	1976	0.18%	0.018%
61	26.213	3973	3978	3988	rVB10	9533	23122	2.08%	0.212%
62	26.366	4002	4004	4010	rVB5	2325	4511	0.41%	0.041%
63	26.407	4010	4011	4015	rBV4	1737	2130	0.19%	0.020%
64	27.106	4127	4130	4133	rBV5	1974	2789	0.25%	0.026%
65	27.212	4146	4148	4152	rVB3	1848	1568	0.14%	0.014%
66	27.265	4155	4157	4159	rVB2	2697	2186	0.20%	0.020%
67	27.282	4159	4160	4162	rBV2	1926	1608	0.14%	0.015%
68	27.564	4204	4208	4209	rBV4	3188	4396	0.40%	0.040%
69	27.605	4209	4215	4216	rVV6	5261	8481	0.76%	0.078%
70	28.099	4296	4299	4303	rVB5	2268	2967	0.27%	0.027%
71	28.140	4303	4306	4307	rBV3	2384	2335	0.21%	0.021%

Data Path : Z:\HPCHEM1\BNA G\DATA\BG060216\
 Data File : BG022148.D
 Acq On : 2 Jun 2016 11:27
 Operator : UM/SJ
 Sample : PB90942BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK42

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG052116.M
 Title : SVOA CALIBRATION

72	28.469	4358	4362	4364	rBV4	2535	3182	0.29%	0.029%
73	28.493	4364	4366	4367	rBV2	1967	1660	0.15%	0.015%
74	28.587	4381	4382	4385	rBV2	2538	2162	0.19%	0.020%
75	28.698	4399	4401	4404	rVB3	1980	1472	0.13%	0.014%
76	28.810	4418	4420	4427	rVB8	1960	3258	0.29%	0.030%
77	28.969	4446	4447	4450	rVB3	2392	2134	0.19%	0.020%
78	28.998	4450	4452	4453	rBV2	1931	1609	0.14%	0.015%
79	29.233	4488	4492	4494	rBV5	2804	3634	0.33%	0.033%
80	29.256	4494	4496	4497	rBV2	3062	2523	0.23%	0.023%
81	29.280	4498	4500	4503	rVV4	3017	3885	0.35%	0.036%
82	29.409	4520	4522	4524	rVB3	2253	2068	0.19%	0.019%
83	29.433	4524	4526	4528	rVV3	1948	1427	0.13%	0.013%
84	29.468	4528	4532	4534	rVV5	2394	3630	0.33%	0.033%
85	29.486	4534	4535	4538	rVB2	3246	2759	0.25%	0.025%
86	29.944	4612	4613	4616	rBV3	1502	1728	0.16%	0.016%
87	29.967	4616	4617	4619	rVV2	2423	1306	0.12%	0.012%
88	30.003	4622	4623	4626	rBV3	1720	2261	0.20%	0.021%
89	30.056	4629	4632	4634	rBV4	1522	2015	0.18%	0.018%
90	30.173	4650	4652	4655	rVB4	2548	1872	0.17%	0.017%
91	30.761	4750	4752	4754	rBV3	2155	2051	0.18%	0.019%
92	30.960	4784	4786	4788	rBV3	1768	1330	0.12%	0.012%
93	31.148	4816	4818	4820	rVB3	1782	1444	0.13%	0.013%
94	31.178	4820	4823	4826	rBV4	1644	1999	0.18%	0.018%
95	31.201	4826	4827	4829	rBV2	1710	1606	0.14%	0.015%
96	31.454	4868	4870	4872	rBV3	2221	1868	0.17%	0.017%
97	31.472	4872	4873	4875	rBV2	1539	1363	0.12%	0.013%
98	32.047	4968	4971	4973	rBV4	1975	2214	0.20%	0.020%
99	32.088	4976	4978	4980	rBV2	1592	1462	0.13%	0.013%
100	32.253	5004	5006	5009	rVB3	1591	1373	0.12%	0.013%


Sum of corrected areas: 10900426

Data Path : Z:\HPCHEM1\BNA G\DATA\BG060216\
Data File : BG022148.D
Acq On : 2 Jun 2016 11:27
Operator : UM/SJ
Sample : PB90942BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK42

Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG052116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

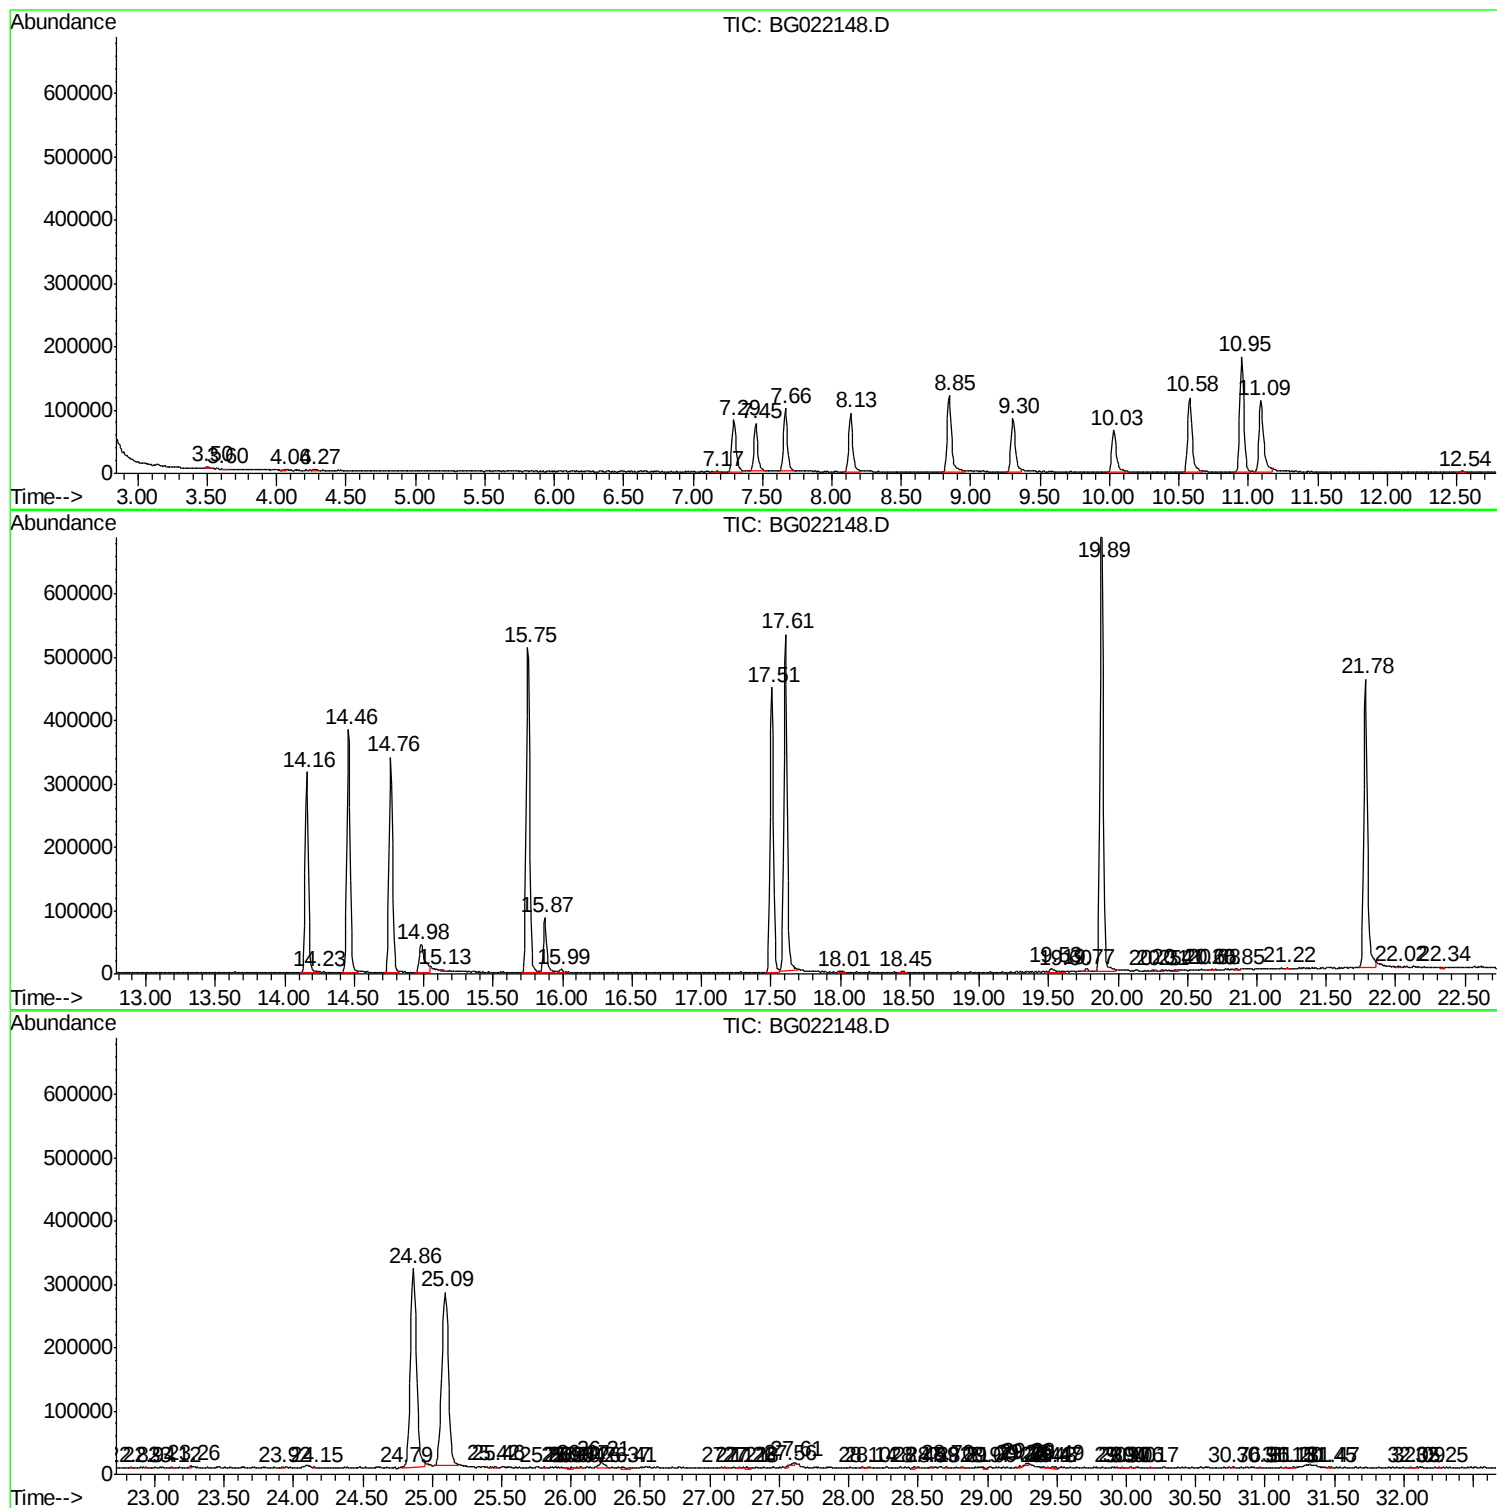

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG060216\
Data File : BG022148.D
Acq On : 2 Jun 2016 11:27
Operator : UM/SJ
Sample : PB90942BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK42

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG052116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG060216\
Data File : BG022148.D
Acq On : 2 Jun 2016 11:27
Operator : UM/SJ
Sample : PB90942BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK42

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG052116.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc