


Data Path : Z:\HPCHEM1\BNA G\Data\BG060216\
 Data File : BG022146.D
 Acq On : 2 Jun 2016 9:16
 Operator : UM/SJ
 Sample : DFTPP18
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP18

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG052116.M
 Title : SVOA CALIBRATION
 Last Update : Fri Jun 03 01:08:24 2016

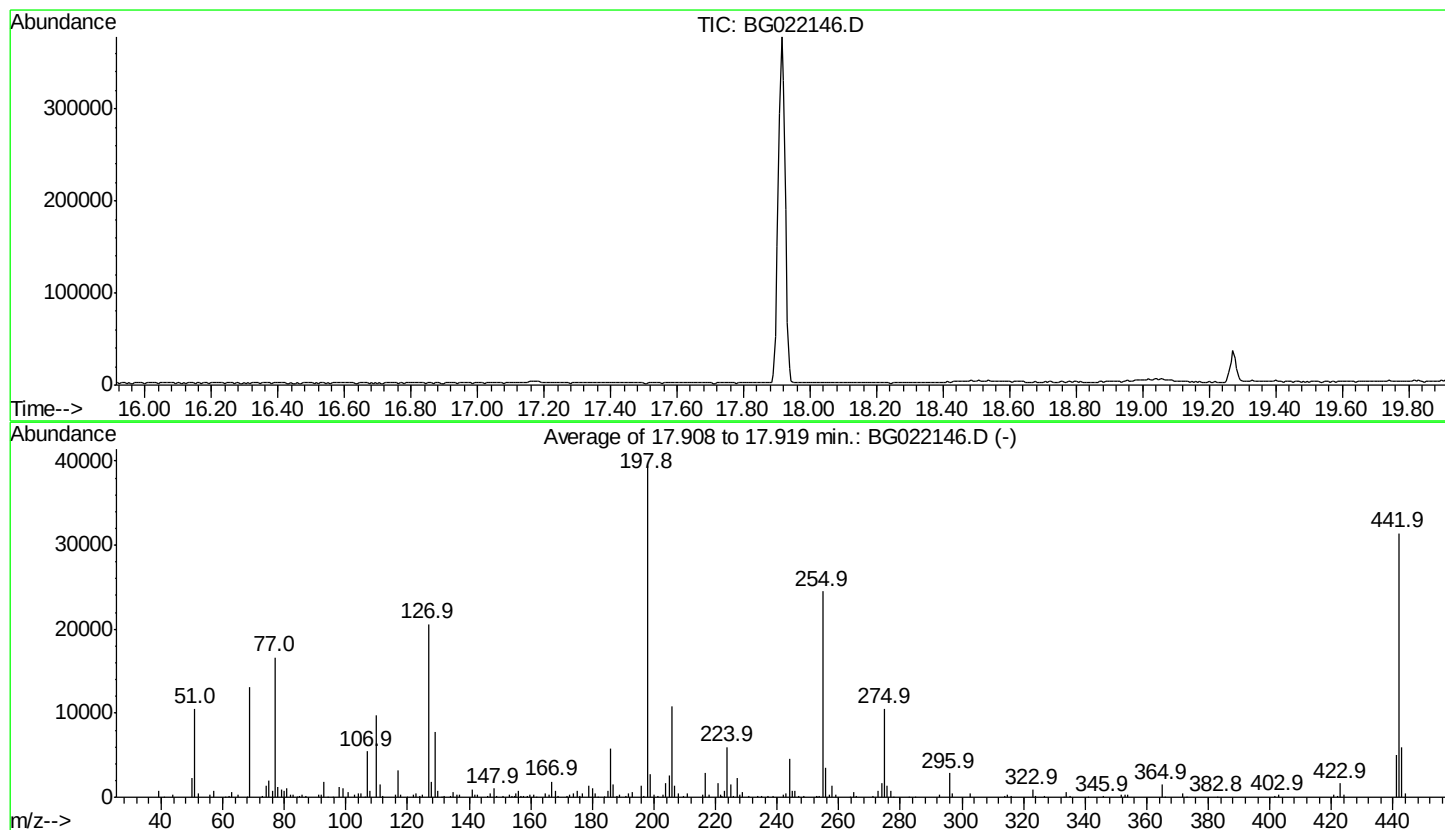

AutoFind: Scans 2565, 2566, 2567; Background Corrected with Scan 2560

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.7	10549	PASS
68	69	0.00	2	0.5	72	PASS
69	198	0.00	100	33.2	13117	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.2	20594	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	39456	PASS
199	198	5	9	7.1	2813	PASS
275	198	10	60	26.7	10547	PASS
365	198	1	100	3.7	1461	PASS
441	442	0.01	100	15.9	4987	PASS
442	198	50	100	79.5	31384	PASS
443	442	15	24	18.9	5933	PASS

Scan 2560 (17.878 min): BG022146.D
DFTPP18

m/z	Abundance
39.90	1797.0
43.90	542.0
206.80	161.0

Instrument :
BNA_G
ClientSampleId :
DFTPP18

m/z	Abundance
39.00	734.0
39.90	1541.0
43.90	651.0
50.00	2089.0
51.00	10782.0
52.00	530.0
55.90	263.0
57.00	645.0
62.00	180.0
62.90	585.0
65.00	297.0
68.00	216.0
68.90	13293.0
73.00	204.0
74.00	1221.0
74.90	2111.0
76.00	877.0
77.00	16440.0
78.00	1334.0
79.00	868.0
79.90	751.0
80.90	1043.0
81.90	414.0
82.90	268.0
83.90	167.0
85.00	247.0
85.90	273.0
87.00	247.0
90.90	253.0
91.90	408.0
92.90	1817.0
97.90	1093.0
98.90	1000.0
100.90	606.0
102.80	243.0
103.90	432.0
104.90	362.0
106.00	203.0
106.90	5192.0
107.90	641.0
109.90	9112.0
110.90	1239.0
112.00	173.0
116.00	386.0
116.90	2860.0
117.90	233.0
119.90	156.0
121.80	272.0
122.90	354.0
123.80	223.0
124.90	304.0
126.90	20480.0
127.90	1860.0
128.90	6997.0
129.90	664.0
133.90	195.0
134.90	525.0
135.90	339.0
137.00	224.0
140.90	809.0
141.90	225.0
142.90	305.0
146.00	299.0
146.90	576.0
147.90	949.0
148.90	196.0
150.90	167.0
152.90	323.0
153.90	278.0
154.80	493.0
155.90	674.0
156.80	189.0
157.90	205.0
158.90	220.0
159.90	292.0
160.80	377.0
164.90	413.0
165.90	401.0
166.90	1739.0
167.90	635.0
168.90	192.0
172.80	329.0
173.90	503.0
174.90	944.0
176.90	421.0
178.90	1355.0
179.90	913.0
180.90	436.0
183.80	222.0
184.90	822.0
185.90	5413.0
186.90	1658.0

Instrument :
BNA_G
ClientSampleId :
DFTPP18

187.80	157.0
188.90	393.0
191.80	458.0
192.90	461.0
195.90	1198.0
197.90	34720.0
198.80	2513.0
199.80	315.0
202.80	240.0
203.90	1254.0
204.90	2405.0
205.90	9241.0
206.90	1476.0
207.80	351.0
210.90	321.0
215.80	163.0
216.90	2448.0
217.90	389.0
220.90	1759.0
221.70	306.0
222.80	604.0
223.90	5494.0
224.90	1612.0
226.90	1662.0
227.80	334.0
228.80	621.0
230.80	159.0
234.90	234.0
236.80	205.0
241.80	259.0
242.90	445.0
243.90	3594.0
244.80	723.0
245.90	694.0
246.80	220.0
248.80	155.0
253.00	159.0
253.80	220.0
254.90	20416.0
255.90	3069.0
257.90	1109.0
258.80	244.0
264.80	593.0
272.80	693.0
273.80	1413.0
274.90	8414.0
275.90	1209.0
276.80	656.0
277.80	234.0
292.80	273.0
295.90	2288.0
296.80	285.0
302.90	380.0
314.80	358.0
322.90	729.0
333.90	582.0
351.80	279.0
352.80	177.0
353.90	223.0
364.80	1056.0
371.90	341.0
401.70	217.0
402.80	230.0
420.90	310.0
422.90	1326.0
423.80	192.0
440.90	3322.0
441.90	20744.0
442.90	4307.0
443.90	426.0

Instrument :
BNA_G
ClientSampleId :
DFTPP18

m/z	Abundance
39.00	759.0
39.90	1860.0
41.00	161.0
44.00	1039.0
50.00	2544.0
51.00	11375.0
52.00	564.0
55.90	447.0
57.00	821.0
62.00	264.0
63.00	596.0
65.00	365.0
68.90	14259.0
73.00	174.0
74.00	1615.0
74.90	2256.0
76.00	732.0
77.00	18016.0
77.90	1493.0
78.90	963.0
79.90	956.0
80.90	1260.0
82.00	383.0
82.90	296.0
86.00	433.0
86.90	186.0
91.00	195.0
92.00	258.0
92.90	1940.0
93.90	239.0
95.90	178.0
97.90	1432.0
98.90	1266.0
100.90	732.0
102.80	255.0
103.90	436.0
104.90	690.0
106.90	6496.0
108.00	1123.0
109.90	11285.0
110.90	1604.0
111.90	268.0
116.00	363.0
116.90	3584.0
117.90	333.0
121.90	362.0
122.90	602.0
123.90	222.0
125.00	246.0
126.90	22104.0
127.90	2190.0
128.90	8948.0
129.90	880.0
131.90	182.0
134.00	178.0
135.00	763.0
135.90	171.0
136.90	315.0
140.90	872.0
141.90	404.0
142.80	216.0
145.90	211.0
146.90	394.0
147.90	1200.0
148.90	243.0
150.80	162.0
152.90	311.0
153.90	210.0
155.00	731.0
155.90	750.0
156.90	184.0
157.90	267.0
158.80	251.0
159.90	384.0
160.80	362.0
164.80	356.0
165.90	487.0
166.90	2065.0
167.90	773.0
168.90	235.0
171.90	247.0
172.80	225.0
173.90	527.0
174.90	794.0
175.90	267.0
176.80	464.0
178.80	1418.0
179.90	1293.0
180.90	616.0
181.80	169.0
184.00	195.0
184.90	881.0

Instrument :
BNA_G
ClientSampleId :
DFTPP18

185.90	6047.0
186.90	1625.0
187.90	176.0
188.90	545.0
190.80	220.0
191.80	583.0
192.90	727.0
195.90	1540.0
197.80	44456.0
198.80	3156.0
199.90	281.0
201.30	206.0
202.90	236.0
203.90	2115.0
204.90	3183.0
205.90	12025.0
206.90	1530.0
207.90	484.0
209.80	249.0
210.80	571.0
215.80	273.0
216.80	3199.0
217.80	353.0
220.90	1537.0
221.90	551.0
222.80	872.0
223.90	6390.0
224.90	1662.0
226.90	3038.0
227.80	426.0
228.80	622.0
230.90	214.0
233.90	186.0
234.90	275.0
238.80	176.0
241.90	418.0
242.90	365.0
243.90	5483.0
244.90	817.0
245.90	751.0
246.90	204.0
248.80	193.0
252.70	158.0
254.90	28224.0
255.90	4139.0
256.80	401.0
257.90	1517.0
258.90	304.0
263.80	173.0
264.90	562.0
265.70	169.0
270.90	252.0
272.80	790.0
273.90	2051.0
274.90	11508.0
275.80	1781.0
276.80	793.0
282.70	175.0
284.90	158.0
292.80	224.0
295.90	3292.0
296.90	519.0
302.80	395.0
313.90	160.0
314.80	295.0
315.80	173.0
322.90	982.0
323.80	191.0
326.70	192.0
333.90	804.0
334.90	228.0
345.90	264.0
351.90	317.0
352.80	361.0
353.90	326.0
364.80	1752.0
365.90	197.0
371.90	522.0
372.80	191.0
382.80	173.0
402.90	263.0
420.90	214.0
421.80	267.0
422.90	2006.0
423.90	344.0
440.90	5953.0
441.90	37360.0
442.90	6622.0
443.80	553.0

Instrument :
BNA_G
ClientSampleId :
DFTPP18

m/z	Abundance
39.00	585.0
39.90	1797.0
43.90	783.0
50.00	2282.0
51.00	9490.0
51.90	483.0
56.00	364.0
56.90	728.0
60.90	228.0
63.00	515.0
65.00	205.0
68.90	11799.0
73.90	1217.0
74.90	1747.0
76.00	627.0
77.00	15527.0
78.00	812.0
78.90	854.0
79.90	819.0
80.90	1096.0
81.90	345.0
82.80	276.0
85.00	183.0
85.90	303.0
91.00	357.0
91.90	374.0
92.90	1644.0
97.90	1042.0
98.90	883.0
100.90	473.0
102.80	241.0
103.90	490.0
104.90	318.0
106.90	4667.0
107.90	561.0
109.90	8660.0
110.90	1517.0
111.90	169.0
115.90	237.0
116.90	3137.0
117.90	237.0
121.80	385.0
122.90	524.0
123.70	157.0
124.90	216.0
126.90	19200.0
127.90	1600.0
128.90	7242.0
129.90	546.0
130.90	166.0
131.90	182.0
134.90	447.0
135.80	239.0
136.90	316.0
140.90	1048.0
141.90	303.0
142.90	182.0
146.90	478.0
147.90	870.0
148.80	235.0
152.90	251.0
153.90	159.0
154.90	428.0
155.90	759.0
156.80	234.0
157.80	162.0
159.80	236.0
160.90	407.0
161.80	154.0
164.80	445.0
165.90	265.0
166.90	1701.0
167.90	856.0
168.90	231.0
171.90	161.0
172.80	332.0
173.90	359.0
174.90	749.0
175.90	197.0
176.80	430.0
178.80	1317.0
179.90	1072.0
180.90	500.0
184.90	601.0
185.90	5797.0
186.90	1407.0
188.80	203.0
190.90	194.0
191.80	393.0
192.90	563.0
195.90	1179.0
196.60	253.0

Instrument :
BNA_G
ClientSampleId :
DFTPP18

197.80	39192.0
198.80	2771.0
199.90	256.0
201.40	380.0
202.80	361.0
203.90	1502.0
204.90	2371.0
205.90	11196.0
206.90	1411.0
207.90	469.0
210.90	494.0
215.90	282.0
216.90	3178.0
217.90	414.0
220.80	1592.0
221.50	417.0
222.90	746.0
223.90	6009.0
224.90	1495.0
225.90	281.0
226.90	2230.0
227.80	223.0
228.80	437.0
230.80	253.0
233.90	154.0
236.90	292.0
238.90	161.0
241.90	455.0
242.80	396.0
243.90	4873.0
244.90	549.0
245.80	679.0
248.80	191.0
252.90	182.0
253.90	415.0
254.90	24912.0
255.90	3251.0
256.80	408.0
257.90	1295.0
258.90	194.0
264.90	569.0
265.80	236.0
272.90	803.0
273.90	1582.0
274.90	11720.0
275.90	1168.0
276.80	873.0
292.90	267.0
295.90	3089.0
296.80	471.0
302.90	411.0
313.90	228.0
314.80	329.0
315.90	177.0
322.90	958.0
323.90	308.0
326.80	231.0
332.90	171.0
333.80	689.0
334.90	177.0
340.90	184.0
345.80	151.0
351.80	215.0
352.80	220.0
353.90	353.0
364.90	1577.0
371.80	460.0
401.80	235.0
402.80	400.0
420.90	257.0
421.80	329.0
422.90	1618.0
423.90	333.0
440.90	5686.0
441.90	36048.0
442.90	6870.0
443.90	610.0

Instrument :
BNA_G
ClientSampleId :
DFTPP18