
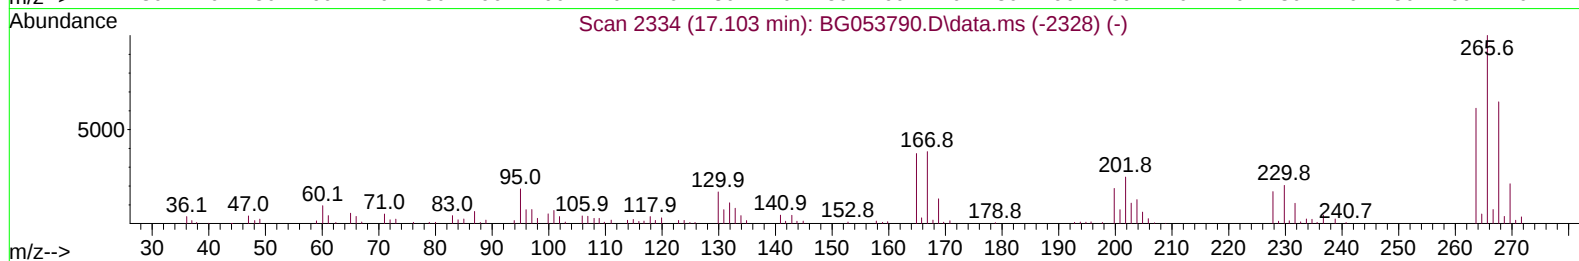
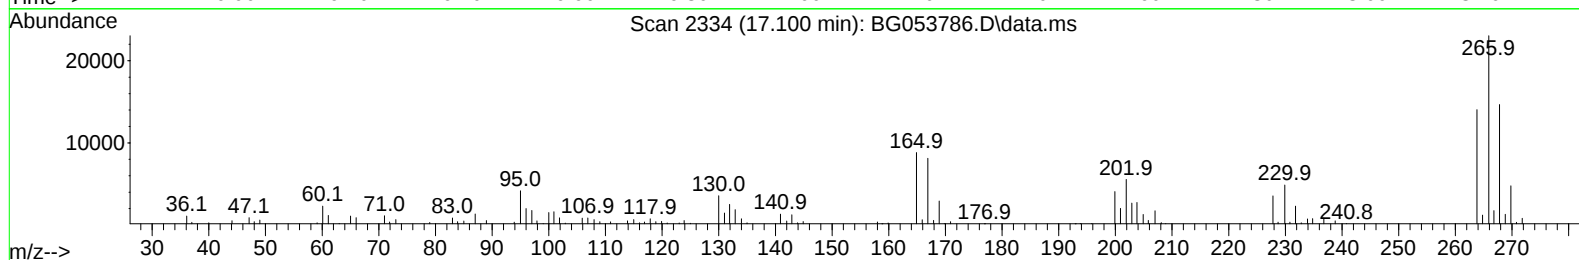


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060222\
Data File : BG053786.D
Acq On : 2 Jun 2022 11:08
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 02 18:55:13 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 02 18:25:54 2022
Response via : Initial Calibration

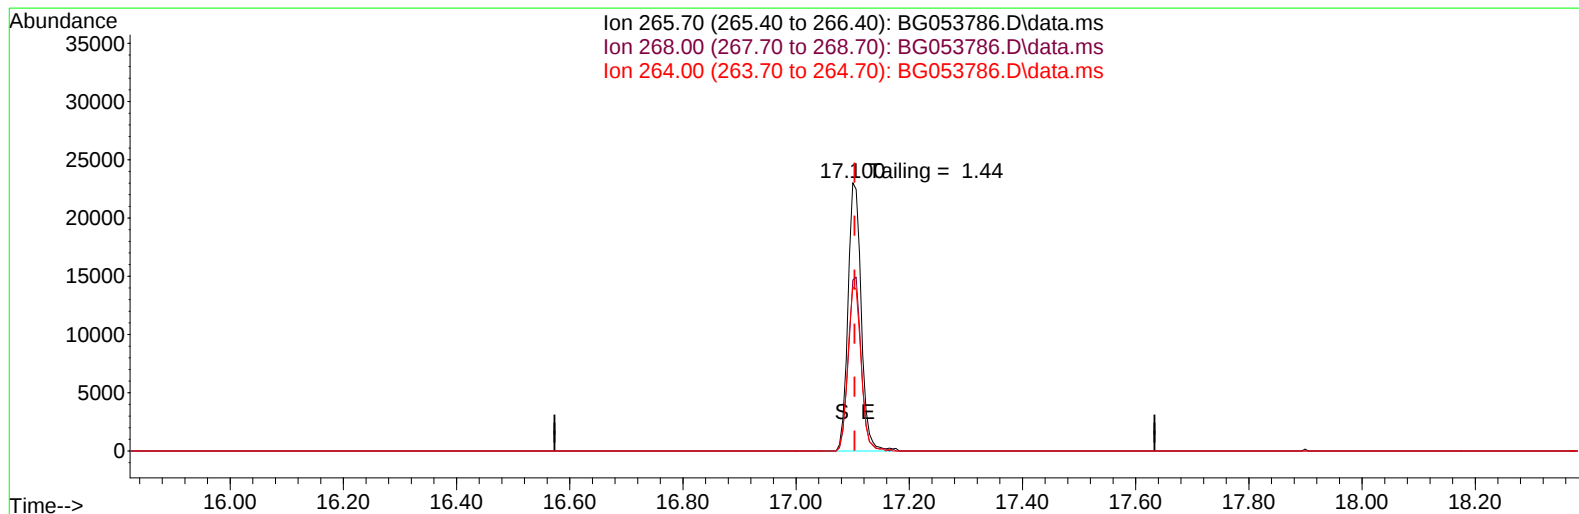

TIC: BG053786.D\data.ms

(70) Pentachlorophenol (C)




17.100min (-0.003) 34616.33 ng

response 37163

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	63.67
264.00	66.20	60.94
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060222\
Data File : BG053786.D
Acq On : 2 Jun 2022 11:08
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 02 18:55:13 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 02 18:25:54 2022
Response via : Initial Calibration

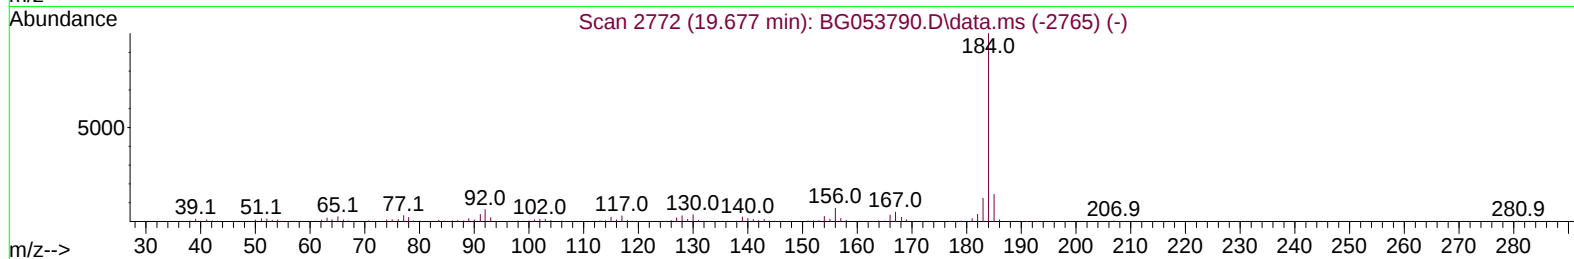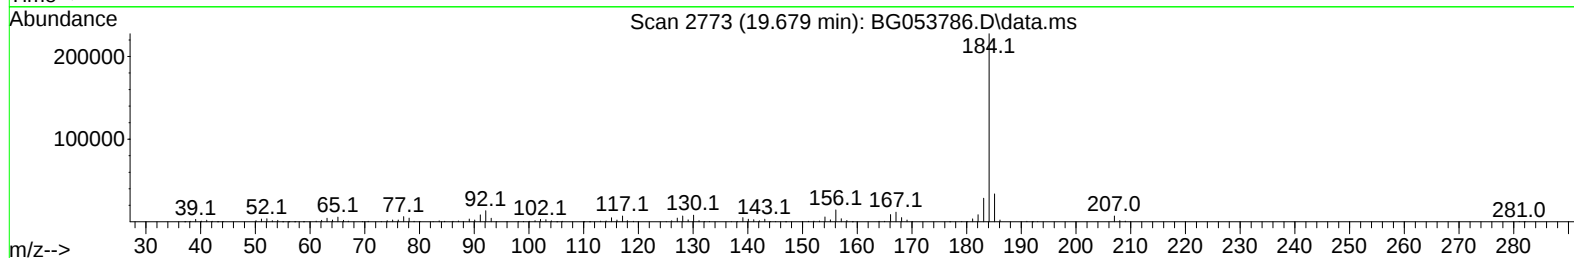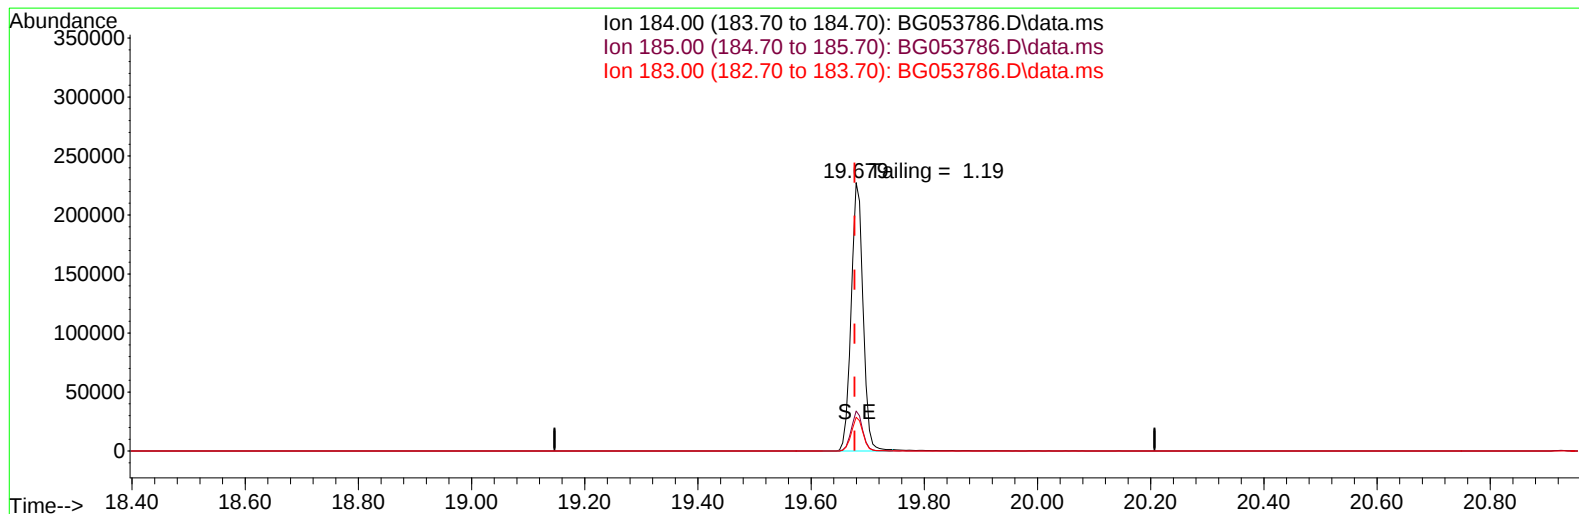

TIC: BG053786.D\data.ms

(77) Benzidine

19.679min (+ 0.003) 0.00 ng

response 332879

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.91
183.00	11.10	12.59
0.00	0.00	0.00