

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060222\
 Data File : BG053795.D
 Acq On : 2 Jun 2022 17:06
 Operator : CG/JU
 Sample : PB145265BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB145265BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG060222.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG053795.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.657	379	386	396	rBV	394802	663231	29.11%	8.596%
2	7.243	647	656	666	rBV	381774	691362	30.35%	8.961%
3	8.095	794	801	808	rVB	72238	127173	5.58%	1.648%
4	9.252	990	998	1006	rBV	222523	414680	18.20%	5.375%
5	10.903	1270	1279	1286	rBV	94297	177841	7.81%	2.305%
6	13.342	1686	1694	1703	rBV	693250	1100982	48.33%	14.270%
7	14.711	1920	1927	1934	rVB	157862	251889	11.06%	3.265%
8	16.197	2173	2180	2191	rBV	470566	746431	32.77%	9.675%
9	17.454	2387	2394	2402	rVB	220387	341909	15.01%	4.432%
10	20.063	2832	2838	2844	rVB	1630740	2278132	100.00%	29.528%
11	21.732	3116	3122	3129	rVB	270512	473420	20.78%	6.136%
12	24.993	3668	3677	3688	rVB2	150628	448198	19.67%	5.809%




Sum of corrected areas: 7715248

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060222\
Data File : BG053795.D
Acq On : 2 Jun 2022 17:06
Operator : CG/JU
Sample : PB145265BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB145265BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

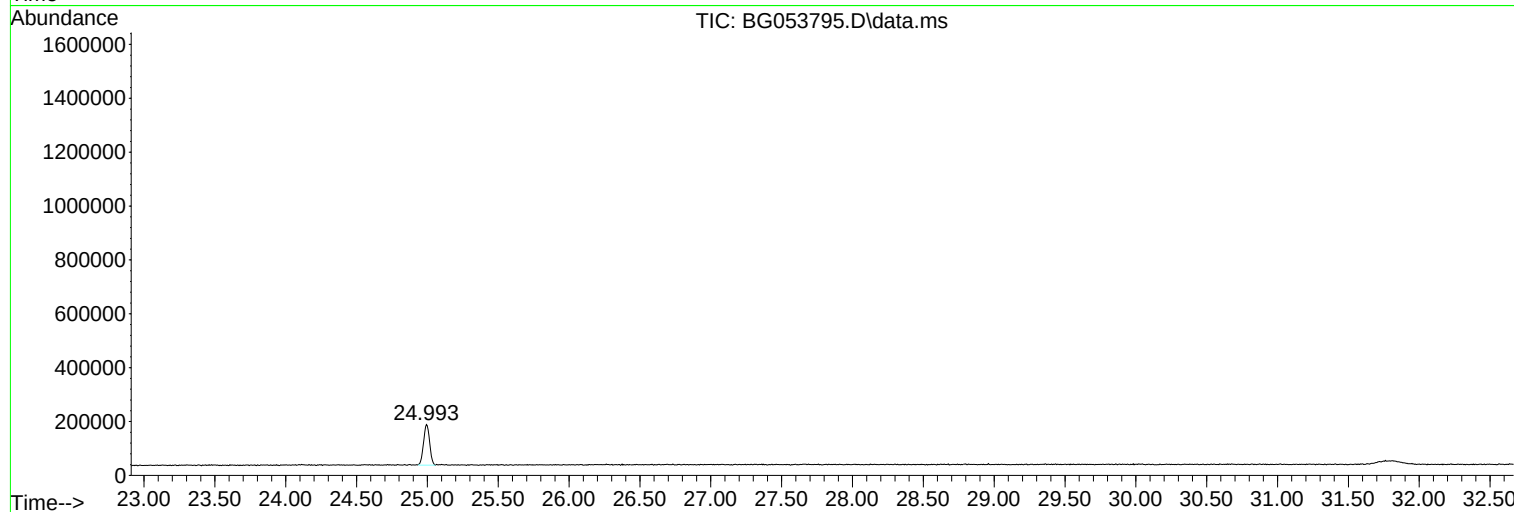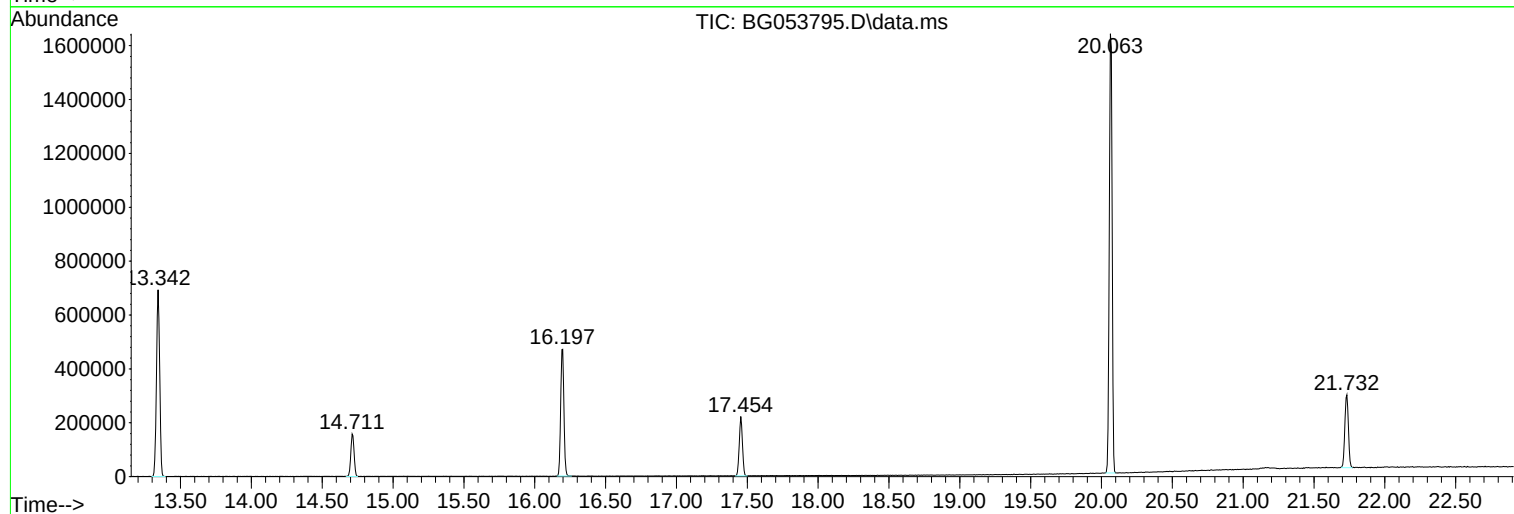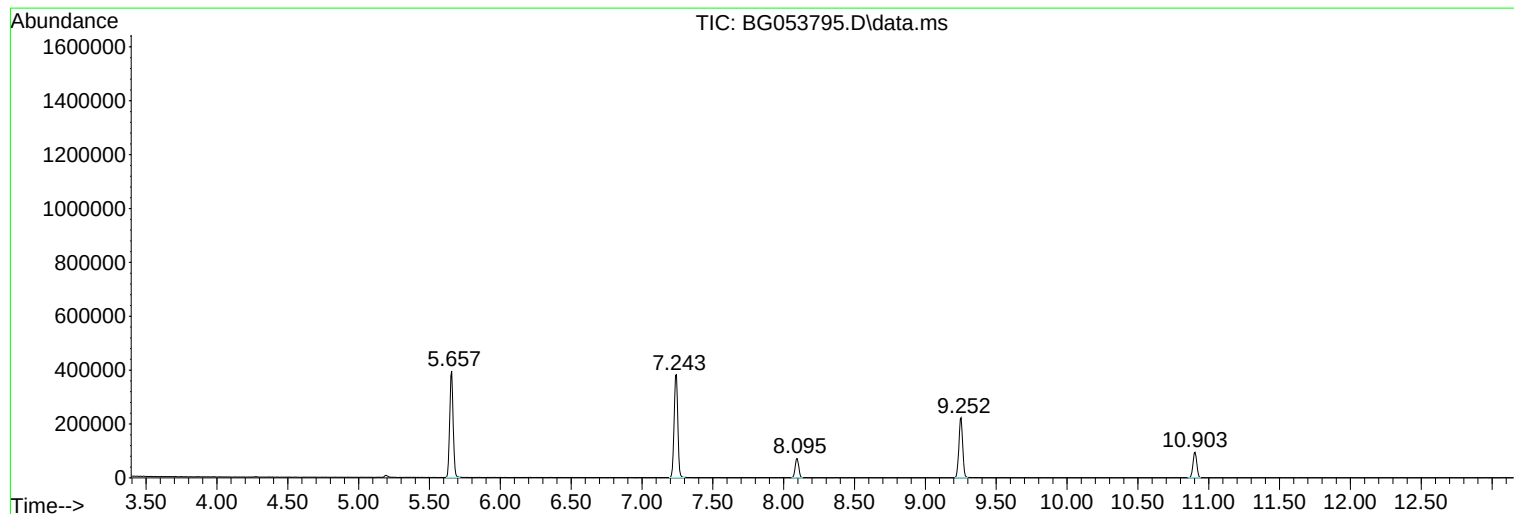

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060222\
Data File : BG053795.D
Acq On : 2 Jun 2022 17:06
Operator : CG/JU
Sample : PB145265BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB145265BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060222\
Data File : BG053795.D
Acq On : 2 Jun 2022 17:06
Operator : CG/JU
Sample : PB145265BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB145265BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------