
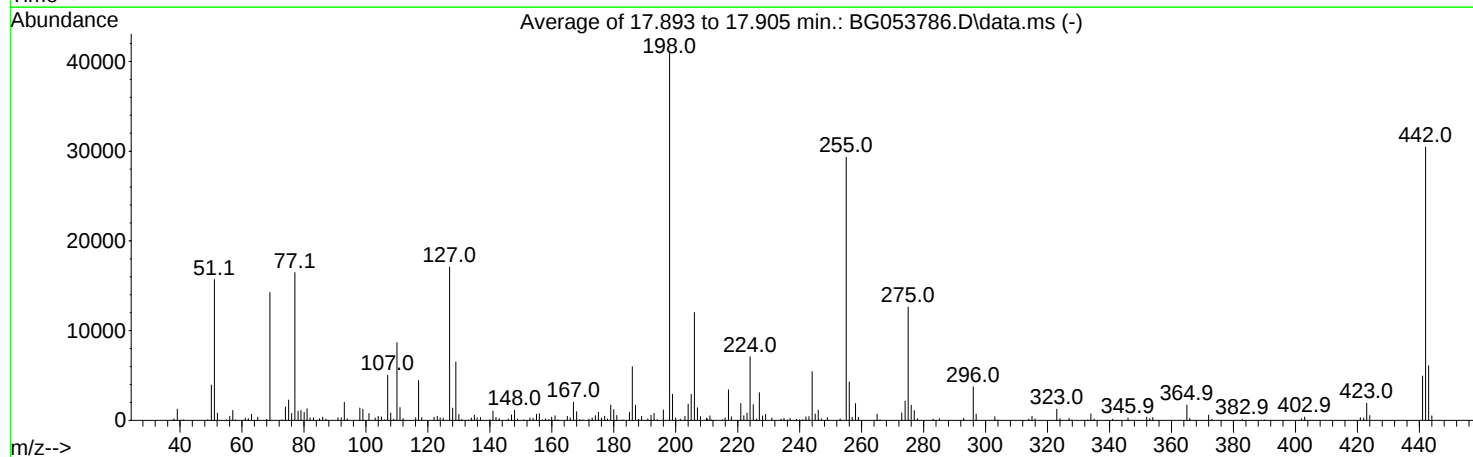


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060222\
 Data File : BG053786.D
 Acq On : 2 Jun 2022 11:08
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG060222.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jun 02 23:22:27 2022

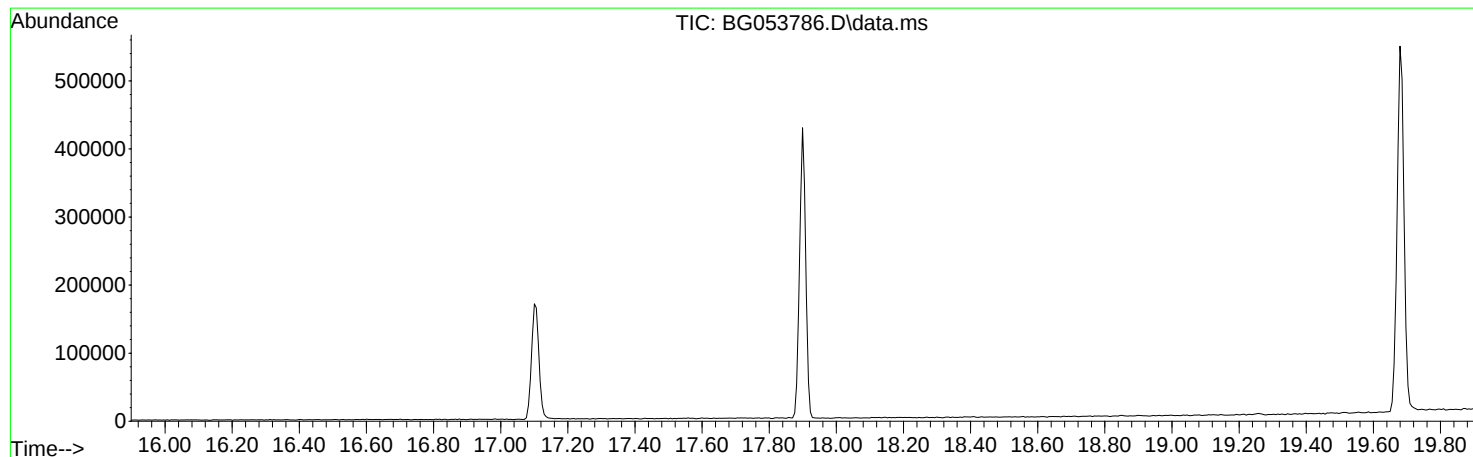

AutoFind: Scans 2469, 2470, 2471; Background Corrected with Scan 2463

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.3	15695	PASS
68	69	0.00	2	0.8	110	PASS
69	198	0.00	100	34.8	14257	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	41.7	17091	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	40995	PASS
199	198	5	9	7.1	2903	PASS
275	198	10	60	30.8	12630	PASS
365	198	1	100	4.2	1712	PASS
441	198	0.01	100	12.0	4938	PASS
442	442	50	100	100.0	30461	PASS
443	442	15	24	20.0	6088	PASS




DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/2/2022	BNA_G	<u>BG053786.D</u>
Compound Name	Response	Retention Time
DDT	125741	20.91
DDD	412	20.53
DDE	0	19.97
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
412	126153	0.33

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060222\
Data File : BG053786.D
Acq On : 2 Jun 2022 11:08
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jun 02 18:55:13 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 02 18:25:54 2022
Response via : Initial Calibration

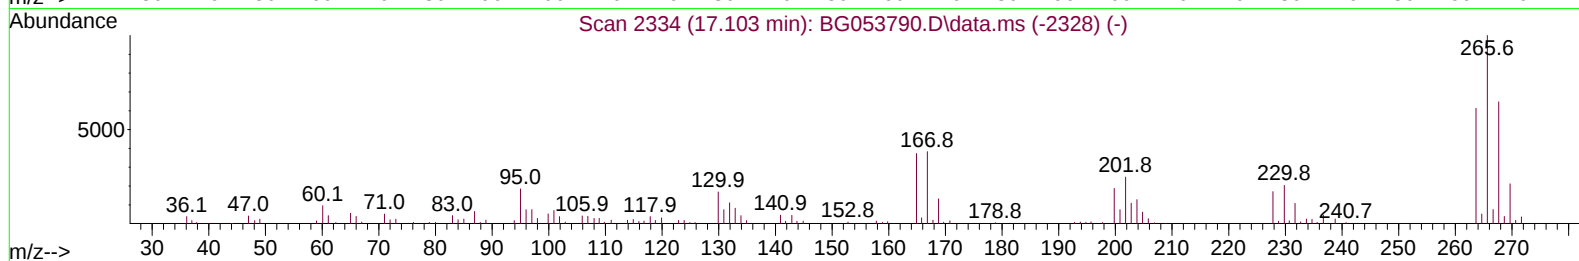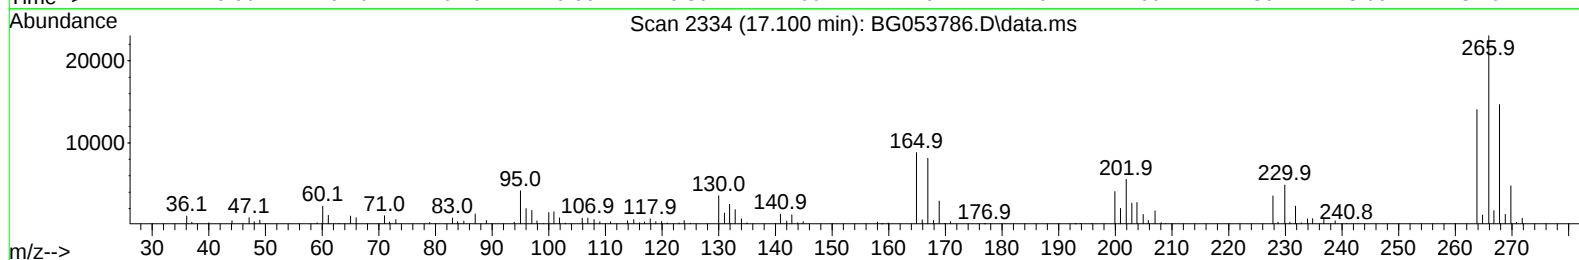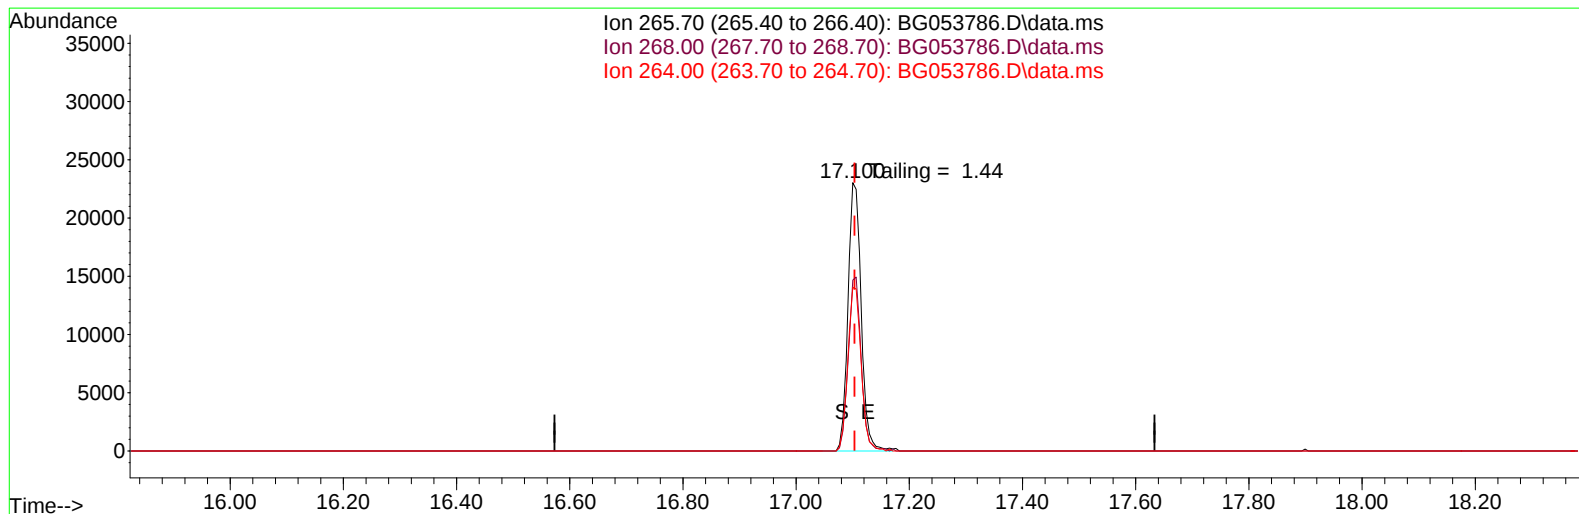

TIC: BG053786.D\data.ms

(70) Pentachlorophenol (C)

17.100min (-0.003) 34616.33 ng




response 37163

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	63.67
264.00	66.20	60.94
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060222\
Data File : BG053786.D
Acq On : 2 Jun 2022 11:08
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jun 02 18:55:13 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 02 18:25:54 2022
Response via : Initial Calibration

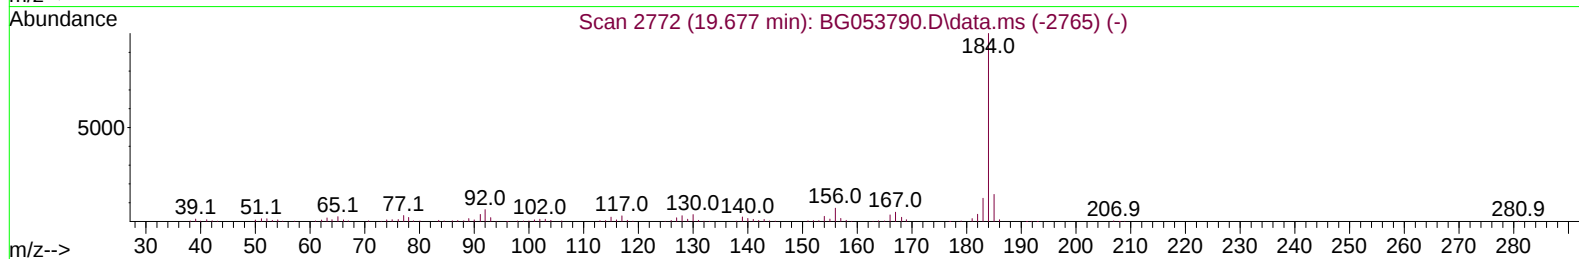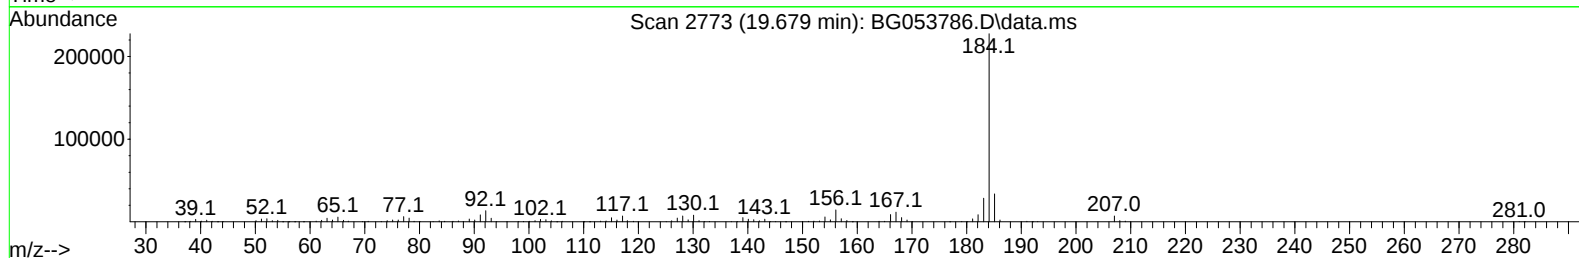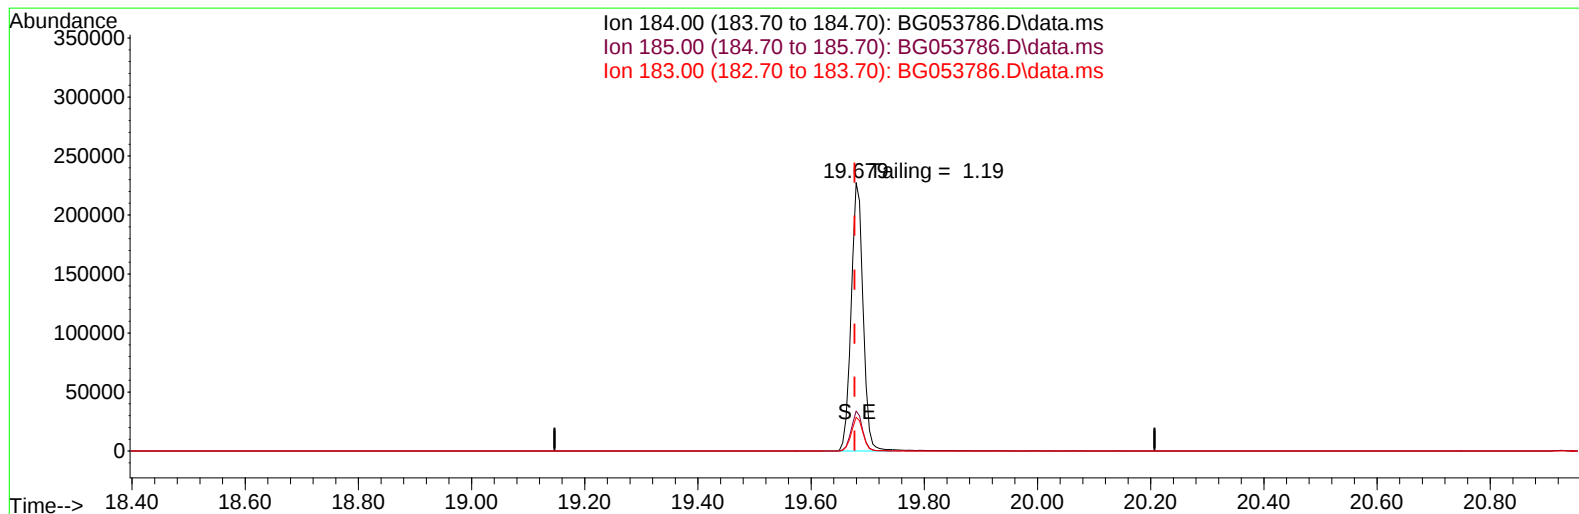

TIC: BG053786.D\data.ms

(77) Benzidine

19.679min (+ 0.003) 0.00 ng

response 332879

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.91
183.00	11.10	12.59
0.00	0.00	0.00