
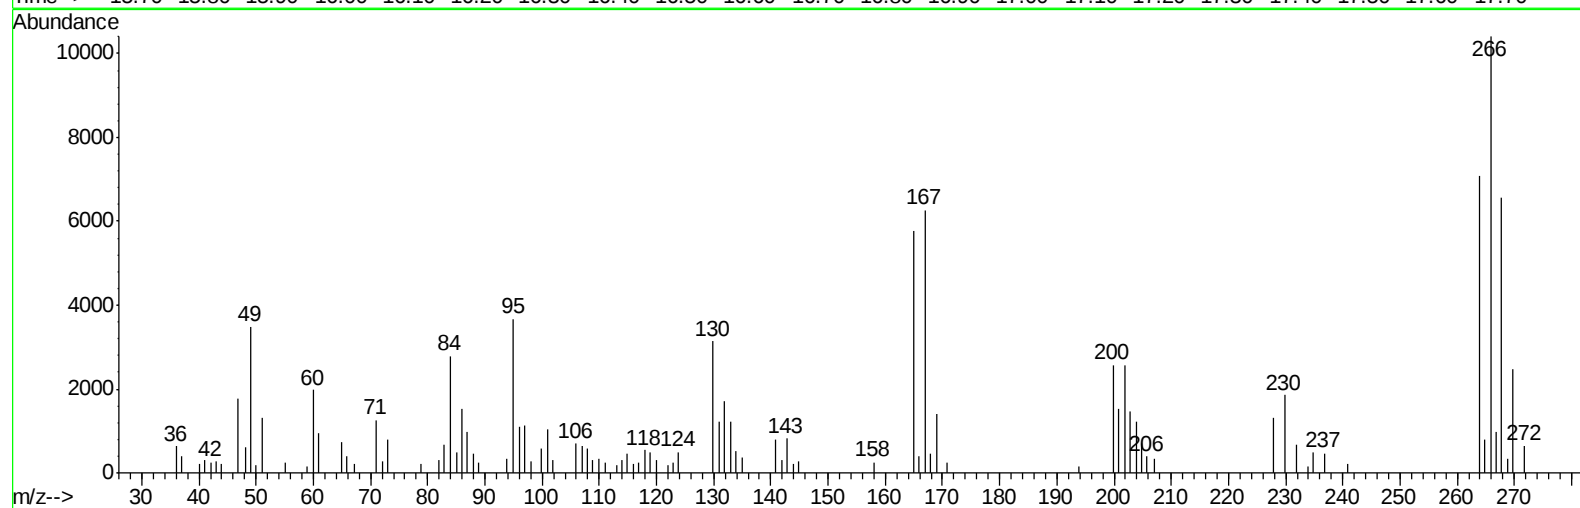


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG060315\
Data File : BG017403.D
Acq On : 3 Jun 2015 12:24
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 04 06:42:55 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 04 01:31:15 2015
Response via : Initial Calibration

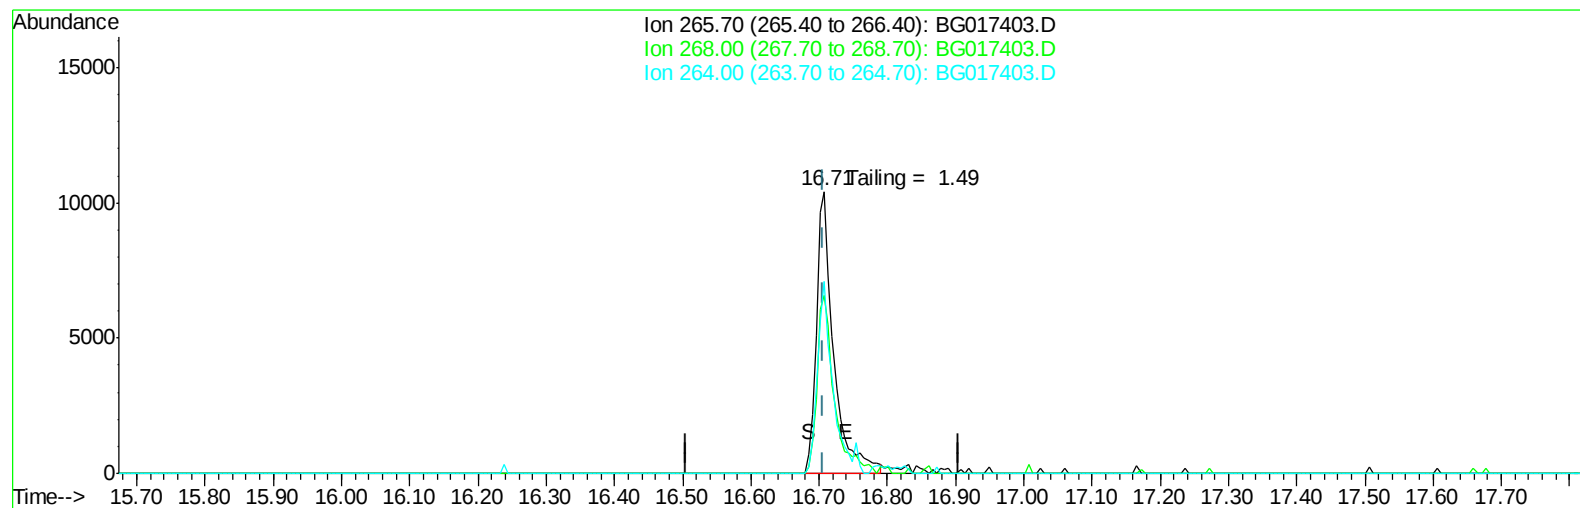

TIC: BG017403.D

(69) Pentachlorophenol (C)



16.708min (+0.002) 0.00ng

response 18779

Ion	Exp%	Act%
265.70	100	100
268.00	58.80	63.03
264.00	57.10	68.05
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG060315\
Data File : BG017403.D
Acq On : 3 Jun 2015 12:24
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 04 06:42:55 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 04 01:31:15 2015
Response via : Initial Calibration

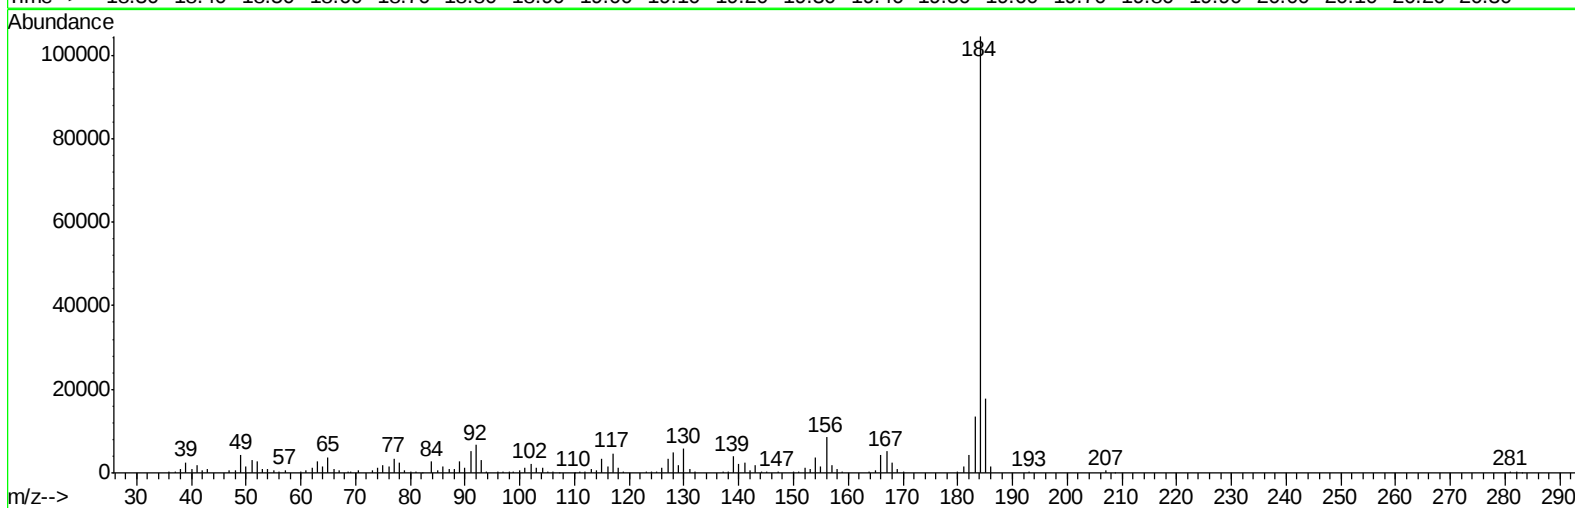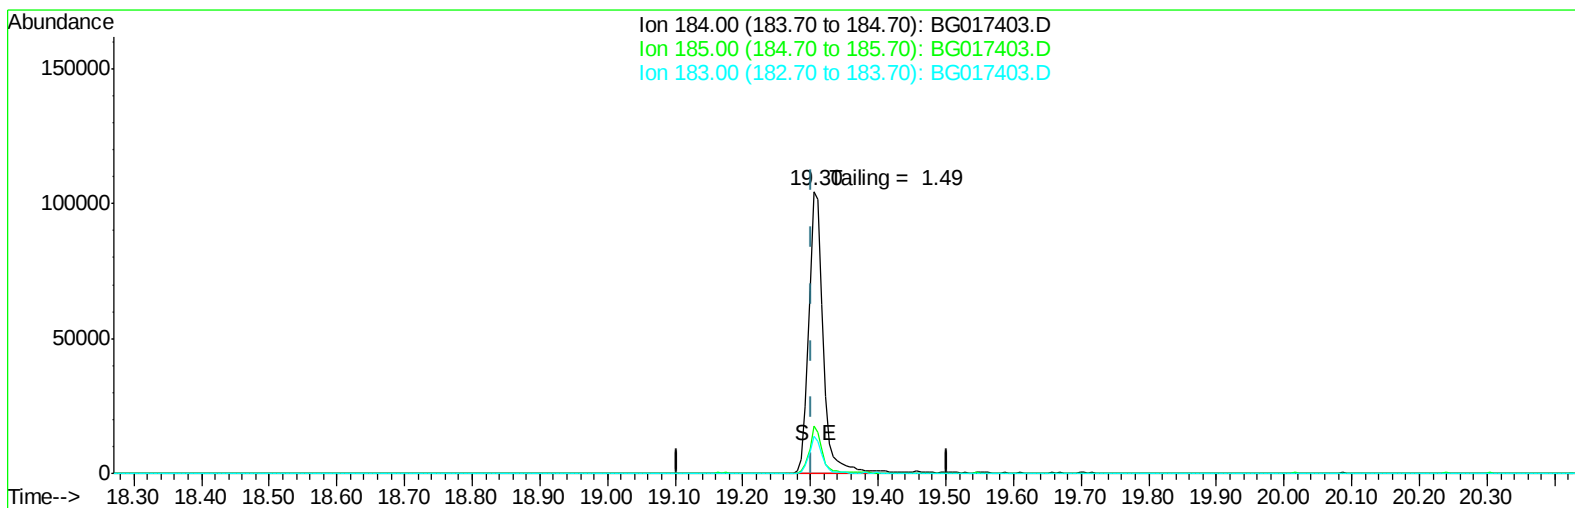

TIC: BG017403.D

(76) Benzidine

19.305min (+0.002) 24744.72ng

response 154779

Ion	Exp%	Act%
184.00	100	100
185.00	13.80	17.01#
183.00	12.30	12.99
0.00	0.00	0.00