
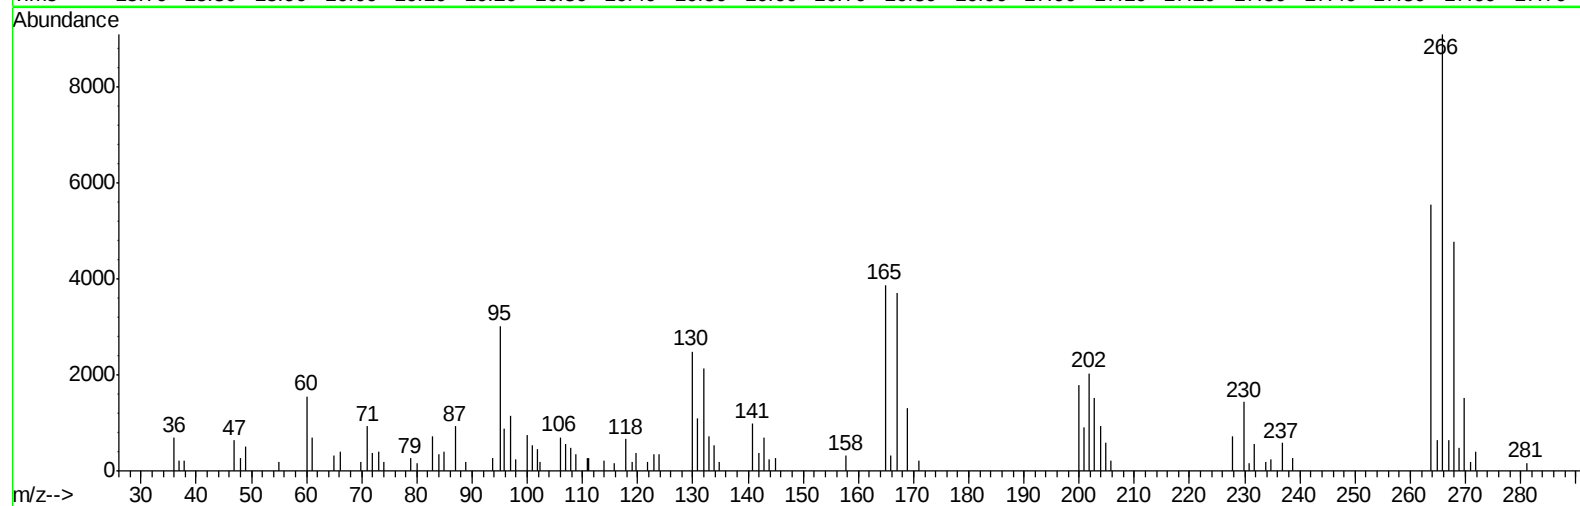


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG060315\
Data File : BG017421.D
Acq On : 4 Jun 2015 00:30
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 04 06:44:01 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 04 01:31:15 2015
Response via : Initial Calibration

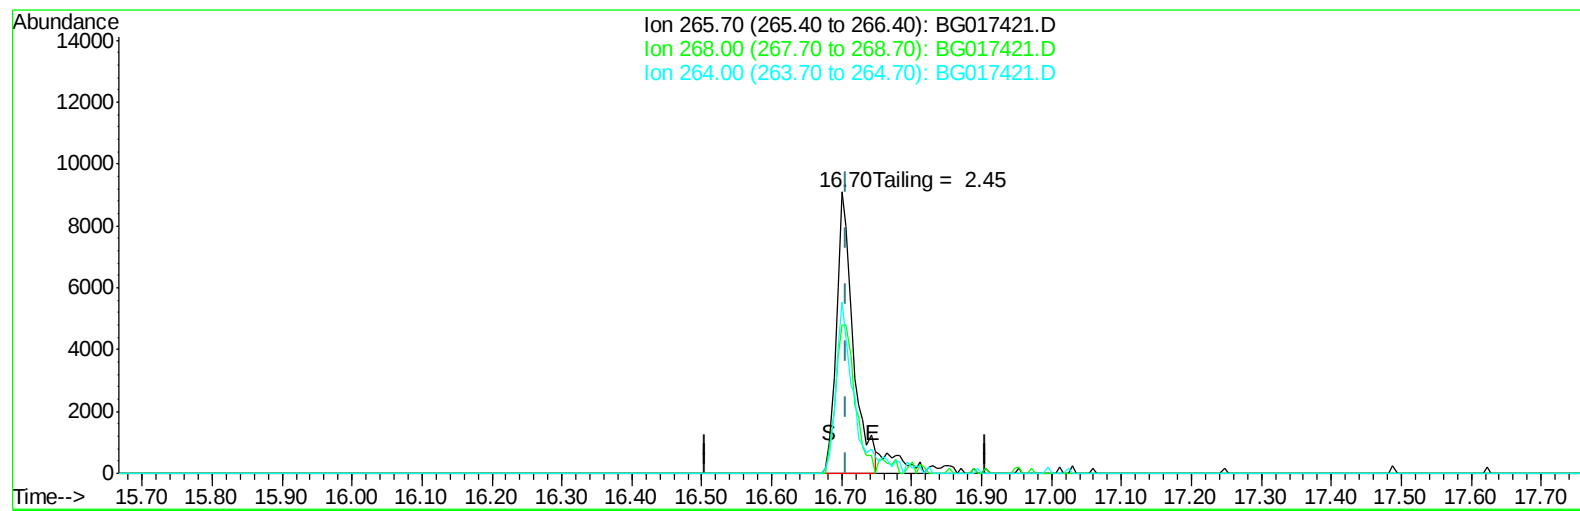

TIC: BG017421.D

(69) Pentachlorophenol (C)



16.701min (-0.005) 0.00ng m

response 14977

Ion	Exp%	Act%
265.70	100	100
268.00	58.80	52.64
264.00	57.10	61.00
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG060315\
Data File : BG017421.D
Acq On : 4 Jun 2015 00:30
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 04 06:44:01 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 04 01:31:15 2015
Response via : Initial Calibration

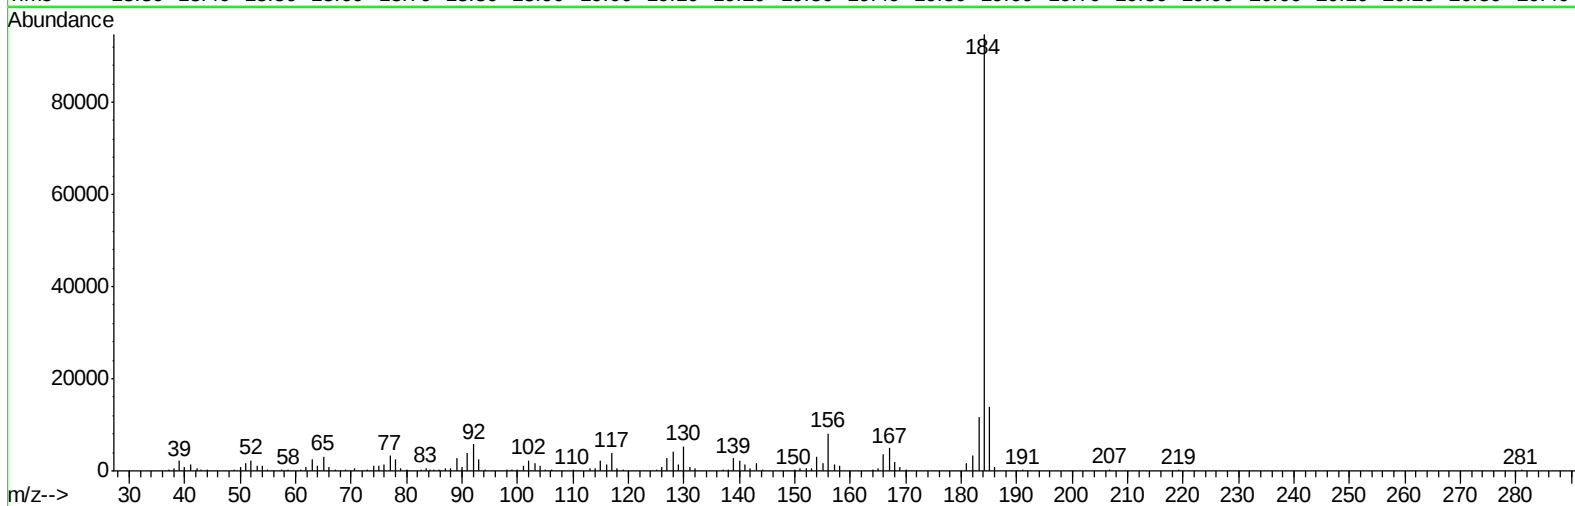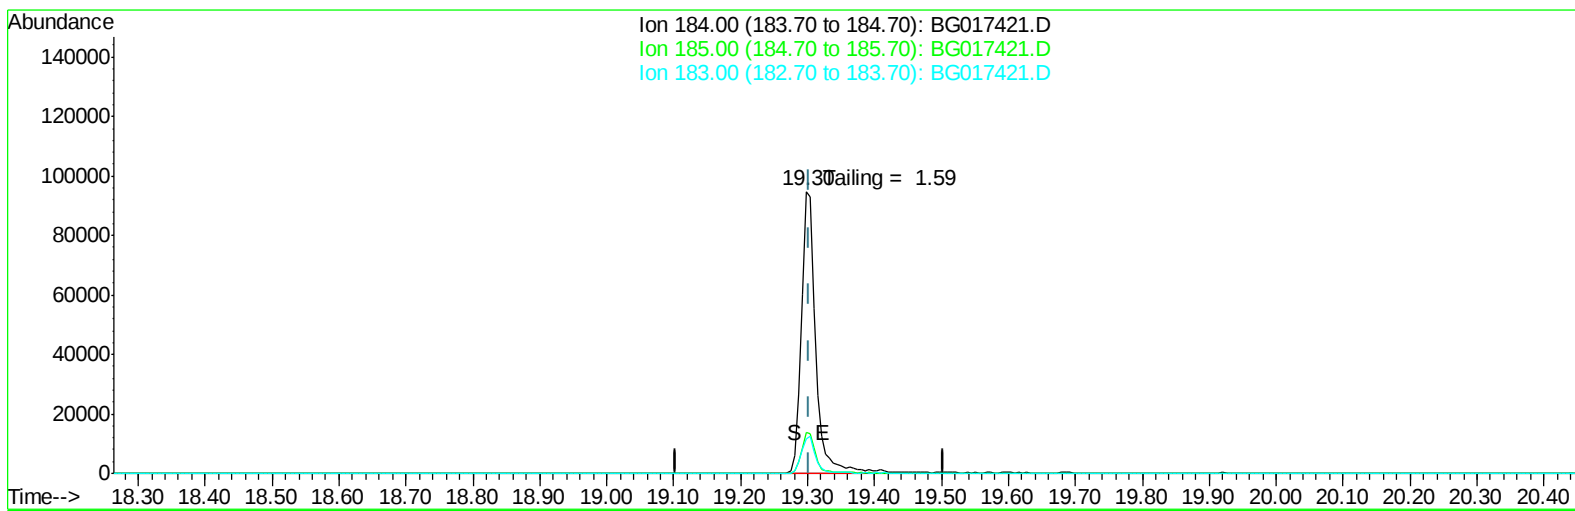

TIC: BG017421.D

(76) Benzidine

19.298min (-0.005) 0.00ng

response 145923

Ion	Exp%	Act%
184.00	100	100
185.00	13.80	14.55
183.00	12.30	12.29
0.00	0.00	0.00