


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG060315\
 Data File : BG017403.D
 Acq On : 3 Jun 2015 12:24
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060315.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jun 04 01:31:15 2015

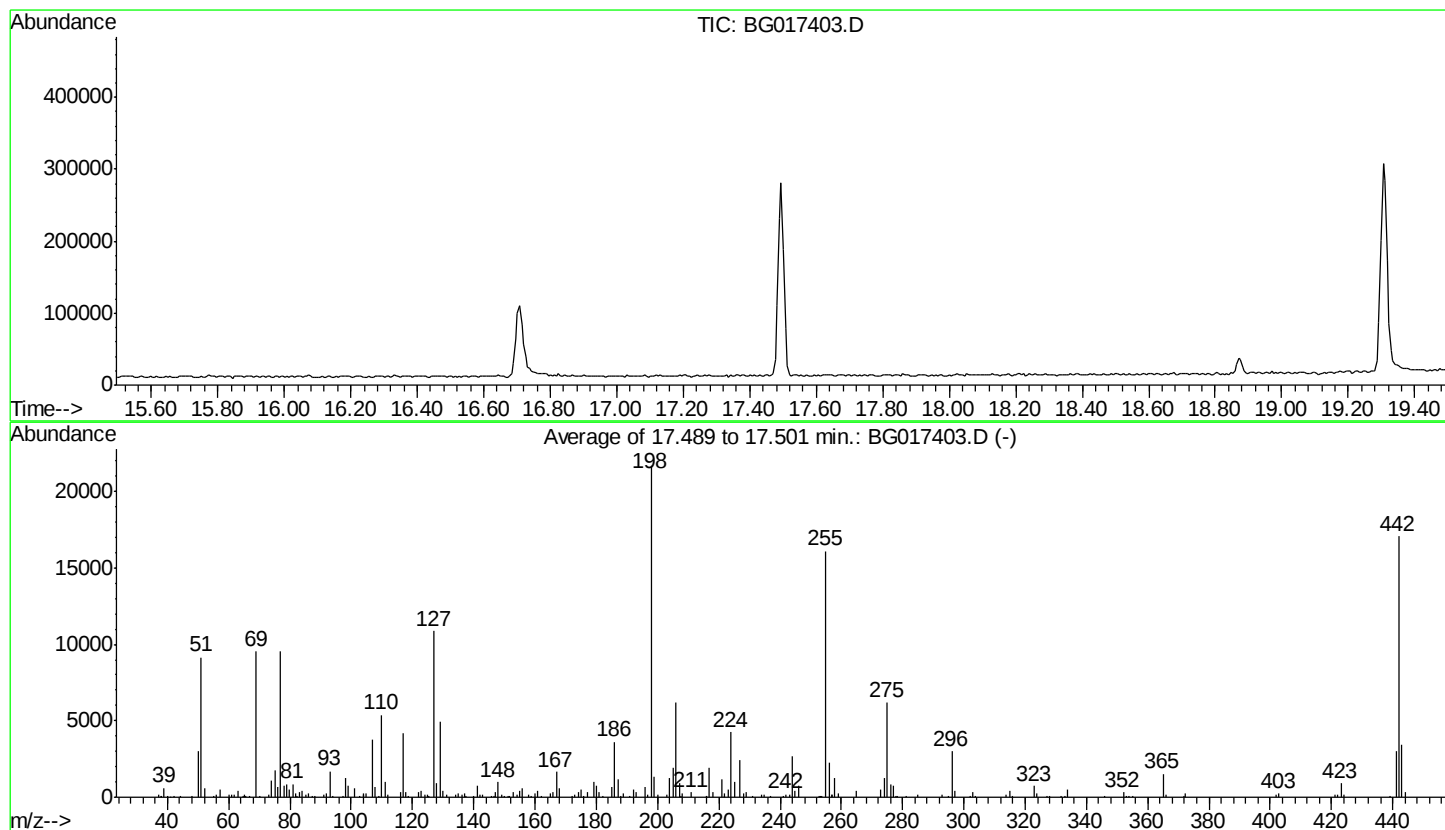

AutoFind: Scans 2519, 2520, 2521; Background Corrected with Scan 2513

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.2	9144	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	43.9	9523	PASS
70	69	0.00	2	0.5	52	PASS
127	198	10	80	50.0	10849	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	21682	PASS
199	198	5	9	6.2	1337	PASS
275	198	10	60	28.6	6192	PASS
365	198	1	100	7.1	1544	PASS
441	442	0.01	24	17.5	2990	PASS
442	198	50	100	78.7	17055	PASS
443	442	15	24	19.9	3393	PASS