


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG060315\
 Data File : BG017421.D
 Acq On : 4 Jun 2015 00:30
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060315.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jun 04 01:31:15 2015

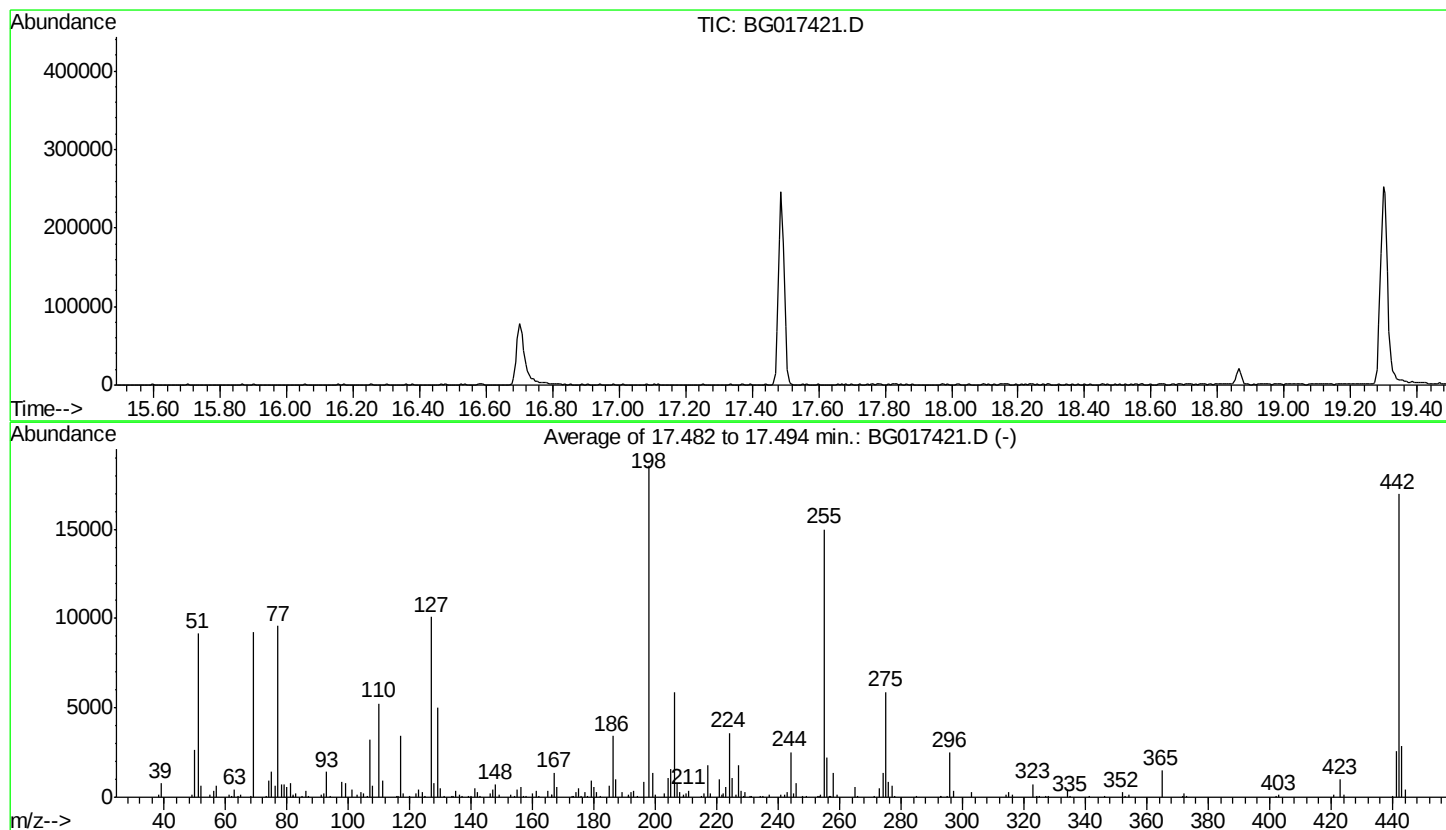

AutoFind: Scans 2518, 2519, 2520; Background Corrected with Scan 2512

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	49.3	9143	PASS
68	69	0.00	2	1.2	109	PASS
69	198	0.00	100	49.6	9213	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	54.3	10078	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	18558	PASS
199	198	5	9	7.2	1328	PASS
275	198	10	60	31.7	5883	PASS
365	198	1	100	8.0	1483	PASS
441	442	0.01	24	15.3	2605	PASS
442	198	50	100	91.5	16974	PASS
443	442	15	24	17.1	2901	PASS