
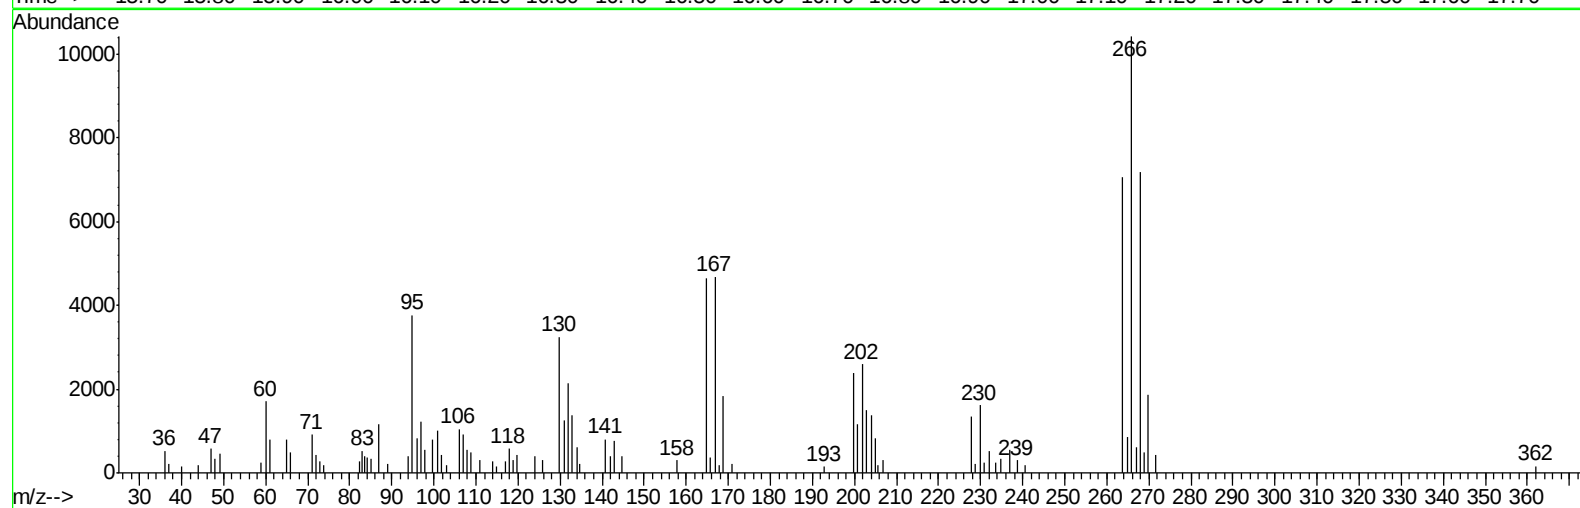


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG060415\
Data File : BG017439.D
Acq On : 4 Jun 2015 13:34
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 05 06:34:23 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 05 04:39:41 2015
Response via : Initial Calibration

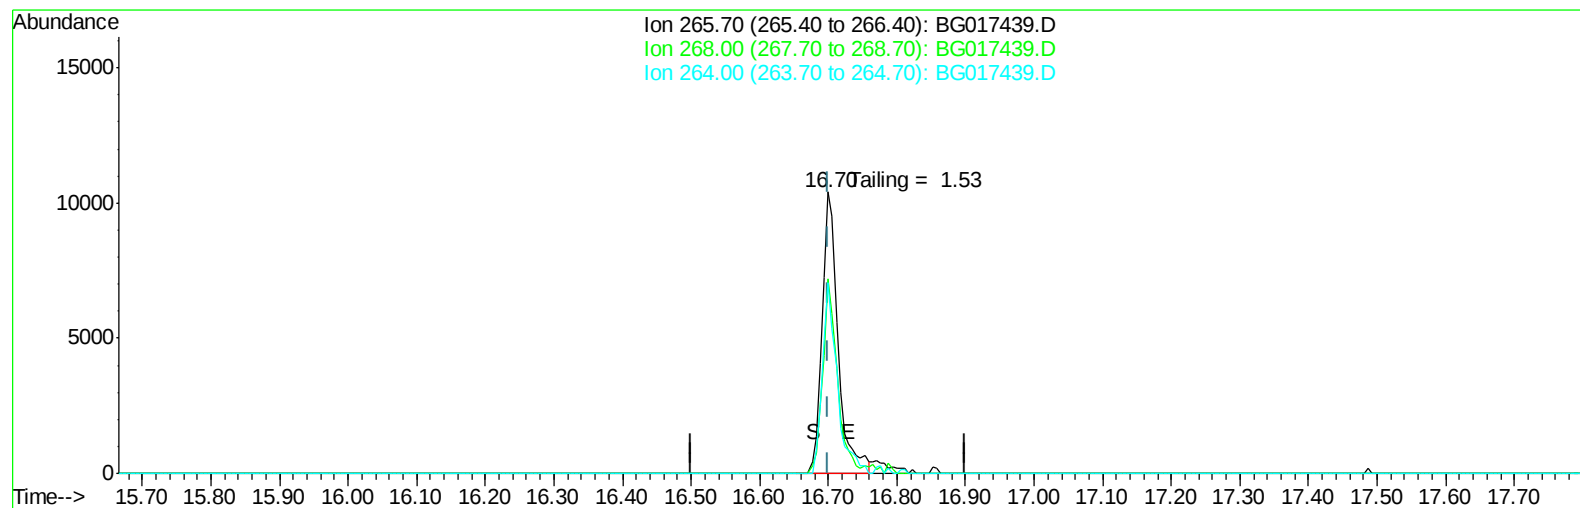

TIC: BG017439.D

(69) Pentachlorophenol (C)



16.700min (-0.001) 4970.81ng

response 17477

Ion	Exp%	Act%
265.70	100	100
268.00	58.80	69.06
264.00	57.10	67.76
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG060415\
Data File : BG017439.D
Acq On : 4 Jun 2015 13:34
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 05 06:34:23 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 05 04:39:41 2015
Response via : Initial Calibration

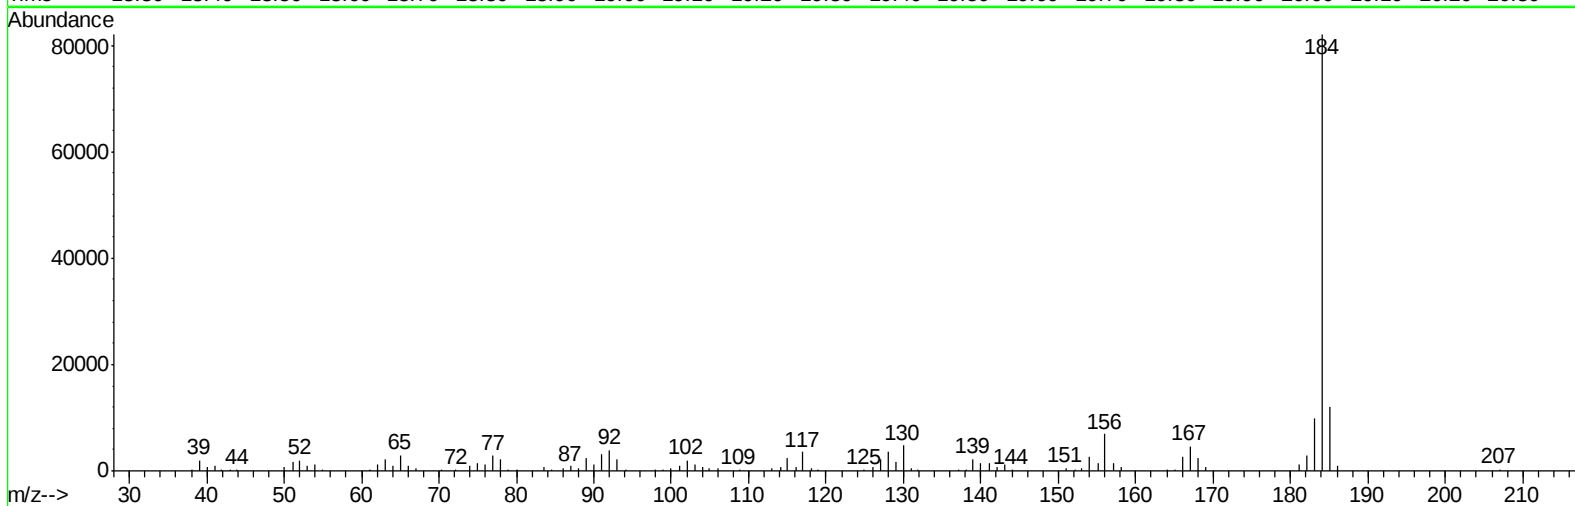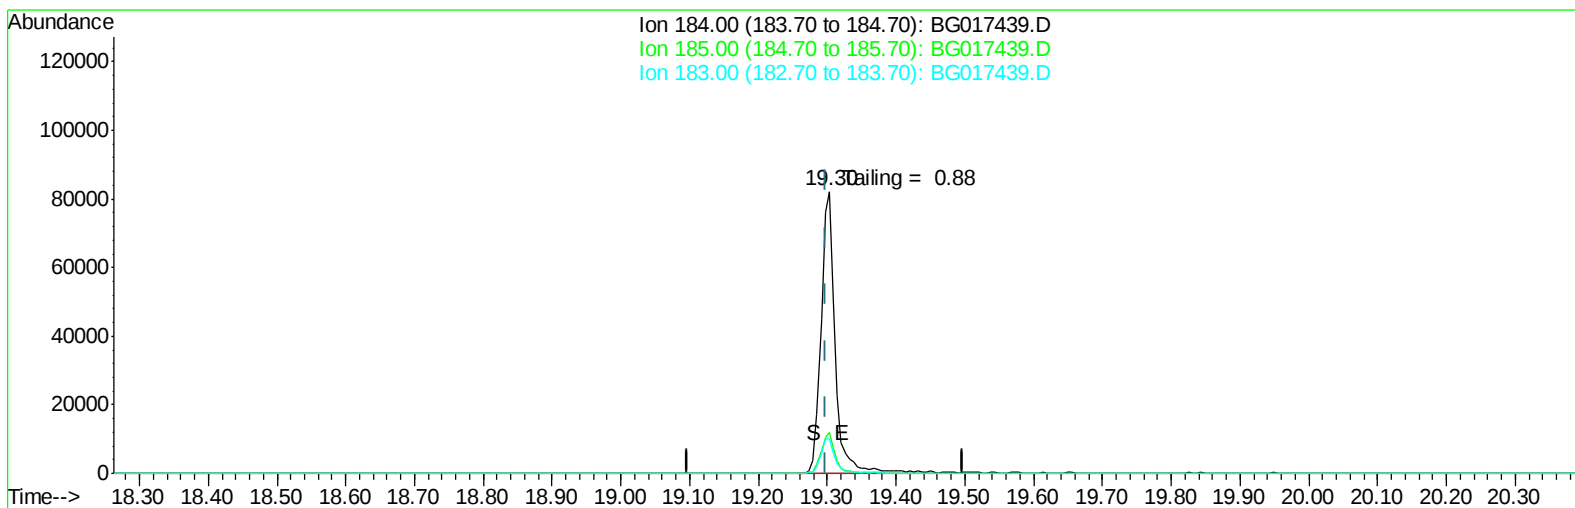

TIC: BG017439.D

(76) Benzidine

19.303min (+0.005) 7657.32ng

response 116847

Ion	Exp%	Act%
184.00	100	100
185.00	13.80	14.64
183.00	12.30	12.17
0.00	0.00	0.00