
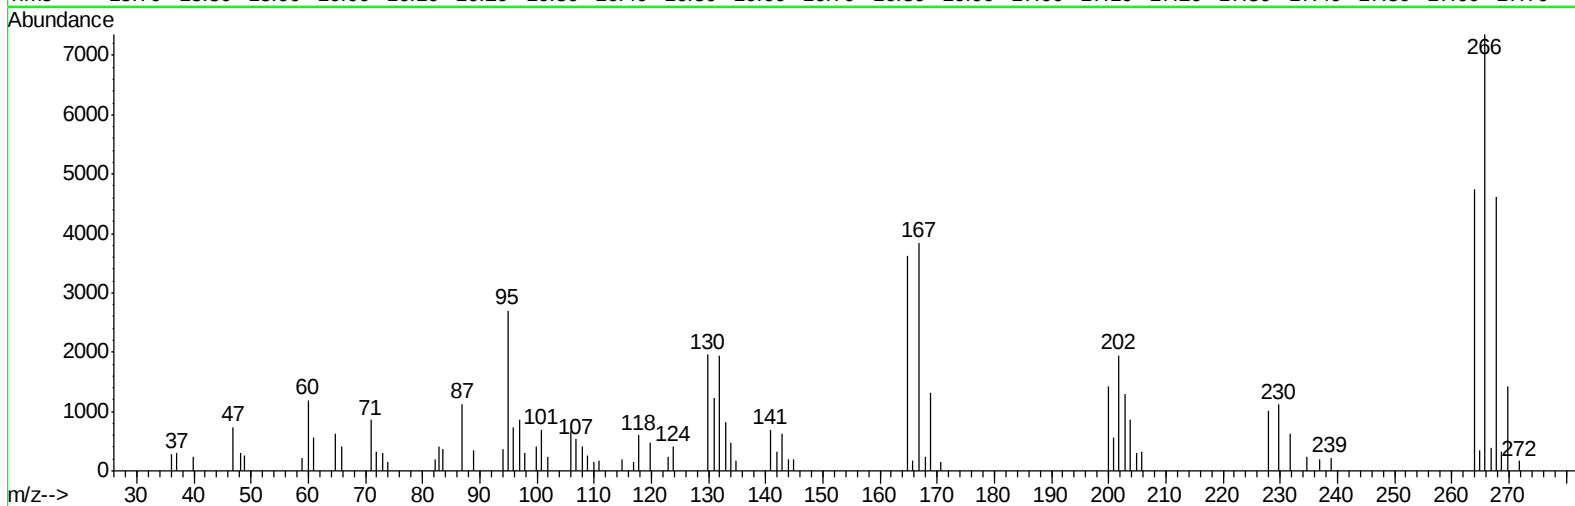


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG060415\
Data File : BG017457.D
Acq On : 5 Jun 2015 1:56
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 05 06:35:57 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 05 04:39:41 2015
Response via : Initial Calibration

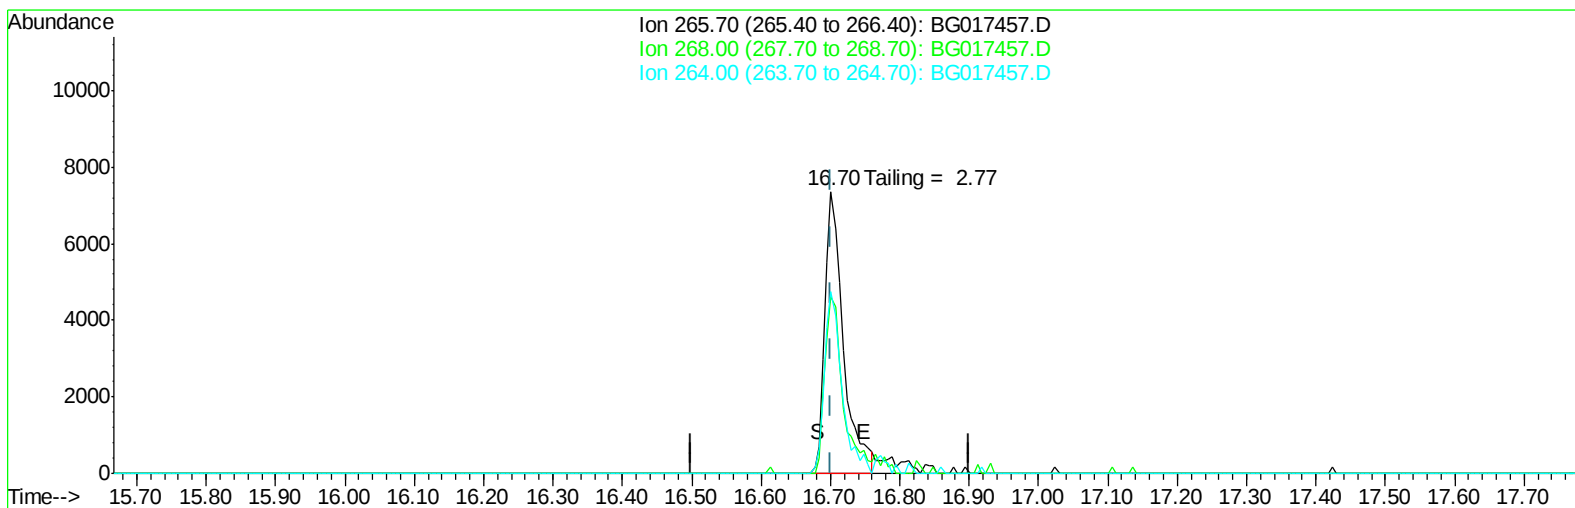

TIC: BG017457.D

(69) Pentachlorophenol (C)



16.701min (0.000) 33096.71ng

response 13977

Ion	Exp%	Act%
265.70	100	100
268.00	58.80	67.23
264.00	57.10	64.64
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG060415\
Data File : BG017457.D
Acq On : 5 Jun 2015 1:56
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 05 06:35:57 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 05 04:39:41 2015
Response via : Initial Calibration

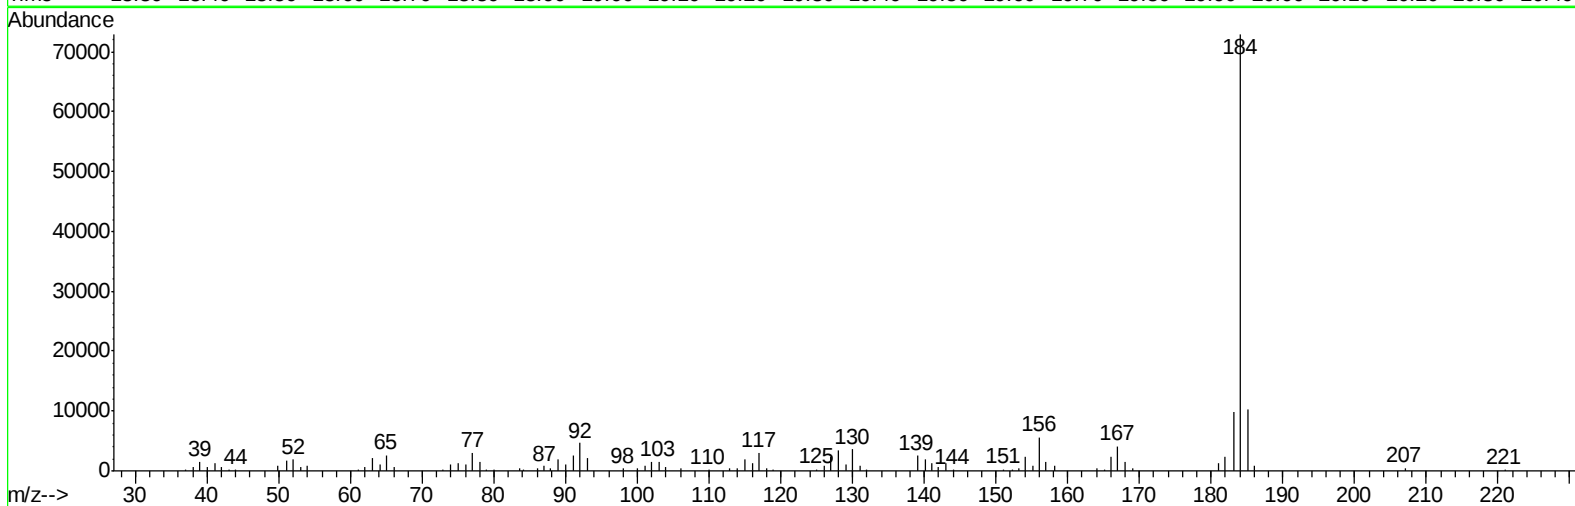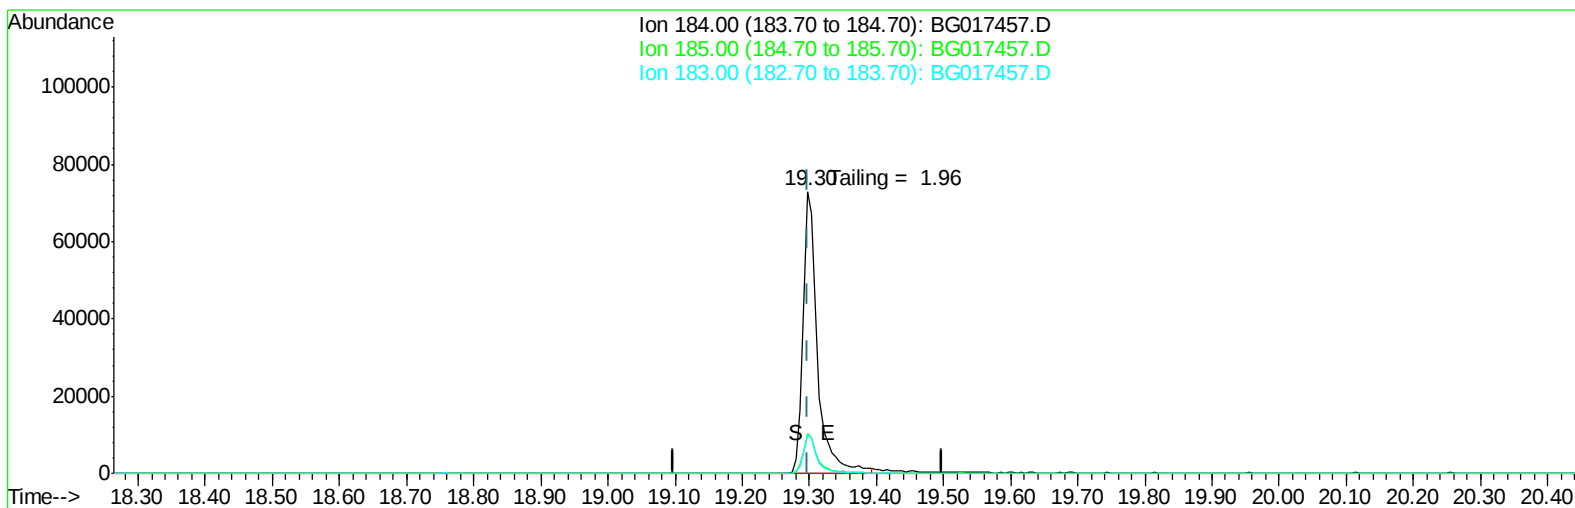

TIC: BG017457.D

(76) Benzidine

19.298min (0.000) 0.00ng

response 112467

Ion	Exp%	Act%
184.00	100	100
185.00	13.80	14.09
183.00	12.30	13.63
0.00	0.00	0.00