


Data Path : Z:\HPCHEM1\BNA G\Data\BG060415\
 Data File : BG017439.D
 Acq On : 4 Jun 2015 13:34
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060315.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jun 04 01:31:15 2015

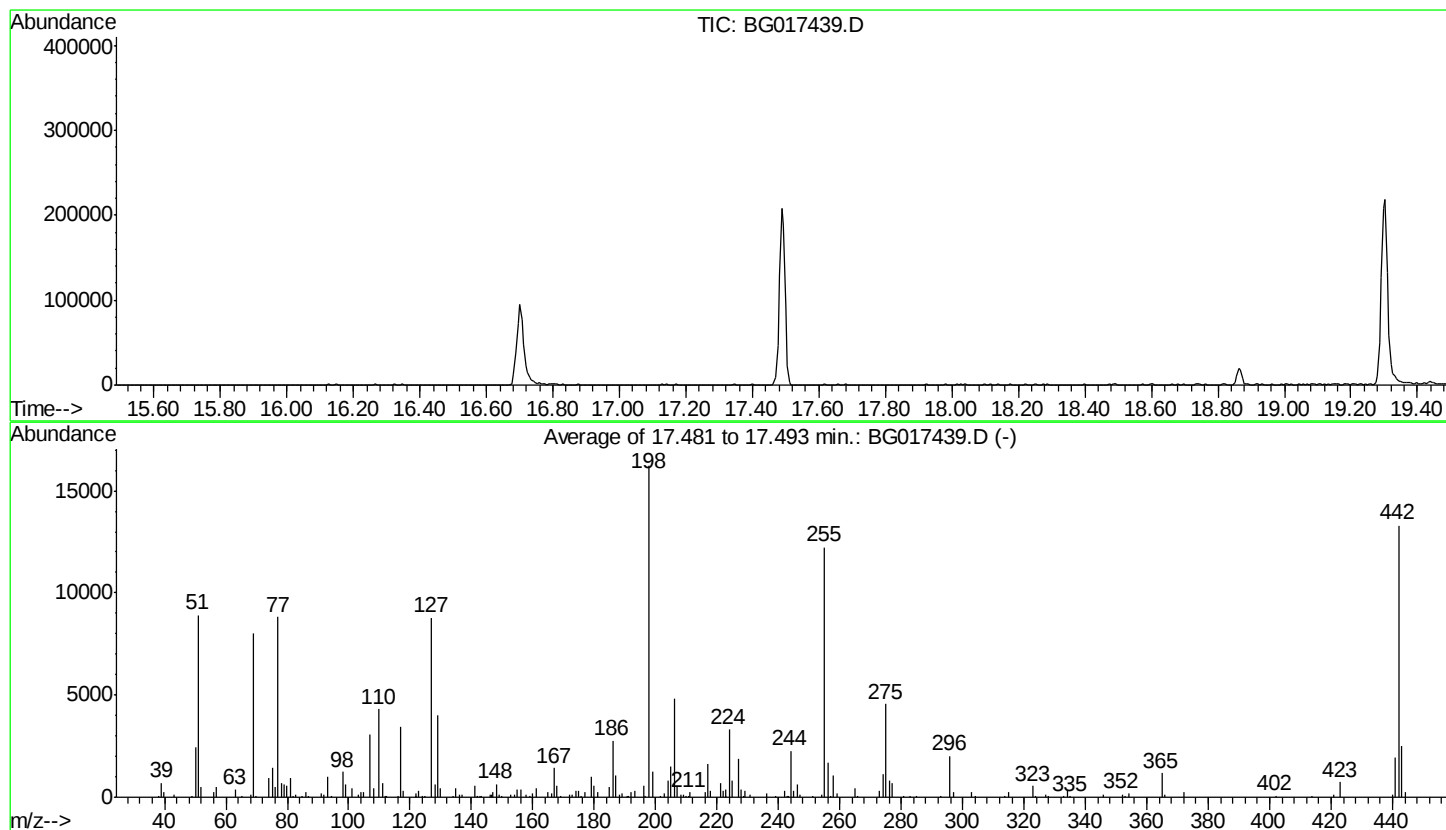

AutoFind: Scans 2518, 2519, 2520; Background Corrected with Scan 2512

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	54.9	8910	PASS
68	69	0.00	2	1.6	130	PASS
69	198	0.00	100	49.4	8014	PASS
70	69	0.00	2	0.6	52	PASS
127	198	10	80	54.2	8790	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	16228	PASS
199	198	5	9	7.9	1274	PASS
275	198	10	60	28.0	4545	PASS
365	198	1	100	7.3	1180	PASS
441	442	0.01	24	14.4	1915	PASS
442	198	50	100	81.9	13288	PASS
443	442	15	24	18.9	2517	PASS