


Data Path : Z:\HPCHEM1\BNA G\Data\BG060415\
 Data File : BG017457.D
 Acq On : 5 Jun 2015 1:56
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060315.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jun 04 01:31:15 2015

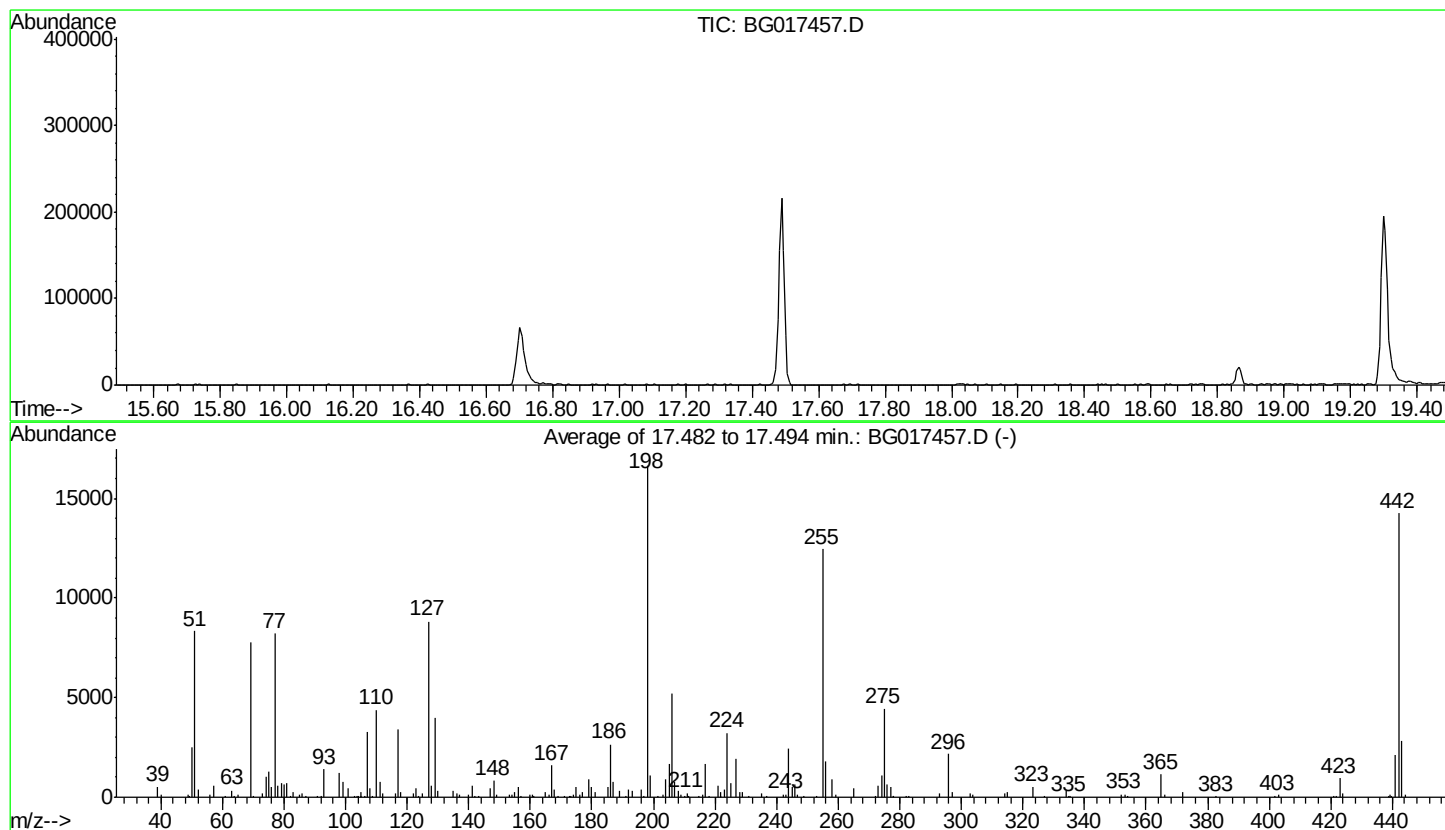

AutoFind: Scans 2518, 2519, 2520; Background Corrected with Scan 2512

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.1	8346	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	46.7	7772	PASS
70	69	0.00	2	1.0	75	PASS
127	198	10	80	52.9	8809	PASS
197	198	0.00	2	0.5	83	PASS
198	198	100	100	100.0	16646	PASS
199	198	5	9	6.5	1079	PASS
275	198	10	60	26.8	4463	PASS
365	198	1	100	6.9	1144	PASS
441	442	0.01	24	14.7	2100	PASS
442	198	50	100	85.6	14249	PASS
443	442	15	24	19.7	2802	PASS