
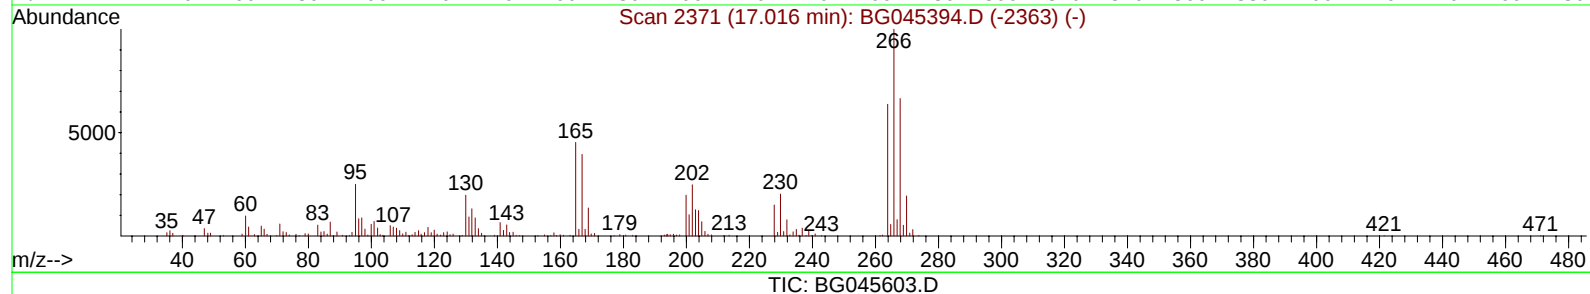
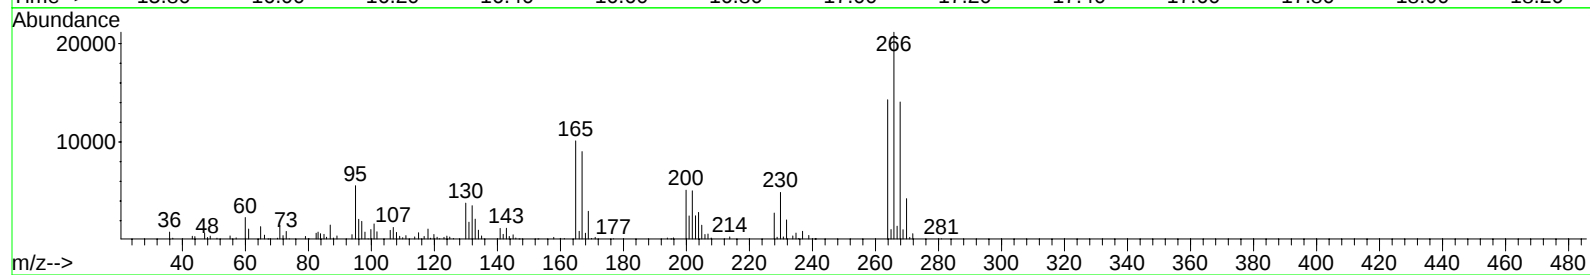


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG060420\
Data File : BG045603.D
Acq On : 4 Jun 2020 13:34
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 04 18:41:05 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG051520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 01 15:07:00 2020
Response via : Initial Calibration

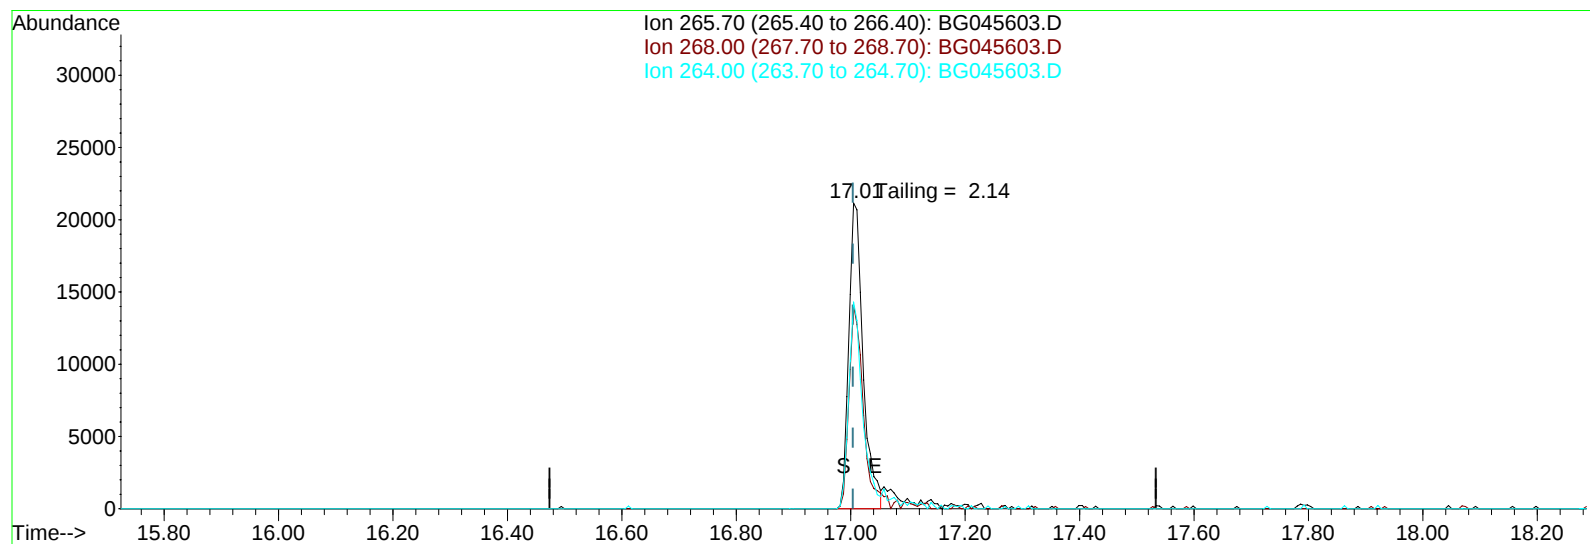

(70) Pentachlorophenol (C)




17.005min (+0.001) 0.00ng

response 39298

Ion	Exp%	Act%
265.70	100	100
268.00	66.50	66.49
264.00	63.70	67.61
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG060420\
Data File : BG045603.D
Acq On : 4 Jun 2020 13:34
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 04 18:41:05 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG051520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 01 15:07:00 2020
Response via : Initial Calibration

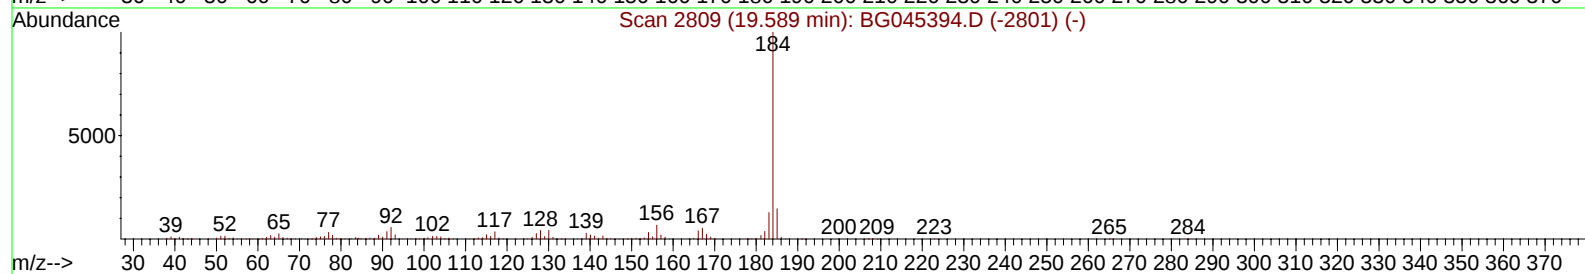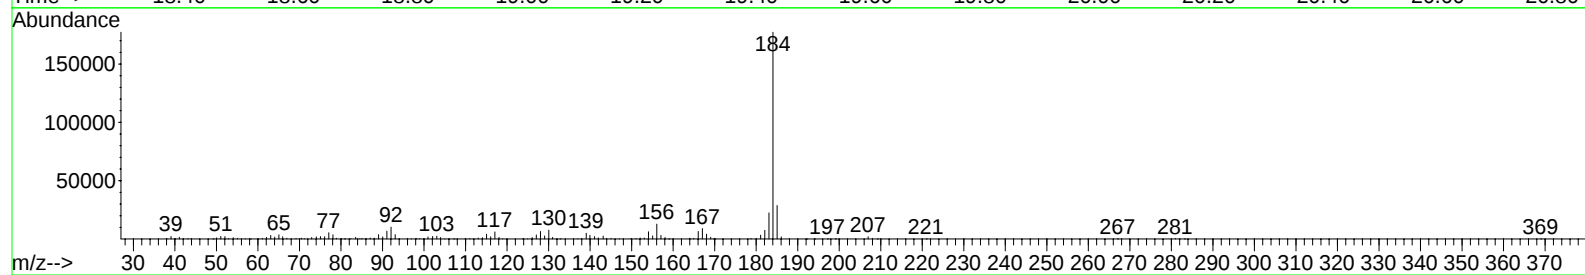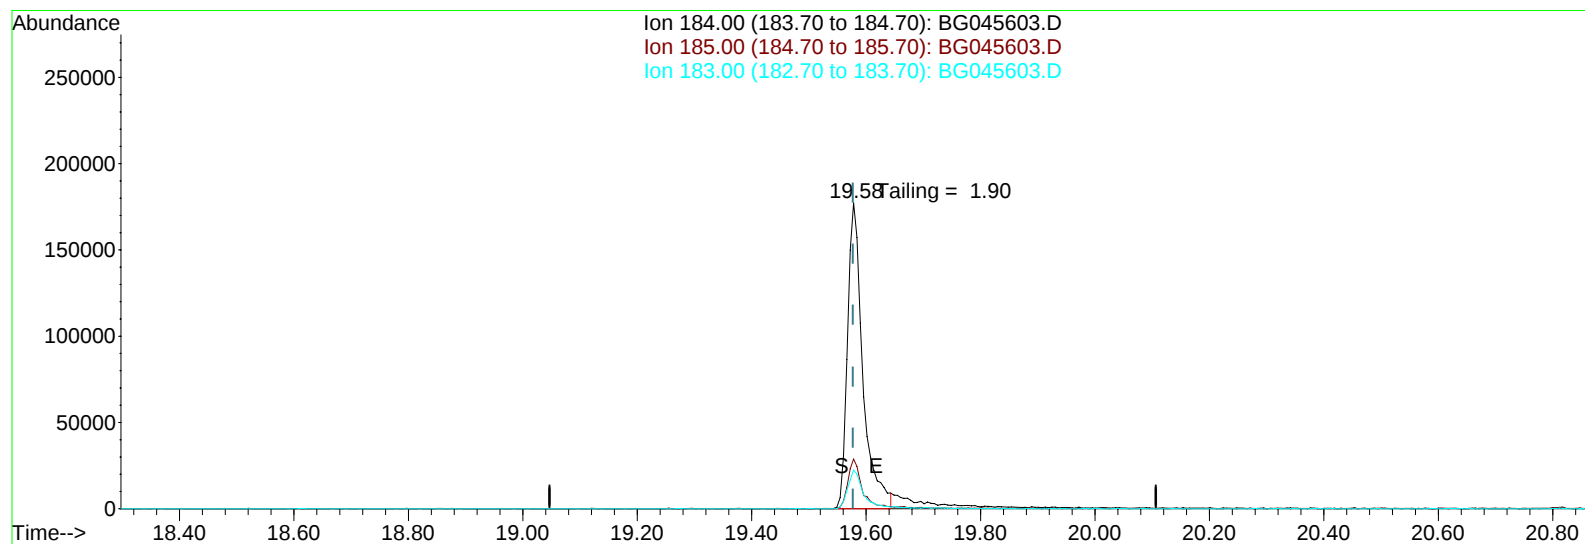

TIC: BG045603.D

(77) Benzidine

19.578min (+0.001) 0.00ng

response 346785

Ion	Exp%	Act%
184.00	100	100
185.00	14.60	16.25
183.00	12.80	12.66
0.00	0.00	0.00