

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060424\
 Data File : BG061486.D
 Acq On : 5 Jun 2024 14:30
 Operator : MA/JU
 Sample : PB161224BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK224

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG052124.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG061486.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.071	9	14	21	rVV3	20425	30060	3.60%	0.366%
2	3.330	54	58	64	rVB4	6258	8388	1.00%	0.102%
3	3.577	98	100	103	rBV2	718	880	0.11%	0.011%
4	3.600	103	104	110	rVB3	1232	1687	0.20%	0.021%
5	3.735	122	127	138	rBV	89764	154820	18.55%	1.885%
6	4.076	180	185	190	rVB3	1660	2646	0.32%	0.032%
7	4.346	228	231	234	rVB	879	1207	0.14%	0.015%
8	4.975	335	338	341	rVB	746	1019	0.12%	0.012%
9	7.067	685	694	705	rBV	115961	202247	24.23%	2.463%
10	7.202	710	717	726	rBV	79058	127207	15.24%	1.549%
11	7.413	746	753	763	rBV	116090	197385	23.65%	2.404%
12	7.877	825	832	838	rBV	108144	183605	22.00%	2.236%
13	8.594	948	954	963	rBV2	147135	260337	31.19%	3.171%
14	9.035	1021	1029	1036	rBV	123555	217480	26.05%	2.649%
15	9.752	1143	1151	1160	rVB2	94562	169008	20.25%	2.058%
16	10.310	1236	1246	1259	rBV	126199	234350	28.08%	2.854%
17	10.668	1298	1307	1319	rBB	136357	235182	28.18%	2.864%
18	10.809	1324	1331	1338	rBV	128823	233636	27.99%	2.845%
19	12.261	1573	1578	1582	rVB4	1385	2353	0.28%	0.029%
20	13.917	1854	1860	1866	rBV	243856	336769	40.35%	4.101%
21	13.964	1866	1868	1873	rVB	1600	1626	0.19%	0.020%
22	14.205	1902	1909	1917	rBV2	252239	397820	47.66%	4.845%
23	14.511	1954	1961	1971	rBV	218515	333139	39.91%	4.057%
24	14.758	1998	2003	2016	rBV	55748	119277	14.29%	1.453%
25	14.875	2021	2023	2025	rVB2	956	870	0.10%	0.011%
26	15.510	2124	2131	2142	rBV	338449	500469	59.96%	6.095%
27	15.657	2150	2156	2165	rBV	72203	119656	14.33%	1.457%
28	15.745	2168	2171	2177	rVB2	1887	1834	0.22%	0.022%
29	17.261	2423	2429	2437	rBV	313085	471387	56.47%	5.741%
30	17.360	2440	2446	2454	rBV	438058	636677	76.27%	7.754%
31	17.966	2547	2549	2553	rVB	1096	1133	0.14%	0.014%
32	18.160	2579	2582	2584	rBV	864	1138	0.14%	0.014%
33	18.230	2587	2594	2595	rBV2	1189	1483	0.18%	0.018%
34	18.776	2683	2687	2690	rVB3	755	1240	0.15%	0.015%
35	18.882	2700	2705	2707	rVB3	745	1217	0.15%	0.015%
36	19.105	2738	2743	2744	rBV2	719	881	0.11%	0.011%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060424\
 Data File : BG061486.D
 Acq On : 5 Jun 2024 14:30
 Operator : MA/JU
 Sample : PB161224BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK224

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG052124.MA.M
 Title : SVOA CALIBRATION

37	19.152	2748	2751	2752	rBV2	953	991	0.12%	0.012%
38	19.223	2755	2763	2768	rBV2	6263	9205	1.10%	0.112%
39	19.294	2771	2775	2781	rVB	5864	7388	0.89%	0.090%
40	19.435	2795	2799	2801	rVB4	1436	1793	0.21%	0.022%
41	19.452	2801	2802	2805	rBV3	1351	1556	0.19%	0.019%
42	19.482	2805	2807	2809	rBV2	1120	1056	0.13%	0.013%
43	19.540	2815	2817	2819	rVB3	1205	952	0.11%	0.012%
44	19.576	2819	2823	2828	rBV6	2152	3946	0.47%	0.048%
45	19.658	2829	2837	2847	rBV	525908	734033	87.94%	8.940%
46	19.728	2847	2849	2851	rVV2	2151	2268	0.27%	0.028%
47	19.764	2853	2855	2858	rVB3	1625	1353	0.16%	0.016%
48	19.787	2858	2859	2861	rBV2	1671	1195	0.14%	0.015%
49	19.828	2864	2866	2869	rVB3	2233	1675	0.20%	0.020%
50	19.852	2869	2870	2872	rBV	2294	1593	0.19%	0.019%
51	19.875	2872	2874	2876	rVB	1190	906	0.11%	0.011%
52	19.910	2878	2880	2883	rBV4	1822	2447	0.29%	0.030%
53	19.993	2892	2894	2895	rBV2	1340	925	0.11%	0.011%
54	20.034	2899	2901	2903	rVB3	1790	1151	0.14%	0.014%
55	20.093	2908	2911	2912	rBV3	2013	1989	0.24%	0.024%
56	20.145	2919	2920	2923	rVB3	2022	1386	0.17%	0.017%
57	20.181	2923	2926	2927	rBV3	2033	1678	0.20%	0.020%
58	20.239	2934	2936	2939	rBV3	2039	2044	0.24%	0.025%
59	20.281	2942	2943	2946	rVB3	2207	1686	0.20%	0.021%
60	20.304	2946	2947	2949	rBV2	1994	1605	0.19%	0.020%
61	20.351	2953	2955	2958	rBV4	1936	2358	0.28%	0.029%
62	20.433	2968	2969	2971	rBV2	2064	1902	0.23%	0.023%
63	20.474	2974	2976	2978	rVV3	1731	1392	0.17%	0.017%
64	20.574	2991	2993	2995	rBV3	2781	2018	0.24%	0.025%
65	20.768	3024	3026	3027	rVB2	2842	1242	0.15%	0.015%
66	20.851	3039	3040	3042	rBV2	2980	2336	0.28%	0.028%
67	20.886	3044	3046	3047	rBV2	2417	1746	0.21%	0.021%
68	21.315	3117	3119	3121	rBV3	3216	3518	0.42%	0.043%
69	21.373	3127	3129	3130	rBV2	3830	2163	0.26%	0.026%
70	21.415	3133	3136	3138	rBV3	3996	5194	0.62%	0.063%
71	21.456	3142	3143	3147	rBV4	5458	7351	0.88%	0.090%
72	21.520	3147	3154	3162	rBV2	365967	592885	71.03%	7.221%
73	21.785	3197	3199	3201	rBV3	4356	3437	0.41%	0.042%
74	22.678	3350	3351	3352	rVB	5407	1906	0.23%	0.023%
75	22.948	3394	3397	3401	rVB4	10849	16722	2.00%	0.204%
76	23.277	3452	3453	3456	rVB3	6455	4445	0.53%	0.054%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060424\
 Data File : BG061486.D
 Acq On : 5 Jun 2024 14:30
 Operator : MA/JU
 Sample : PB161224BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK224

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG052124.MA.M
 Title : SVOA CALIBRATION

77	23.342	3462	3464	3465	rBV2	4086	3040	0.36%	0.037%
78	23.712	3522	3527	3533	rVB7	13773	30137	3.61%	0.367%
79	24.405	3635	3645	3664	rBV	300459	834717	100.00%	10.166%
80	24.617	3671	3681	3695	rBV2	210979	604130	72.38%	7.357%
81	25.498	3829	3831	3832	rBV2	4987	2950	0.35%	0.036%
82	25.686	3854	3863	3866	rBV5	17022	45350	5.43%	0.552%
83	26.068	3926	3928	3931	rBV4	3589	2417	0.29%	0.029%
84	26.532	4005	4007	4009	rBV3	3964	4103	0.49%	0.050%
85	26.967	4076	4081	4082	rBV5	8927	15431	1.85%	0.188%
86	27.337	4142	4144	4146	rBV3	5879	6410	0.77%	0.078%
87	27.361	4146	4148	4150	rVV3	3586	2791	0.33%	0.034%
88	27.619	4191	4192	4193	rBV	4306	1829	0.22%	0.022%
89	28.494	4337	4341	4342	rBV4	7934	9427	1.13%	0.115%
90	29.558	4520	4522	4524	rVB3	4287	2117	0.25%	0.026%
91	29.722	4548	4550	4551	rBV2	4588	3338	0.40%	0.041%
92	29.905	4579	4581	4584	rBV4	4625	4806	0.58%	0.059%
93	30.140	4619	4621	4622	rBV2	3597	2090	0.25%	0.025%
94	30.580	4694	4696	4697	rBV2	3506	2438	0.29%	0.030%
95	30.721	4718	4720	4721	rBV2	3499	2189	0.26%	0.027%
96	31.526	4855	4857	4861	rBV4	3988	4419	0.53%	0.054%
97	32.472	5016	5018	5019	rBV2	3450	1434	0.17%	0.017%




Sum of corrected areas: 8211112

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060424\
Data File : BG061486.D
Acq On : 5 Jun 2024 14:30
Operator : MA/JU
Sample : PB161224BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK224

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG052124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

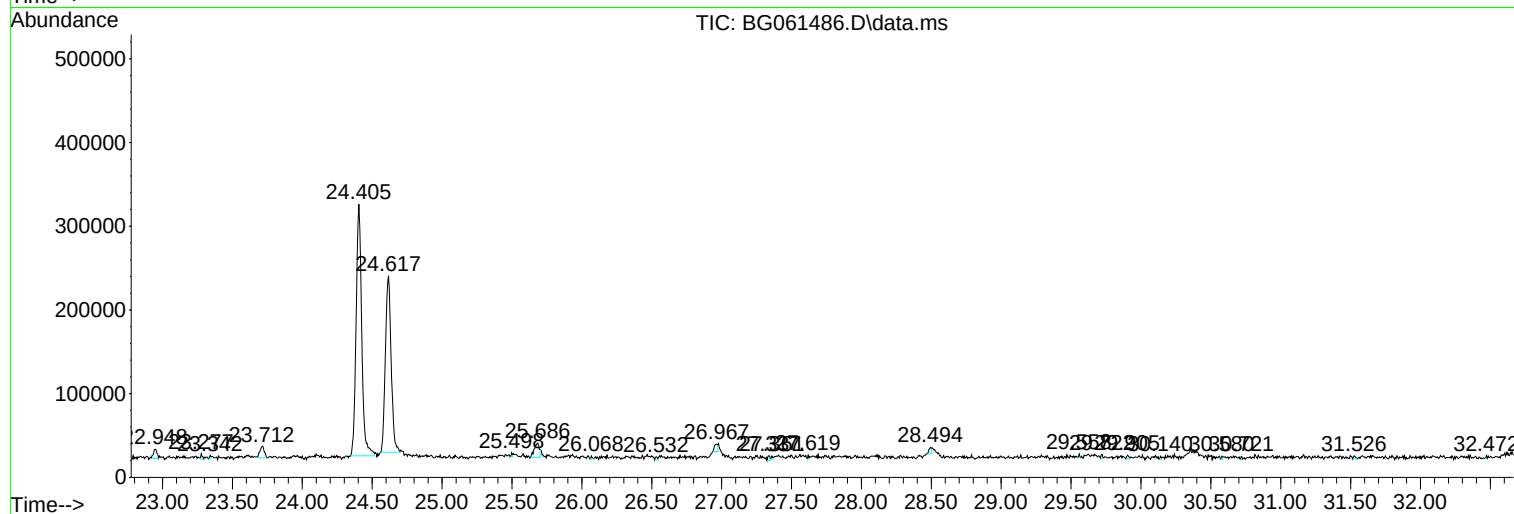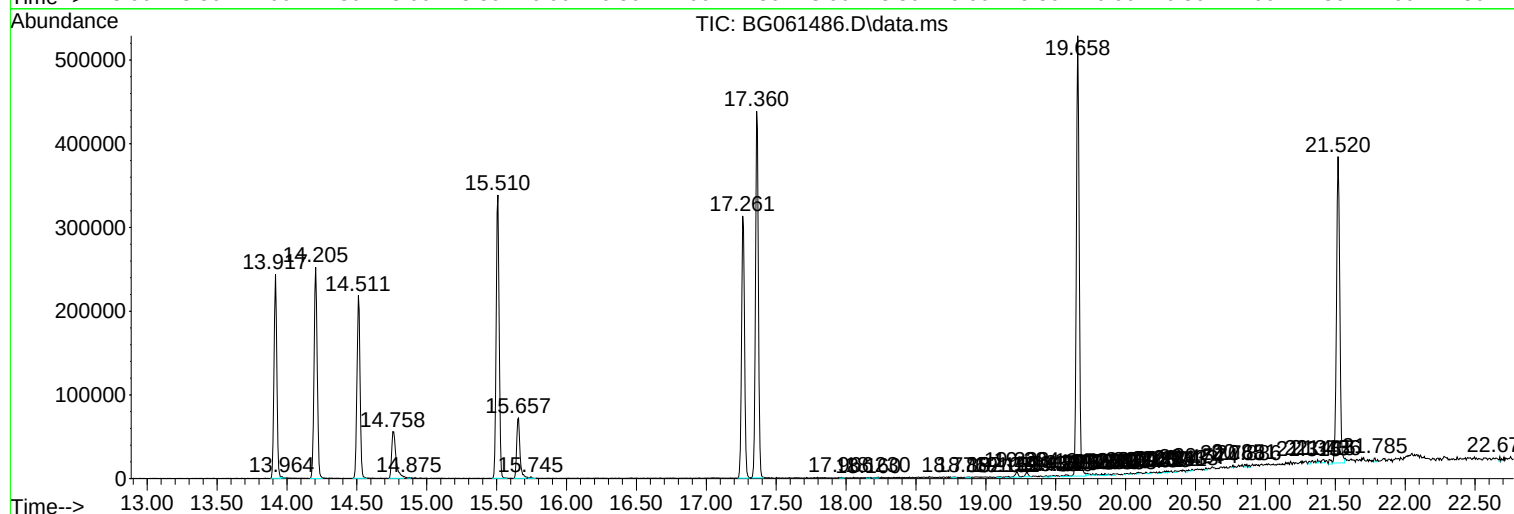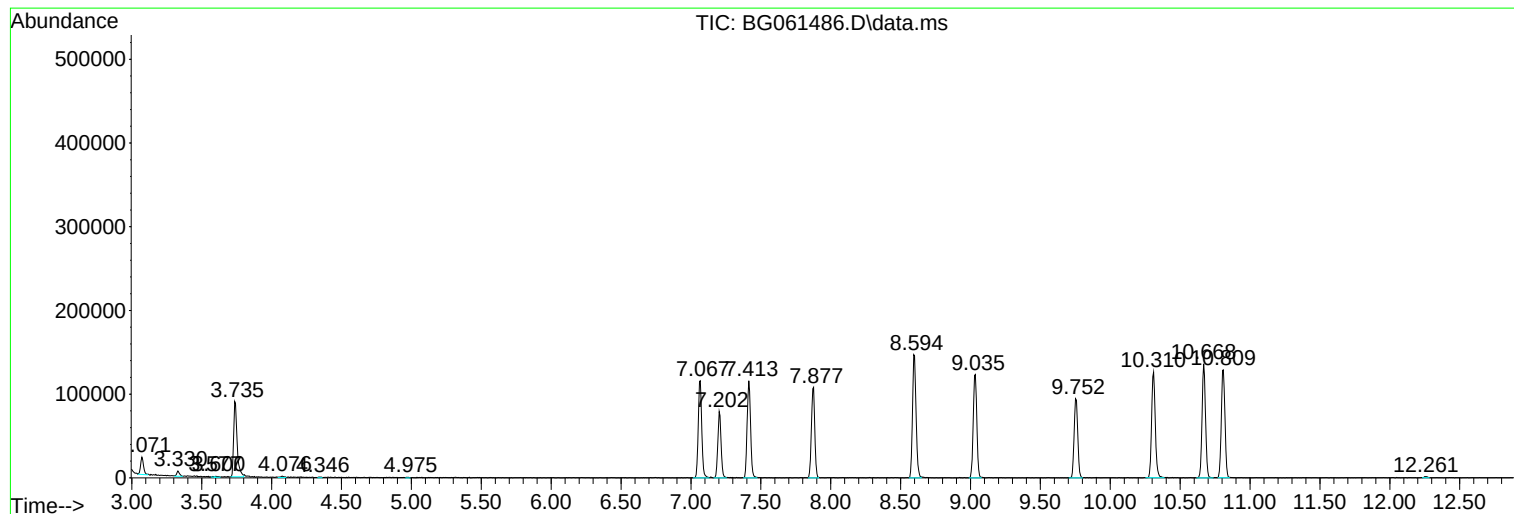

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060424\
Data File : BG061486.D
Acq On : 5 Jun 2024 14:30
Operator : MA/JU
Sample : PB161224BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK224










Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG052124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.071	3.27 ng/ul	30060	1,4-Dichlorobenzene-d4	7.877

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	72
2			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	50
3			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	39
4			3-Pentanol, 2,4-dimethyl-	116	C7H16O	000600-36-2	23
5			(R)-3-Pyrrolidinol	87	C4H9NO	002799-21-5	9

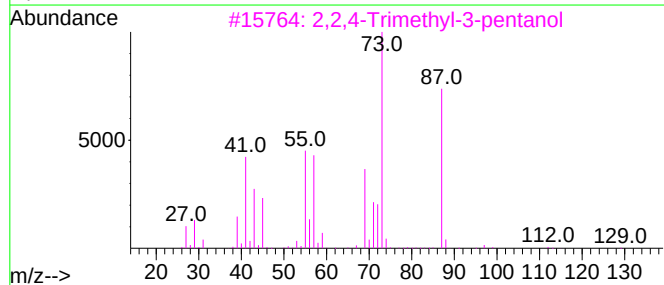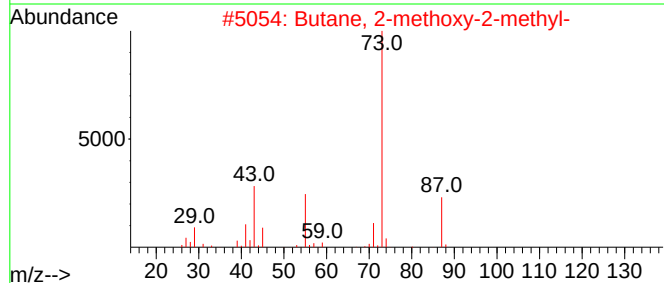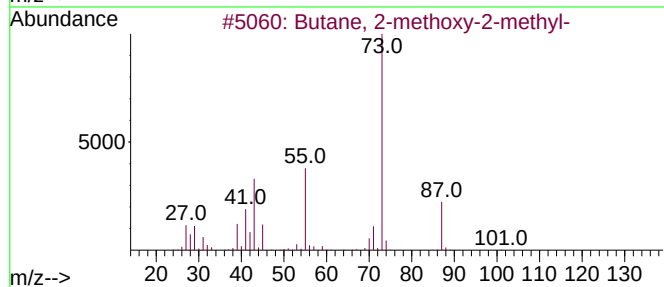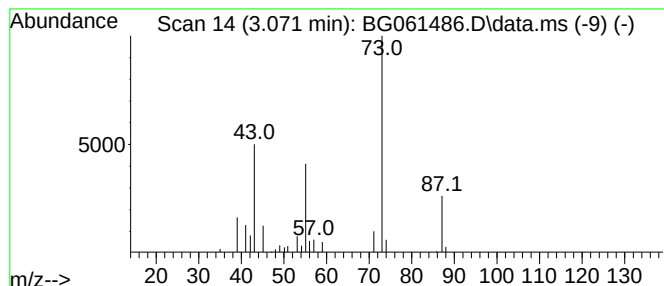

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG060424\
Data File : BG061486.D
Acq On : 5 Jun 2024 14:30
Operator : MA/JU
Sample : PB161224BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK224

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG052124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	3.071	3.3	ng/ul	30060	1	7.877	183605	20.0