

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG060515\
 Data File : BG017498.D
 Acq On : 6 Jun 2015 7:53
 Operator : TP/IZ
 Sample : G2518-01
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 WC060415

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060315.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.765	8	13	21	rBV	187531	250512	5.88%	0.710%
2	4.722	340	346	354	rBV	82979	121188	2.84%	0.344%
3	5.221	425	431	444	rBV	437653	663079	15.55%	1.880%
4	6.837	700	706	722	rBV	407023	678432	15.91%	1.924%
5	7.166	755	762	773	rBV	480730	761245	17.86%	2.158%
6	7.624	834	840	845	rVB	86856	137980	3.24%	0.391%
7	7.941	888	894	906	rVB	350875	550545	12.91%	1.561%
8	8.153	923	930	938	rVB	67169	106413	2.50%	0.302%
9	8.787	1029	1038	1046	rBV	292464	465496	10.92%	1.320%
10	9.269	1112	1120	1126	rBV2	29558	44913	1.05%	0.127%
11	9.340	1126	1132	1141	rVV3	64872	98387	2.31%	0.279%
12	9.951	1227	1236	1248	rBV	366474	568347	13.33%	1.611%
13	10.421	1309	1316	1319	rBV	113865	186433	4.37%	0.529%
14	10.468	1319	1324	1331	rVB	199816	325728	7.64%	0.924%
15	12.307	1631	1637	1646	rVB6	21614	44023	1.03%	0.125%
16	12.512	1666	1672	1681	rBV2	52147	83592	1.96%	0.237%
17	12.906	1733	1739	1750	rVB	715963	1057160	24.80%	2.997%
18	13.259	1793	1799	1812	rBV	618577	900141	21.12%	2.552%
19	14.293	1969	1975	1982	rBV2	186590	271403	6.37%	0.770%
20	15.010	2091	2097	2104	rBV2	32314	46655	1.09%	0.132%
21	15.192	2123	2128	2136	rVB4	31092	45262	1.06%	0.128%
22	15.368	2151	2158	2168	rBV	110944	161047	3.78%	0.457%
23	15.662	2204	2208	2212	rBV2	39618	47767	1.12%	0.135%
24	15.797	2224	2231	2240	rBV	709965	986030	23.13%	2.796%
25	15.950	2248	2257	2268	rBV	1666126	2077347	48.73%	5.890%
26	17.048	2438	2444	2449	rBV2	257822	353467	8.29%	1.002%
27	17.236	2471	2476	2486	rVB2	33667	47986	1.13%	0.136%
28	17.389	2495	2502	2512	rBV2	47327	65780	1.54%	0.187%
29	17.536	2521	2527	2533	rBV	168747	235757	5.53%	0.668%
30	17.959	2594	2599	2605	rBV3	35163	52686	1.24%	0.149%
31	18.035	2605	2612	2628	rVV	2578205	3307275	77.58%	9.377%
32	19.064	2783	2787	2792	rBV	40323	56250	1.32%	0.159%
33	19.193	2804	2809	2814	rBV2	56705	83806	1.97%	0.238%
34	19.310	2825	2829	2837	rBV	212693	266090	6.24%	0.754%

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG060515\
 Data File : BG017498.D
 Acq On : 6 Jun 2015 7:53
 Operator : TP/IZ
 Sample : G2518-01
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 WC060415

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060315.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	19.686	2888	2893	2895	rBV	1652424	2080382	48.80%	5.899%
36	19.716	2895	2898	2909	rVB	3162943	3909705	91.71%	11.085%
37	20.239	2981	2987	2992	rBV3	28172	50607	1.19%	0.143%
38	20.509	3028	3033	3039	rBV	40091	60287	1.41%	0.171%
39	20.621	3048	3052	3057	rBV	53692	72605	1.70%	0.206%
40	20.720	3064	3069	3079	rBV	202616	275582	6.46%	0.781%
41	21.061	3119	3127	3141	rBV	3646979	4262958	100.00%	12.087%
42	21.243	3153	3158	3163	rBV	370331	448676	10.52%	1.272%
43	21.490	3196	3200	3210	rBV3	31179	57305	1.34%	0.162%
44	21.578	3211	3215	3223	rVV	31190	54622	1.28%	0.155%
45	21.825	3254	3257	3263	rBV2	36549	53374	1.25%	0.151%
46	21.919	3269	3273	3285	rBV	131320	224740	5.27%	0.637%
47	22.277	3327	3334	3351	rBV	2434156	3587189	84.15%	10.171%
48	23.212	3487	3493	3499	rBV7	17680	43811	1.03%	0.124%
49	23.329	3508	3513	3530	rVB3	62951	149034	3.50%	0.423%
50	23.488	3533	3540	3547	rVB	243109	458090	10.75%	1.299%
51	23.817	3587	3596	3612	rBV	1272563	2662462	62.46%	7.549%
52	25.327	3847	3853	3858	rBV10	22602	52040	1.22%	0.148%
53	26.055	3965	3977	4001	rBV2	463219	1617593	37.95%	4.586%


Sum of corrected areas: 35269284

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG060515\
Data File : BG017498.D
Acq On : 6 Jun 2015 7:53
Operator : TP/IZ
Sample : G2518-01
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
WC060415

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

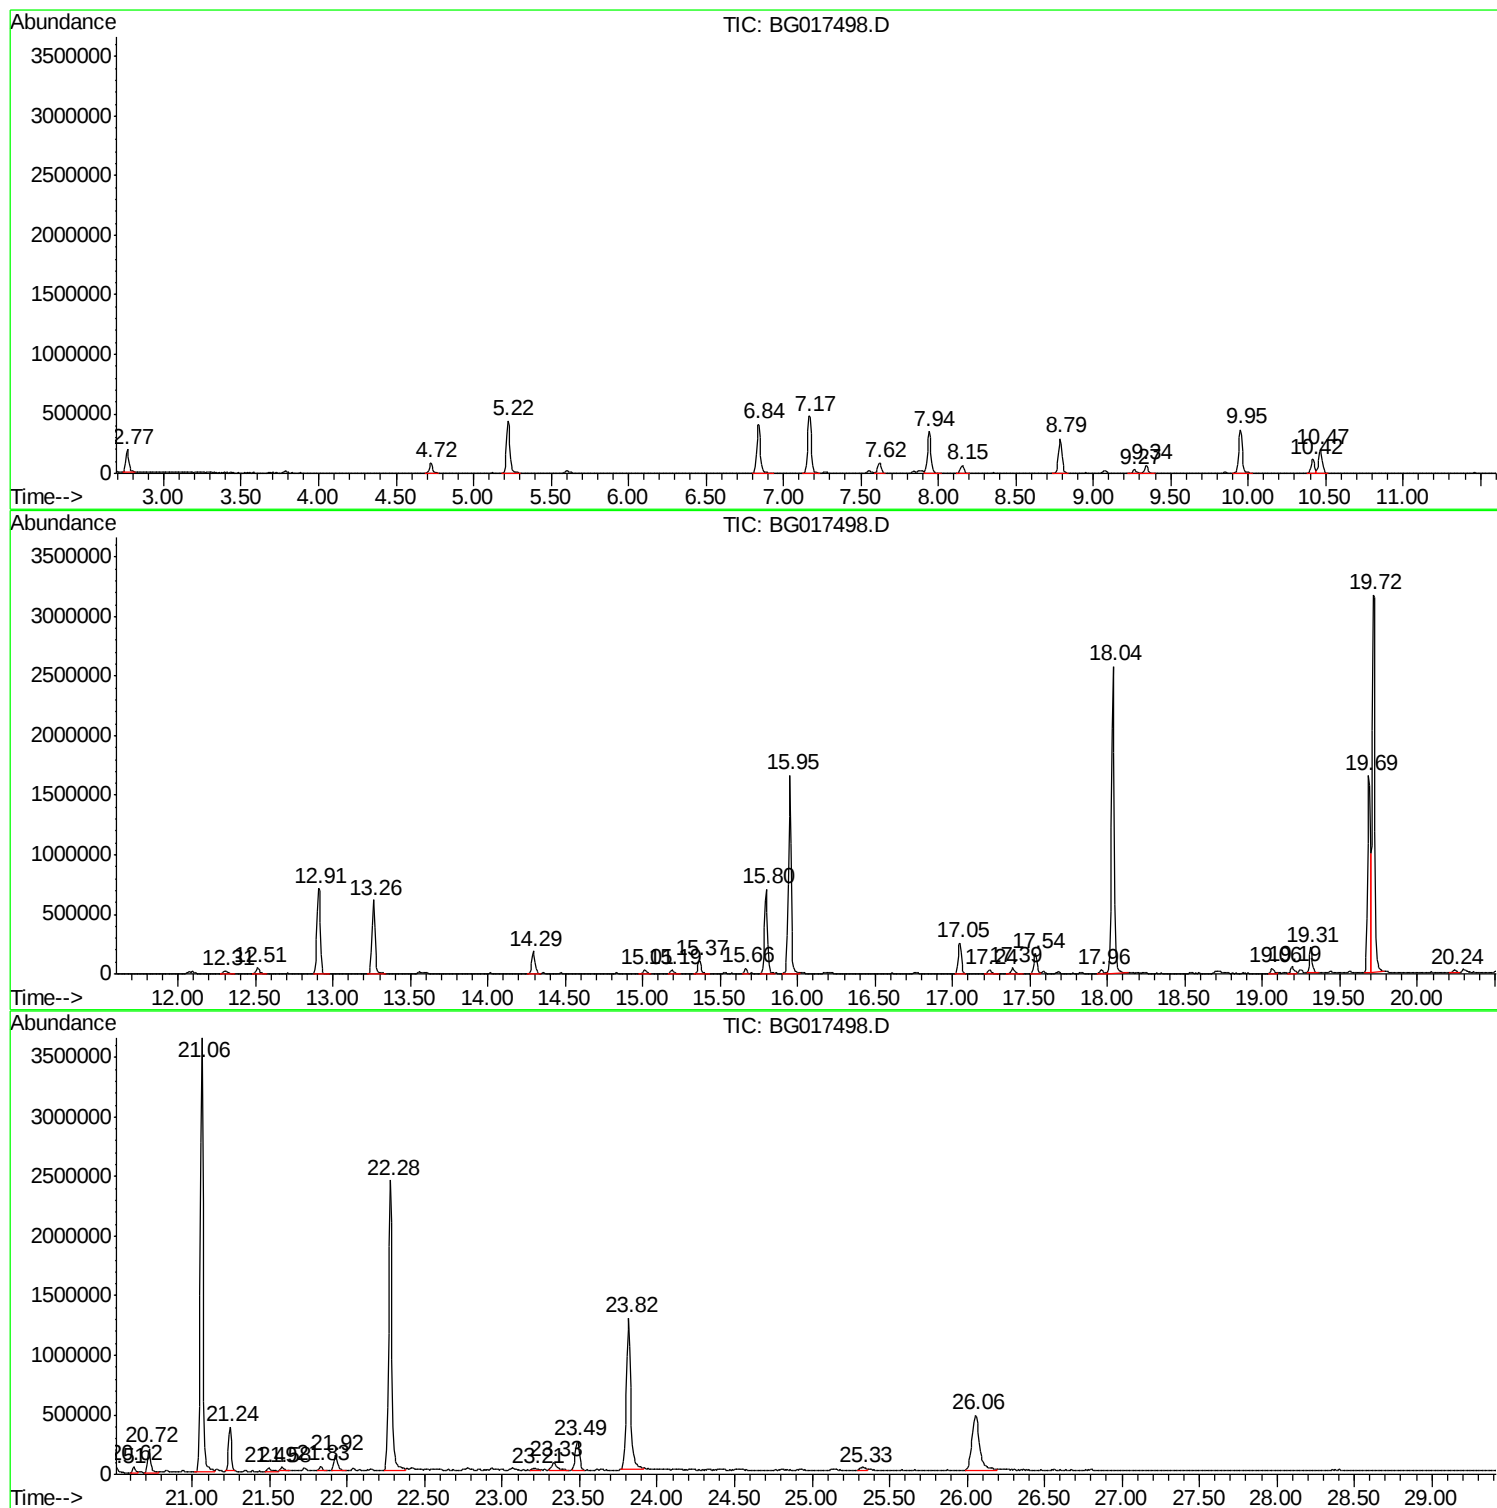

DbaaaPathh::ZZ\NRPBHHM1BBAAGGDBAAAB0000055\
 DbaaaFile::BB0017098DD
 Aeqq00n :: 66Jun2005 77593
 Opeaaor ::TPPIZ
 Sample ::G0258801
 Misc ::
 ASSVaal ::224 SampleMultiplier:11

Instrument :
 BNA_G
 ClientSampleId :
 WC060415

QqaabMebbdd::ZZ\NRPBHHM1BBAAGGMEH00S8270BB000035MM
 QqaabTitle ::ASBPBNASSANDBBSF00R55P000NTC6AIBRATION

TICLibrary ::CC\DATA\BBS6EN055002LL
 TICIntegratíonParameters:LS6CNTPP

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
				#	RT Resp Conc

No Library Search Compounds Detected
