


Data Path : Z:\HPCHEM1\BNA_G\Data\BG060515\
 Data File : BG017472.D
 Acq On : 5 Jun 2015 12:55
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060315.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jun 04 01:31:15 2015

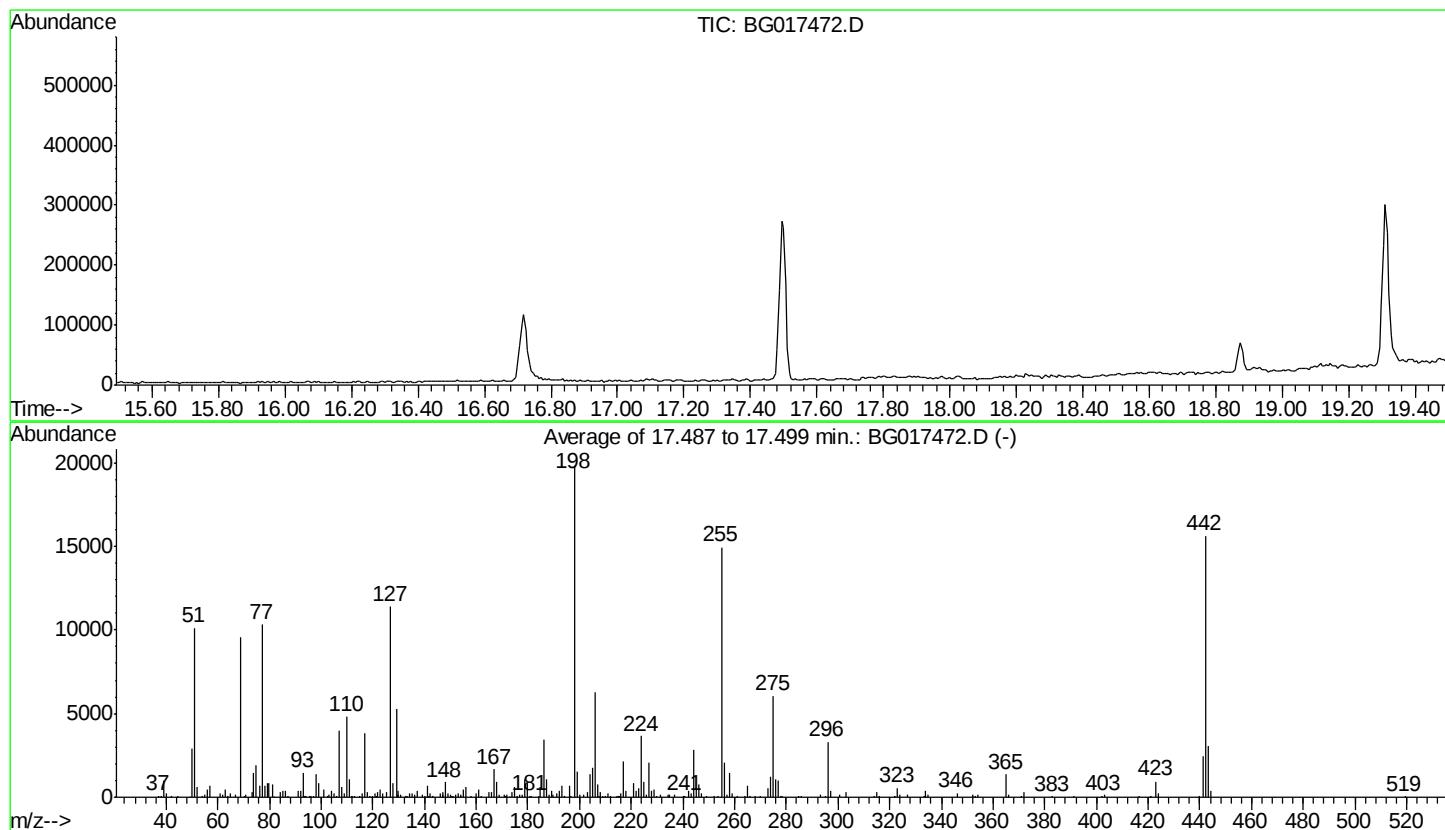

AutoFind: Scans 2519, 2520, 2521; Background Corrected with Scan 2514

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	51.1	10123	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	48.2	9556	PASS
70	69	0.00	2	0.6	62	PASS
127	198	10	80	57.5	11384	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	19815	PASS
199	198	5	9	7.8	1547	PASS
275	198	10	60	30.7	6079	PASS
365	198	1	100	6.9	1369	PASS
441	442	0.01	24	15.7	2455	PASS
442	198	50	100	78.8	15619	PASS
443	442	15	24	19.4	3029	PASS