


Data Path : Z:\HPCHEM1\BNA_G\Data\BG060515\
 Data File : BG017487.D
 Acq On : 6 Jun 2015 00:56
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060315.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jun 04 01:31:15 2015

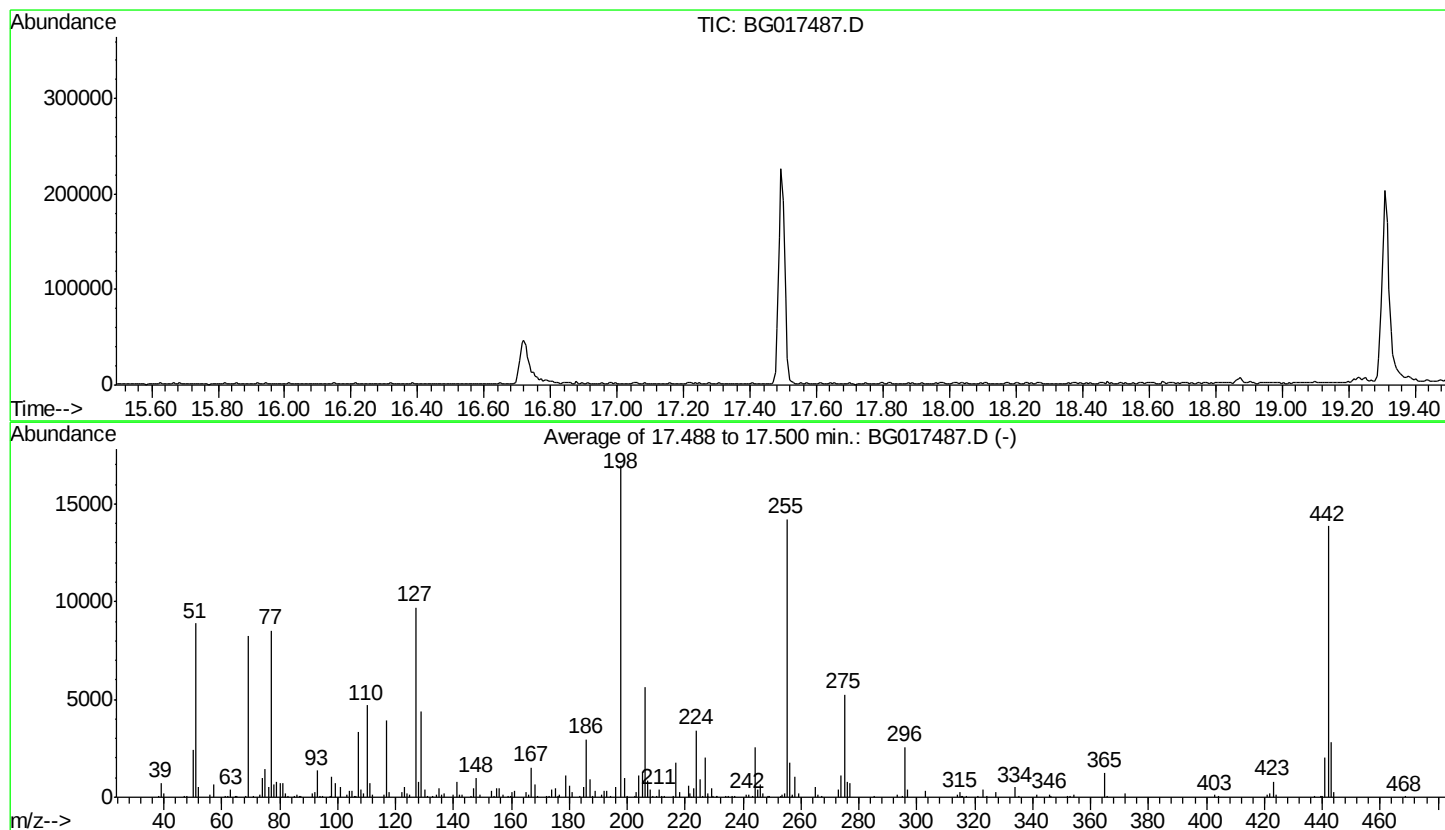

AutoFind: Scans 2519, 2520, 2521; Background Corrected with Scan 2513

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	52.5	8897	PASS
68	69	0.00	2	1.2	100	PASS
69	198	0.00	100	48.8	8281	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	57.2	9701	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	16957	PASS
199	198	5	9	6.0	1012	PASS
275	198	10	60	31.1	5267	PASS
365	198	1	100	7.5	1268	PASS
441	442	0.01	24	14.7	2039	PASS
442	198	50	100	81.7	13859	PASS
443	442	15	24	20.2	2794	PASS