



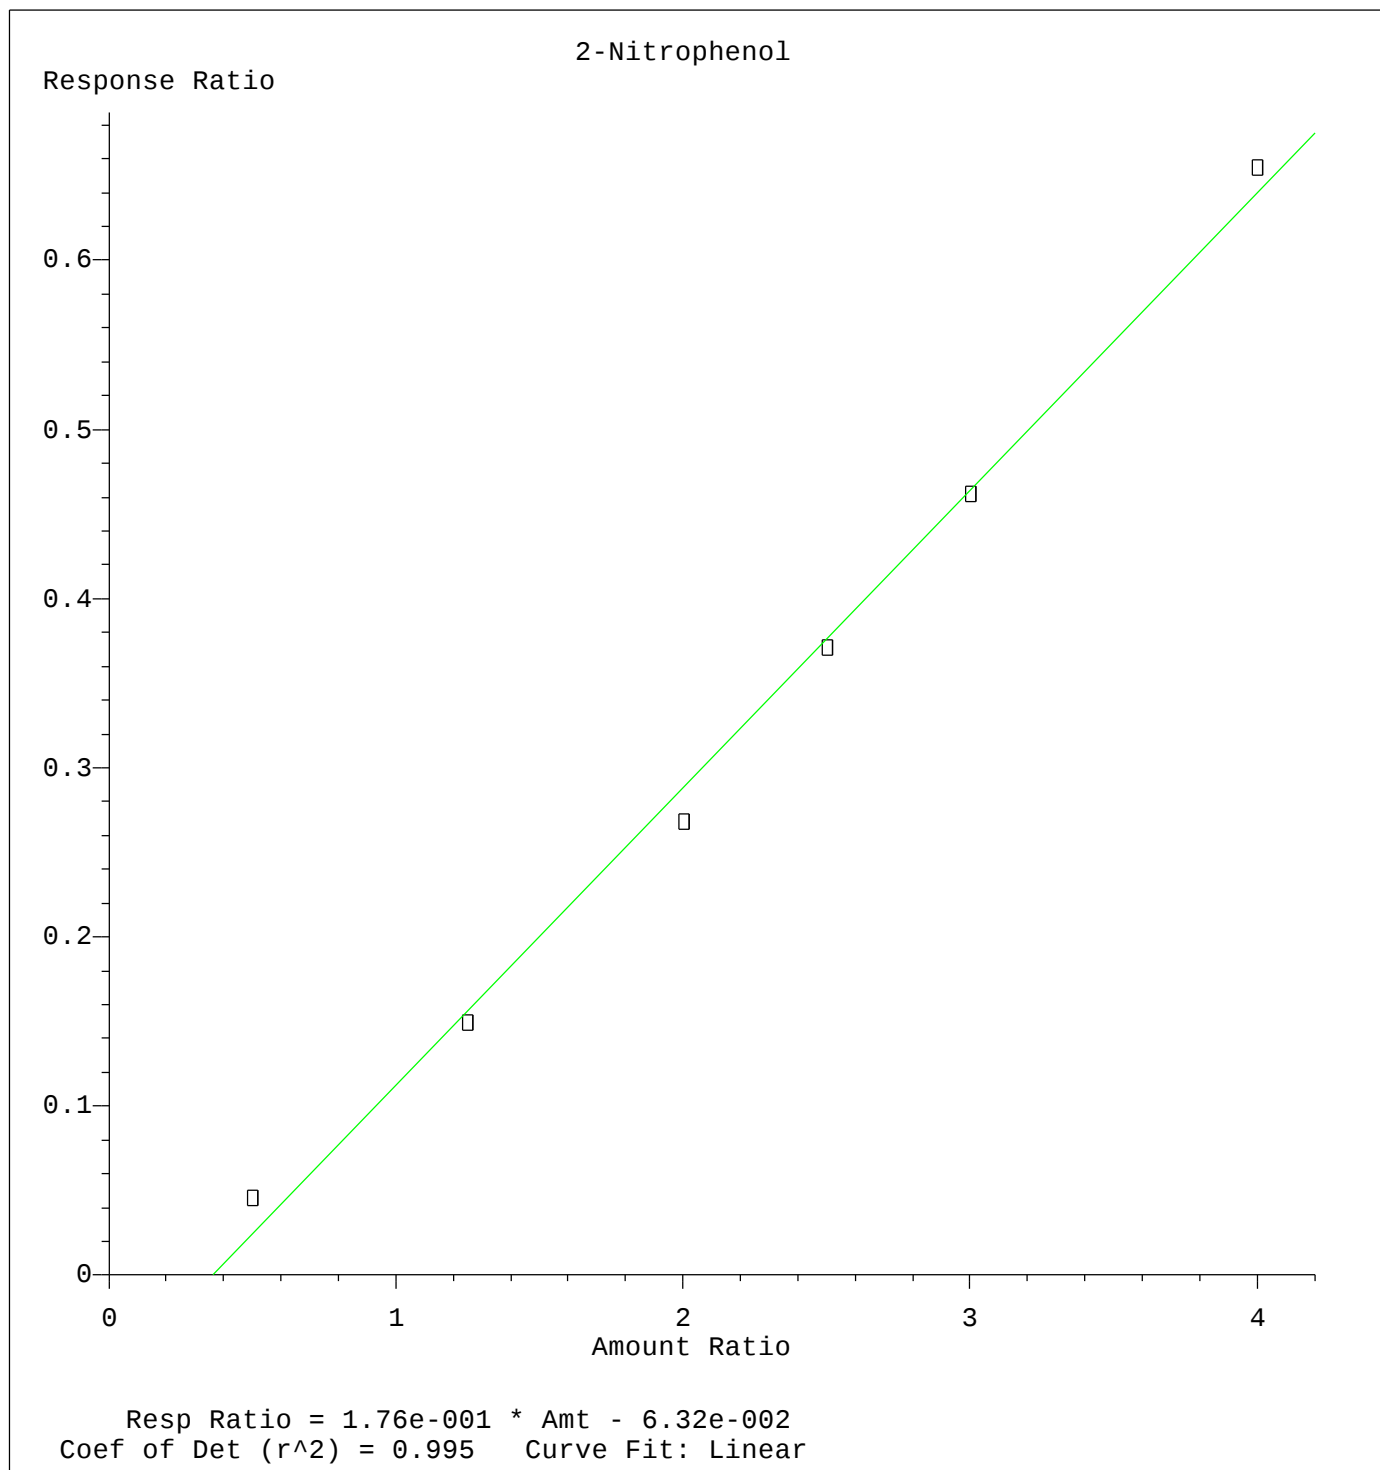


Method Name: Z:\HPCHEM1\BNA_G\METHODS\8270-BG060517.M
Calibration Table Last Updated: Mon Jun 05 16:00:35 2017

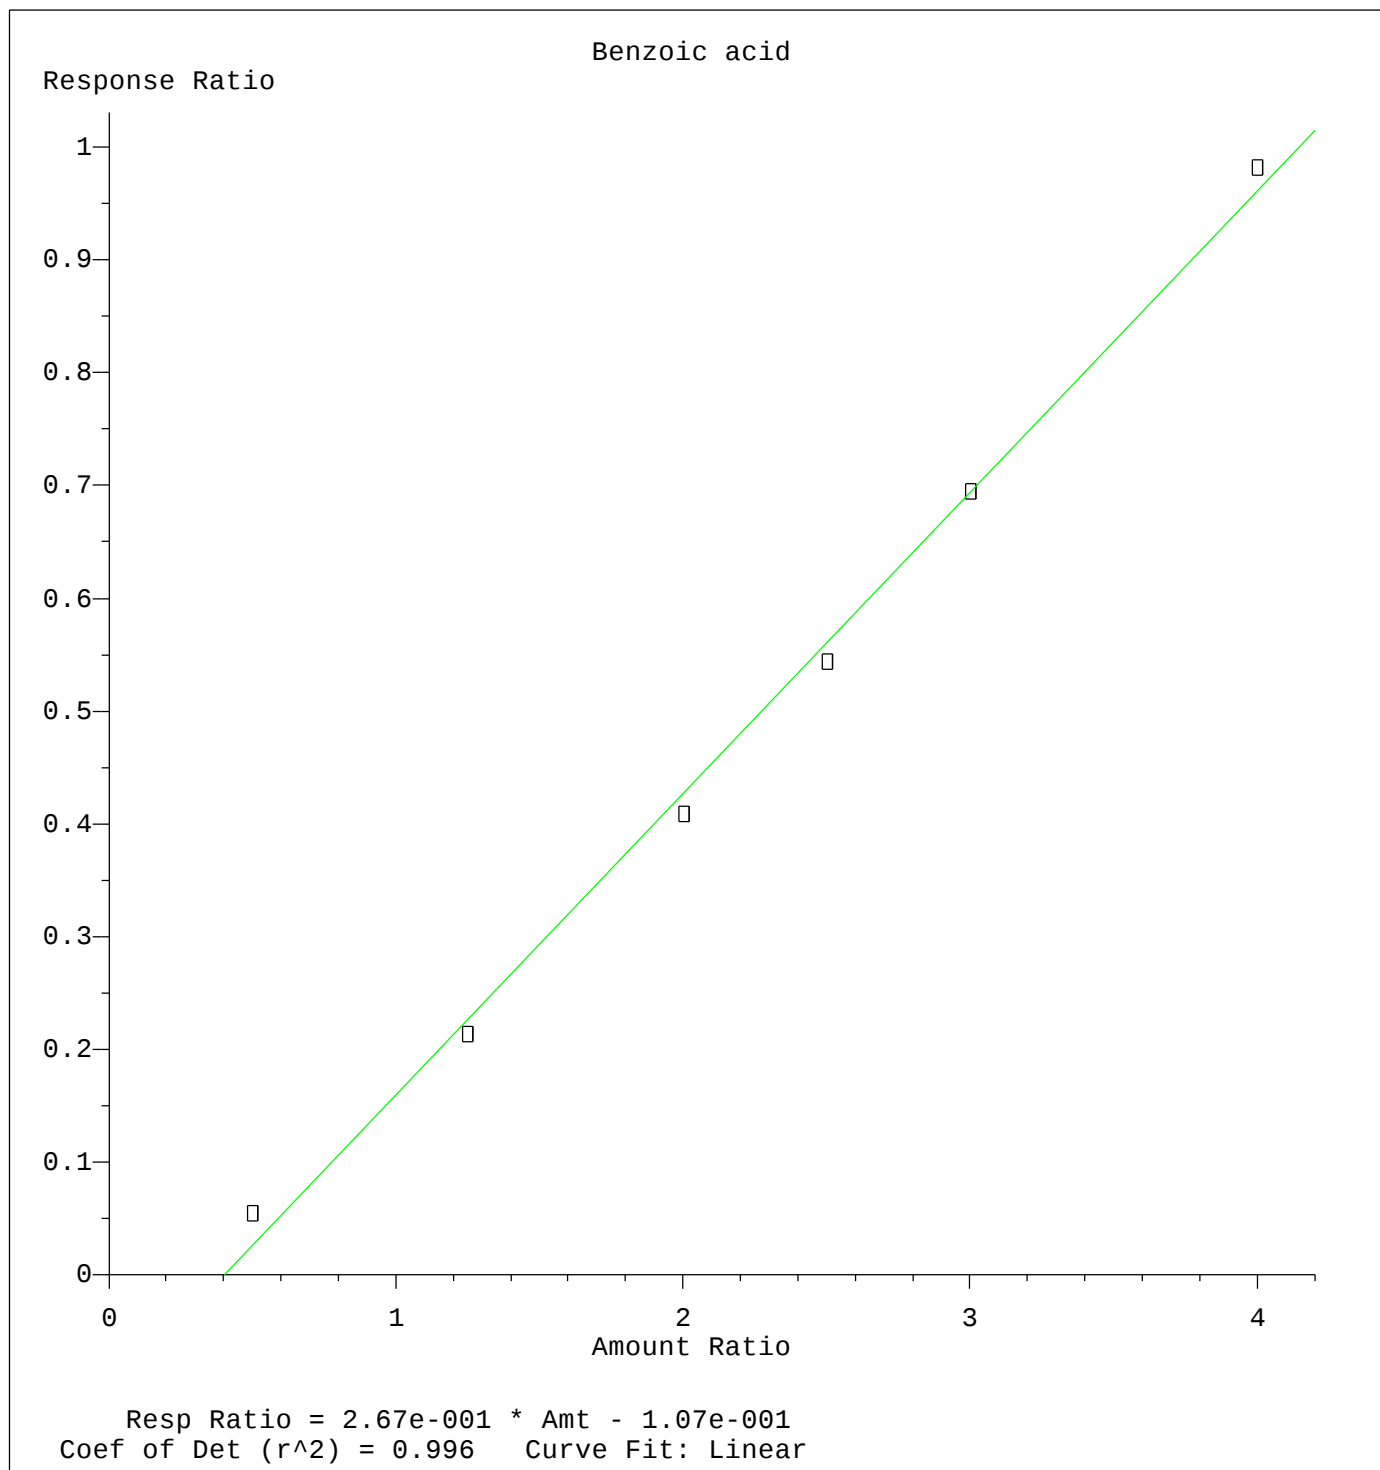

Method Name: Z:\HPCHEM1\BNA_G\METHODS\8270-BG060517.M
Calibration Table Last Updated: Mon Jun 05 16:00:35 2017

2-Nitroaniline

Response Ratio

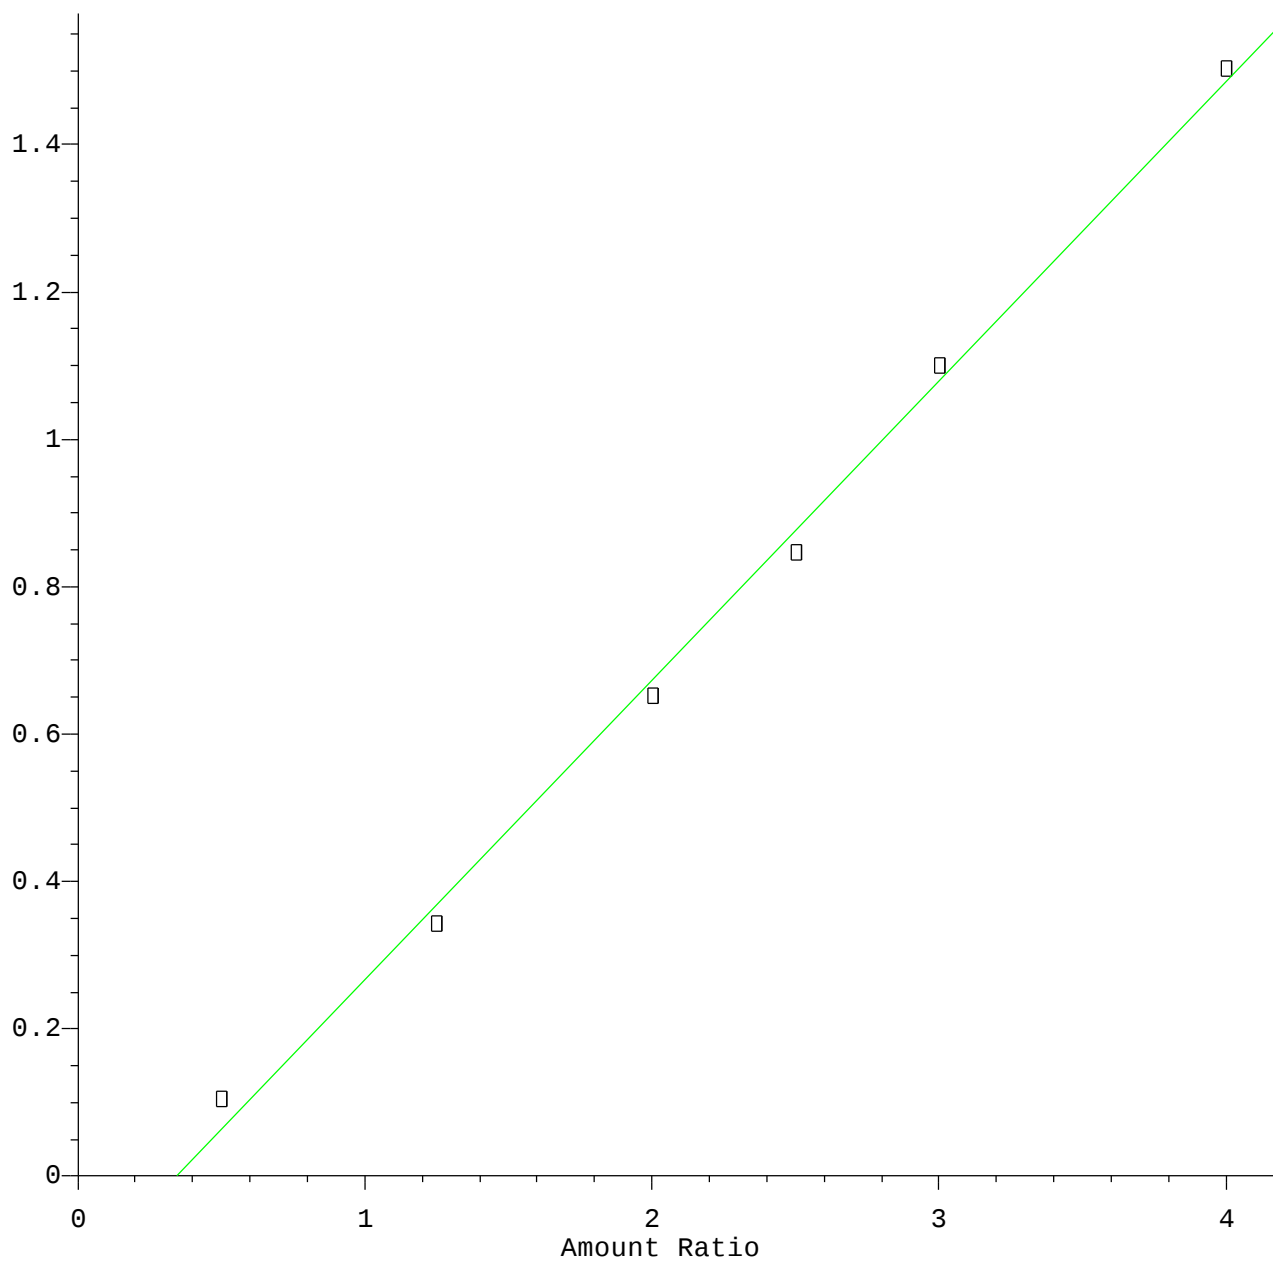


Resp Ratio = $4.06 \times 10^{-1} \times \text{Amt} - 1.39 \times 10^{-1}$
Coef of Det (r^2) = 0.997 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA_G\METHODS\8270-BG060517.M
Calibration Table Last Updated: Mon Jun 05 16:00:35 2017


2,6-Dinitrotoluene

Response Ratio

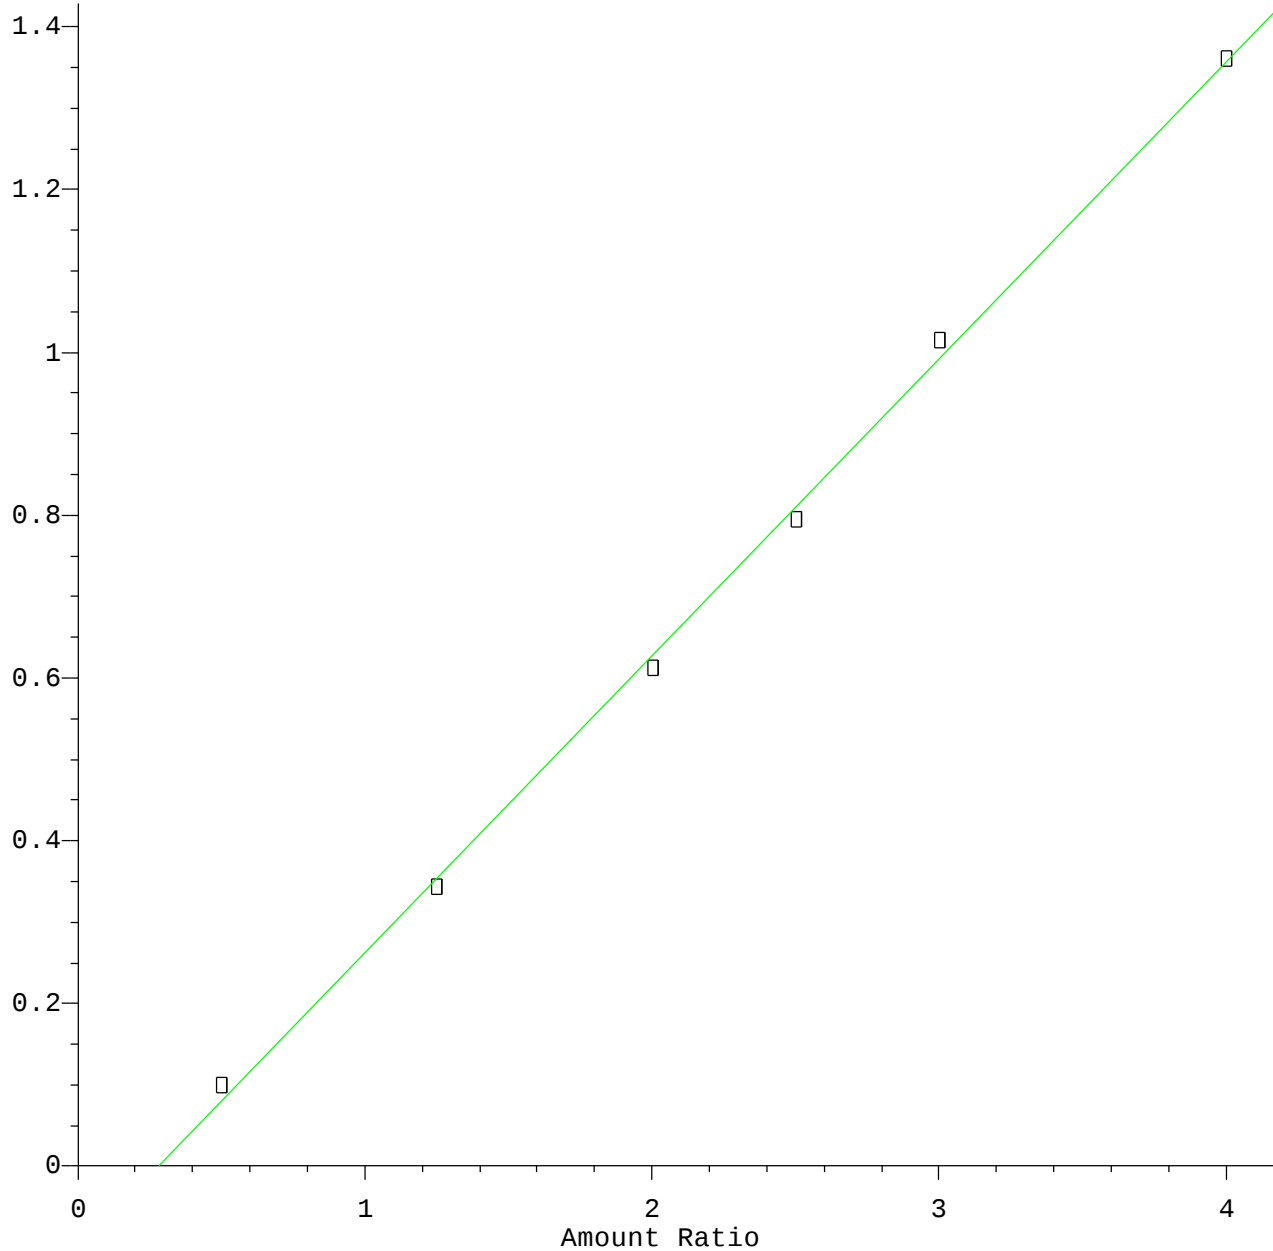


Resp Ratio = 3.65e-001 * Amt - 1.02e-001
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA_G\METHODS\8270-BG060517.M
Calibration Table Last Updated: Mon Jun 05 16:00:35 2017

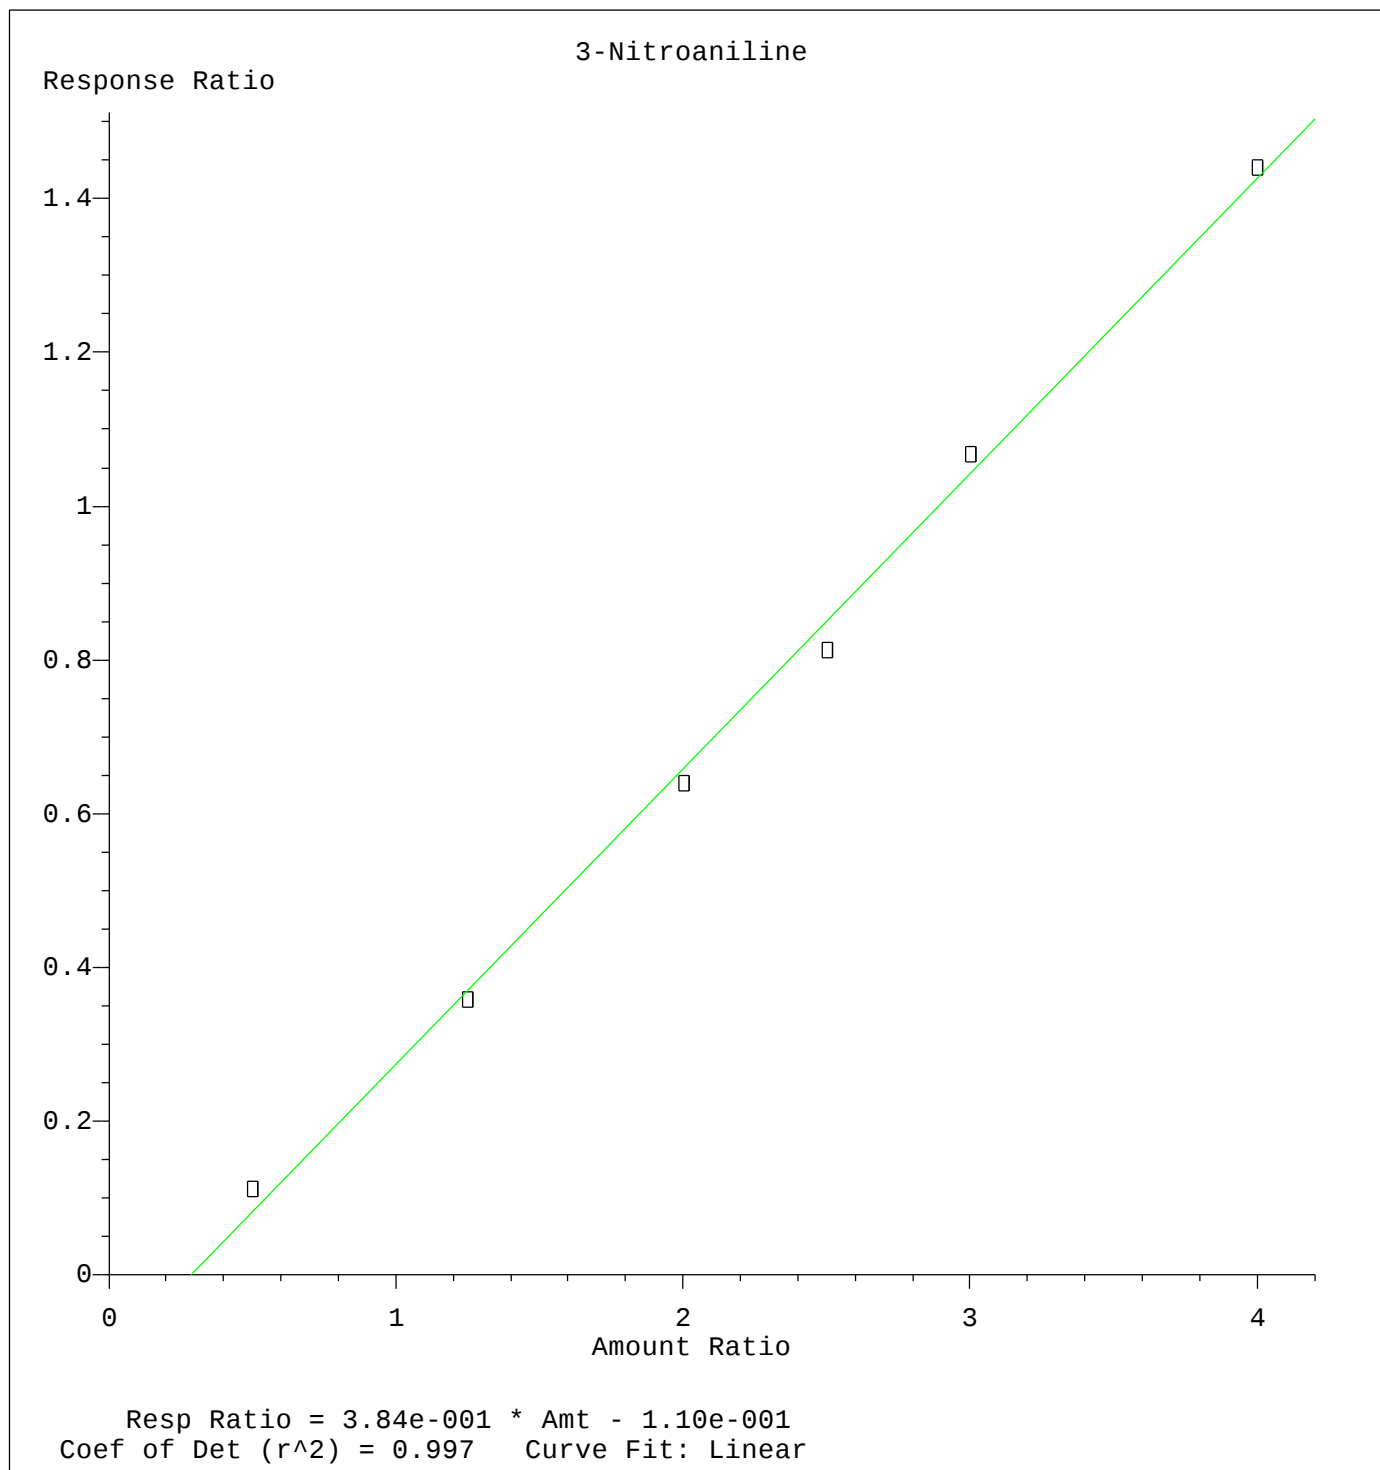


Method Name: Z:\HPCHEM1\BNA_G\METHODS\8270-BG060517.M
Calibration Table Last Updated: Mon Jun 05 16:00:35 2017

2,4-Dinitrophenol

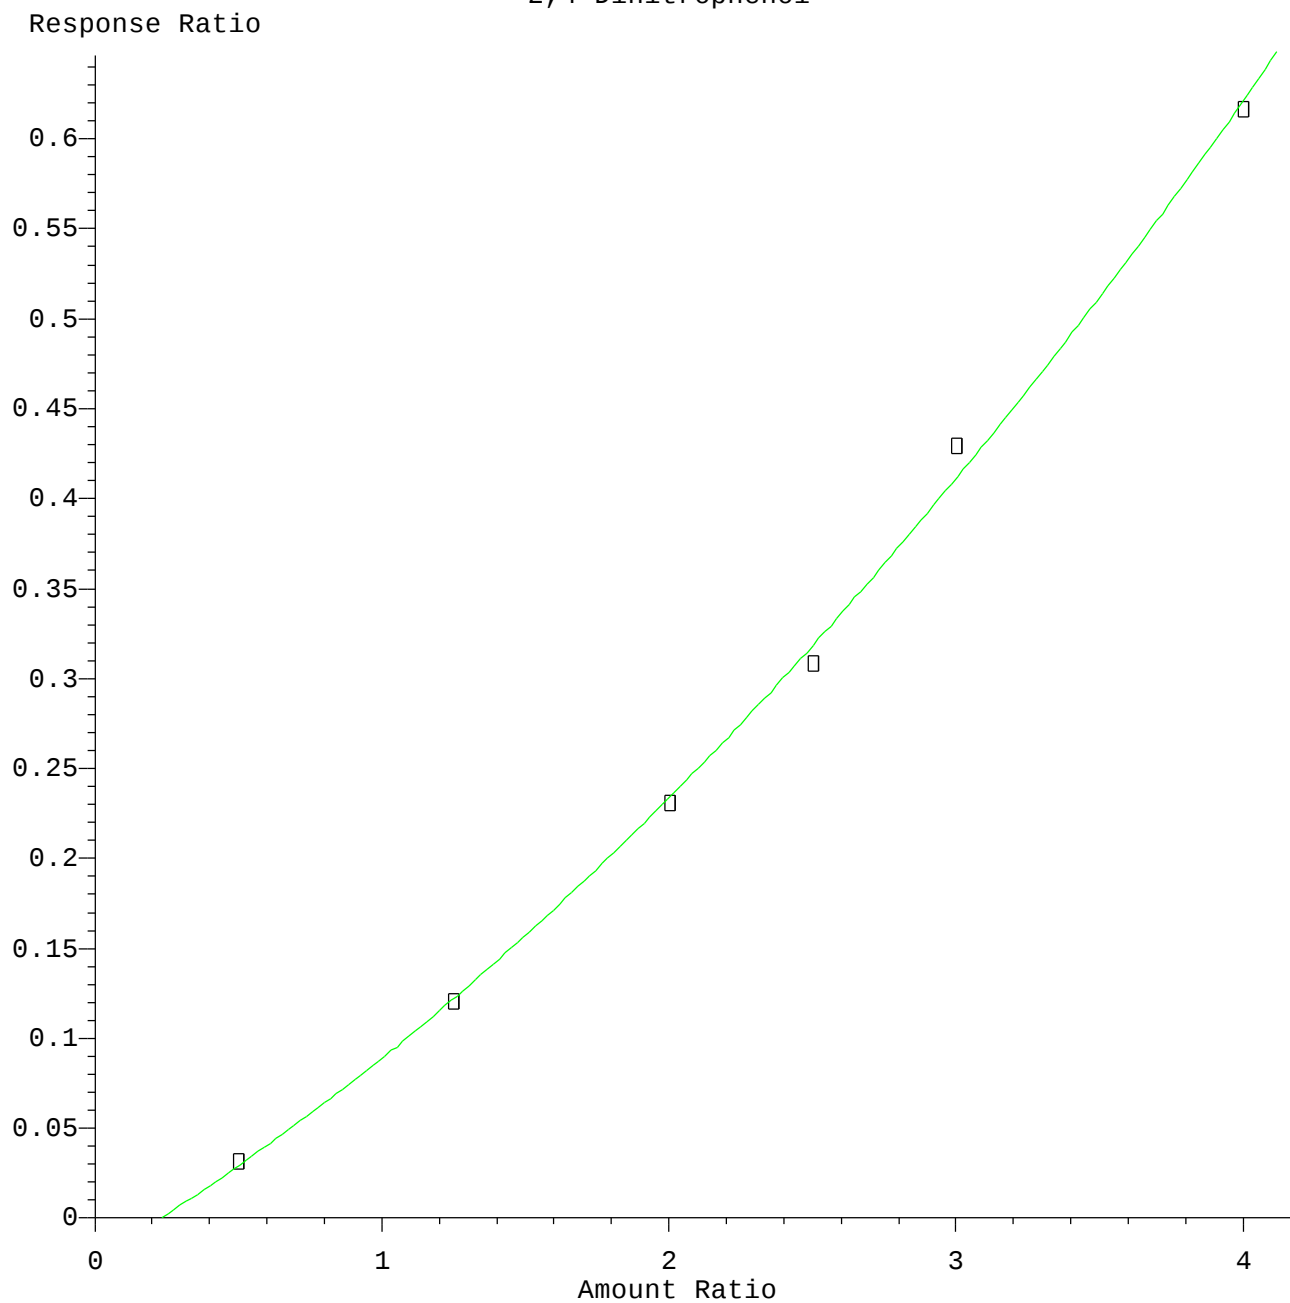

$R = 1.64e-002 A^2 + 9.56e-002 A - 2.29e-002$
Coef of Det (r^2) = 0.998 Curve Fit: Quadratic


Method Name: Z:\HPCHEM1\BNA_G\METHODS\8270-BG060517.M
Calibration Table Last Updated: Mon Jun 05 16:00:35 2017

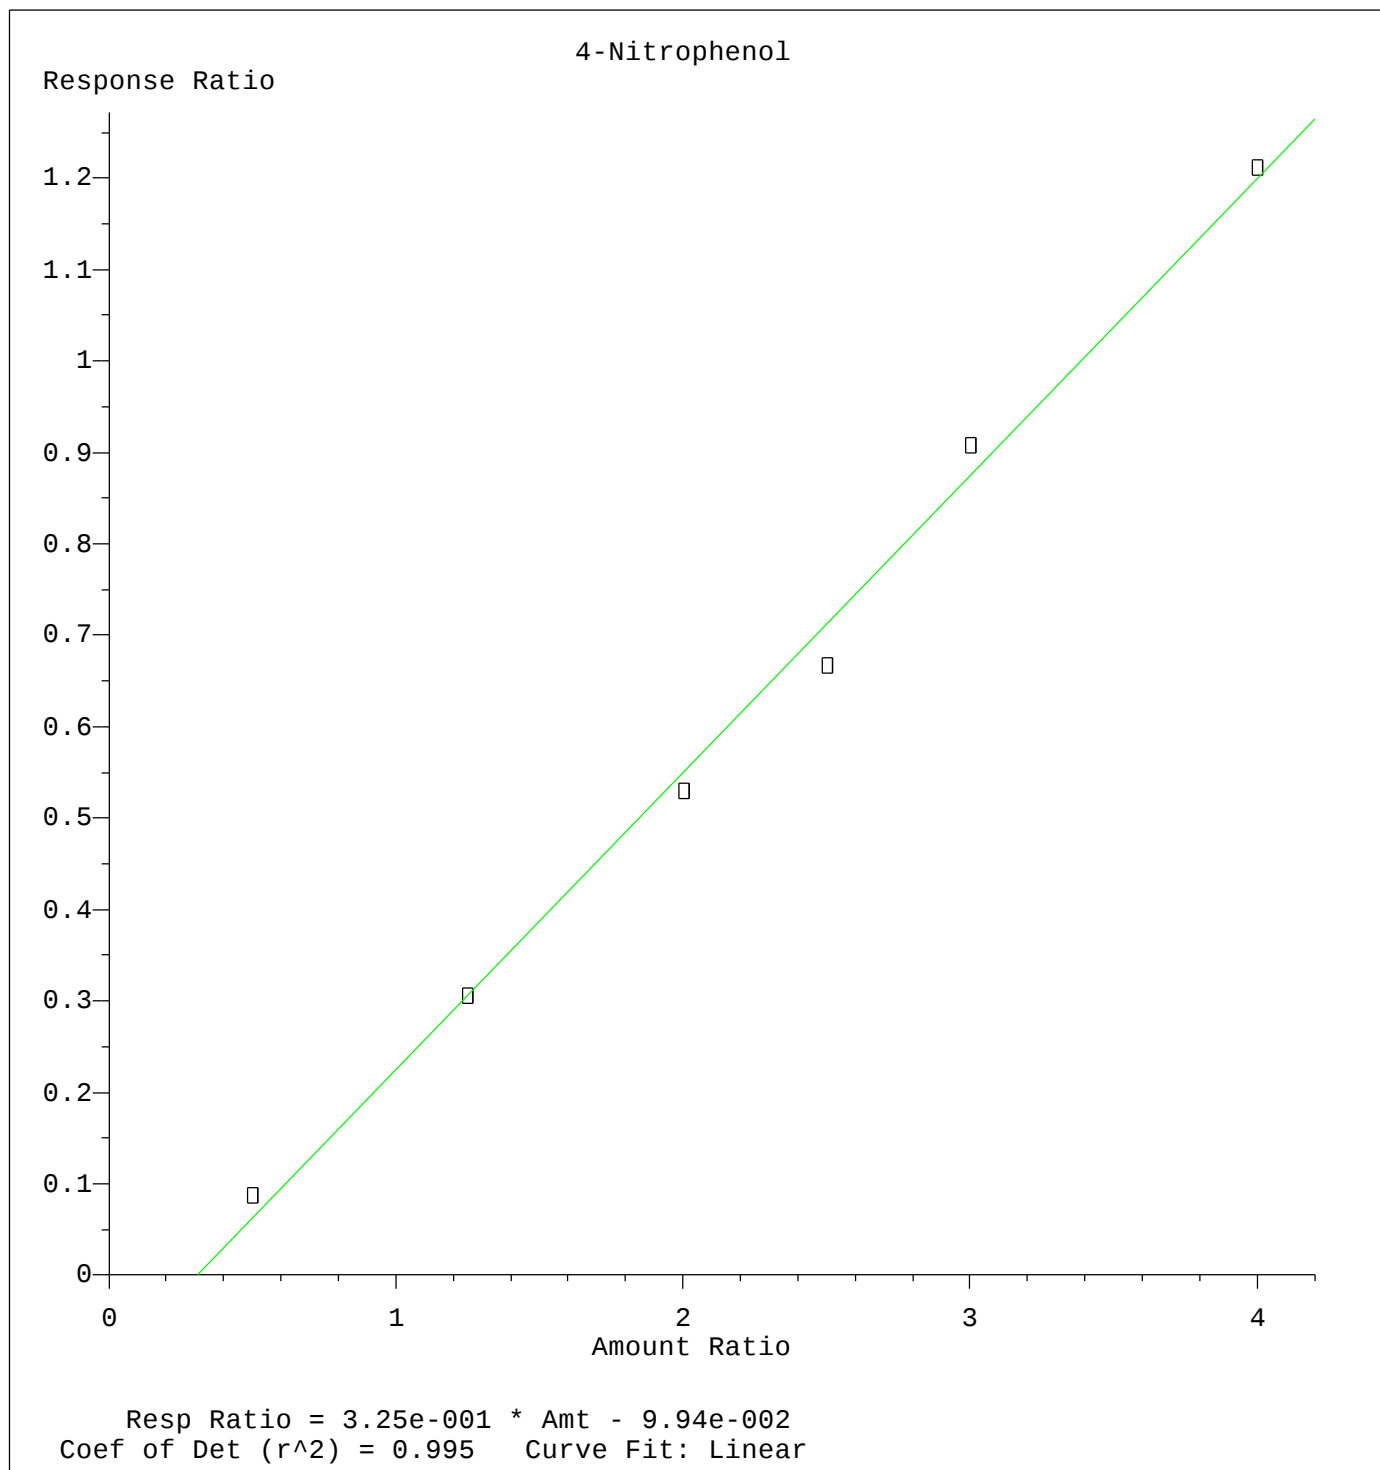

Method Name: Z:\HPCHEM1\BNA_G\METHODS\8270-BG060517.M
Calibration Table Last Updated: Mon Jun 05 16:00:35 2017


2,4-Dinitrotoluene

Response Ratio

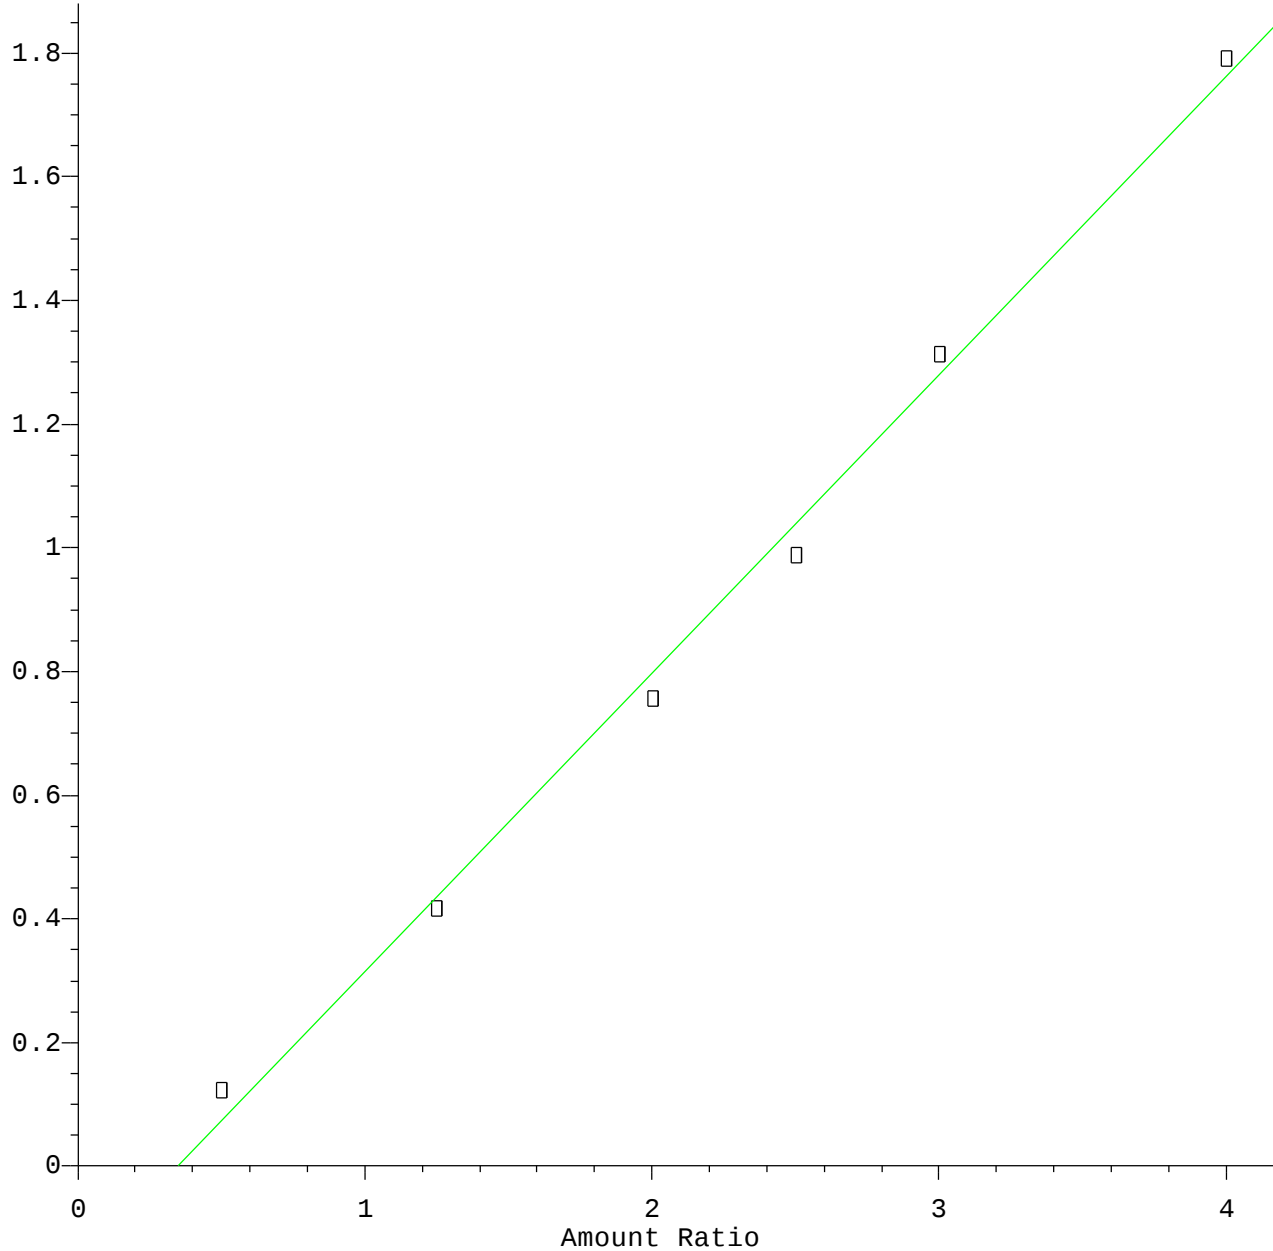


Resp Ratio = $4.83 \times 10^{-1} \times \text{Amt} - 1.69 \times 10^{-1}$
Coef of Det (r^2) = 0.995 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA_G\METHODS\8270-BG060517.M
Calibration Table Last Updated: Mon Jun 05 16:00:35 2017

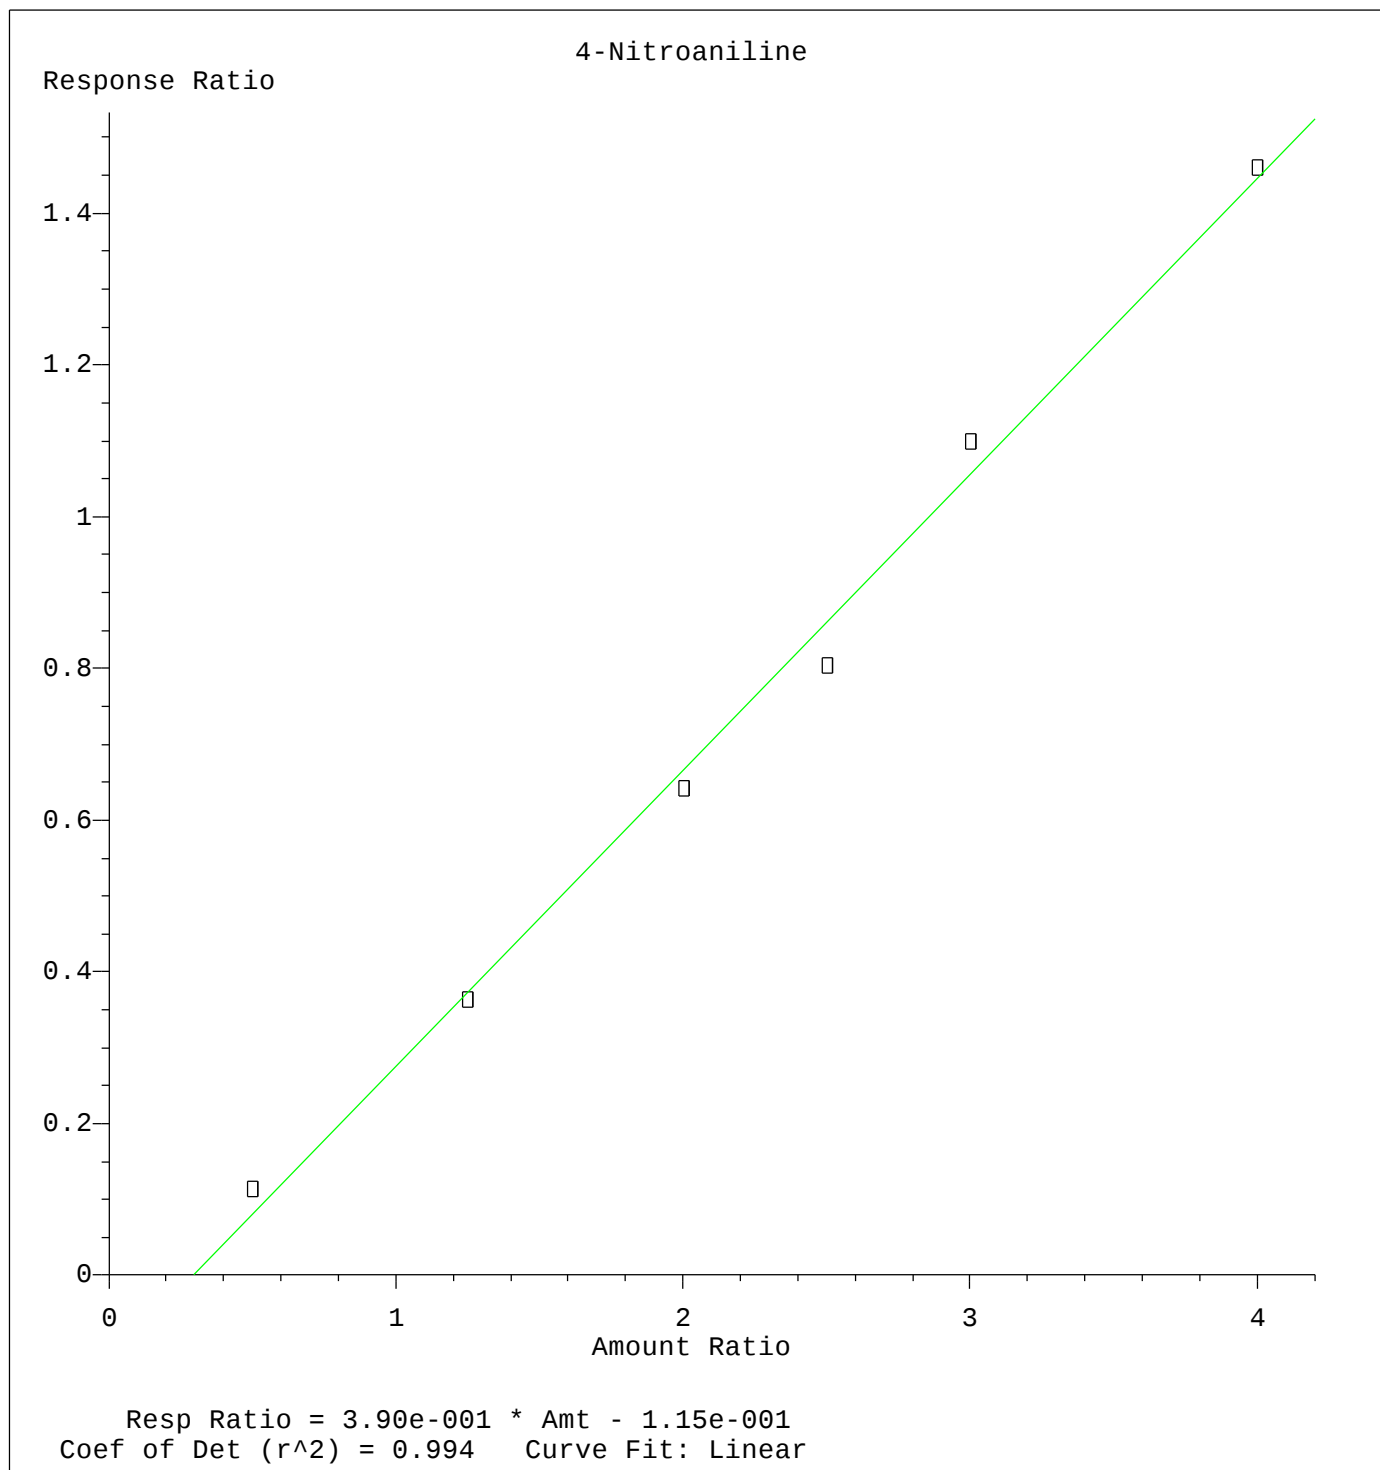

Method Name: Z:\HPCHEM1\BNA_G\METHODS\8270-BG060517.M
Calibration Table Last Updated: Mon Jun 05 16:00:35 2017

4,6-Dinitro-2-methylphenol

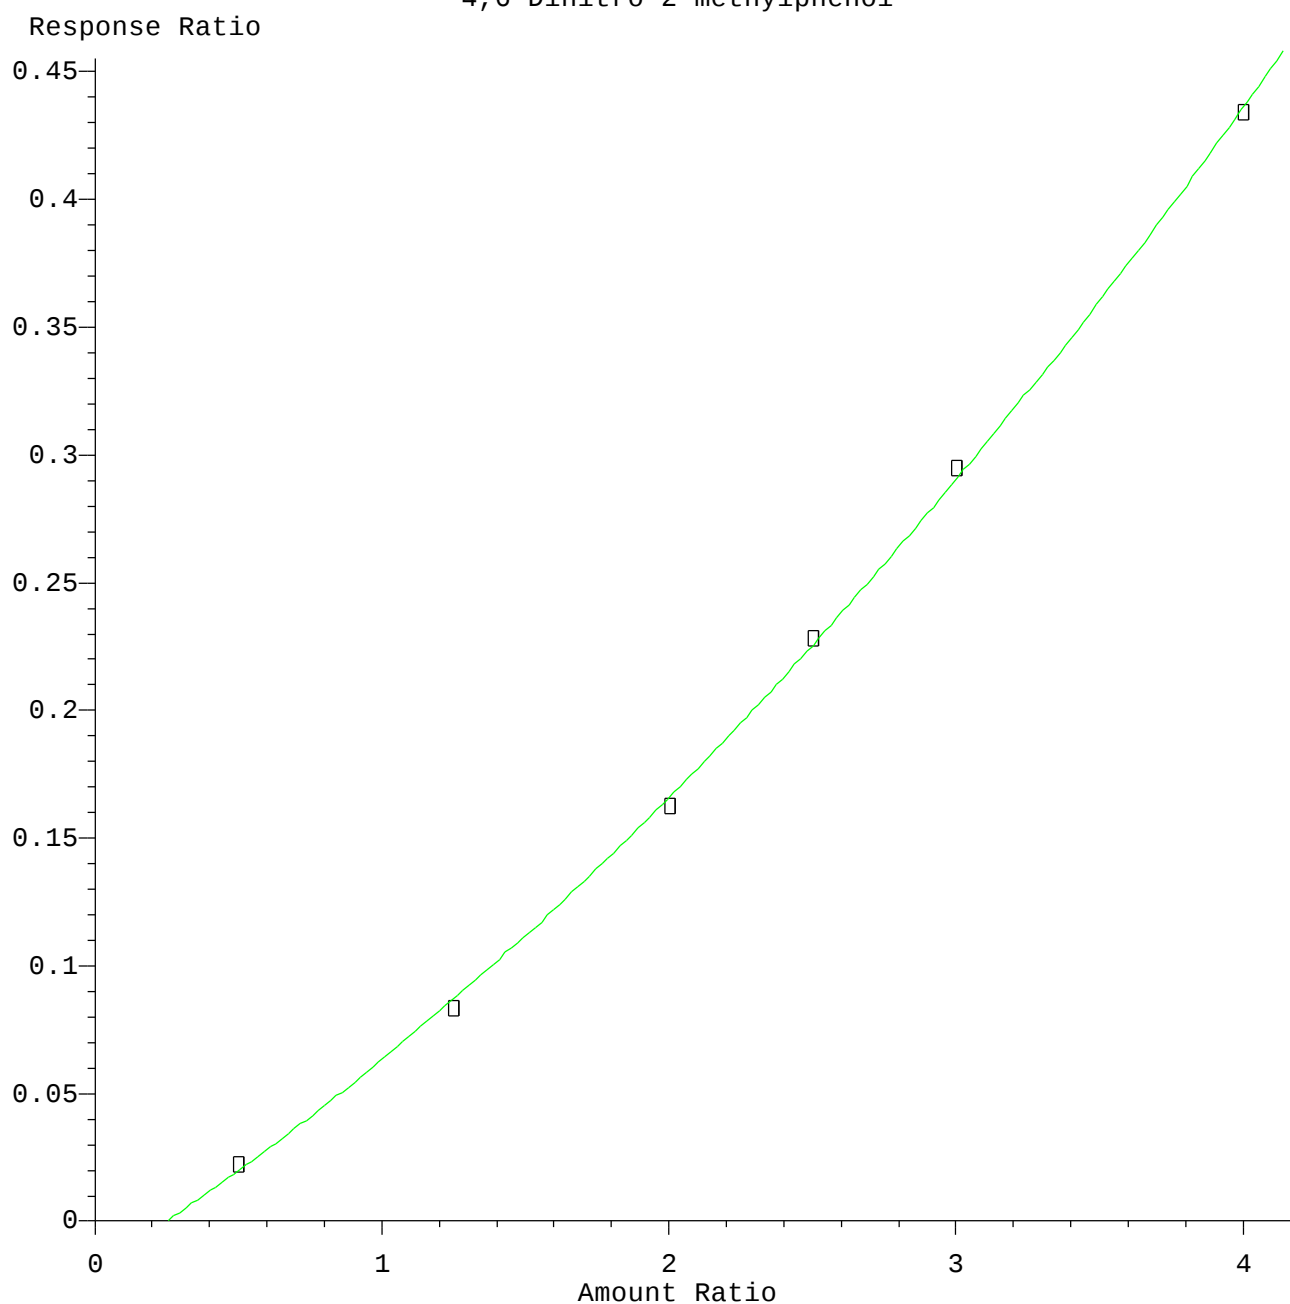

$R = 1.07e-002 A^2 + 7.08e-002 A - 1.84e-002$
Coef of Det (r^2) = 0.999 Curve Fit: Quadratic

Method Name: Z:\HPCHEM1\BNA_G\METHODS\8270-BG060517.M
Calibration Table Last Updated: Mon Jun 05 16:00:35 2017