
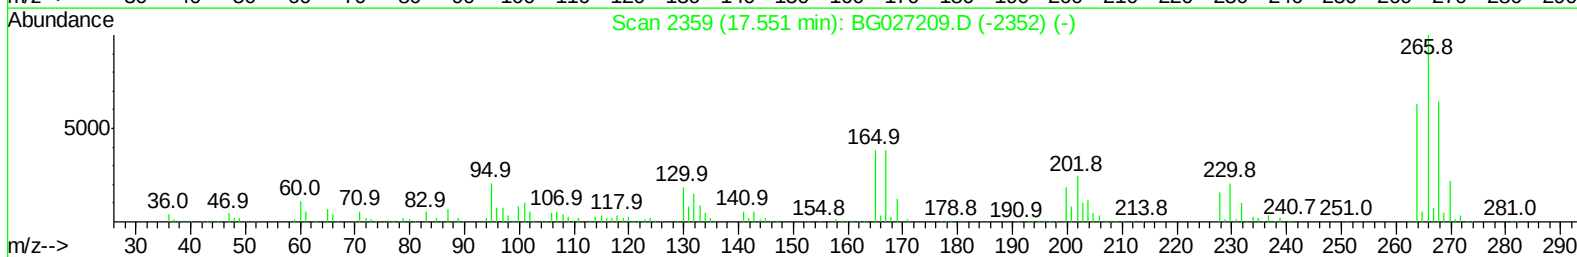
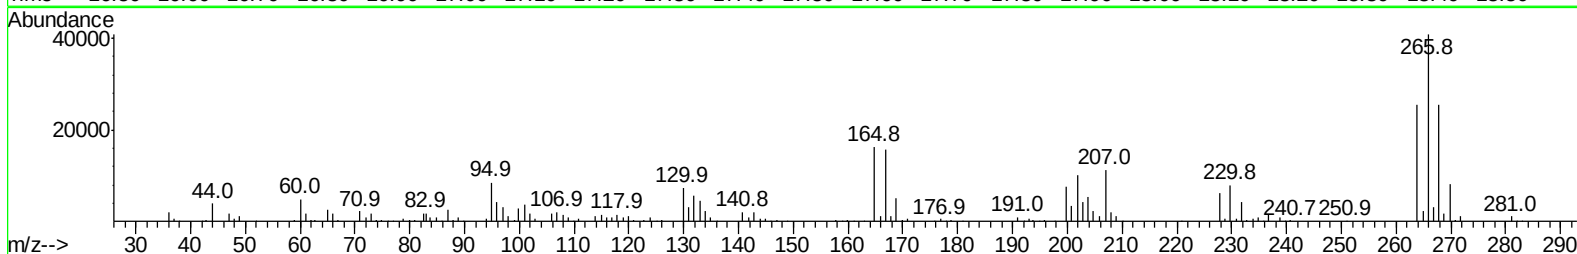


Data Path : Z:\HPCHEM1\BNA G\Data\BG060517\
Data File : BG027205.D
Acq On : 5 Jun 2017 9:55
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 06 14:57:16 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 05 16:00:35 2017
Response via : Initial Calibration

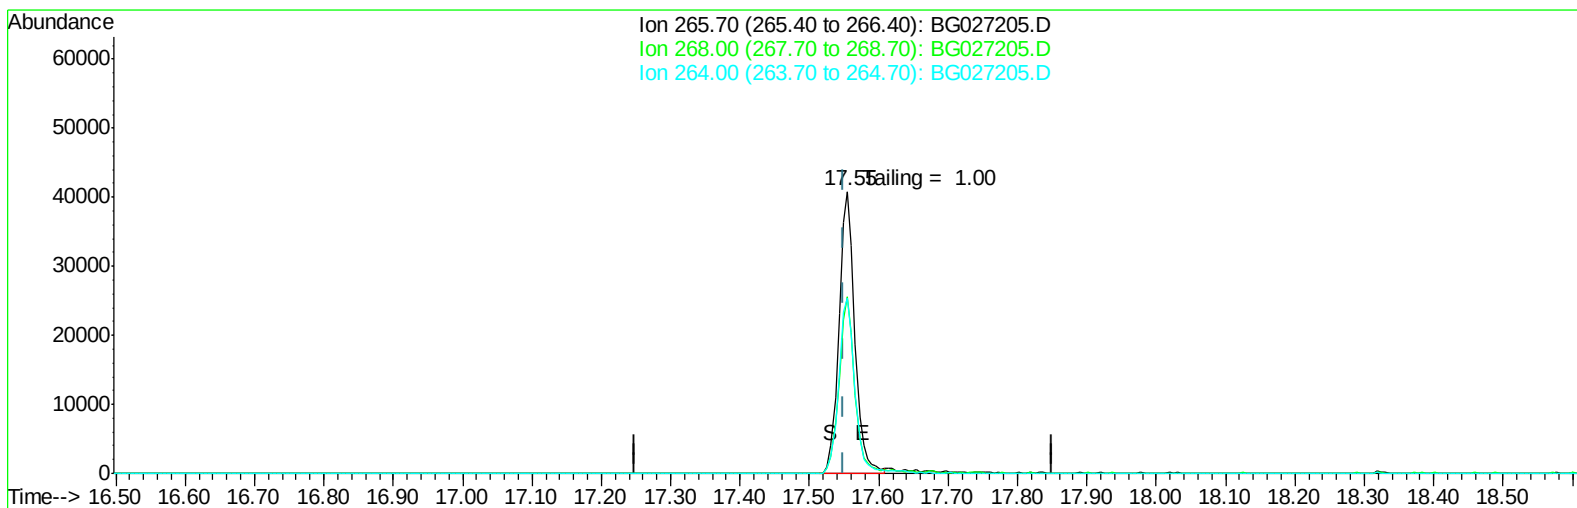

TIC: BG027205.D

(69) Pentachlorophenol (C)




17.555min (+0.005) 0.00ng

response 65577

Ion	Exp%	Act%
265.70	100	100
268.00	60.70	62.53
264.00	62.60	62.32
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\Data\BG060517\
 Data File : BG027205.D
 Acq On : 5 Jun 2017 9:55
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 06 14:57:16 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG060517.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 05 16:00:35 2017
 Response via : Initial Calibration

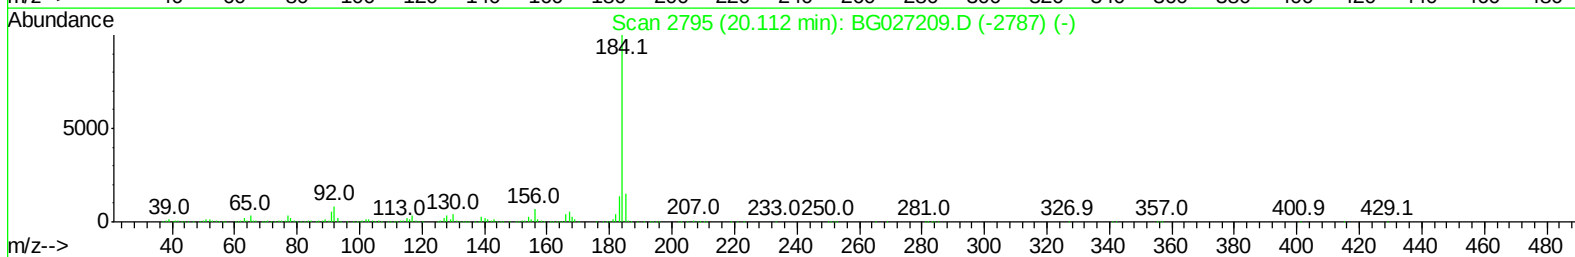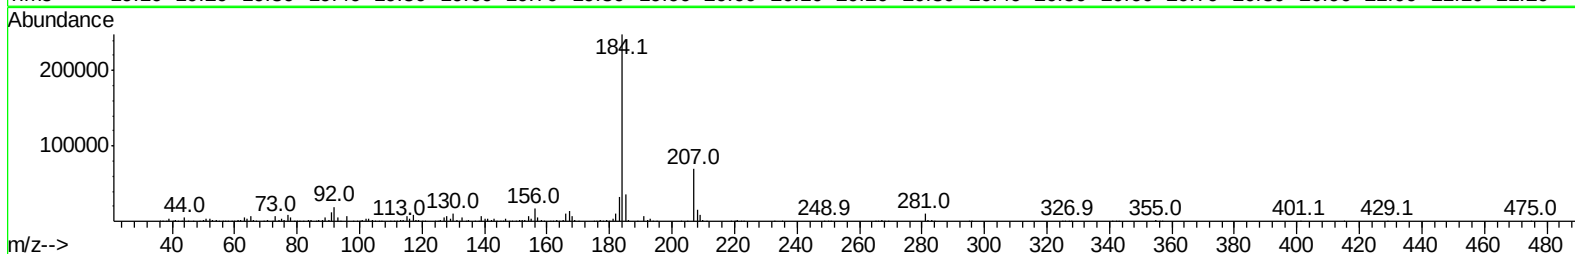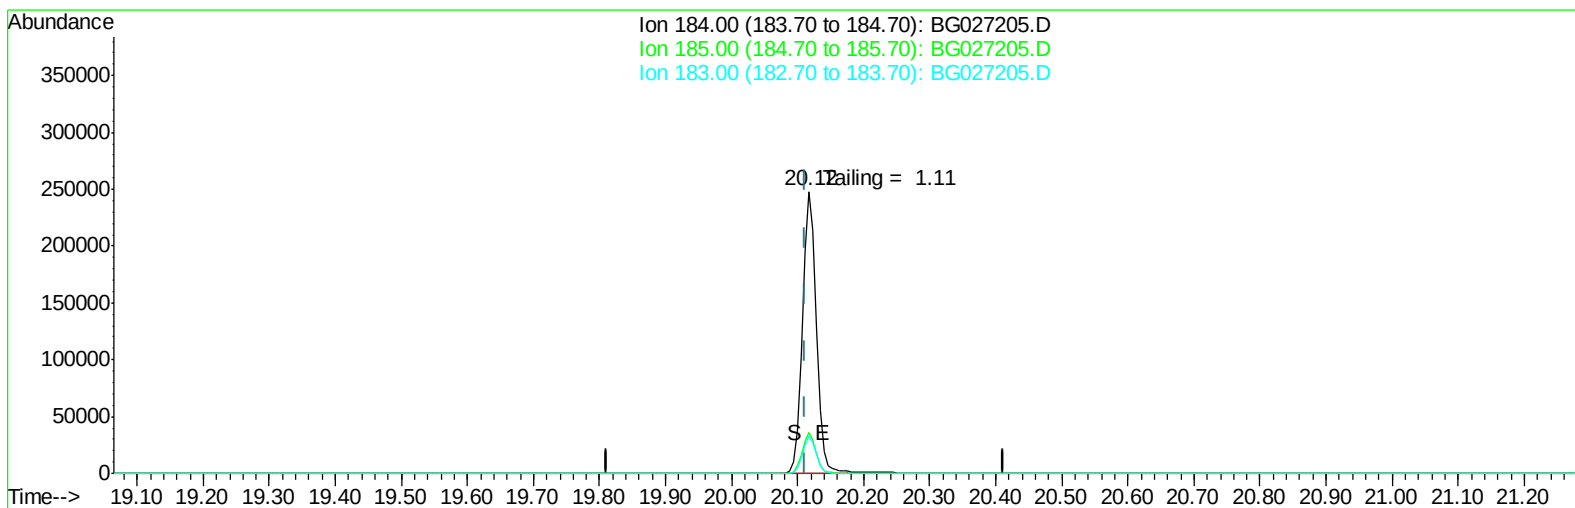

TIC: BG027205.D

(76) Benzidine

20.116min (+0.004) 0.00ng

response 368157

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	14.53
183.00	13.80	13.29
0.00	0.00	0.00