
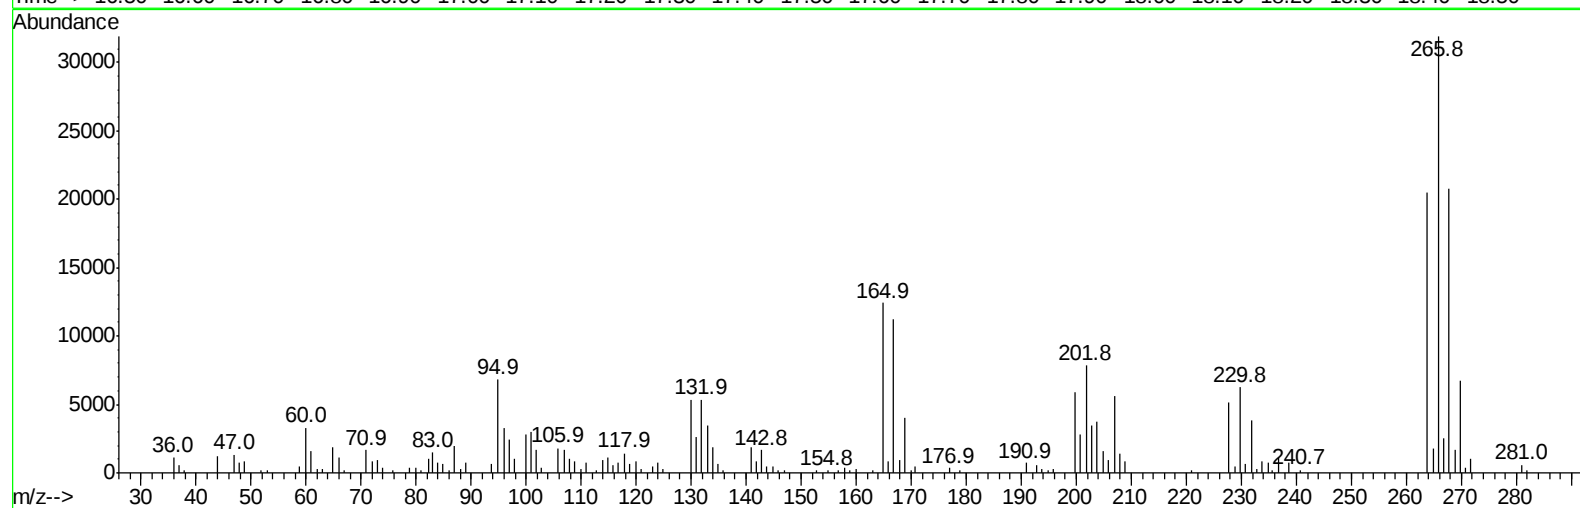


Data Path : Z:\HPCHEM1\BNA G\DATA\BG060517\
Data File : BG027221.D
Acq On : 5 Jun 2017 20:33
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 06 08:45:29 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 05 16:00:35 2017
Response via : Initial Calibration

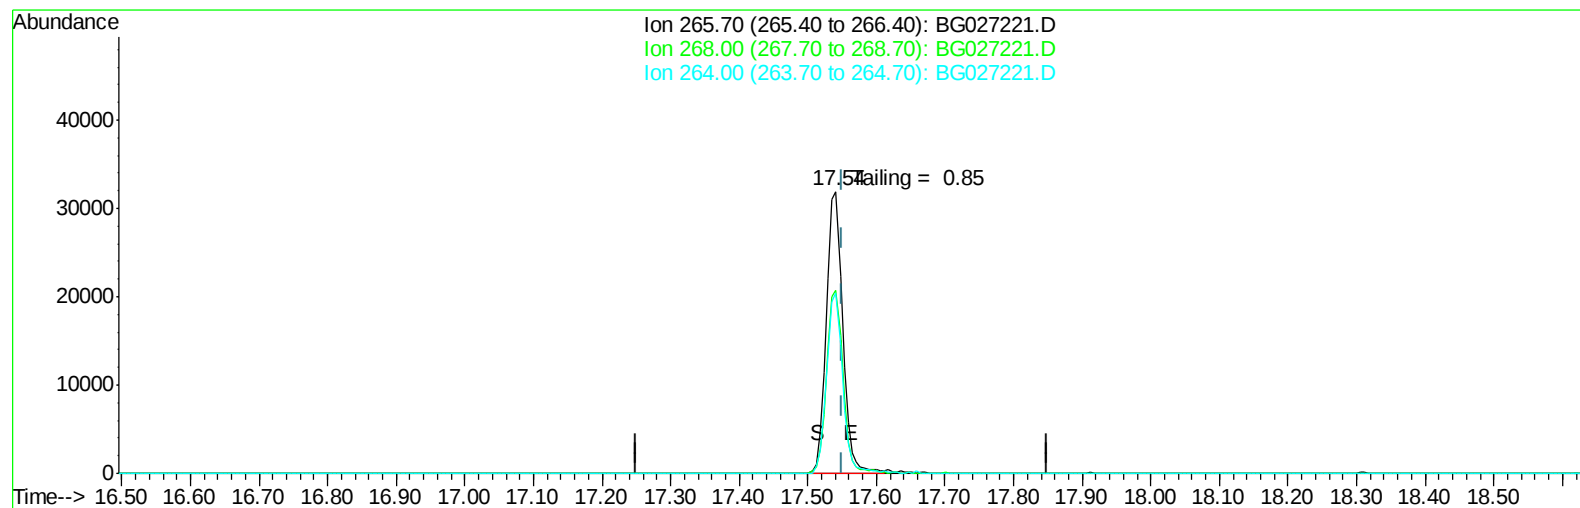

TIC: BG027221.D

(69) Pentachlorophenol (C)



17.541min (-0.009) 0.00ng

response 52948

Ion	Exp%	Act%
265.70	100	100
268.00	60.70	65.20
264.00	62.60	64.15
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG060517\
Data File : BG027221.D
Acq On : 5 Jun 2017 20:33
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 06 08:45:29 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 05 16:00:35 2017
Response via : Initial Calibration

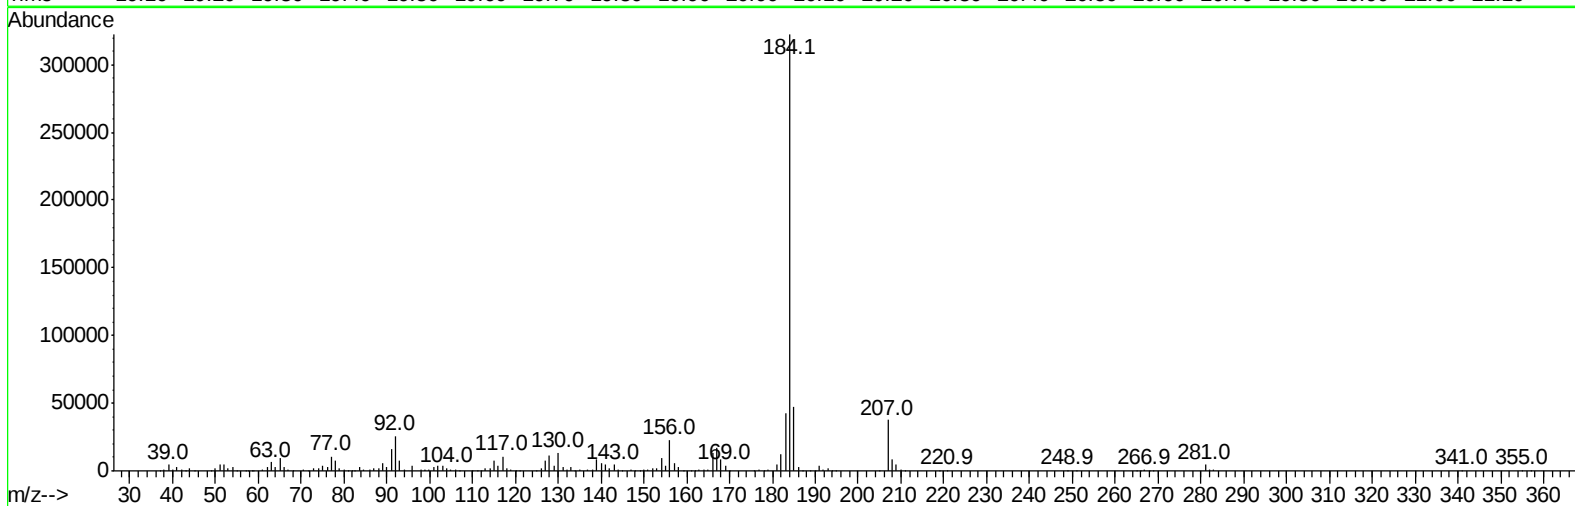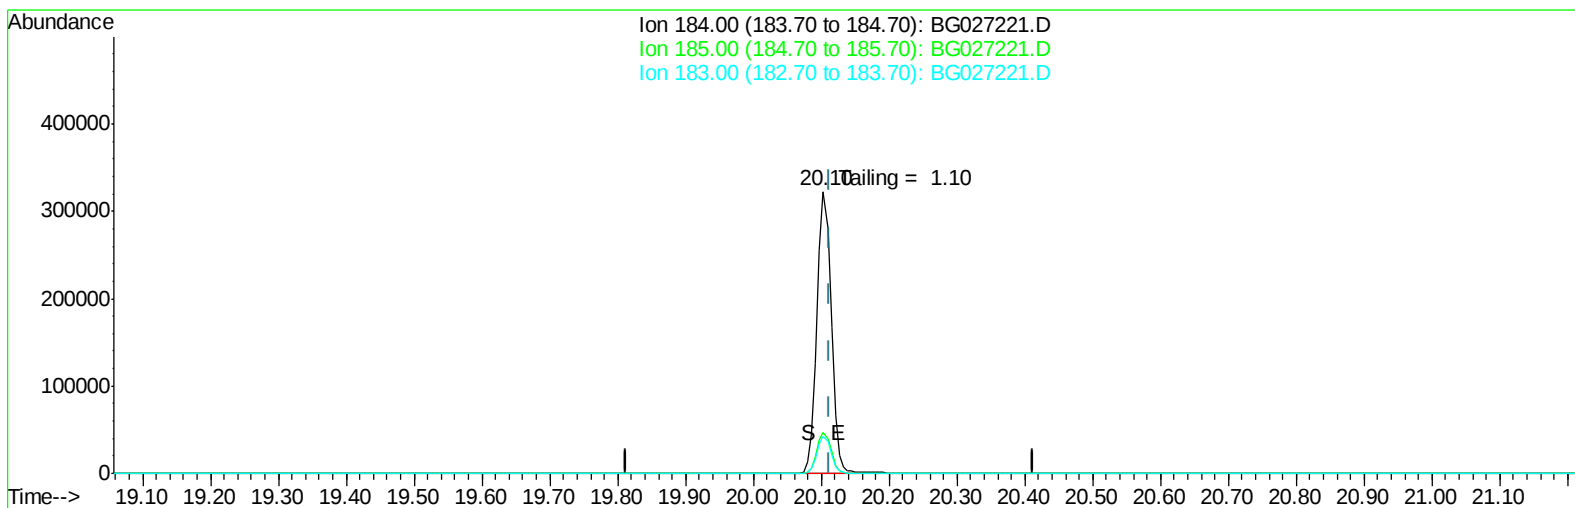

TIC: BG027221.D

(76) Benzidine

20.103min (-0.009) 0.00ng

response 466639

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	14.58
183.00	13.80	13.17
0.00	0.00	0.00