


Data Path : Z:\HPCHEM1\BNA G\Data\BG060517\
 Data File : BG027205.D
 Acq On : 5 Jun 2017 9:55
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 05 16:00:35 2017

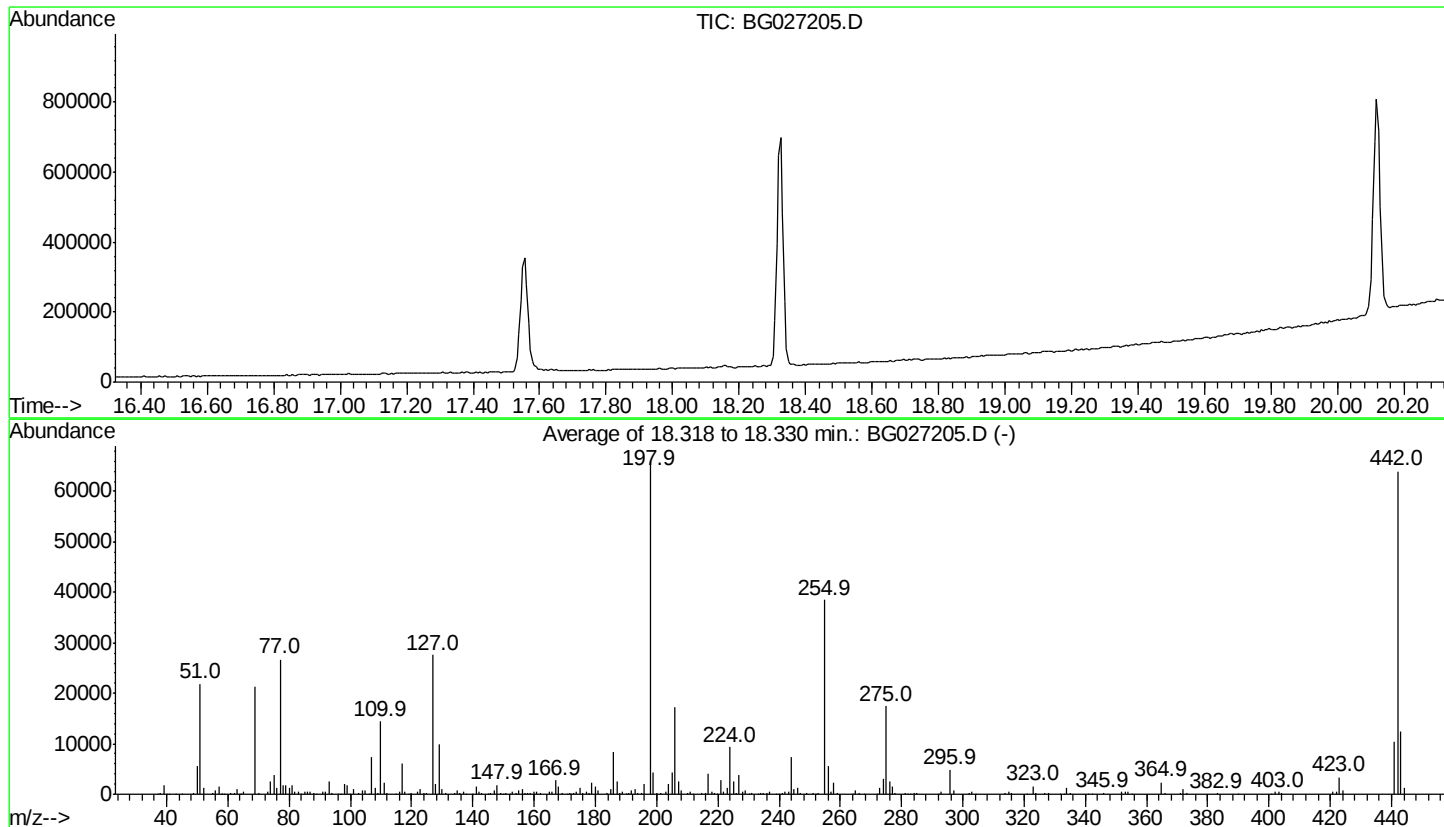

AutoFind: Scans 2490, 2491, 2492; Background Corrected with Scan 2483

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.3	21913	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	32.4	21267	PASS
70	69	0.00	2	0.8	178	PASS
127	198	10	80	42.0	27586	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	65712	PASS
199	198	5	9	6.7	4395	PASS
275	198	10	60	26.6	17460	PASS
365	198	1	100	3.5	2328	PASS
441	442	0.01	24	16.3	10434	PASS
442	198	50	100	97.4	64002	PASS
443	442	15	24	19.3	12353	PASS