


Data Path : Z:\HPCHEM1\BNA G\Data\BG060517\
 Data File : BG027221.D
 Acq On : 5 Jun 2017 20:33
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 05 16:00:35 2017

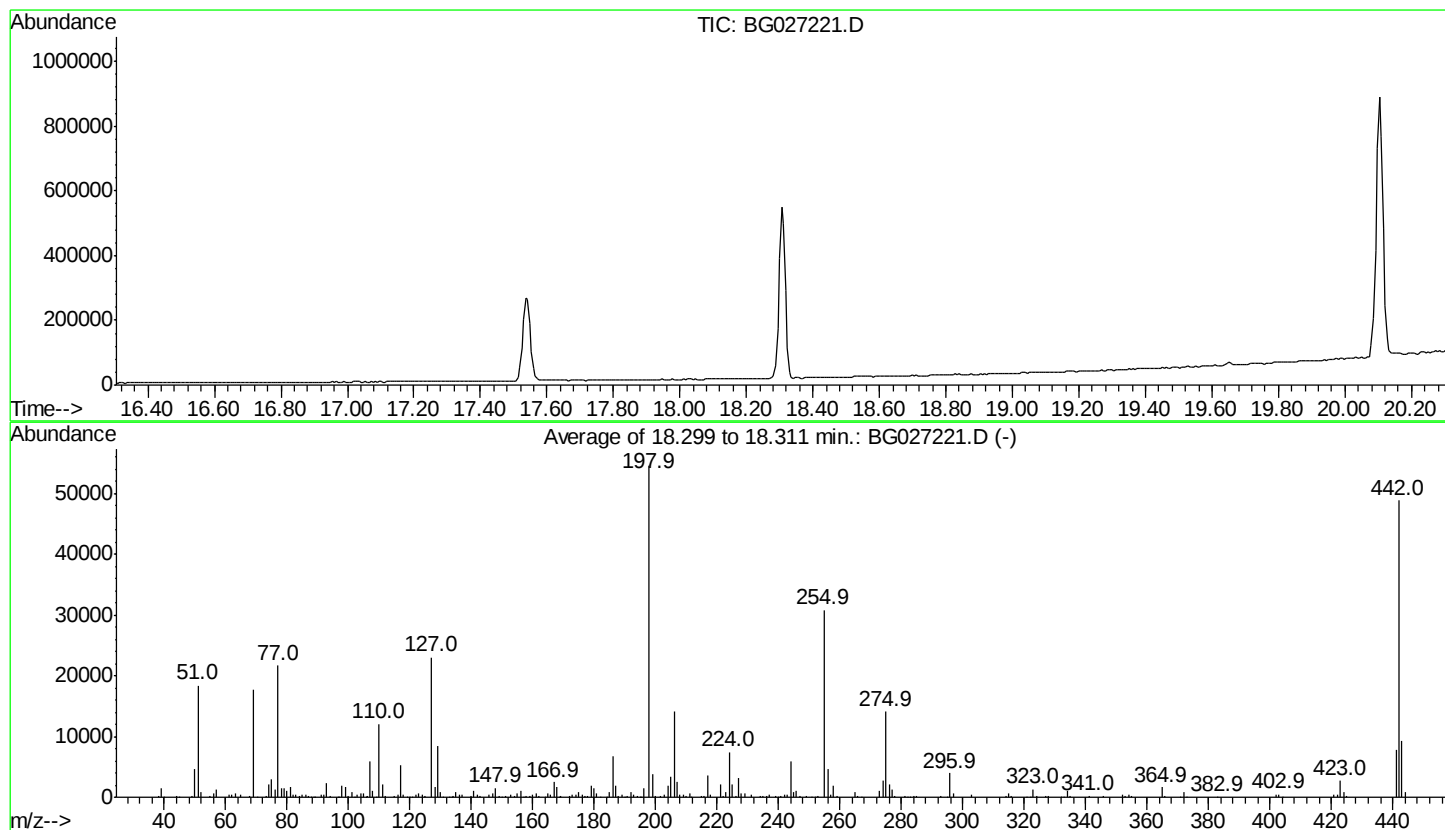

AutoFind: Scans 2487, 2488, 2489; Background Corrected with Scan 2481

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.7	18402	PASS
68	69	0.00	2	1.1	191	PASS
69	198	0.00	100	32.5	17741	PASS
70	69	0.00	2	0.3	58	PASS
127	198	10	80	42.1	22962	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	54568	PASS
199	198	5	9	7.0	3801	PASS
275	198	10	60	25.8	14084	PASS
365	198	1	100	3.0	1620	PASS
441	442	0.01	24	16.2	7886	PASS
442	198	50	100	89.4	48778	PASS
443	442	15	24	19.2	9348	PASS