
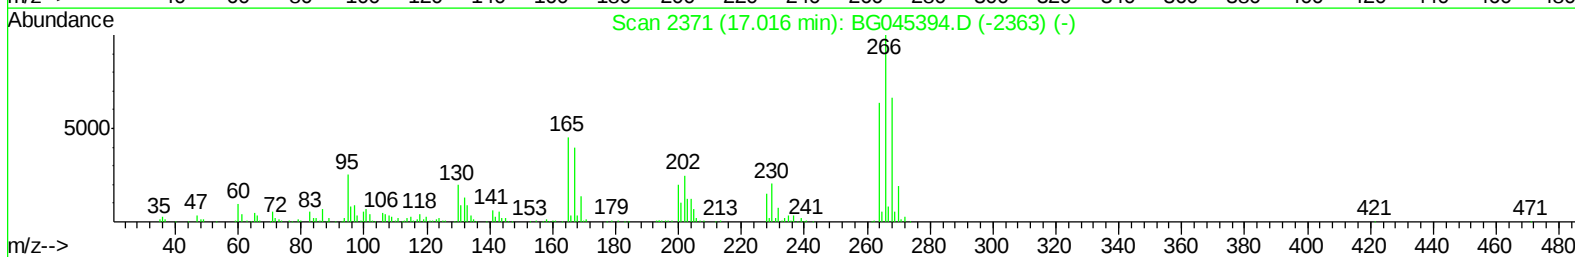
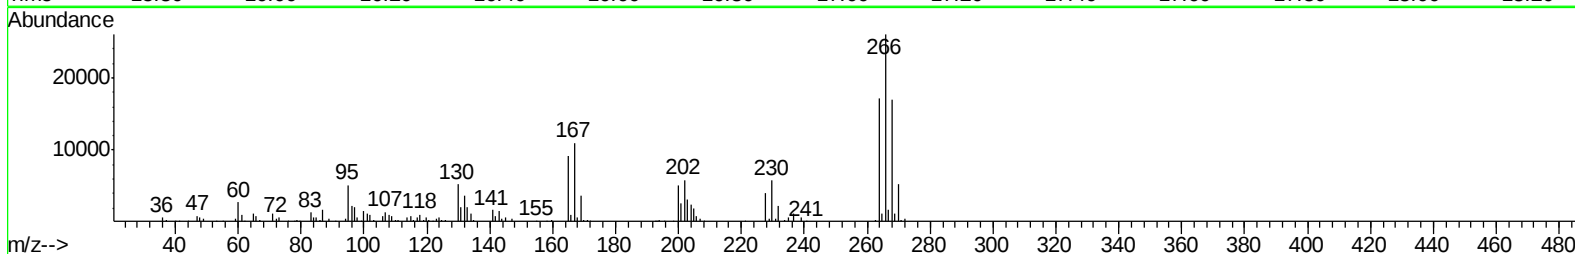


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG060520\
 Data File : BG045629.D
 Acq On : 5 Jun 2020 23:36
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 06 00:14:34 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG051520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 01 15:07:00 2020
 Response via : Initial Calibration

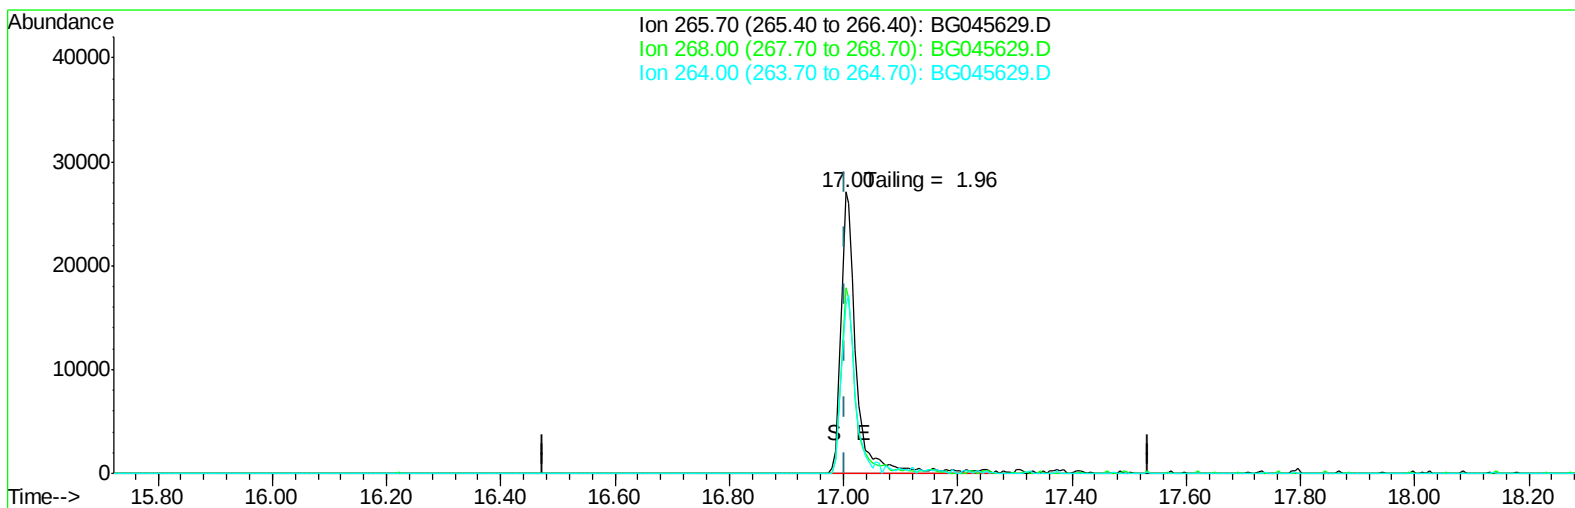

TIC: BG045629.D

(70) Pentachlorophenol (C)




17.003min (-0.001) 0.00ng

response 48132

Ion	Exp%	Act%
265.70	100	100
268.00	66.50	65.95
264.00	63.70	59.82
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG060520\
 Data File : BG045629.D
 Acq On : 5 Jun 2020 23:36
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 06 00:14:34 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG051520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 01 15:07:00 2020
 Response via : Initial Calibration

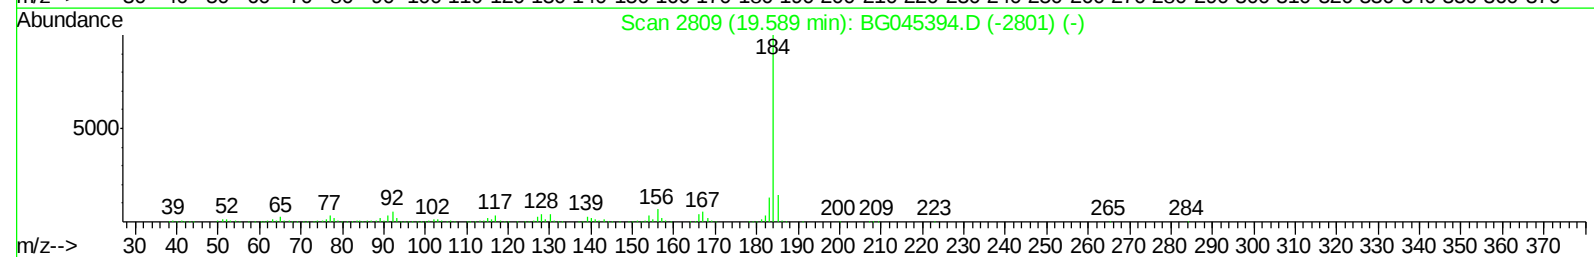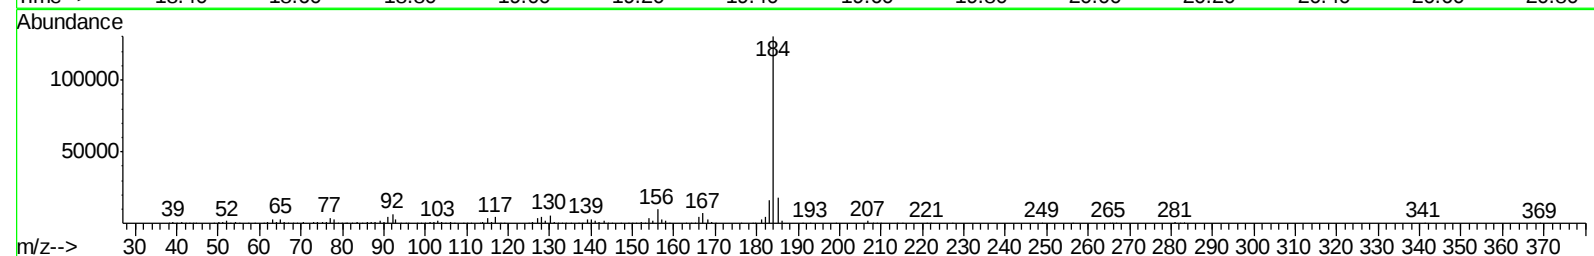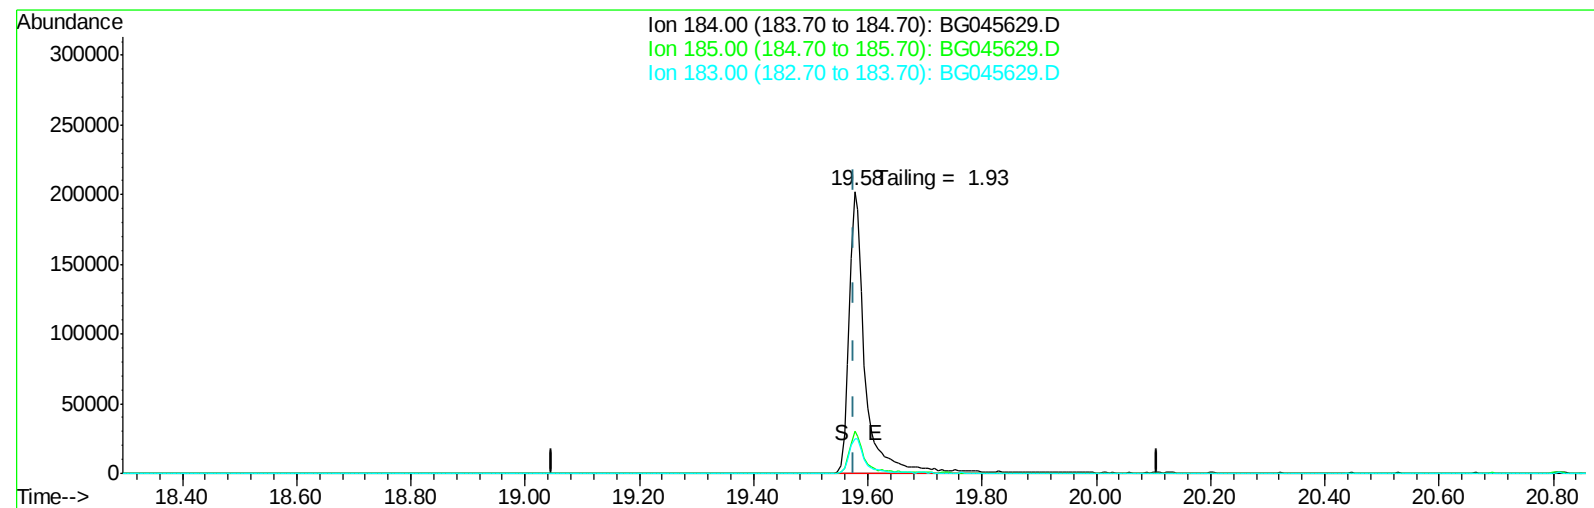

TIC: BG045629.D

(77) Benzidine

19.576min (-0.001) 252073.89ng

response 389379

Ion	Exp%	Act%
184.00	100	100
185.00	14.60	15.04
183.00	12.80	12.42
0.00	0.00	0.00