


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG060520\
 Data File : BG045611.D
 Acq On : 5 Jun 2020 10:58
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG051520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 01 15:07:00 2020

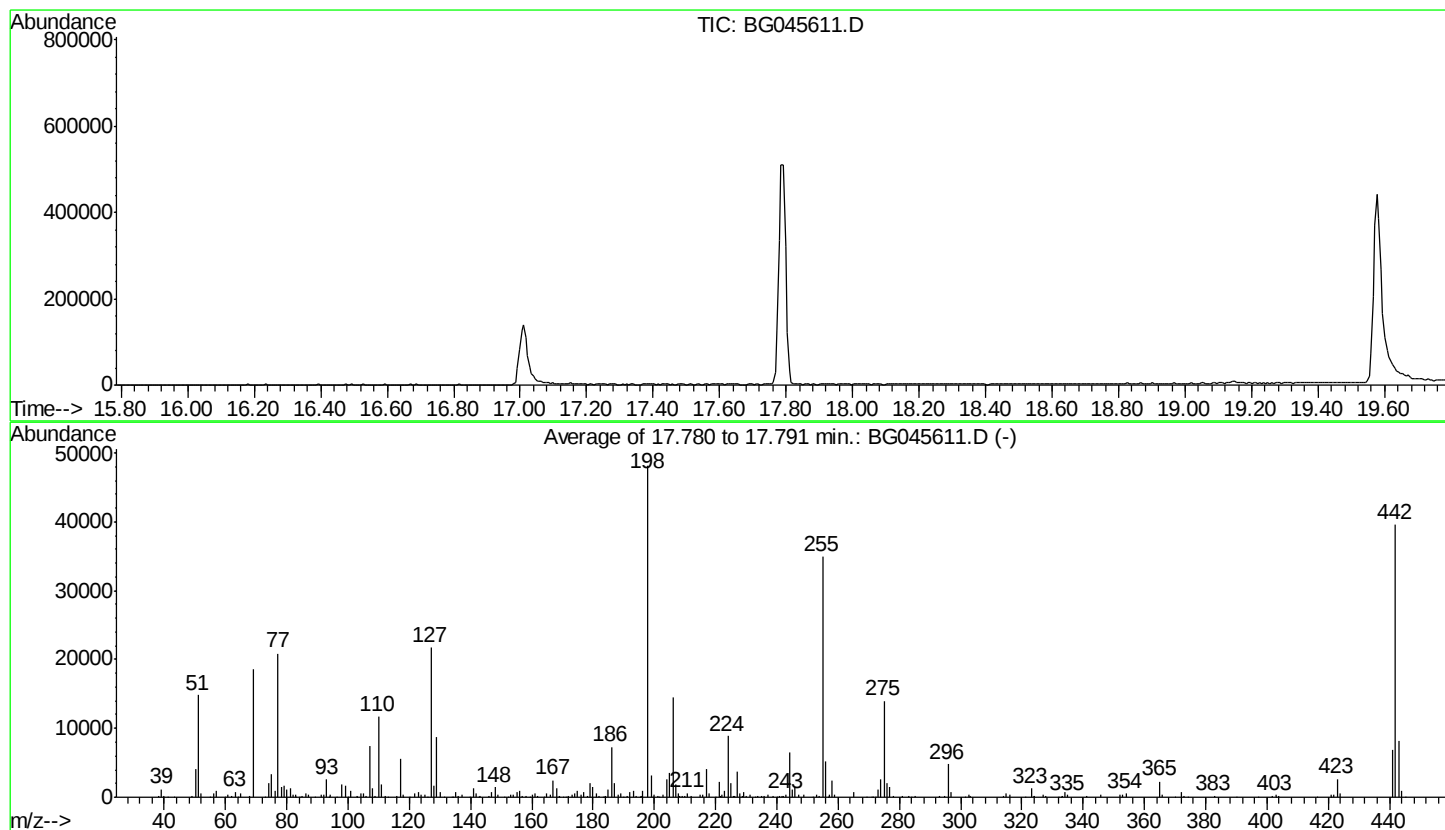

AutoFind: Scans 2501, 2502, 2503; Background Corrected with Scan 2495

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.9	14865	PASS
68	69	0.00	2	1.0	184	PASS
69	198	0.00	100	38.7	18658	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	45.1	21744	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	48162	PASS
199	198	5	9	6.7	3245	PASS
275	198	10	60	29.1	14022	PASS
365	198	1	100	4.8	2320	PASS
441	198	0.01	100	14.3	6895	PASS
442	198	50	100	82.2	39584	PASS
443	442	15	24	20.5	8125	PASS