


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG060520\
 Data File : BG045629.D
 Acq On : 5 Jun 2020 23:36
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG051520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 01 15:07:00 2020

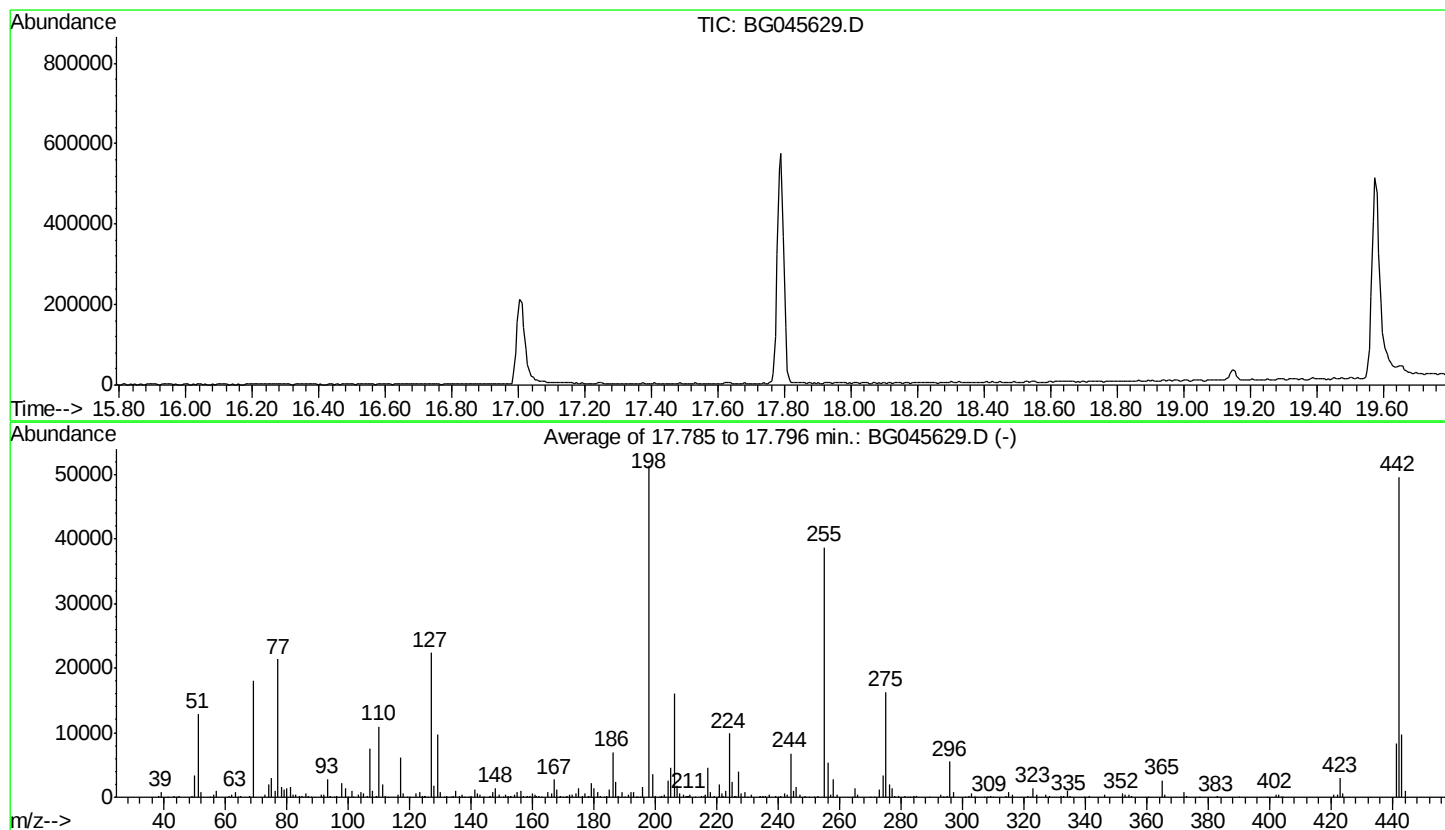

AutoFind: Scans 2502, 2503, 2504; Background Corrected with Scan 2495

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.2	12948	PASS
68	69	0.00	2	1.5	262	PASS
69	198	0.00	100	34.9	17948	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	43.5	22323	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	51354	PASS
199	198	5	9	7.1	3638	PASS
275	198	10	60	31.9	16357	PASS
365	198	1	100	5.1	2599	PASS
441	198	0.01	100	16.0	8241	PASS
442	198	50	100	96.6	49602	PASS
443	442	15	24	19.7	9772	PASS