

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG060615\
 Data File : BG017515.D
 Acq On : 7 Jun 2015 1:51
 Operator : TP/IZ
 Sample : G2457-27
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SP-6

Quant Time: Jun 08 05:18:36 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060315.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 04 01:31:15 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	14677	20.00	ng	0.00
21) Naphthalene-d8	10.42	136	61131	20.00	ng	0.00
38) Acenaphthene-d10	14.29	164	44063	20.00	ng	0.00
63) Phenanthrene-d10	17.05	188	107274	20.00	ng	0.00
75) Chrysene-d12	21.24	240	118407	20.00	ng	0.00
86) Perylene-d12	23.48	264	120276	20.00	ng	0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.22	112	111072	133.33	ng	0.00
7) Phenol-d6	6.83	99	136840	120.57	ng	0.00
23) Nitrobenzene-d5	8.79	82	111930	91.40	ng	0.00
41) 2,4,6-Tribromophenol	15.79	330	80529	131.58	ng	0.00
44) 2-Fluorobiphenyl	12.90	172	262573	89.89	ng	0.00
78) Terphenyl-d14	19.68	244	520004	90.77	ng	0.00


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG060615\
Data File : BG017515.D
Acq On : 7 Jun 2015 1:51
Operator : TP/IZ
Sample : G2457-27
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SP-6

Quant Time: Jun 08 05:18:36 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 04 01:31:15 2015
Response via : Initial Calibration

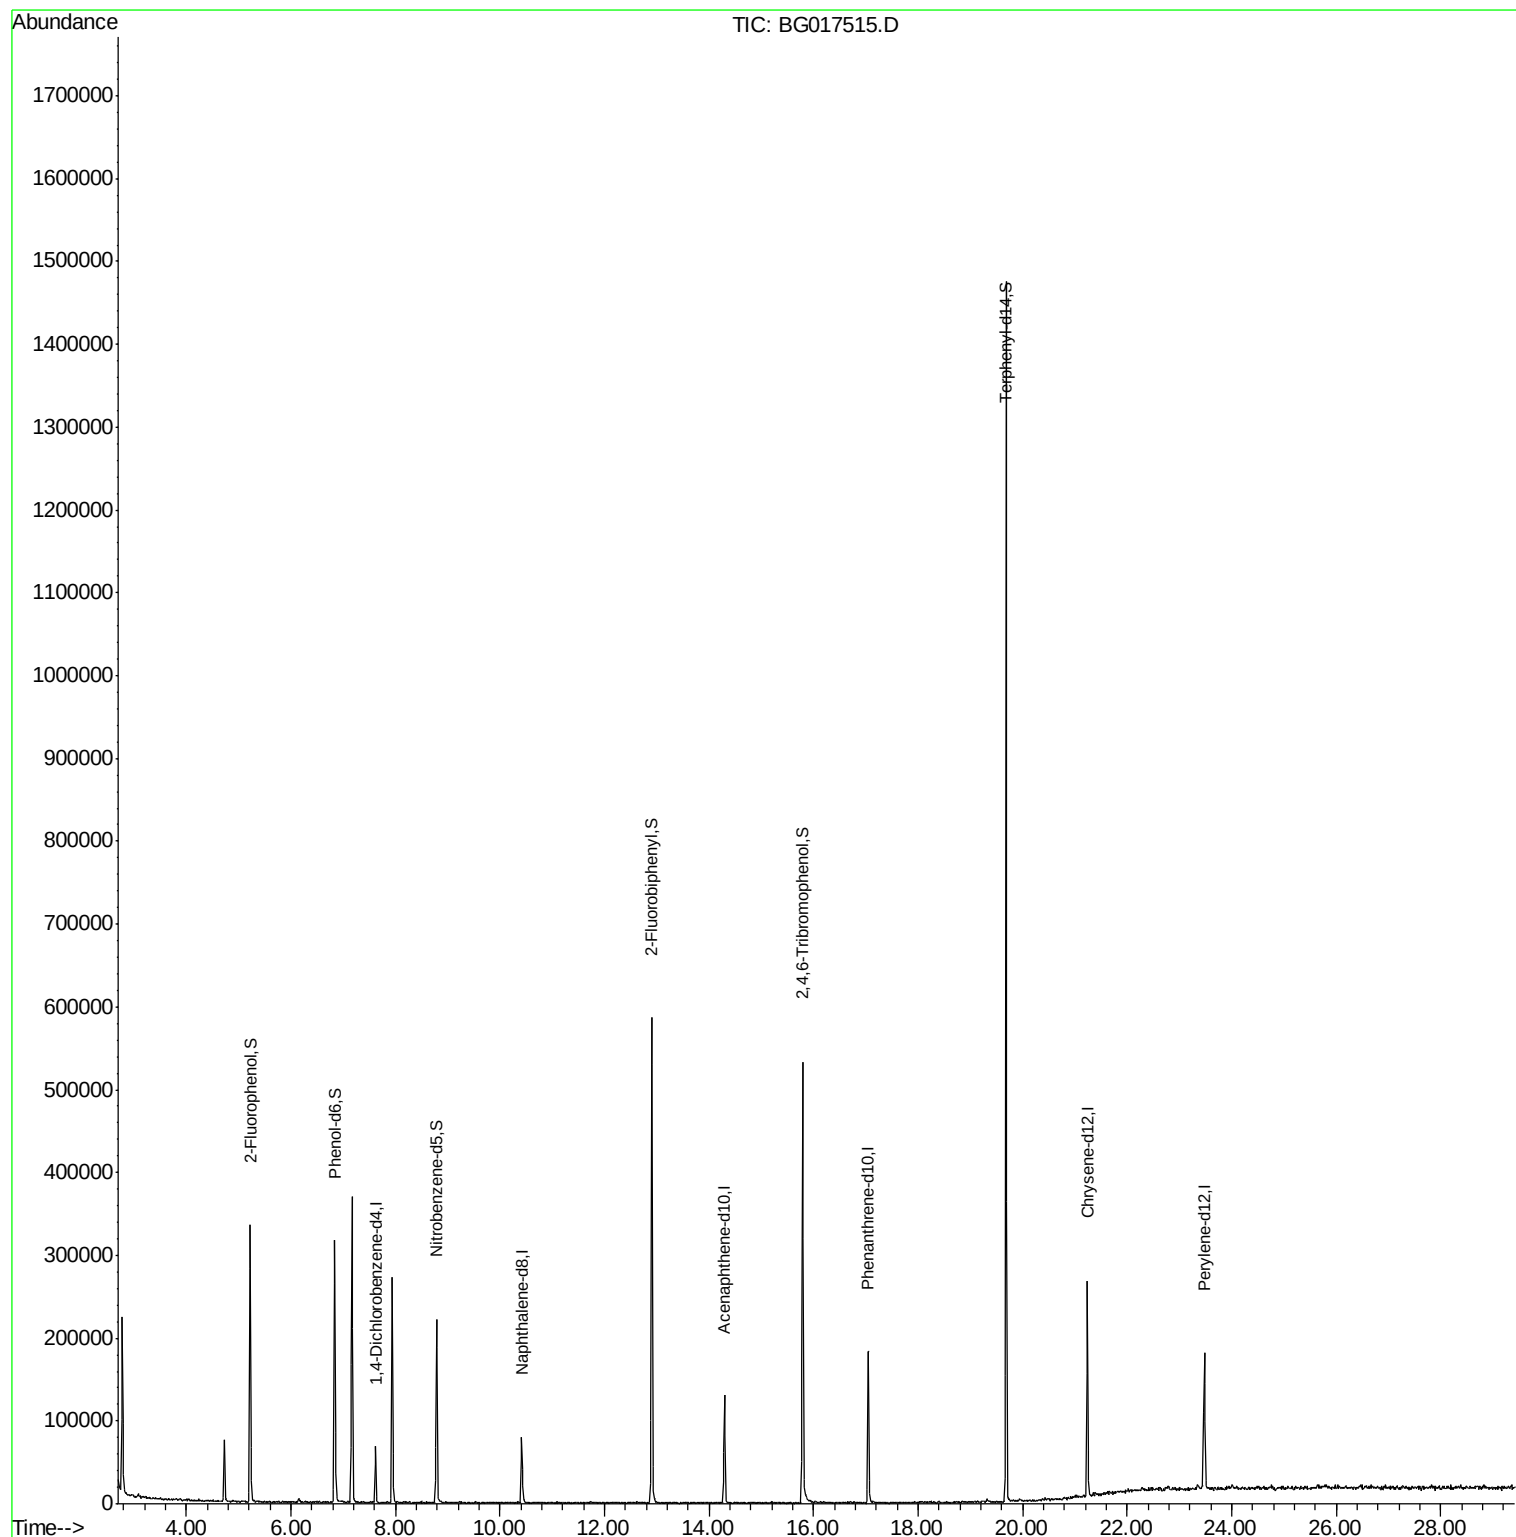

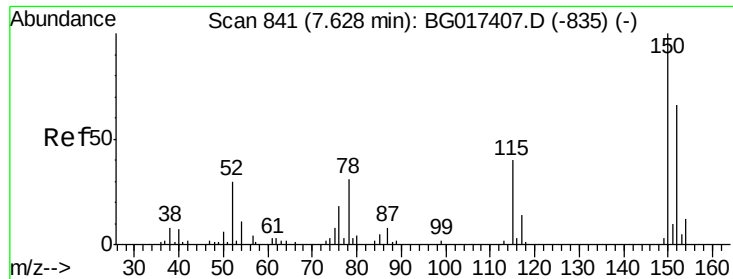

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 7.62 min Scan# 840

Delta R.T. -0.01 min

Lab File: BG017515.D

Acq: 7 Jun 2015 1:51

Instrument :

BNA_G

ClientSampleId :

SP-6


Tgt Ion:152 Resp: 14677

Ion Ratio Lower Upper

152 100

150 149.7 121.7 182.5




115 54.2 48.6 73.0

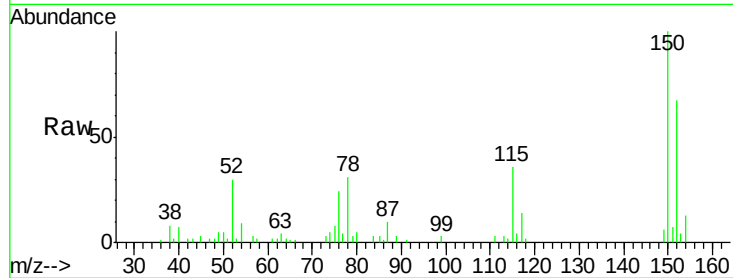

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

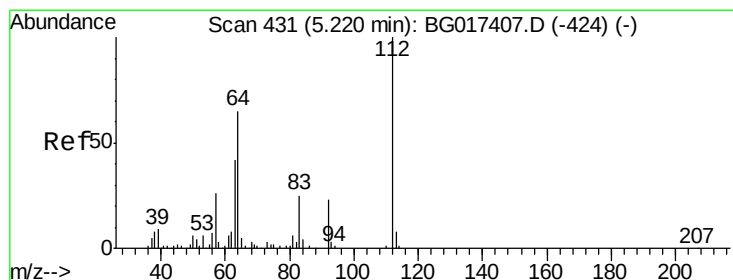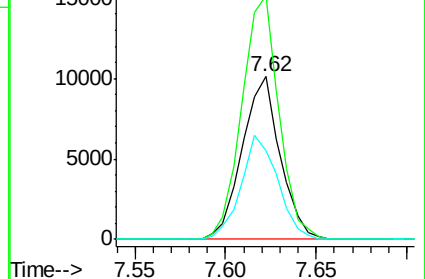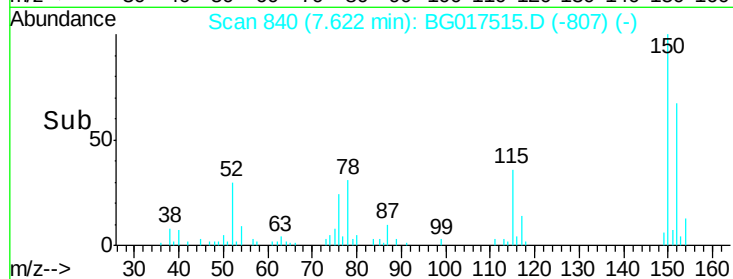

#5

2-Fluorophenol

Concen: 133.33 ng

RT: 5.22 min Scan# 431

Delta R.T. -0.00 min

Lab File: BG017515.D

Acq: 7 Jun 2015 1:51


Tgt Ion:112 Resp: 111072

Ion Ratio Lower Upper

112 100

64 68.6 51.6 77.4



63 44.0 33.3 49.9

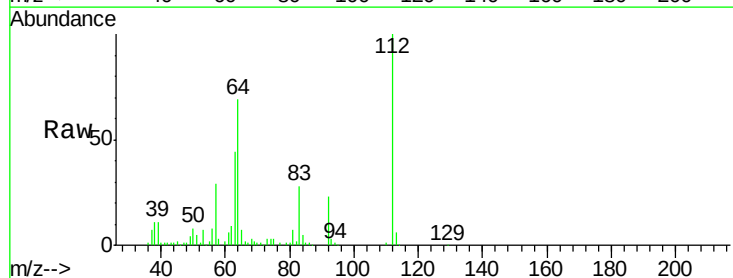


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BGC

Ion 63.00 (62.70 to 63.70): BGC

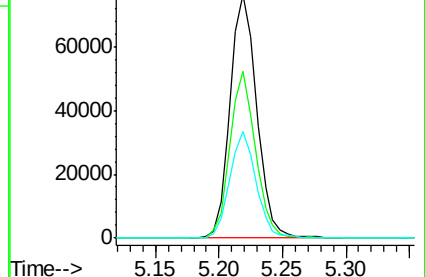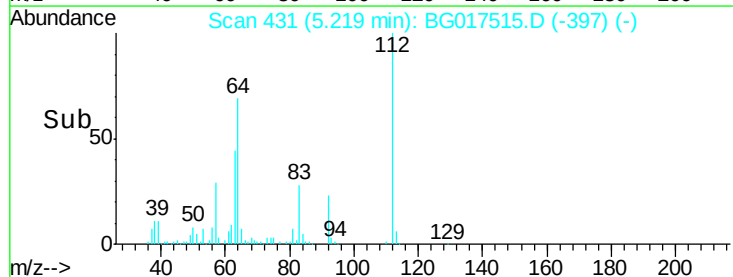

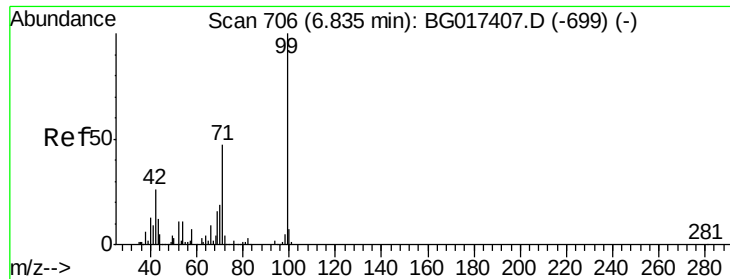

#7

Phenol-d6

Concen: 120.57 ng

RT: 6.83 min Scan# 706

Delta R.T. -0.00 min

Lab File: BG017515.D

Acq: 7 Jun 2015 1:51

Instrument :

BNA_G

ClientSampleId :

SP-6





Tgt Ion: 99 Resp: 136840

Ion Ratio Lower Upper

99 100

42 32.1 21.0 31.6#

71 55.1 37.2 55.8

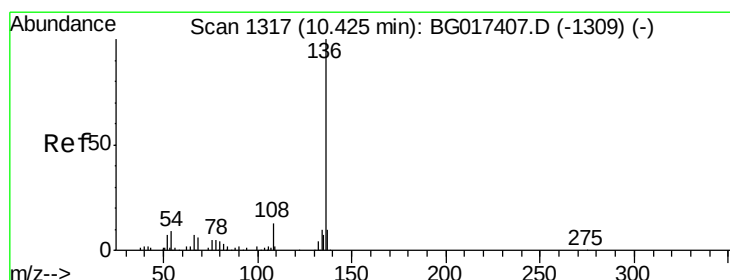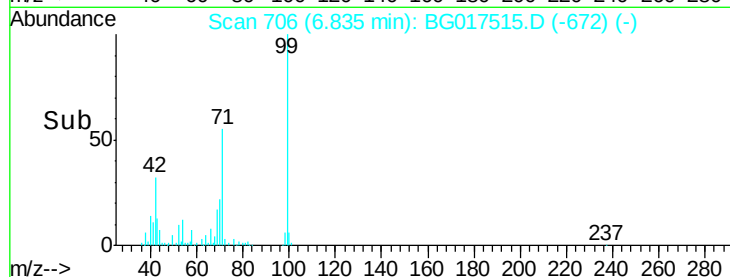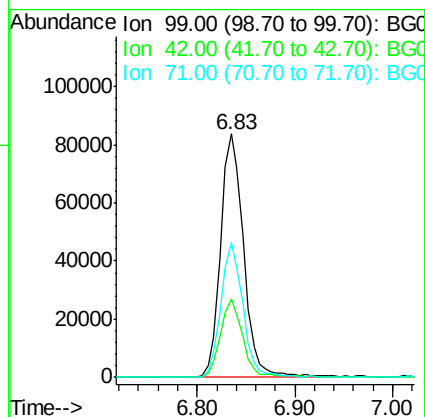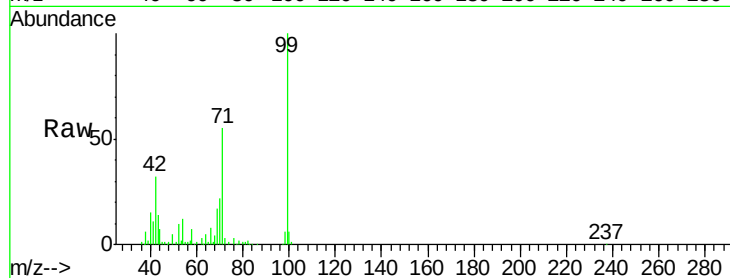

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.42 min Scan# 1316

Delta R.T. -0.01 min

Lab File: BG017515.D

Acq: 7 Jun 2015 1:51

Tgt Ion: 136 Resp: 61131




Ion Ratio Lower Upper


136 100

137 10.4 7.9 11.9

54 10.7 7.2 10.8

68 5.8 4.5 6.7


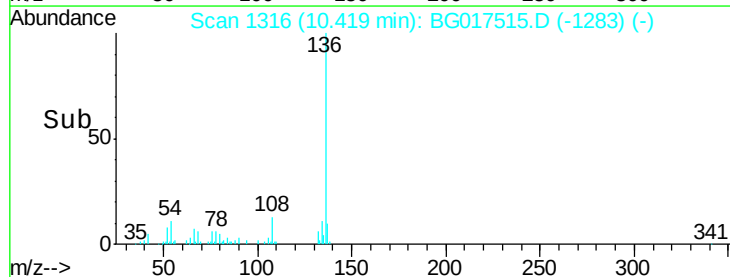
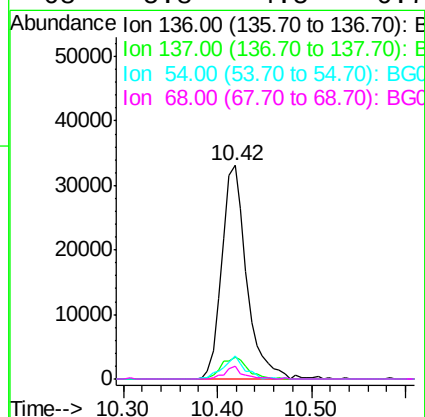
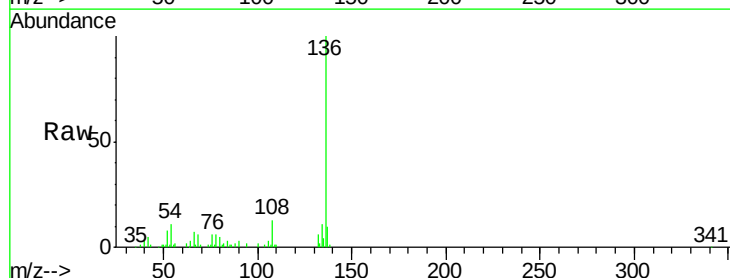


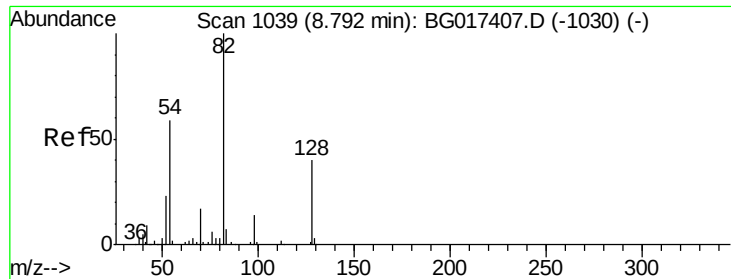

#23
 Nitrobenzene-d5
 Concen: 91.40 ng
 RT: 8.79 min Scan# 1038
 Delta R.T. -0.01 min
 Lab File: BG017515.D
 Acq: 7 Jun 2015 1:51




Instrument :
 BNA_G
 ClientSampleId :
 SP-6


Tgt Ion: 82 Resp: 111930
 Ion Ratio Lower Upper
 82 100
 128 37.7 32.2 48.4
 54 62.3 47.4 71.2

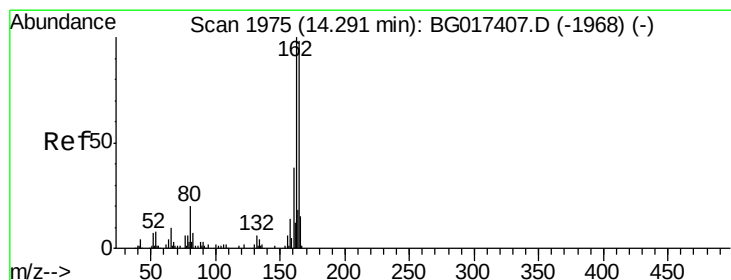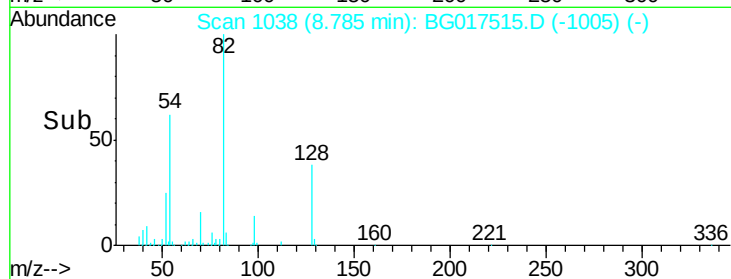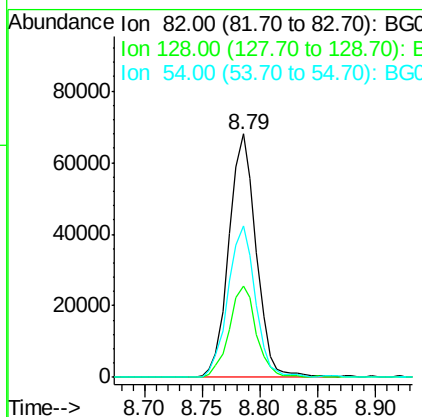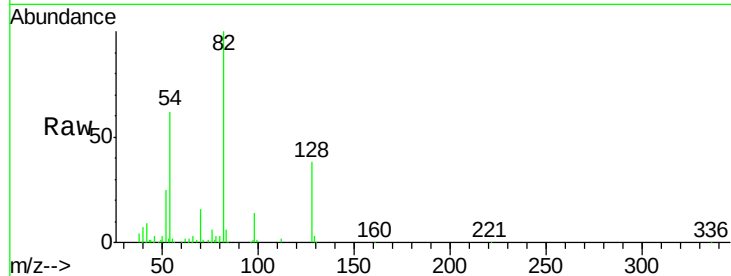

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 14.29 min Scan# 1975
 Delta R.T. -0.00 min
 Lab File: BG017515.D
 Acq: 7 Jun 2015 1:51

Tgt Ion: 164 Resp: 44063
 Ion Ratio Lower Upper
 164 100
 162 105.3 81.8 122.6
 160 45.2 31.0 46.4

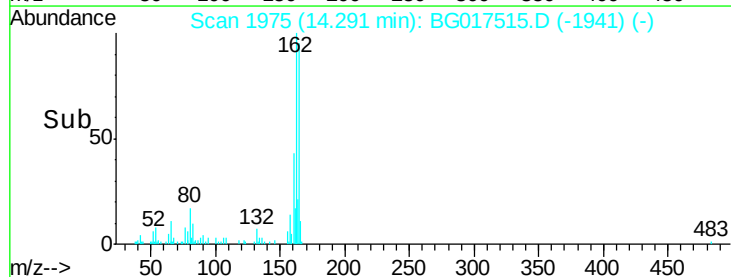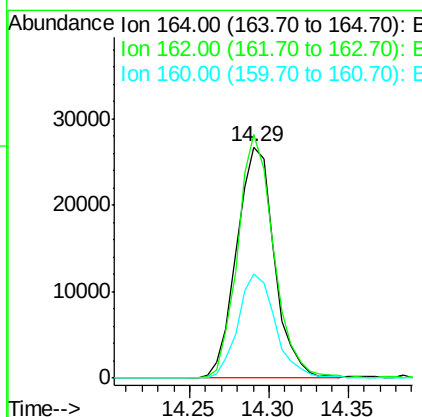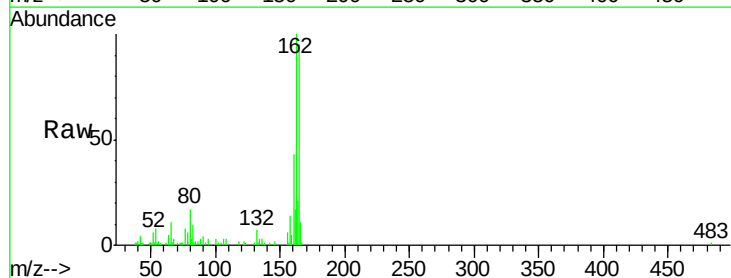


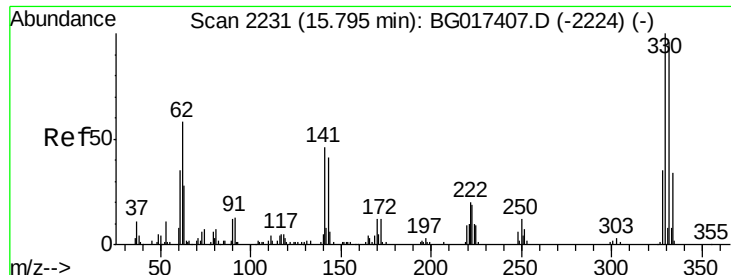




#41
 2,4,6-Tribromophenol
 Concen: 131.58 ng
 RT: 15.79 min Scan# 2231
 Delta R.T. -0.00 min
 Lab File: BG017515.D
 Acq: 7 Jun 2015 1:51

Instrument :
 BNA_G
 ClientSampleId :
 SP-6

Tgt Ion:330 Resp: 80529
 Ion Ratio Lower Upper
 330 100
 332 97.6 75.9 113.9
 141 51.2 40.2 60.4

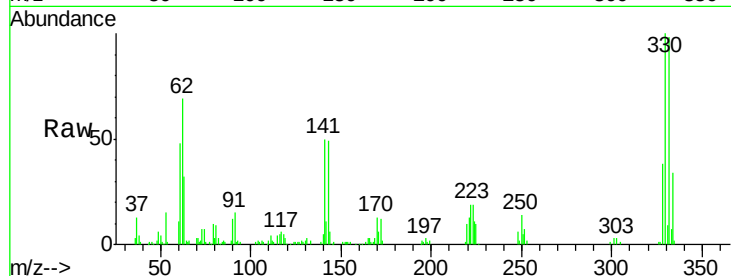


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

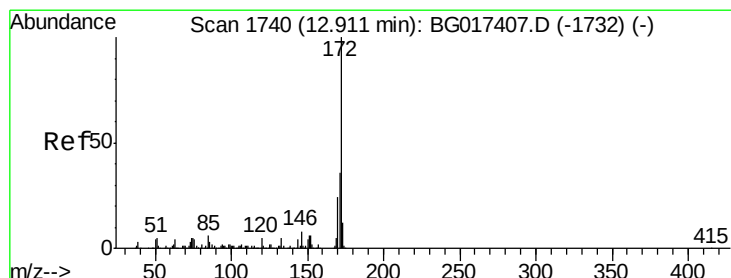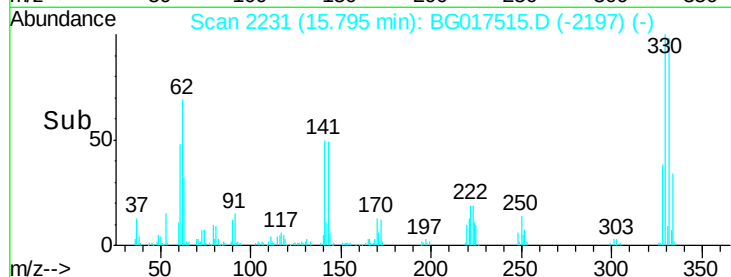
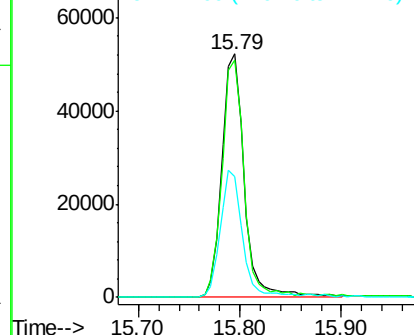



#44
 2-Fluorobiphenyl
 Concen: 89.89 ng
 RT: 12.90 min Scan# 1739
 Delta R.T. -0.01 min
 Lab File: BG017515.D
 Acq: 7 Jun 2015 1:51

Tgt Ion:172 Resp: 262573
 Ion Ratio Lower Upper
 172 100
 171 37.1 29.0 43.6
 170 22.3 18.9 28.3

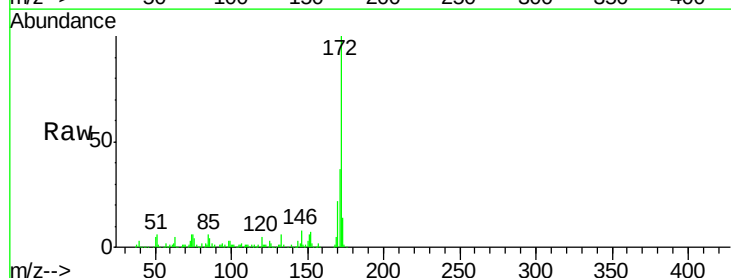

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

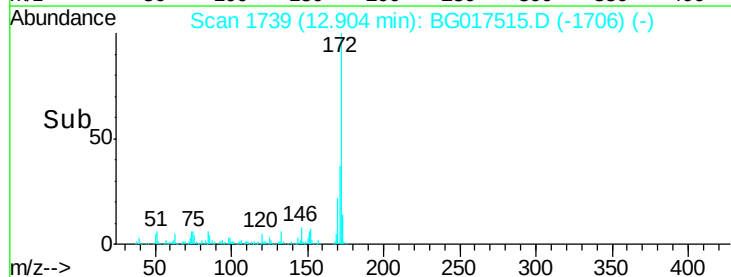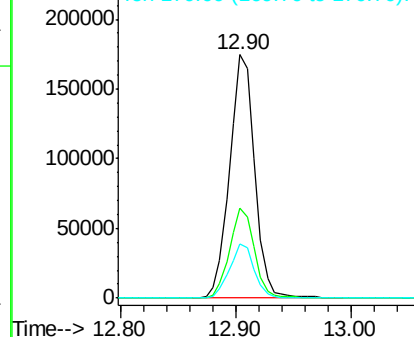


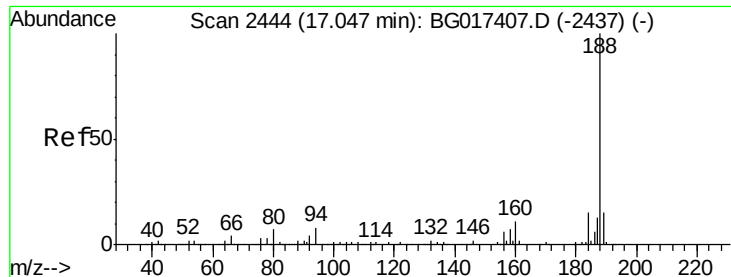




#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 17.05 min Scan# 2444
Delta R.T. -0.00 min
Lab File: BG017515.D
Acq: 7 Jun 2015 1:51

Instrument :
BNA_G
ClientSampleId :
SP-6

Tgt Ion:188 Resp: 107274
Ion Ratio Lower Upper
188 100
94 7.0 6.3 9.5
80 7.5 5.2 7.8

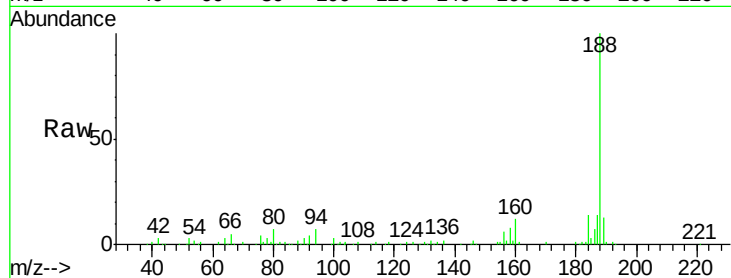


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BGC
Ion 80.00 (79.70 to 80.70): BGC

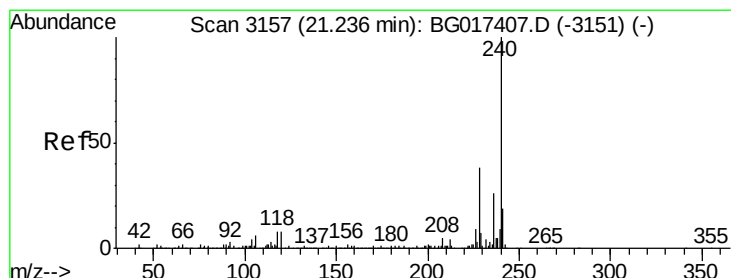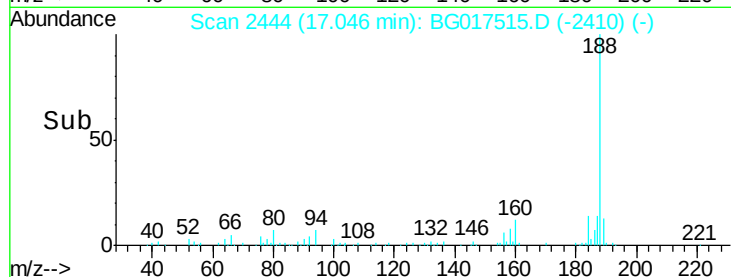
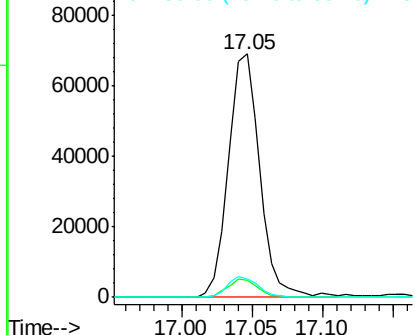



#75
Chrysene-d12
Concen: 20.00 ng
RT: 21.24 min Scan# 3158
Delta R.T. 0.01 min
Lab File: BG017515.D
Acq: 7 Jun 2015 1:51

Tgt Ion:240 Resp: 118407
Ion Ratio Lower Upper
240 100
120 7.6 6.5 9.7
236 24.4 20.8 31.2

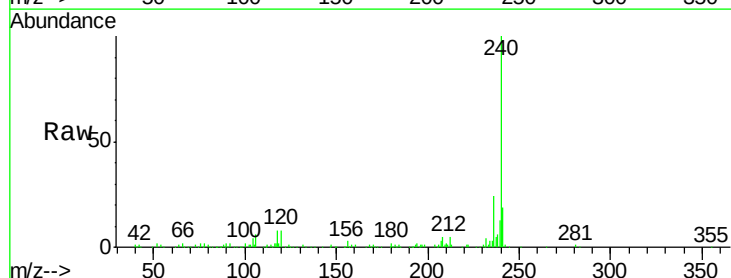

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

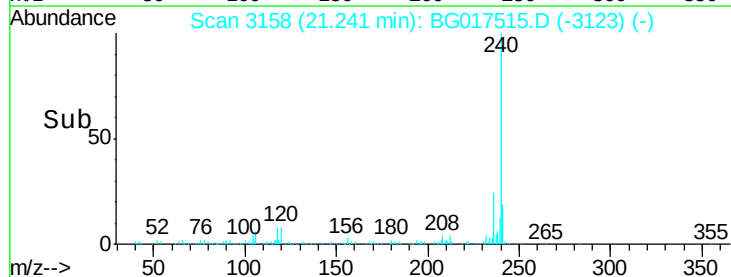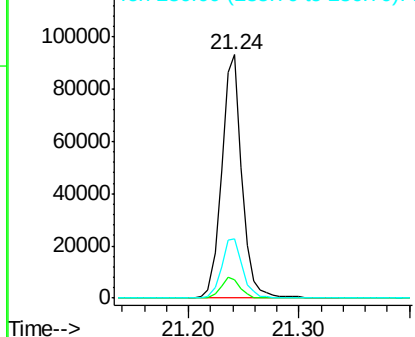

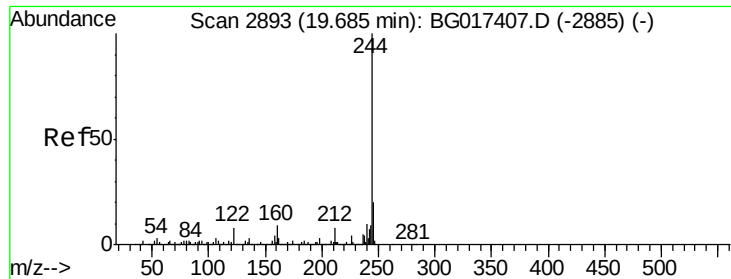

#78

Terphenyl-d14

Concen: 90.77 ng

RT: 19.68 min Scan# 2893

Delta R.T. -0.00 min

Lab File: BG017515.D

Acq: 7 Jun 2015 1:51

Instrument :

BNA_G

ClientSampleId :

SP-6


Tgt Ion:244 Resp: 520004

Ion Ratio Lower Upper

244 100

212 9.1 6.4 9.6




122 9.6 6.6 10.0

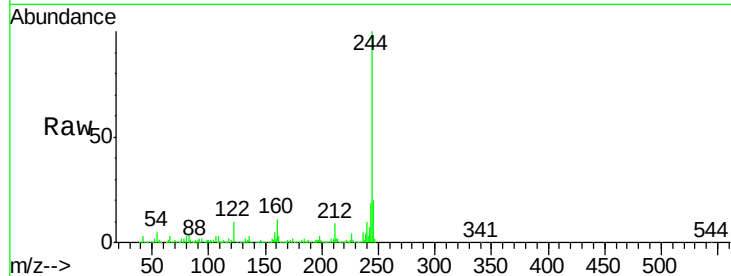

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

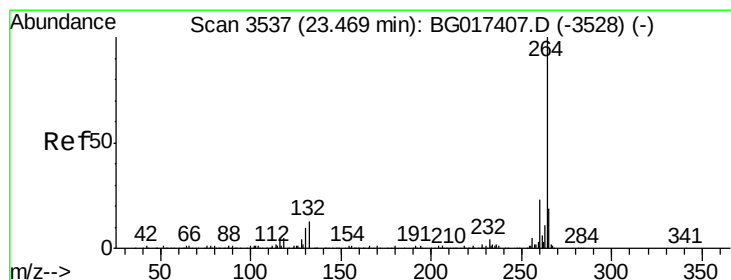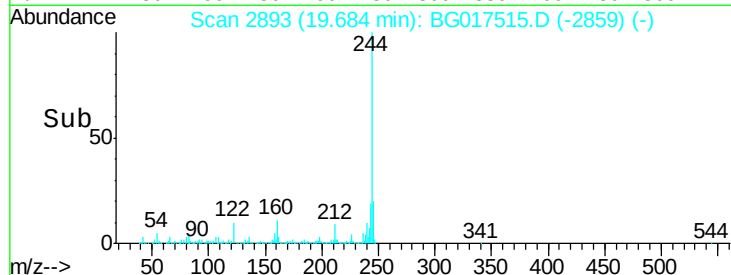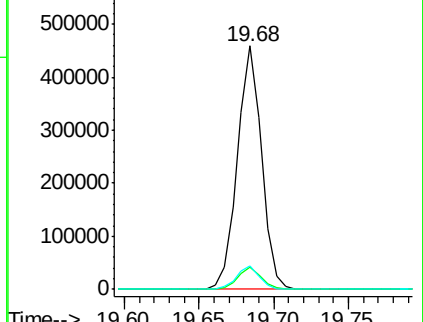

#86

Perylene-d12

Concen: 20.00 ng

RT: 23.48 min Scan# 3539

Delta R.T. 0.01 min

Lab File: BG017515.D

Acq: 7 Jun 2015 1:51


Tgt Ion:264 Resp: 120276

Ion Ratio Lower Upper

264 100

260 23.2 18.2 27.4

265 20.8 15.8 23.6

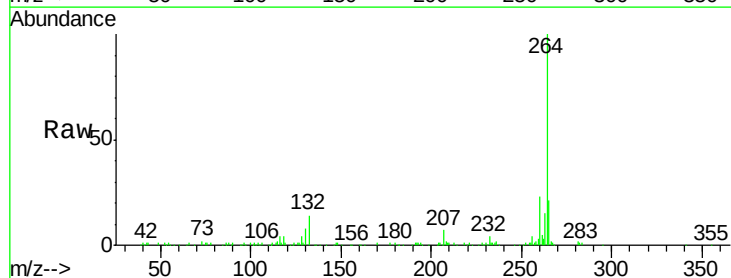

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

