

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG060615\
 Data File : BG017524.D
 Acq On : 7 Jun 2015 8:47
 Operator : TP/IZ
 Sample : G2517-01
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DCW-WW-147-6415

Quant Time: Jun 08 07:18:07 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060315.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 04 01:31:15 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	17343	20.00	ng	-0.01
21) Naphthalene-d8	10.41	136	66728	20.00	ng	-0.01
38) Acenaphthene-d10	14.29	164	46314	20.00	ng	0.00
63) Phenanthrene-d10	17.04	188	107998	20.00	ng	0.00
75) Chrysene-d12	21.24	240	125484	20.00	ng	0.00
86) Perylene-d12	23.47	264	124704	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.22	112	44761	45.47	ng	0.00
7) Phenol-d6	6.83	99	34377	25.63	ng	0.00
23) Nitrobenzene-d5	8.79	82	108533	81.19	ng	0.00
41) 2,4,6-Tribromophenol	15.79	330	80461	125.08	ng	0.00
44) 2-Fluorobiphenyl	12.90	172	258224	84.11	ng	0.00
78) Terphenyl-d14	19.68	244	454748	74.90	ng	0.00


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG060615\
Data File : BG017524.D
Acq On : 7 Jun 2015 8:47
Operator : TP/IZ
Sample : G2517-01
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DCW-WW-147-6415

Quant Time: Jun 08 07:18:07 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 04 01:31:15 2015
Response via : Initial Calibration

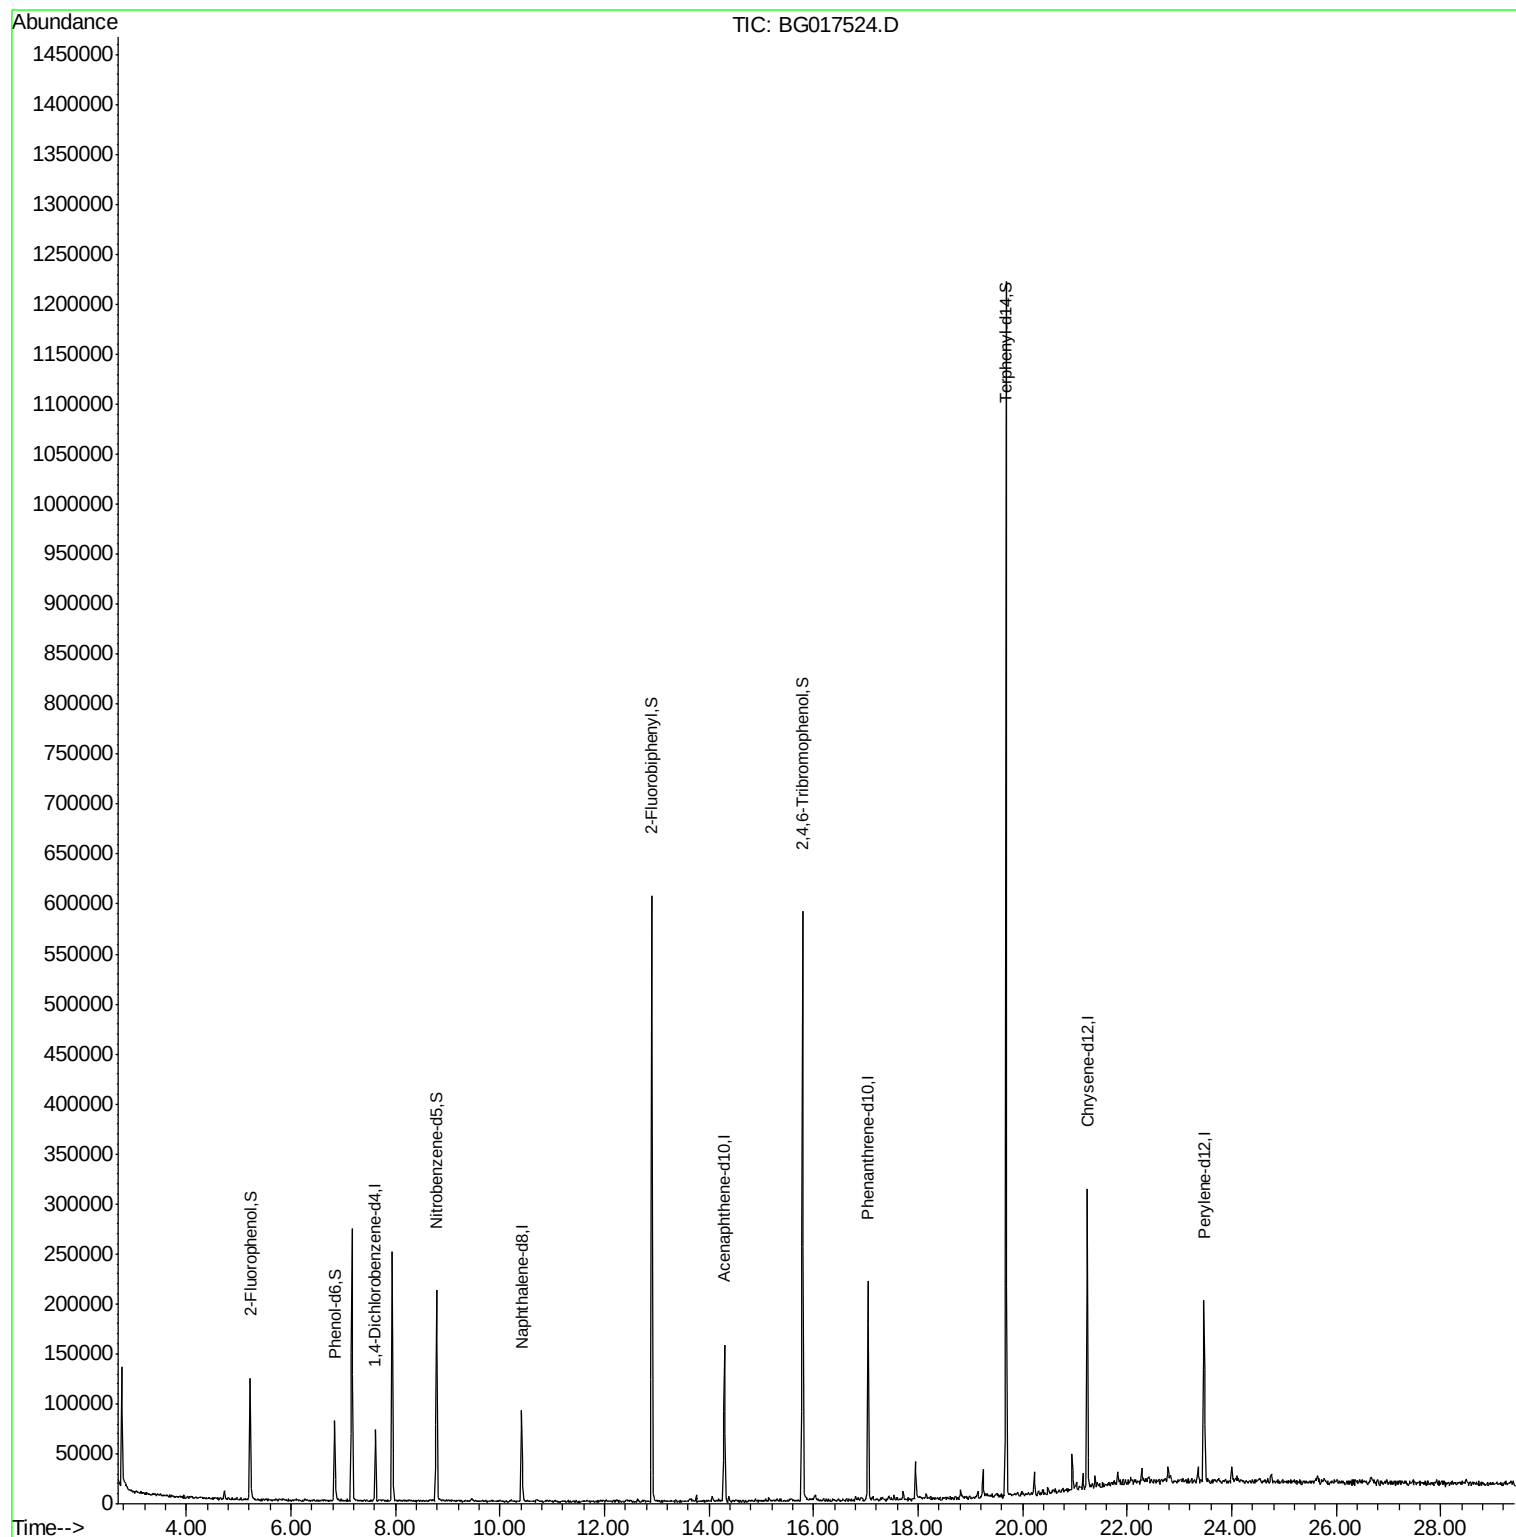

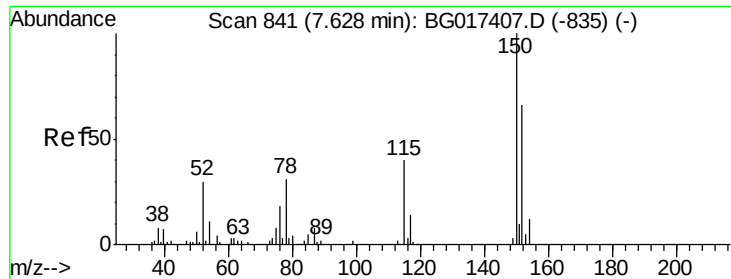


#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 7.62 min Scan# 839
Delta R.T. -0.01 min
Lab File: BG017524.D
Acq: 7 Jun 2015 8:47

Instrument :
BNA_G
ClientSampleId :
DCW-WW-147-6415

Tgt Ion:152 Resp: 17343
Ion Ratio Lower Upper
152 100
150 146.8 121.7 182.5
115 59.9 48.6 73.0

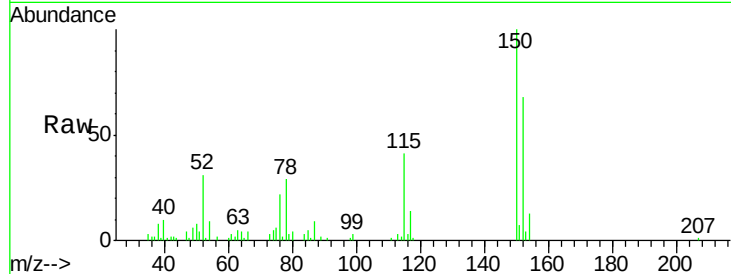


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

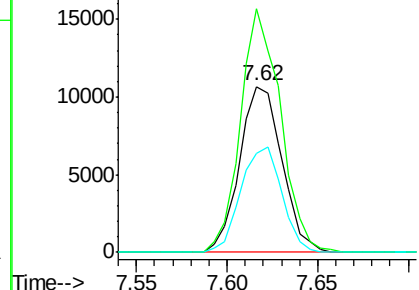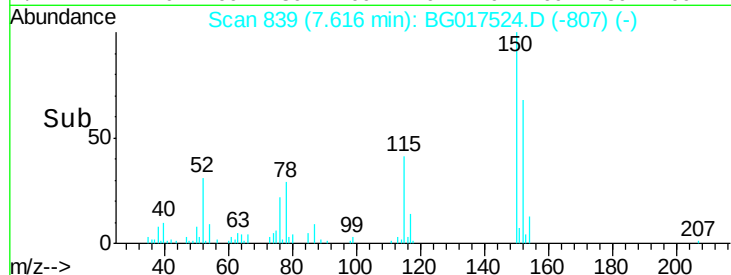



#5


2-Fluorophenol
Concen: 45.47 ng
RT: 5.22 min Scan# 431
Delta R.T. -0.00 min
Lab File: BG017524.D
Acq: 7 Jun 2015 8:47

Tgt Ion:112 Resp: 44761
Ion Ratio Lower Upper
112 100
64 65.4 51.6 77.4
63 37.3 33.3 49.9

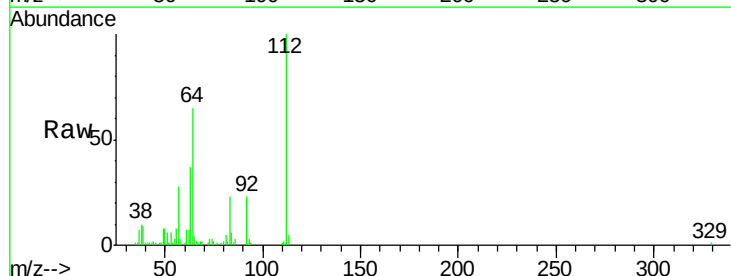

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BGO
Ion 63.00 (62.70 to 63.70): BGO

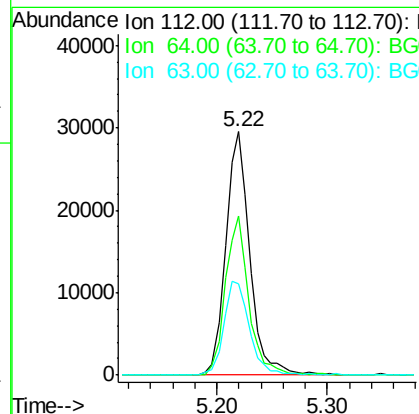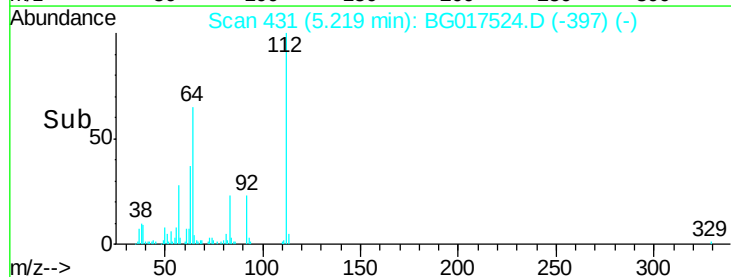

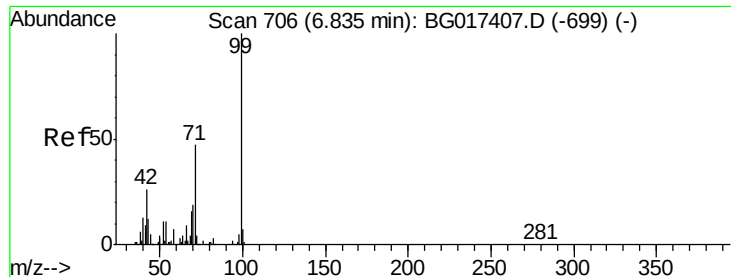

#7

Phenol-d6

Concen: 25.63 ng

RT: 6.83 min Scan# 706

Delta R.T. -0.00 min

Lab File: BG017524.D

Acq: 7 Jun 2015 8:47

Instrument :

BNA_G

ClientSampleId :

DCW-WW-147-6415


Tgt Ion: 99 Resp: 34377

Ion Ratio Lower Upper




99 100

42 29.7 21.0 31.6

71 50.7 37.2 55.8

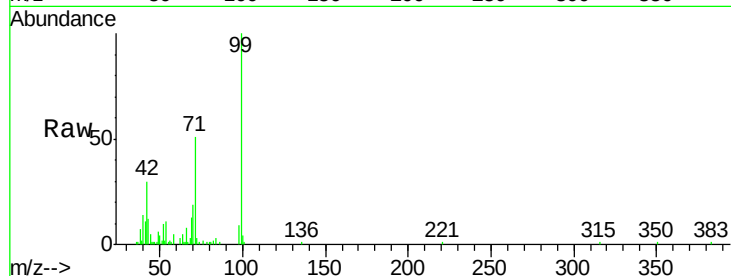

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

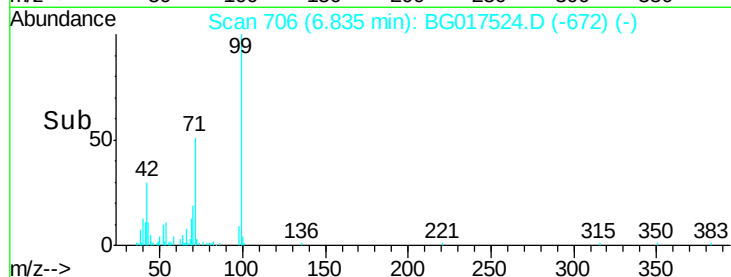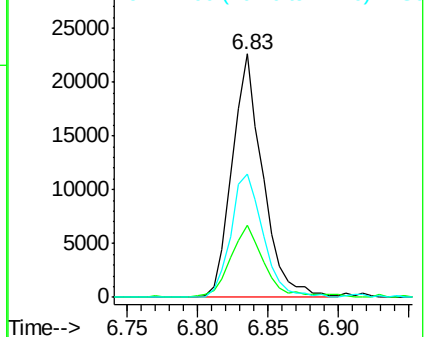

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.41 min Scan# 1315

Delta R.T. -0.01 min

Lab File: BG017524.D

Acq: 7 Jun 2015 8:47

Tgt Ion: 136 Resp: 66728


Ion Ratio Lower Upper

136 100



137 11.8 7.9 11.9


54 8.9 7.2 10.8

68 5.1 4.5 6.7



Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



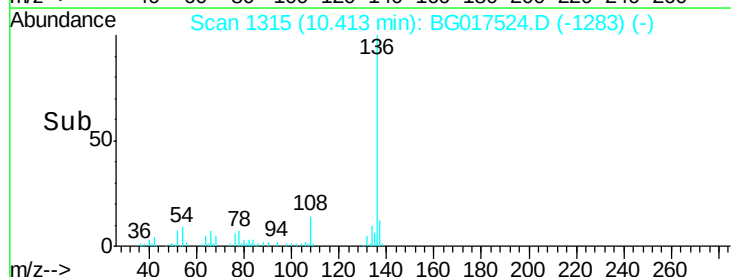
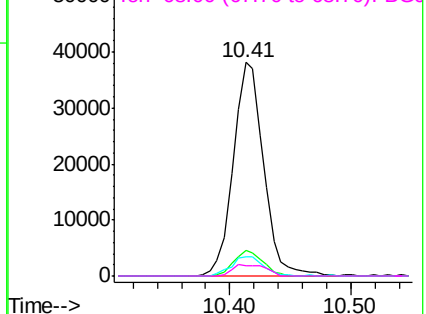


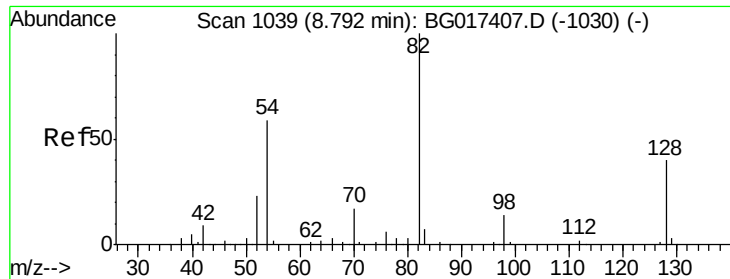

#23
 Nitrobenzene-d5
 Concen: 81.19 ng
 RT: 8.79 min Scan# 1038
 Delta R.T. -0.01 min
 Lab File: BG017524.D
 Acq: 7 Jun 2015 8:47




Instrument :
 BNA_G
 ClientSampleId :
 DCW-WW-147-6415


Tgt Ion: 82 Resp: 108533
 Ion Ratio Lower Upper
 82 100
 128 39.9 32.2 48.4
 54 61.5 47.4 71.2

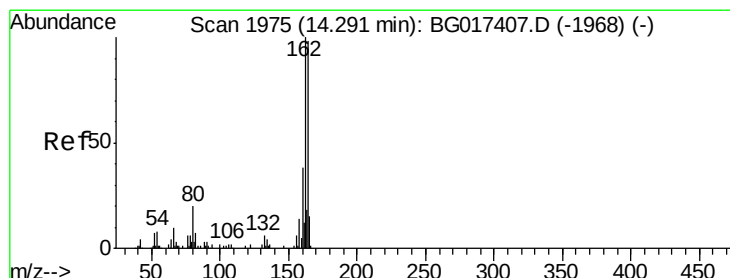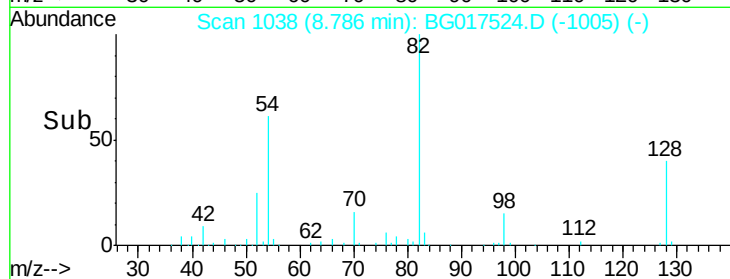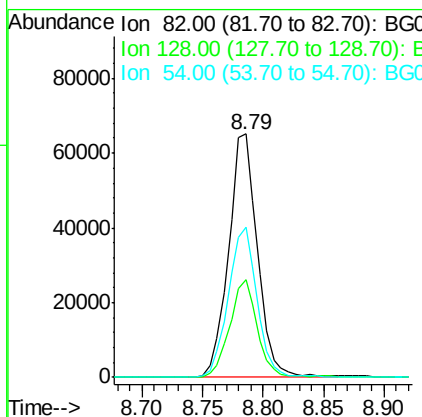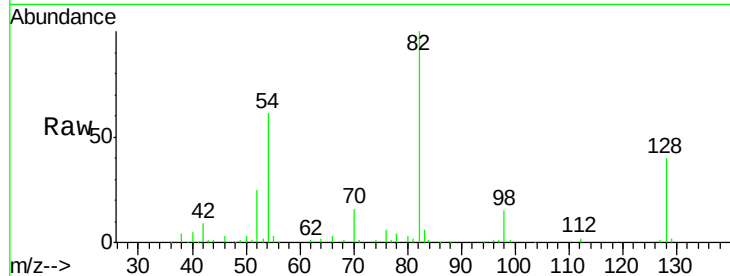

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 14.29 min Scan# 1975
 Delta R.T. -0.00 min
 Lab File: BG017524.D
 Acq: 7 Jun 2015 8:47

Tgt Ion: 164 Resp: 46314
 Ion Ratio Lower Upper
 164 100
 162 101.9 81.8 122.6
 160 46.7 31.0 46.4#

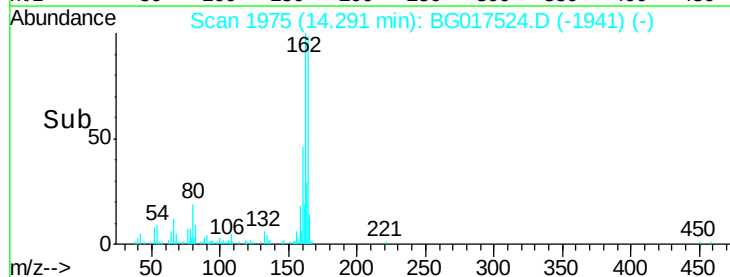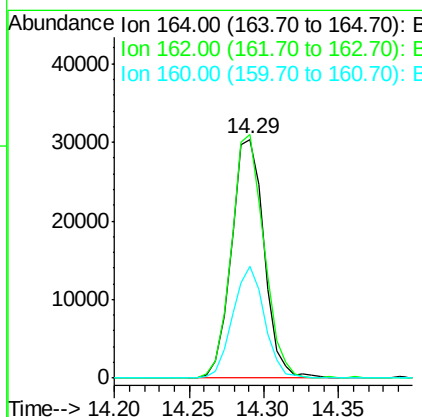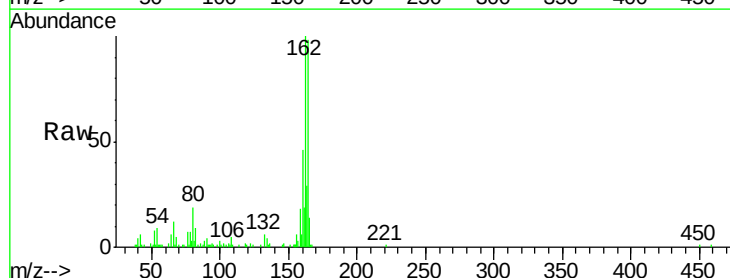


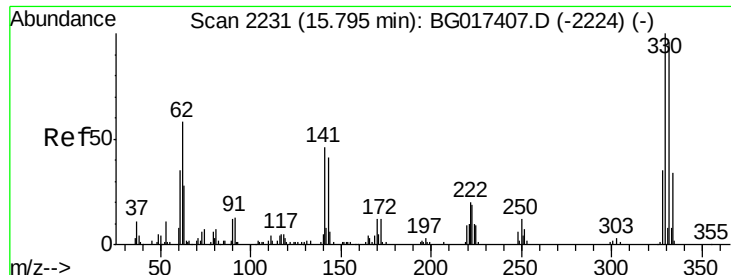




#41
 2,4,6-Tribromophenol
 Concen: 125.08 ng
 RT: 15.79 min Scan# 2230
 Delta R.T. -0.01 min
 Lab File: BG017524.D
 Acq: 7 Jun 2015 8:47

Instrument :
 BNA_G
 ClientSampleId :
 DCW-WW-147-6415

Tgt Ion:330 Resp: 80461
 Ion Ratio Lower Upper
 330 100
 332 94.3 75.9 113.9
 141 53.0 40.2 60.4

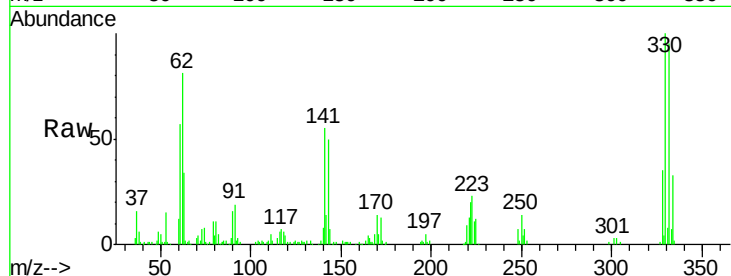


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

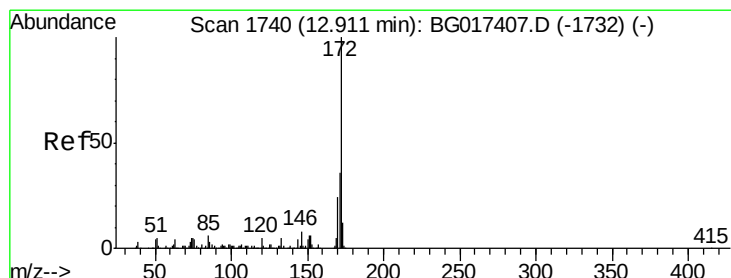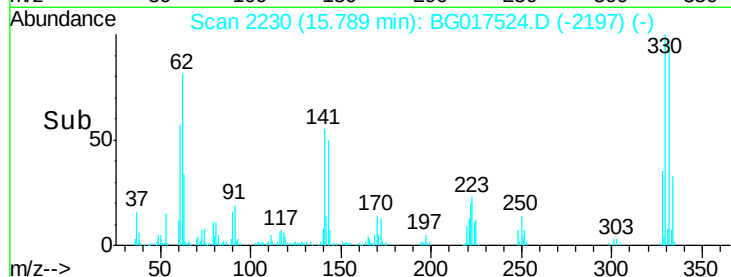
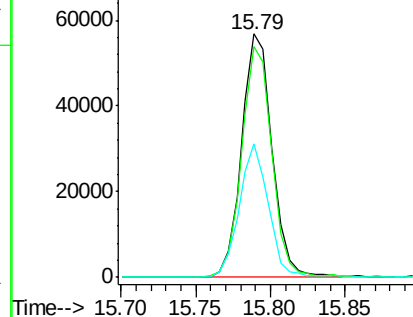



#44
 2-Fluorobiphenyl
 Concen: 84.11 ng
 RT: 12.90 min Scan# 1739
 Delta R.T. -0.01 min
 Lab File: BG017524.D
 Acq: 7 Jun 2015 8:47

Tgt Ion:172 Resp: 258224
 Ion Ratio Lower Upper
 172 100
 171 36.2 29.0 43.6
 170 21.5 18.9 28.3



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

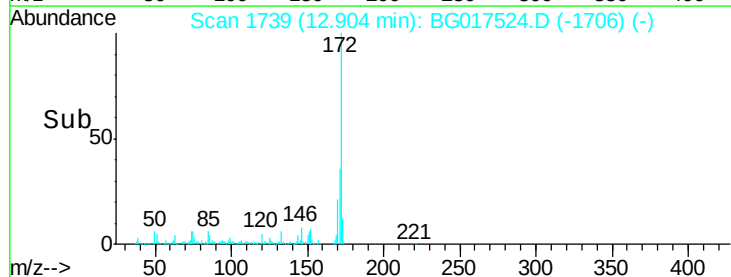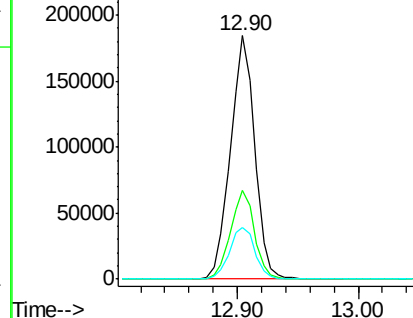


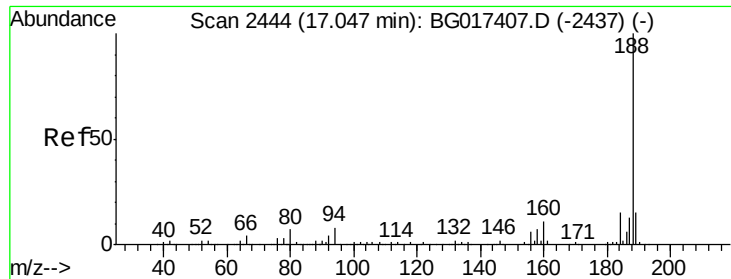




#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 17.04 min Scan# 2443
Delta R.T. -0.01 min
Lab File: BG017524.D
Acq: 7 Jun 2015 8:47

Instrument :
BNA_G
ClientSampleId :
DCW-WW-147-6415

Tgt Ion:188 Resp: 107998
Ion Ratio Lower Upper
188 100
94 9.0 6.3 9.5
80 7.6 5.2 7.8




Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BGC
Ion 80.00 (79.70 to 80.70): BGC

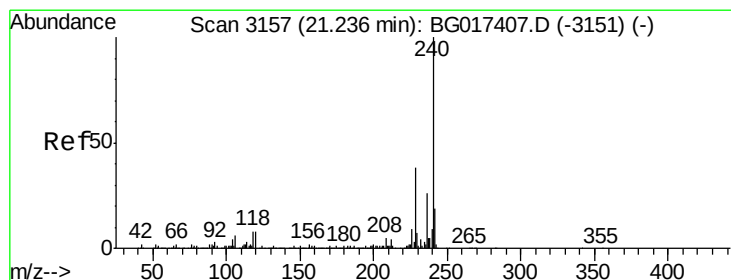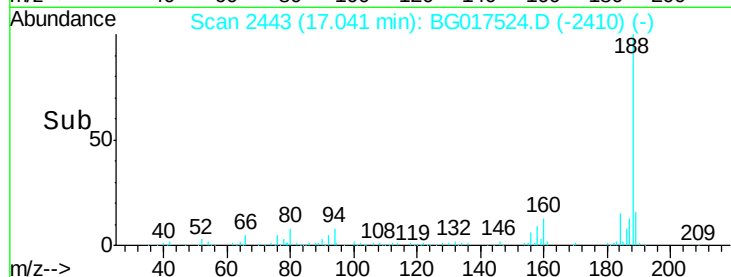
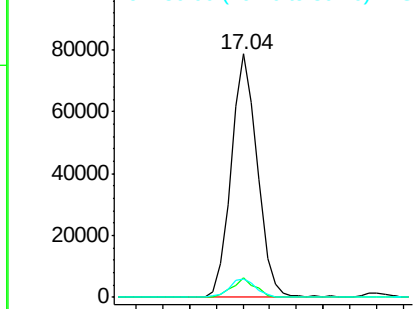



#75
Chrysene-d12
Concen: 20.00 ng
RT: 21.24 min Scan# 3157
Delta R.T. -0.00 min
Lab File: BG017524.D
Acq: 7 Jun 2015 8:47

Tgt Ion:240 Resp: 125484
Ion Ratio Lower Upper
240 100
120 7.8 6.5 9.7
236 25.0 20.8 31.2



Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

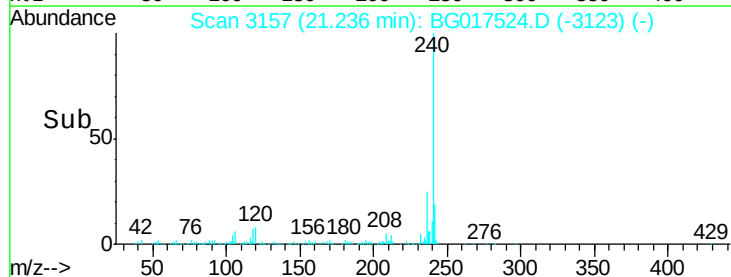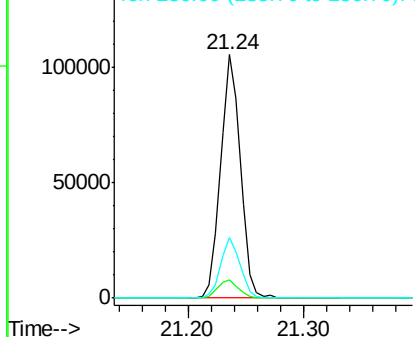

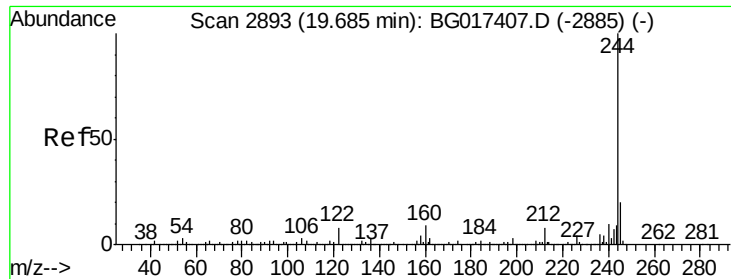

#78

Terphenyl-d14

Concen: 74.90 ng

RT: 19.68 min Scan# 2893

Delta R.T. -0.00 min

Lab File: BG017524.D

Acq: 7 Jun 2015 8:47

Instrument :

BNA_G

ClientSampleId :

DCW-WW-147-6415


Tgt Ion:244 Resp: 454748

Ion Ratio Lower Upper

244 100

212 8.9 6.4 9.6




122 8.6 6.6 10.0



Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

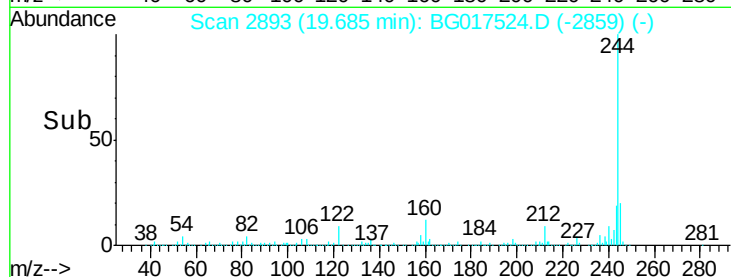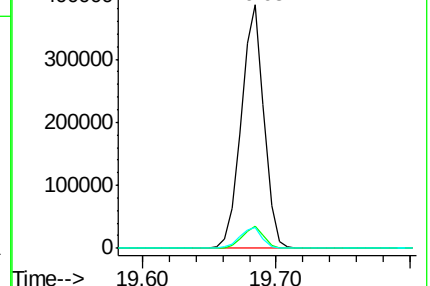

#86

Perylene-d12

Concen: 20.00 ng

RT: 23.47 min Scan# 3538

Delta R.T. 0.01 min

Lab File: BG017524.D

Acq: 7 Jun 2015 8:47


Tgt Ion:264 Resp: 124704

Ion Ratio Lower Upper

264 100

260 21.9 18.2 27.4

265 23.2 15.8 23.6



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

