

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG060615\
 Data File : BG017510.D
 Acq On : 6 Jun 2015 22:58
 Operator : TP/IZ
 Sample : G2505-04
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BE-2

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060315.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.758	8	12	17	rBV	77423	87877	5.09%	0.980%
2	3.328	105	109	115	rBV	14000	22415	1.30%	0.250%
3	4.721	341	346	352	rBV	48062	60978	3.53%	0.680%
4	5.220	422	431	442	rBV	383054	573540	33.21%	6.394%
5	6.137	584	587	596	rVB2	11643	20045	1.16%	0.223%
6	6.836	700	706	718	rBV	418952	658253	38.11%	7.339%
7	7.165	754	762	772	rBV	420629	649006	37.57%	7.236%
8	7.617	833	839	846	rBV	74276	118868	6.88%	1.325%
9	7.941	885	894	903	rBV	292293	446366	25.84%	4.977%
10	8.787	1027	1038	1048	rBV	251219	414480	24.00%	4.621%
11	10.414	1310	1315	1324	rBV	96299	163910	9.49%	1.827%
12	12.635	1687	1693	1701	rBV4	19993	31800	1.84%	0.355%
13	12.905	1732	1739	1747	rBV	674578	981799	56.84%	10.946%
14	13.751	1878	1883	1892	rBV	97461	147539	8.54%	1.645%
15	14.292	1967	1975	1984	rBV2	174049	260635	15.09%	2.906%
16	15.150	2116	2121	2127	rVB2	20075	25089	1.45%	0.280%
17	15.555	2184	2190	2194	rVB3	12607	21837	1.26%	0.243%
18	15.790	2222	2230	2245	rBV	630608	933200	54.03%	10.404%
19	16.013	2264	2268	2270	rBV2	32789	45243	2.62%	0.504%
20	16.807	2398	2403	2407	rBV2	33610	41323	2.39%	0.461%
21	16.859	2408	2412	2416	rVB3	19647	25212	1.46%	0.281%
22	17.047	2438	2444	2451	rBV	242190	343389	19.88%	3.828%
23	17.547	2525	2529	2533	rBV	33555	39545	2.29%	0.441%
24	17.952	2594	2598	2604	rBV3	58971	85394	4.94%	0.952%
25	18.240	2643	2647	2651	rBV	25195	32622	1.89%	0.364%
26	18.881	2752	2756	2760	rBV3	18885	24310	1.41%	0.271%
27	19.245	2811	2818	2824	rBV4	21901	41757	2.42%	0.466%
28	19.686	2887	2893	2898	rBV	1470159	1727246	100.00%	19.257%
29	20.949	3104	3108	3114	rBV2	86477	111458	6.45%	1.243%
30	21.243	3152	3158	3163	rBV	306637	400386	23.18%	4.464%
31	22.412	3350	3357	3363	rBV6	18876	31118	1.80%	0.347%
32	23.475	3532	3538	3546	rBV	210454	383132	22.18%	4.272%
33	25.767	3921	3928	3930	rBV7	11004	19584	1.13%	0.218%

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG060615\
Data File : BG017510.D
Acq On : 6 Jun 2015 22:58
Operator : TP/IZ
Sample : G2505-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BE-2

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060315.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION


Sum of corrected areas: 8969356

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG060615\
Data File : BG017510.D
Acq On : 6 Jun 2015 22:58
Operator : TP/IZ
Sample : G2505-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BE-2

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

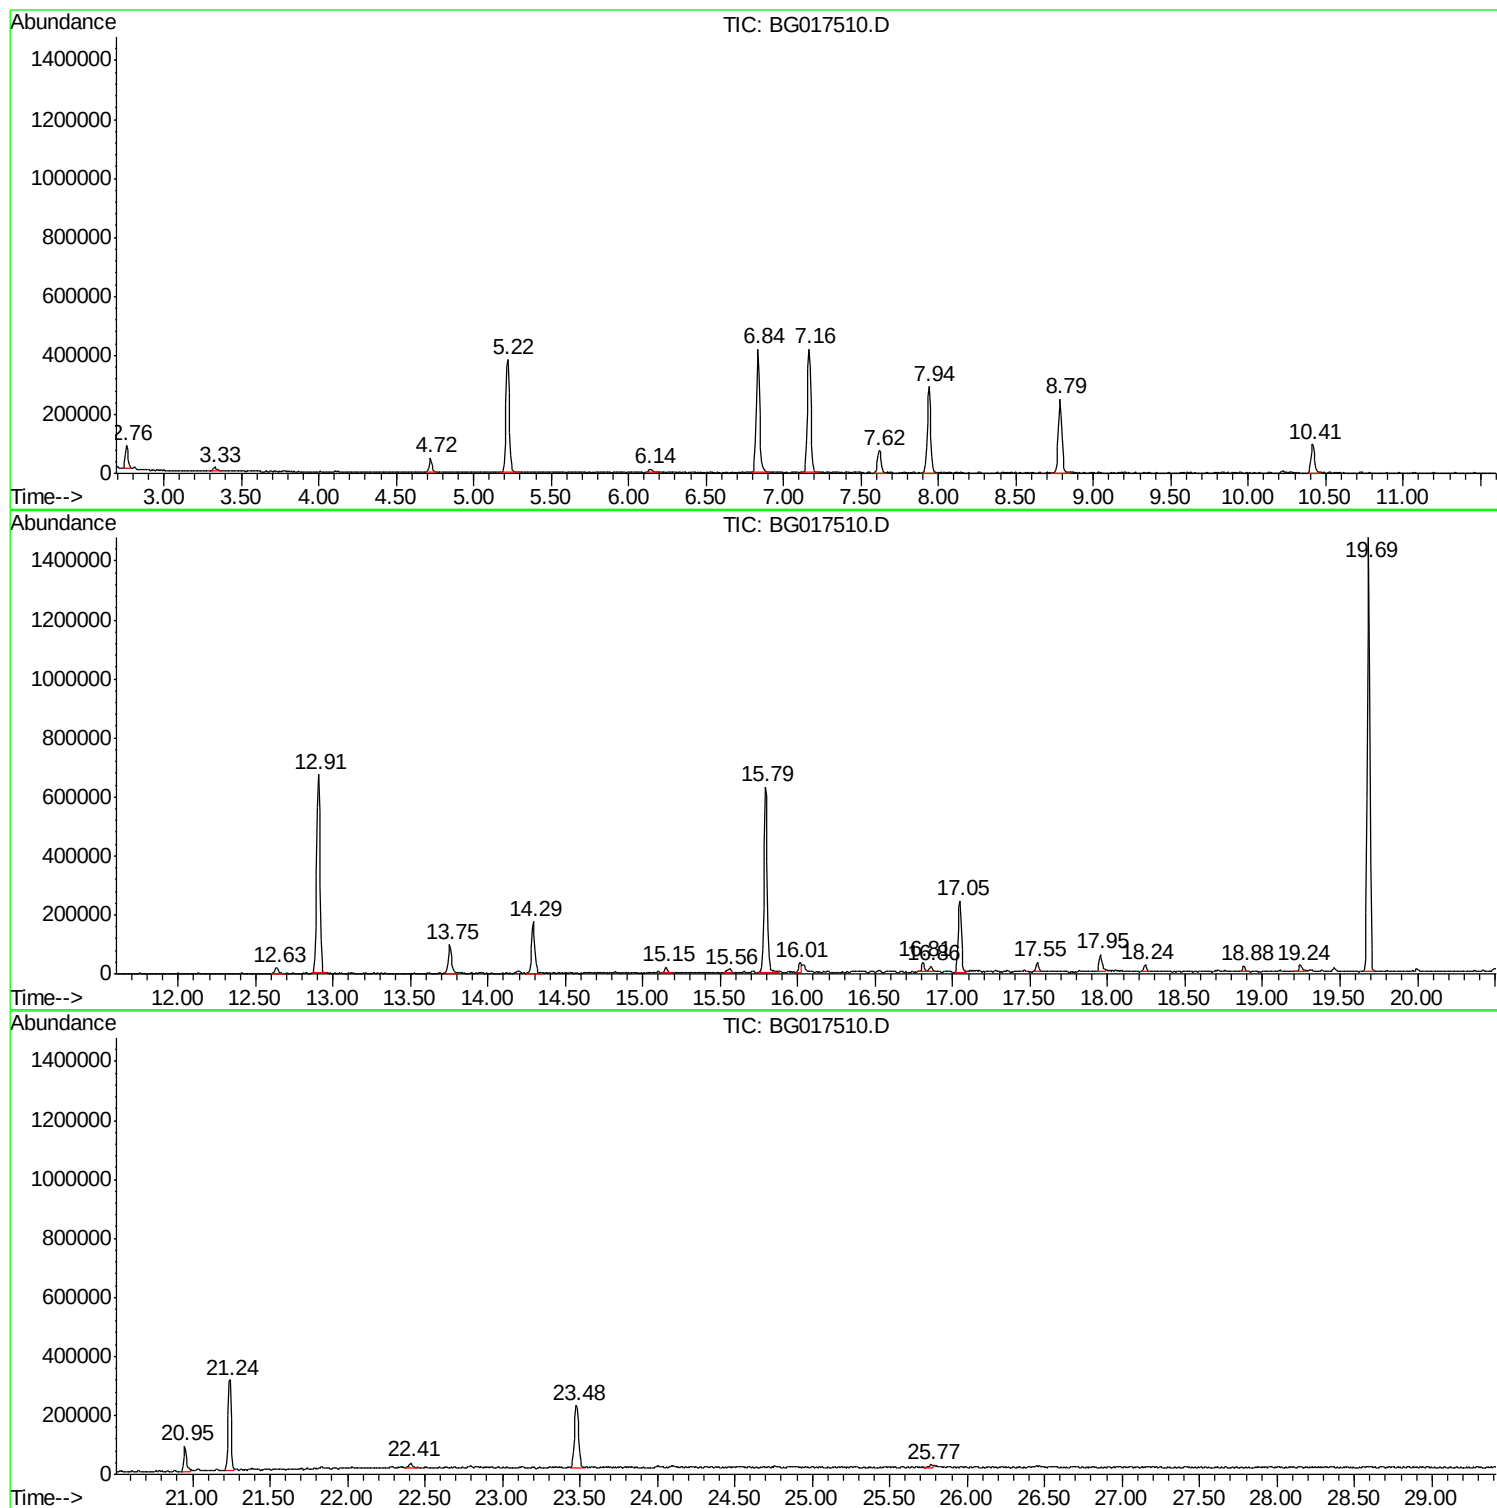

DbaaaPath::ZZ\NRPBMM1BNAAGCDBAA\BB0000655\
 DbaaaFile::BB0013500DD
 AcqQOn :: 66Jun2005 222588
 Operator::TPPIZ
 Sample::G02005004
 Misc::
 ASSVal::88 SampleMultiplier:11

Instrument :
 BNA_G
 ClientSampleId :
 BE-2

QcadtMebdd::ZZ\NRPBMM1BNAAGCMEH00S8270BB000035MM
 QcadtTitle::ASBPBNASSANDABBSF00R55P000NTCALIBRATION

TICLibrary::CC\DATA\BBSSEN05002LL
 TICIntegratIonParameters:LS6CNTPP

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
				#	RT Resp Conc

No Library Search Compounds Detected
