

Data Path : Z:\HPCHEM1\BNA\_G\DATA\BG060615\  
 Data File : BG017511.D  
 Acq On : 6 Jun 2015 23:33  
 Operator : TP/IZ  
 Sample : G2457-19  
 Misc :  
 ALS Vial : 9 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 SP-2

Integration Parameters: rteint.p  
 Integrator: RTE  
 Smoothing : ON Filtering: 5  
 Sampling : 1 Min Area: 3 % of largest Peak  
 Start Thrs: 0.2 Max Peaks: 100  
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
 Peak separation: 5

Method : Z:\HPCHEM1\BNA\_G\METHODS\8270-BG060315.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 2.781       | 10            | 16          | 23           | rVB      | 197730         | 293811        | 15.54%          | 3.567%        |
| 2         | 4.726       | 343           | 347         | 353          | rVB      | 47489          | 60937         | 3.22%           | 0.740%        |
| 3         | 5.219       | 424           | 431         | 442          | rBV      | 368912         | 528846        | 27.96%          | 6.421%        |
| 4         | 6.835       | 700           | 706         | 716          | rBV      | 341686         | 535144        | 28.30%          | 6.498%        |
| 5         | 7.164       | 755           | 762         | 772          | rBV      | 409790         | 622413        | 32.91%          | 7.557%        |
| 6         | 7.616       | 834           | 839         | 846          | rVB      | 74671          | 114834        | 6.07%           | 1.394%        |
| 7         | 7.939       | 888           | 894         | 902          | rVB      | 291823         | 451801        | 23.89%          | 5.486%        |
| 8         | 8.786       | 1031          | 1038        | 1049         | rBV      | 241103         | 403084        | 21.31%          | 4.894%        |
| 9         | 10.419      | 1309          | 1316        | 1326         | rVB      | 84846          | 149502        | 7.90%           | 1.815%        |
| 10        | 12.904      | 1733          | 1739        | 1751         | rBV      | 671783         | 949396        | 50.20%          | 11.527%       |
| 11        | 14.291      | 1966          | 1975        | 1984         | rBV2     | 153421         | 231689        | 12.25%          | 2.813%        |
| 12        | 15.795      | 2221          | 2231        | 2246         | rBV      | 594868         | 926770        | 49.00%          | 11.253%       |
| 13        | 17.046      | 2438          | 2444        | 2452         | rVB2     | 208920         | 302586        | 16.00%          | 3.674%        |
| 14        | 17.957      | 2595          | 2599        | 2608         | rBV9     | 15966          | 37505         | 1.98%           | 0.455%        |
| 15        | 19.685      | 2887          | 2893        | 2898         | rBV      | 1624832        | 1891283       | 100.00%         | 22.964%       |
| 16        | 21.236      | 3152          | 3157        | 3169         | rBV      | 286479         | 379308        | 20.06%          | 4.606%        |
| 17        | 23.480      | 3531          | 3539        | 3546         | rBV      | 191351         | 357062        | 18.88%          | 4.335%        |


Sum of corrected areas: 8235971

Data Path : Z:\HPCHEM1\BNA\_G\DATA\BG060615\  
Data File : BG017511.D  
Acq On : 6 Jun 2015 23:33  
Operator : TP/IZ  
Sample : G2457-19  
Misc :  
ALS Vial : 9 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
SP-2

Quant Method : Z:\HPCHEM1\BNA\_G\METHODS\8270-BG060315.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L  
TIC Integration Parameters: LSCINT.P

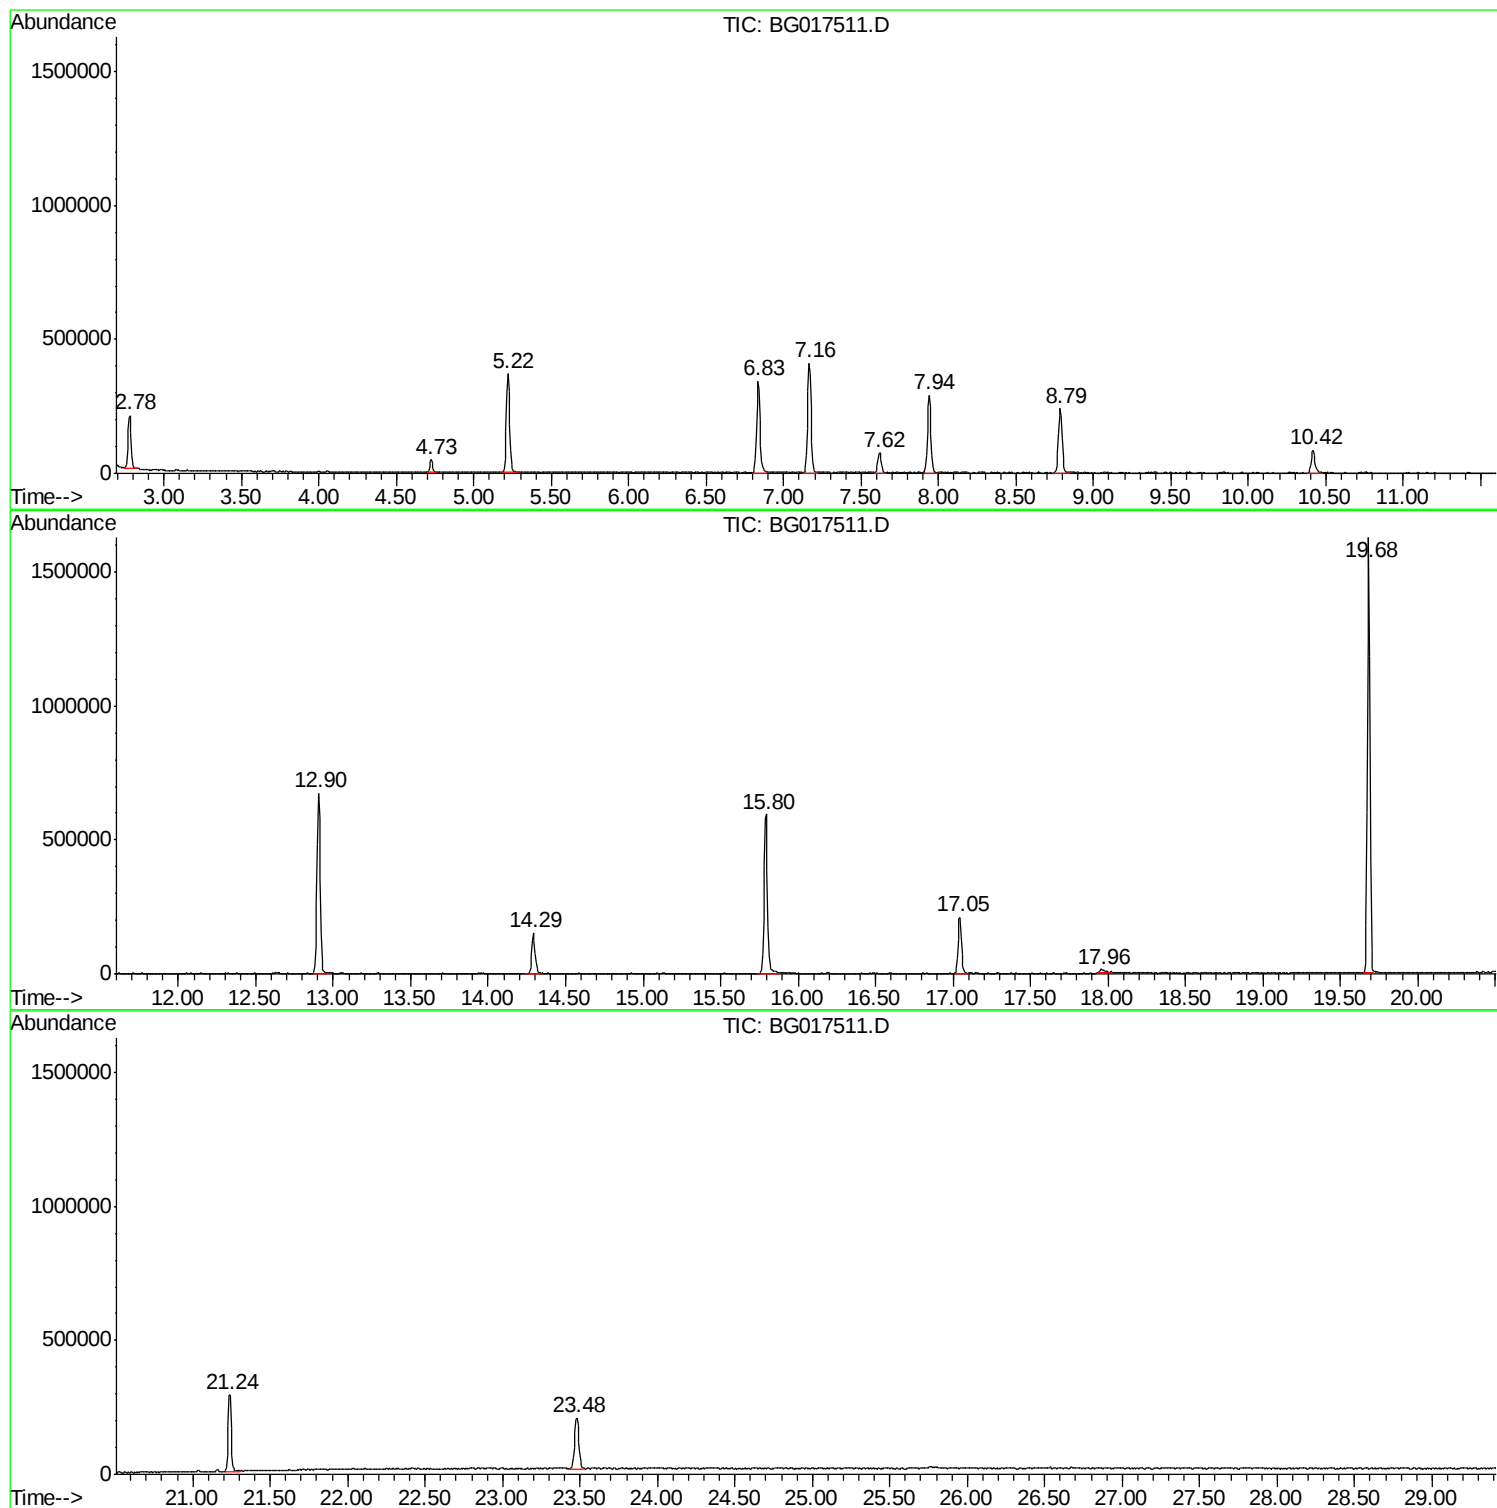

DbaaaPathh::ZZ\NRPBHHM1BBAAGCDBAAAB00000655\  
 DbaaaFile::BB0073511DD  
 Aeqq00n :: 66Jun2005 233333  
 Opeaaor ::TPPIZ  
 Sample ::G02337199  
 Misc ::  
 AASSVal ::99 SampleMultiplier:11

Instrument :  
 BNA\_G  
 ClientSampleId :  
 SP-2

QqaabMebbdd::ZZ\NRPBHHM1BBAAGCMEEH00S8270BB000035MM  
 QqaabTitle ::ASBPBNAASSANDBBSF00R55P000NTCALIBRATION

TICCLibbaay ::CC\DATAABASSEN0\$5002LL  
 TICIntegratioonPaaameess:LS6CNTPP

| TIC Top Hit name | RT | EstConc | Units | Response | ---Internal Standard--- |
|------------------|----|---------|-------|----------|-------------------------|
|                  |    |         |       | #        | RT Resp Conc            |

No Library Search Compounds Detected

\*\*\*\*\*